
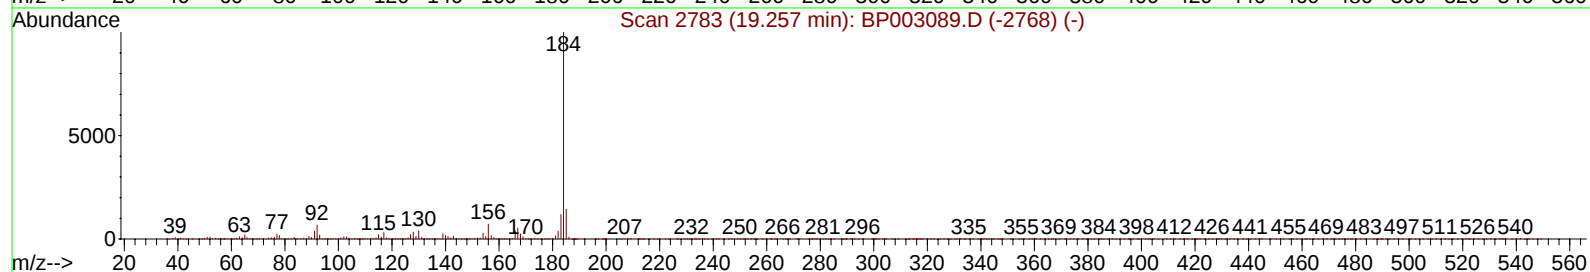
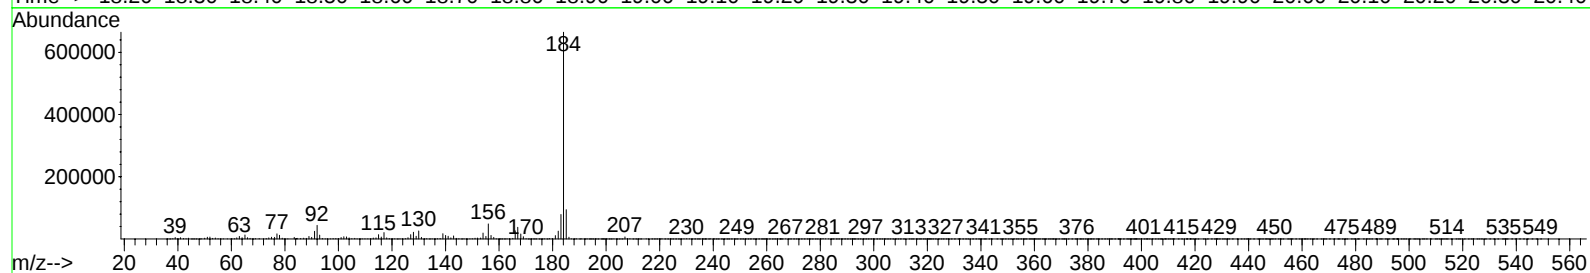


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP090320\
 Data File : BP003196.D
 Acq On : 03 Sep 2020 08:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 18:47:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 01 14:37:05 2020
 Response via : Initial Calibration

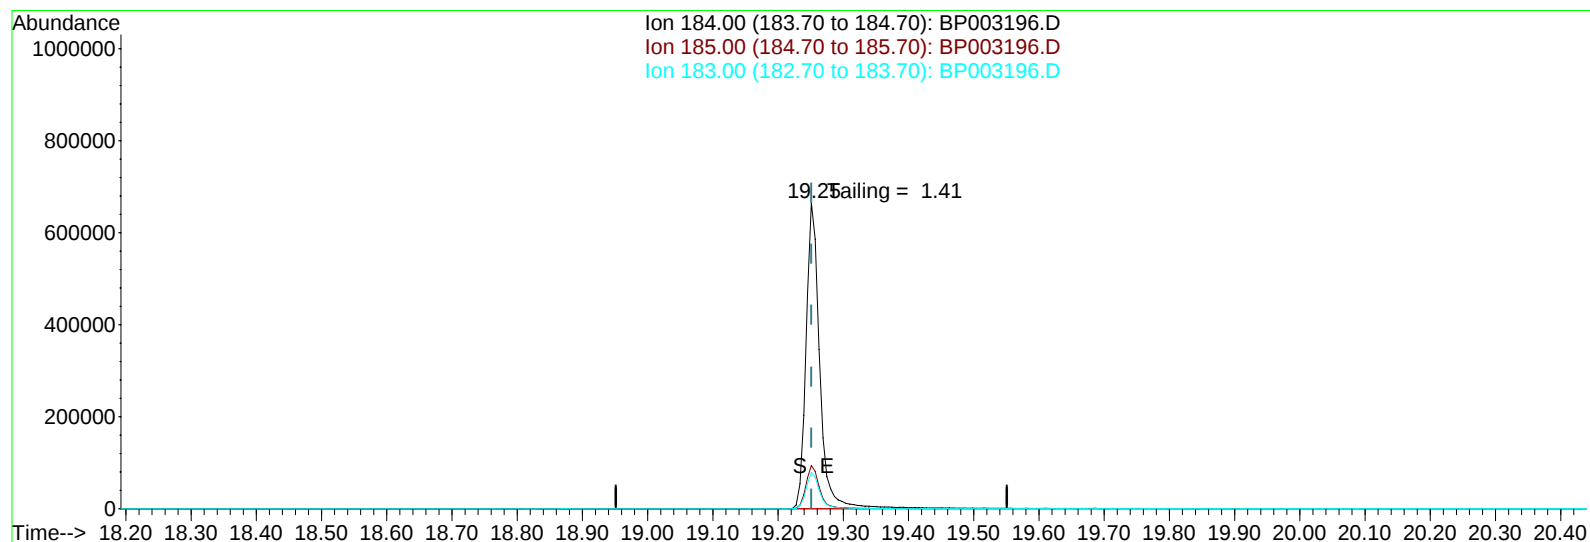

TIC: BP003196.D

(77) Benzidine




19.251min (-0.000) 155614.81ng

response 974500

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.18
183.00	12.00	11.87
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP090320\
 Data File : BP003196.D
 Acq On : 03 Sep 2020 08:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 18:47:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 01 14:37:05 2020
 Response via : Initial Calibration

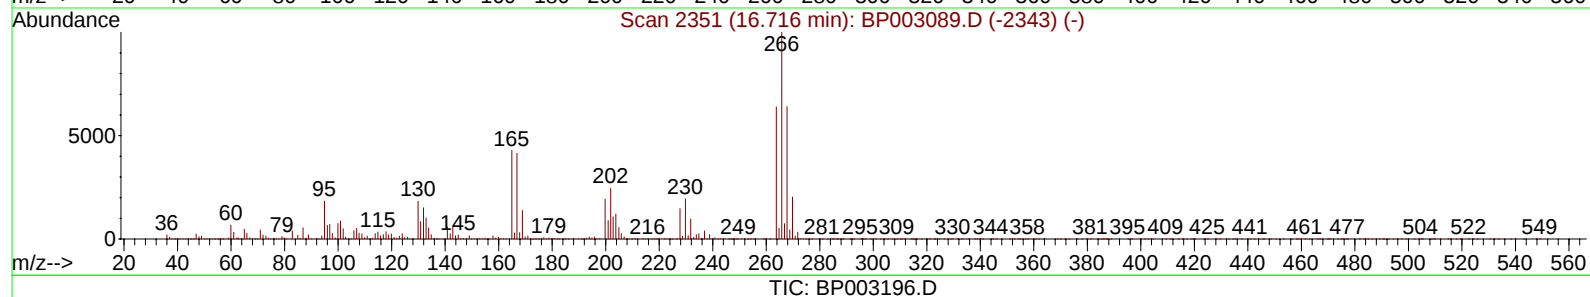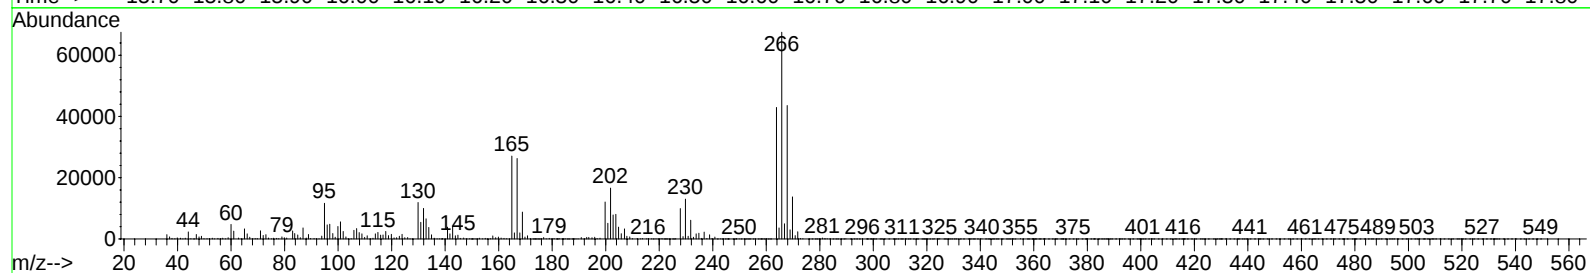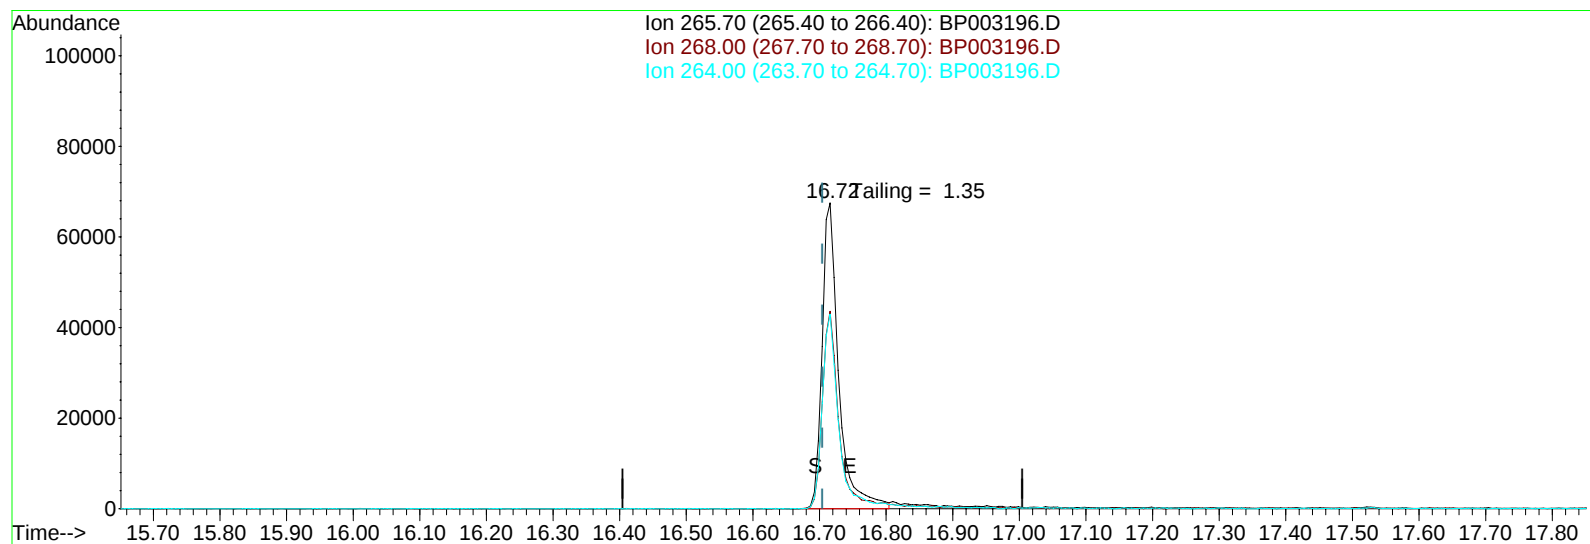

(70) Pentachlorophenol (C)

16.716min (+0.012) 221617.08ng

response 119755

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.58
264.00	63.30	63.65
0.00	0.00	0.00