


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090320\
 Data File : BP003196.D
 Acq On : 03 Sep 2020 08:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 01 14:37:05 2020

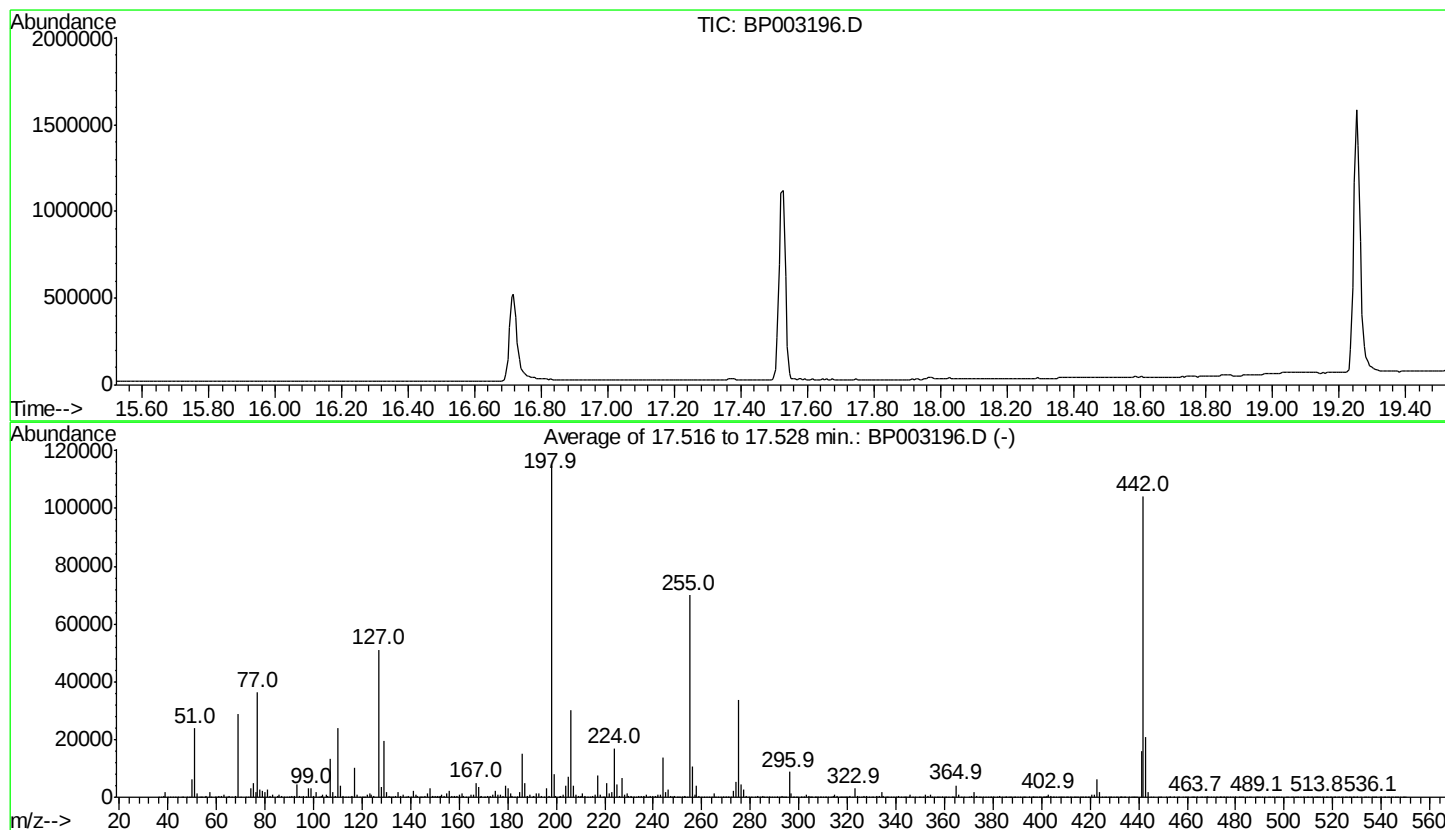

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.8	23825	PASS
68	69	0.00	2	1.9	558	PASS
69	198	0.00	100	25.2	28949	PASS
70	69	0.00	2	0.4	106	PASS
127	198	10	80	44.5	51058	PASS
197	198	0.00	2	0.5	591	PASS
198	198	100	100	100.0	114808	PASS
199	198	5	9	7.0	8023	PASS
275	198	10	60	29.2	33531	PASS
365	198	1	100	3.6	4156	PASS
441	198	0.01	100	14.0	16033	PASS
442	198	50	100	90.6	104069	PASS
443	442	15	24	19.8	20656	PASS