

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090324\
Data File : BP021792.D
Acq On : 03 Sep 2024 17:47
Operator : RC/JU
Sample : PB163070BL
Misc :
ALS Vial : 8 Sample Multiplier: 1




Instrument :
BNA_P
ClientSampleId :
SBLK070

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/04/2024
Supervised By :mohammad ahmed 09/07/2024

Supervised By :mohammad
ahmed
09/07/2024

Supervised By :mohammad
ahmed

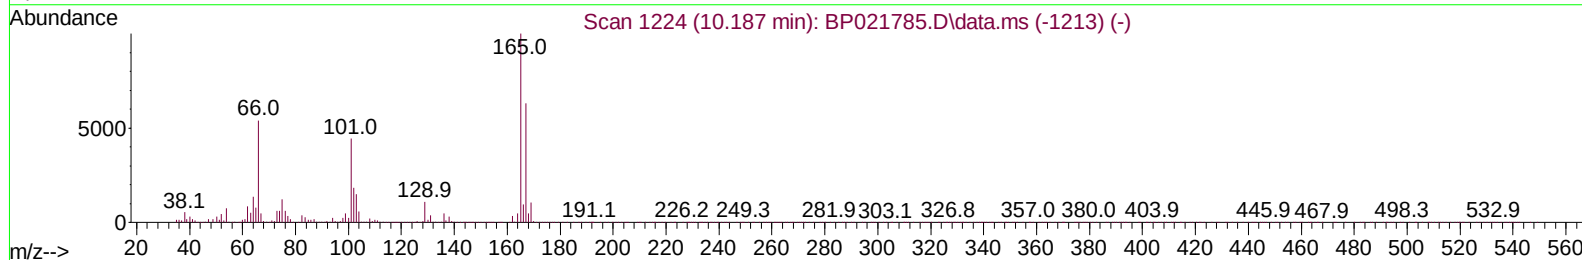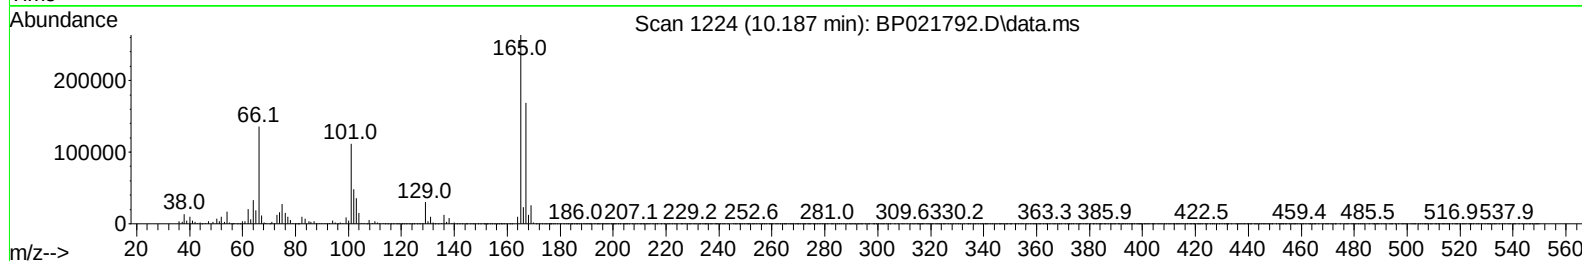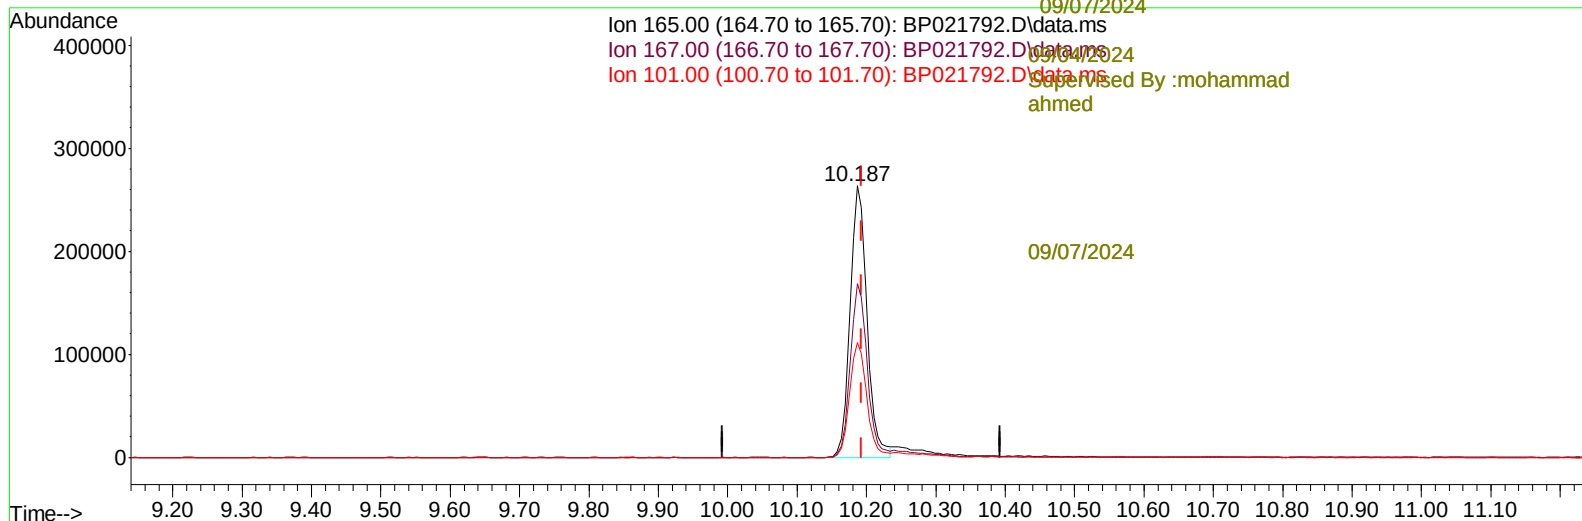

TIC: BP021792.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.187min (-0.006) 22.27 ng/uI

response 446680

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.10	63.91
101.00	41.40	42.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090324\
Data File : BP021792.D
Acq On : 03 Sep 2024 17:47
Operator : RC/JU
Sample : PB163070BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK070


Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/04/2024
Supervised By :mohammad ahmed 09/07/2024


Supervised By :mohammad
ahmed
09/07/2024

Quant Time: Sep 04 04:01:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration


Ion 165.00 (164.70 to 165.70): BP021792.D\data.ms
Ion 167.00 (166.70 to 167.70): BP021792.D\data.ms
Ion 101.00 (100.70 to 101.70): BP021792.D\data.ms

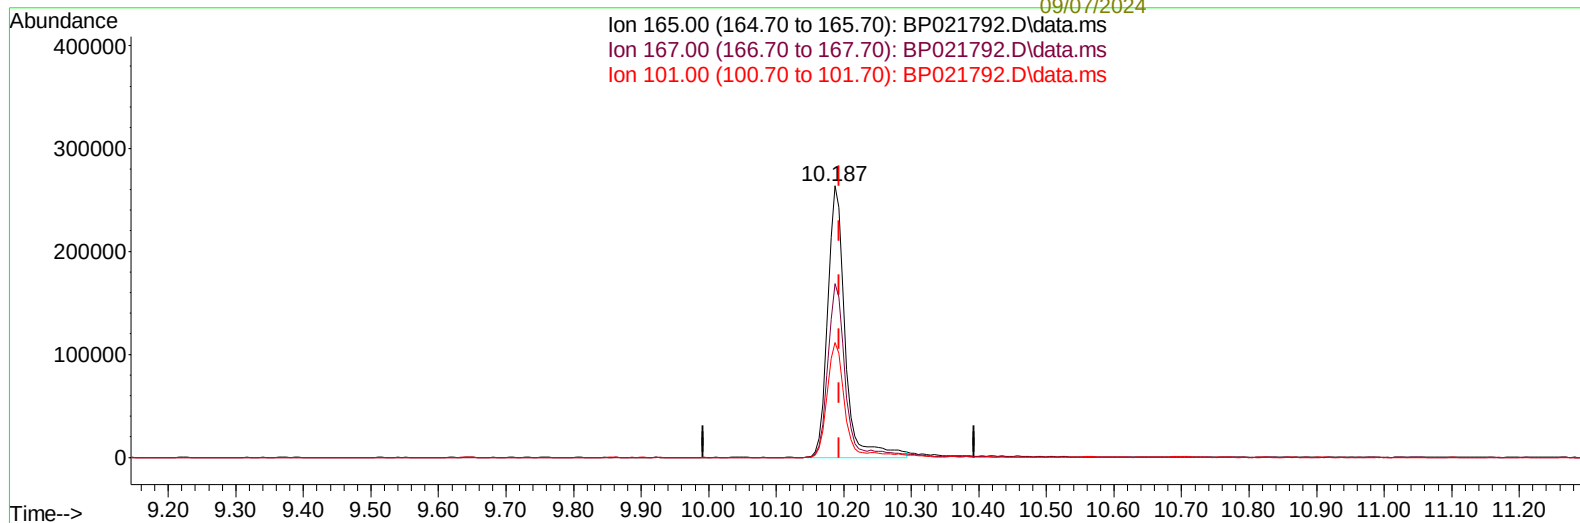

Scan 1224 (10.187 min): BP021792.D\data.ms

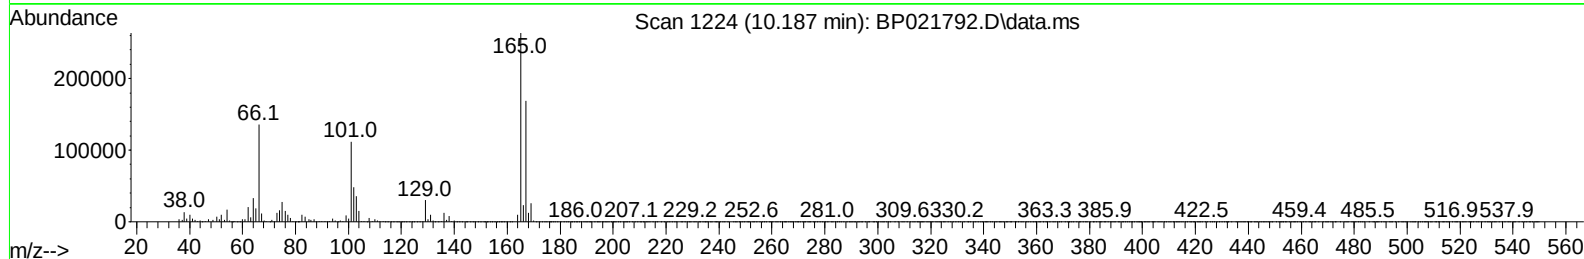

Scan 1224 (10.187 min): BP021785.D\data.ms (-1213) (-)

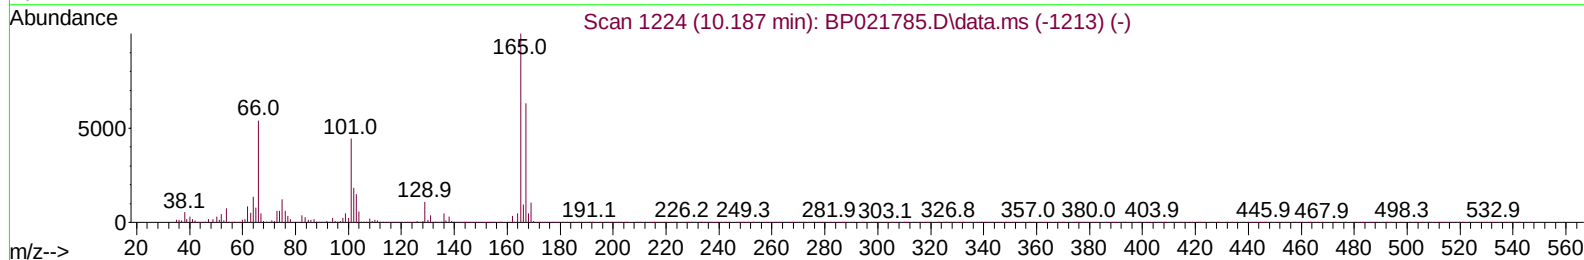

TIC: BP021792.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.187min (-0.006) 23.69 ng/ul m

response 475046

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.10	63.91
101.00	41.40	42.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090324\
Data File : BP021792.D
Acq On : 03 Sep 2024 17:47
Operator : RC/JU
Sample : PB163070BL
Misc :
ALS Vial : 8 Sample Multiplier: 1




Instrument :
BNA_P
ClientSampleId :
SBLK070

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/04/2024
Supervised By :mohammad ahmed 09/07/2024

Supervised By :mohammad
ahmed
09/07/2024

Quant Time: Sep 04 04:01:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration

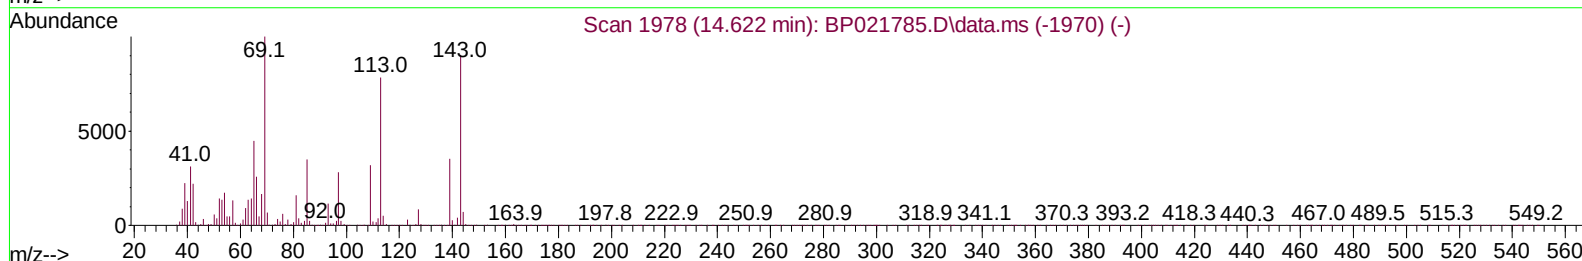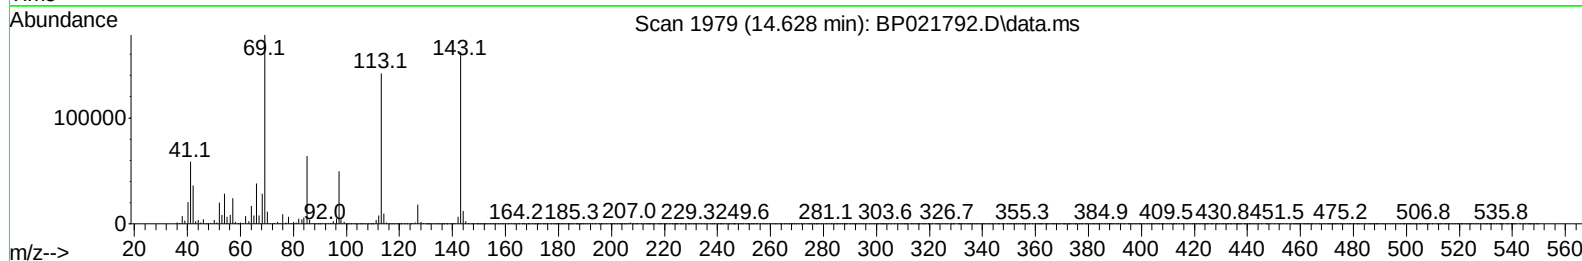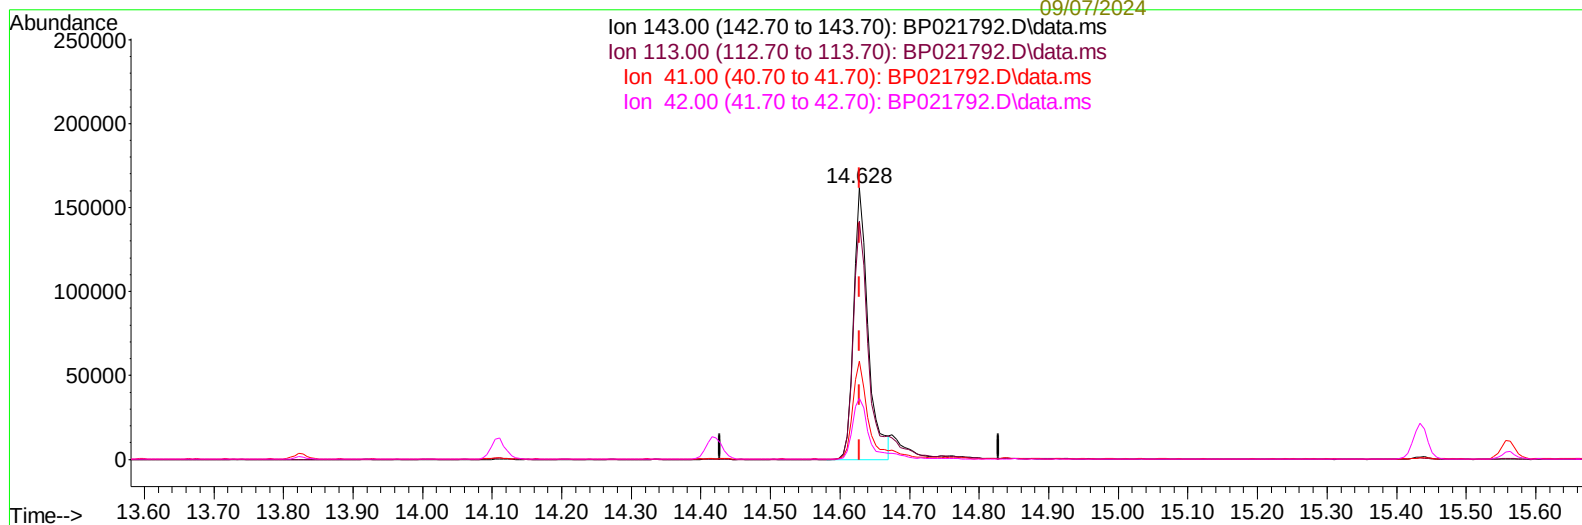

TIC: BP021792.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.628min (+ 0.000) 20.18 ng/ul

response 232448

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	83.10	87.85
41.00	33.90	36.11
42.00	23.00	22.62

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090324\
Data File : BP021792.D
Acq On : 03 Sep 2024 17:47
Operator : RC/JU
Sample : PB163070BL
Misc :
ALS Vial : 8 Sample Multiplier: 1




Instrument :
BNA_P
ClientSampleId :
SBLK070

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/04/2024
Supervised By :mohammad ahmed 09/07/2024

Supervised By :mohammad
ahmed
09/07/2024

Quant Time: Sep 04 04:01:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration

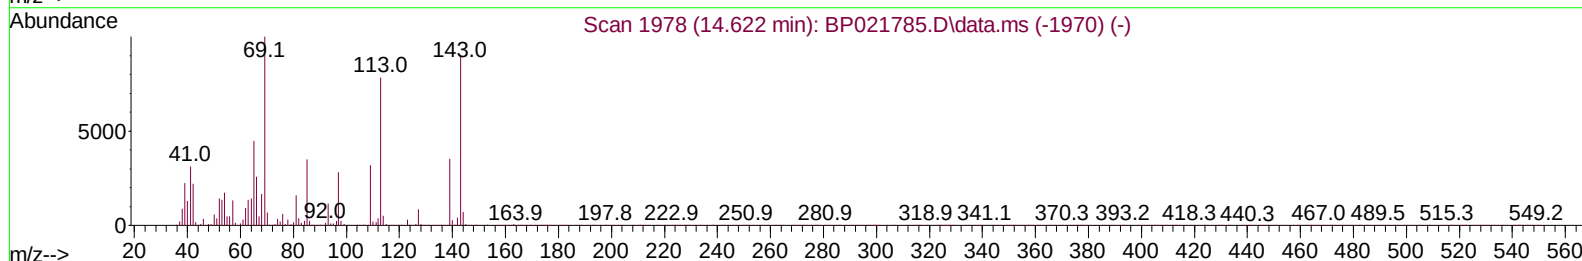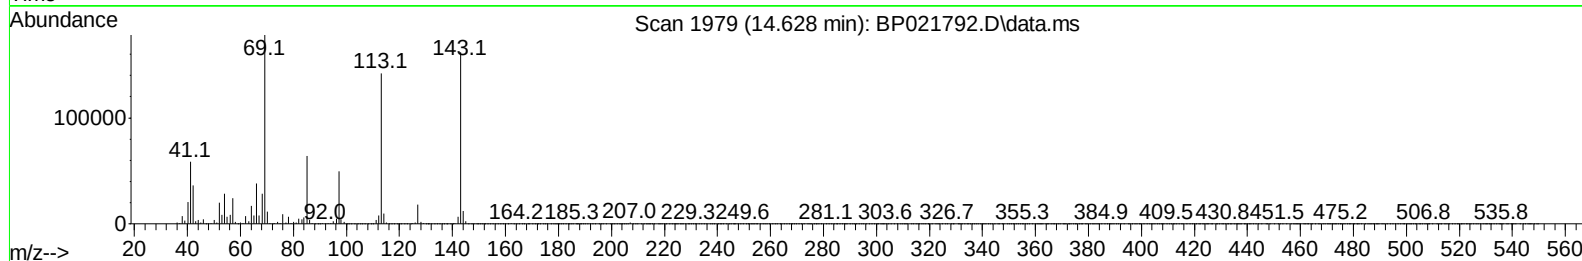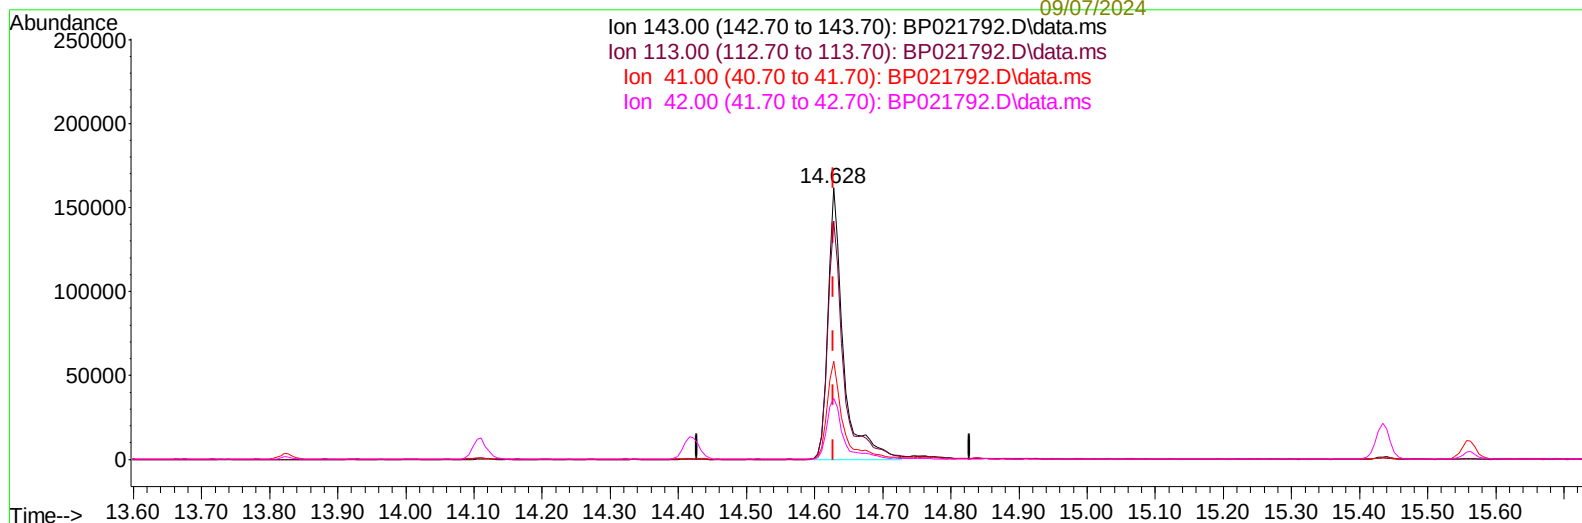

TIC: BP021792.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.628min (+ 0.000) 22.11 ng/ul m

response 254746

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	83.10	87.85
41.00	33.90	36.11
42.00	23.00	22.62

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090324\
 Data File : BP021792.D
 Acq On : 03 Sep 2024 17:47
 Operator : RC/JU
 Sample : PB163070BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK070

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/04/2024
 Supervised By :mohammad ahmed 09/07/2024

Supervised By :mohammad
 ahmed
 09/07/2024

Quant Time: Sep 04 04:42:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 29 23:56:59 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.775	152		315590	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.563	136		1246125	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.422	164		791337	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.240	188		1747453	20.000	ng/ul	0.01
79) Chrysene-d12	21.680	240		1792967	20.000	ng/ul	0.01
88) Perylene-d12	25.092	264		1959725	20.000	ng/ul	0.03
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.270	96		50834	5.348	ng/uL	0.00
4) Pyridine-d5	3.681	84		653871	23.781	ng/ul	0.00
7) Phenol-d5	6.952	99		823499	24.451	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.111	67		465564	25.401	ng/ul	0.00
11) 2-Chlorophenol-d4	7.316	132		542123	24.932	ng/ul	0.00
15) 4-Methylphenol-d8	8.475	113		602692	23.158	ng/ul	-0.01
21) Nitrobenzene-d5	8.928	128		260911	26.025	ng/ul	0.00
24) 2-Nitrophenol-d4	9.646	143		266242	26.162	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.187	165		475046m	23.688	ng/ul	0.00
31) 4-Chloroaniline-d4	10.699	131		685701	23.502	ng/ul	0.00
46) Dimethylphthalate-d6	13.822	166		1643254	27.138	ng/ul	-0.02
49) Acenaphthylene-d8	14.110	160		1740276	25.599	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.628	143		254746m	22.114	ng/ul	0.00
60) Fluorene-d10	15.434	176		1372366	26.959	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.563	200		199590	20.767	ng/ul	0.00
73) Anthracene-d10	17.340	188		2209716	26.645	ng/ul	0.00
81) Pyrene-d10	19.704	212		2758140	26.910	ng/ul	0.01
92) Benzo(a)pyrene-d12	24.851	264		2758714	26.399	ng/ul	0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090324\
Data File : BP021792.D
Acq On : 03 Sep 2024 17:47
Operator : RC/JU
Sample : PB163070BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK070

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/04/2024
Supervised By :mohammad ahmed 09/07/2024

Supervised By :mohammad
ahmed
09/07/2024

Quant Time: Sep 04 04:42:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration

