




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090324\
 Data File : BP021801.D
 Acq On : 04 Sep 2024 00:13
 Operator : RC/JU
 Sample : P3734-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44B1

Manual IntegrationsAPPROVED

Quant Time: Sep 04 04:04:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 29 23:56:59 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/04/2024
 Supervised By :mohammad ahmed 09/07/2024

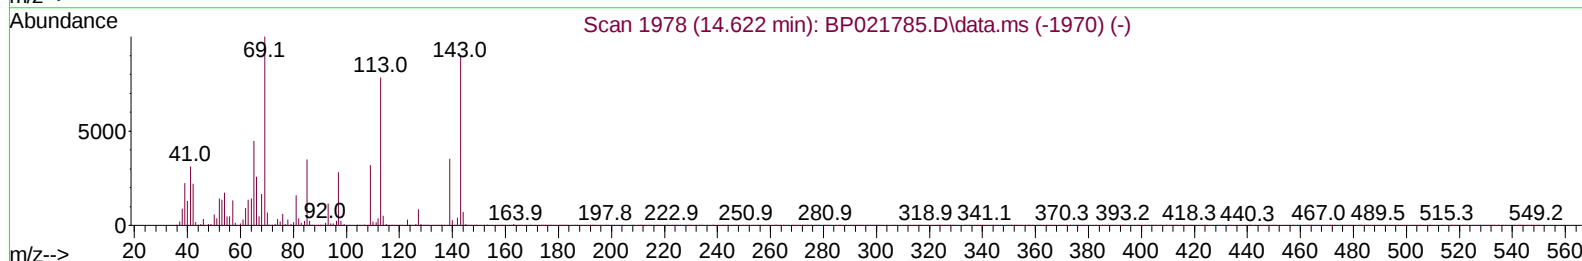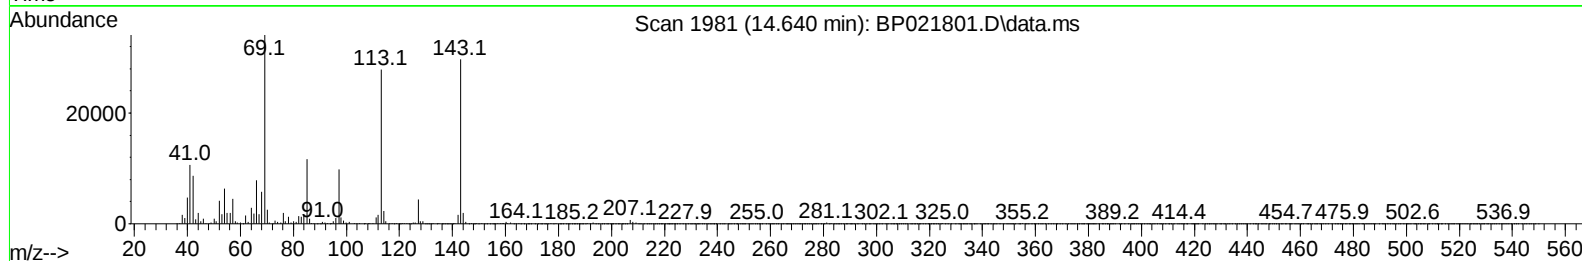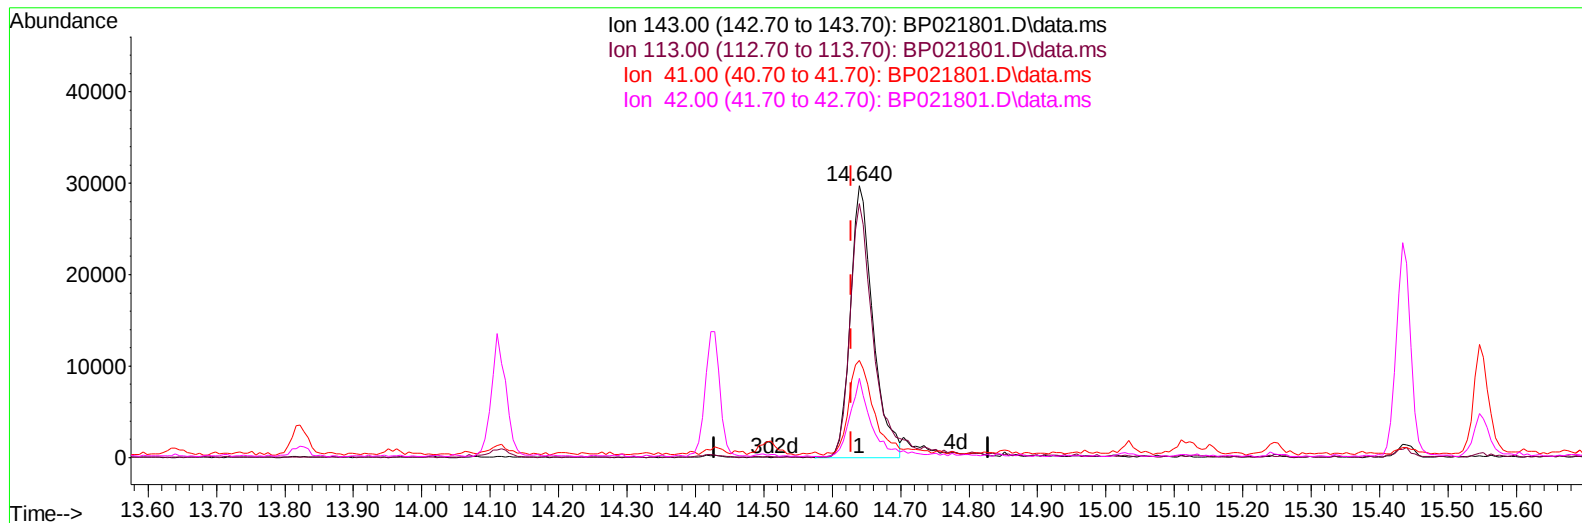

TIC: BP021801.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.640min (+ 0.012) 6.37 ng/u1

response 68252

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	83.10	93.56
41.00	33.90	35.76
42.00	23.00	29.07#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090324\
 Data File : BP021801.D
 Acq On : 04 Sep 2024 00:13
 Operator : RC/JU
 Sample : P3734-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44B1

Manual IntegrationsAPPROVED

Quant Time: Sep 04 04:04:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 29 23:56:59 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/04/2024
 Supervised By :mohammad ahmed 09/07/2024

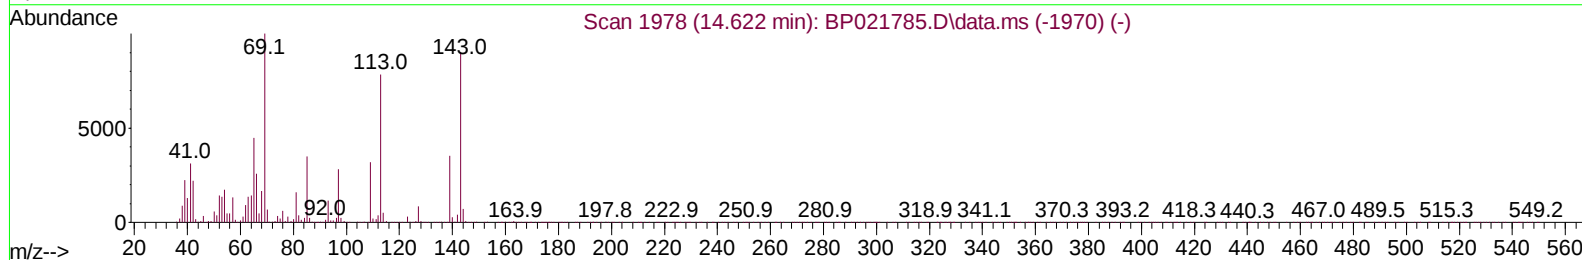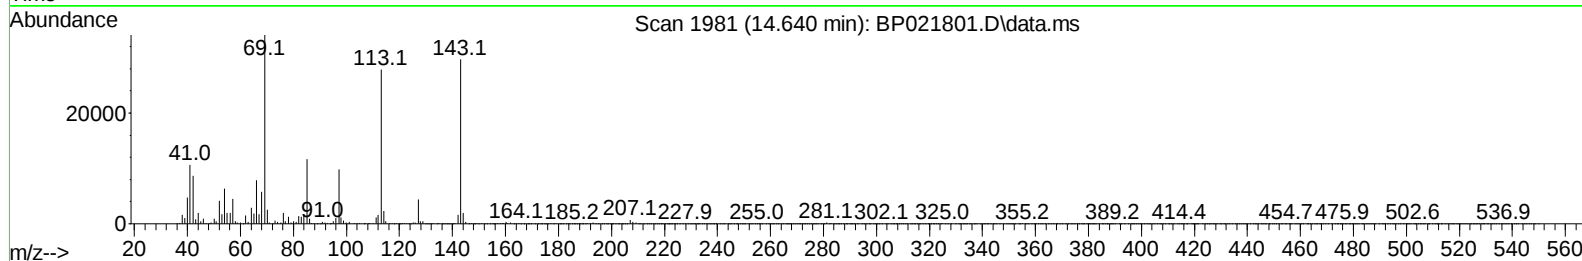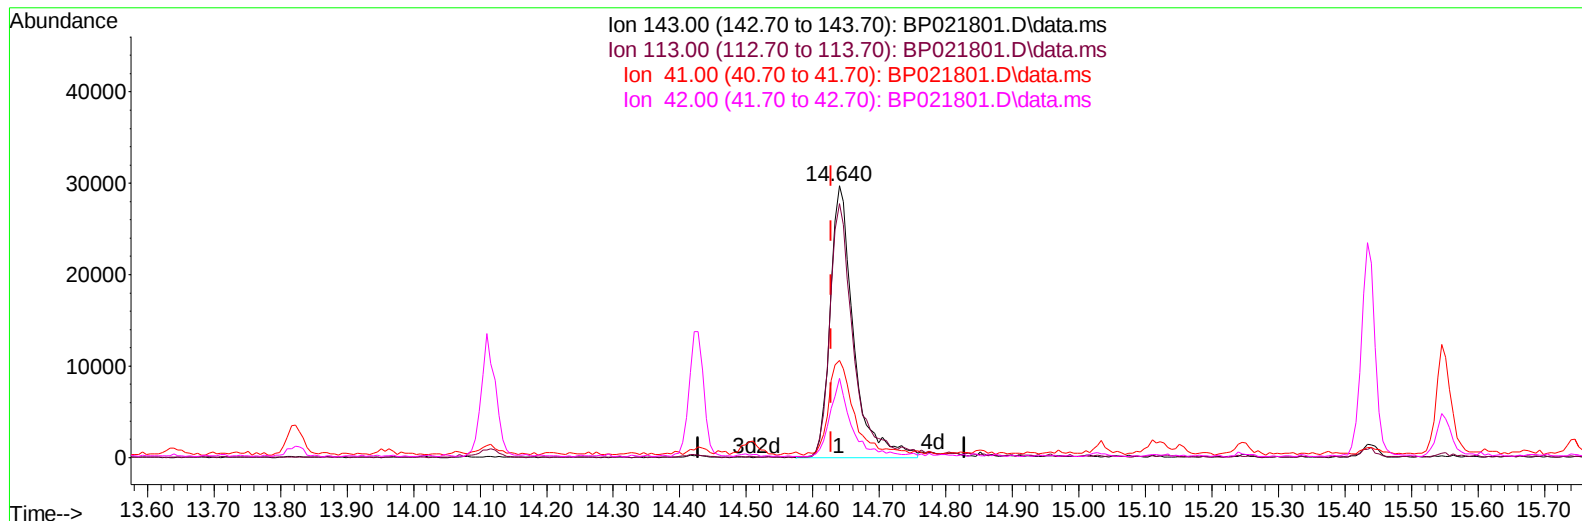

TIC: BP021801.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.640min (+ 0.012) 6.76 ng/ul m

response 72406

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	83.10	93.56
41.00	33.90	35.76
42.00	23.00	29.07#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090324\
 Data File : BP021801.D
 Acq On : 04 Sep 2024 00:13
 Operator : RC/JU
 Sample : P3734-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44B1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/04/2024
 Supervised By :mohammad ahmed 09/07/2024

Quant Time: Sep 04 05:30:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 29 23:56:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	285998	20.000	ng/ul	0.00
20) Naphthalene-d8	10.563	136	1129874	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.428	164	736059	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.228	188	1616801	20.000	ng/ul	0.00
79) Chrysene-d12	21.675	240	1625118	20.000	ng/ul	0.00
88) Perylene-d12	25.063	264	1800051	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.276	96	31299	3.633	ng/uL	0.00
4) Pyridine-d5	3.693	84	67530	2.710	ng/ul	0.00
7) Phenol-d5	6.952	99	207148	6.787	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.111	67	400009	24.082	ng/ul	0.00
11) 2-Chlorophenol-d4	7.317	132	441512	22.406	ng/ul	0.00
15) 4-Methylphenol-d8	8.481	113	351998	14.924	ng/ul	0.00
21) Nitrobenzene-d5	8.928	128	232969	25.628	ng/ul	0.00
24) 2-Nitrophenol-d4	9.646	143	233627	25.319	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.187	165	421523	23.182	ng/ul	0.00
31) 4-Chloroaniline-d4	10.693	131	216681	8.191	ng/ul	0.00
46) Dimethylphthalate-d6	13.822	166	1648825	29.275	ng/ul	-0.02
49) Acenaphthylene-d8	14.110	160	1694674	26.800	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.640	143	72406m	6.757	ng/ul	0.01
60) Fluorene-d10	15.434	176	1390538	29.367	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.546					

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090324\
Data File : BP021801.D
Acq On : 04 Sep 2024 00:13
Operator : RC/JU
Sample : P3734-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44B1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/04/2024
Supervised By :mohammad ahmed 09/07/2024

Quant Time: Sep 04 05:30:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration

