

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090324\
 Data File : BP021786.D
 Acq On : 03 Sep 2024 10:02
 Operator : RC/JU
 Sample : PB163064BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK064

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021786.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	11	rVB	156854	171194	2.81%	0.295%
2	3.117	19	22	27	rVB	23467	27115	0.44%	0.047%
3	3.275	45	49	56	rVB	93309	123076	2.02%	0.212%
4	3.687	114	119	134	rBV	1006612	1458338	23.92%	2.511%
5	4.011	171	174	182	rVB	19880	29314	0.48%	0.050%
6	6.952	666	674	689	rBV	1070992	1788626	29.33%	3.080%
7	7.110	695	701	711	rVB	955541	1446419	23.72%	2.491%
8	7.316	728	736	746	rBV	1021031	1700536	27.89%	2.928%
9	7.781	806	815	824	rBV	855415	1307856	21.45%	2.252%
10	8.481	926	934	944	rBV	1306690	2110950	34.62%	3.635%
11	8.922	1000	1009	1021	rBV	910237	1596232	26.18%	2.749%
12	9.646	1124	1132	1142	rBV	697951	1178493	19.33%	2.029%
13	10.193	1215	1225	1233	rBV	964737	1760539	28.87%	3.032%
14	10.569	1280	1289	1297	rBV	903944	1710122	28.05%	2.945%
15	10.693	1303	1310	1339	rVB	1079048	1864632	30.58%	3.211%
16	12.151	1551	1558	1566	rBV2	16538	32302	0.53%	0.056%
17	13.822	1836	1842	1860	rBV	1997111	2687851	44.08%	4.629%
18	14.122	1884	1893	1899	rBV	2038360	3091536	50.70%	5.324%
19	14.434	1939	1946	1960	rBV	1378510	2159163	35.41%	3.718%
20	14.639	1973	1981	1996	rBV3	425956	1309594	21.48%	2.255%
21	15.434	2109	2116	2127	rBV	2667595	4049898	66.42%	6.974%
22	15.557	2131	2137	2146	rBV	672050	989416	16.23%	1.704%
23	15.681	2154	2158	2165	rVB4	12209	24771	0.41%	0.043%
24	15.957	2200	2205	2208	rBV6	4979	9255	0.15%	0.016%
25	16.239	2249	2253	2259	rBV6	9179	14569	0.24%	0.025%
26	16.569	2305	2309	2314	rBV6	7191	10100	0.17%	0.017%
27	17.228	2414	2421	2430	rBV	1728746	2587096	42.43%	4.455%
28	17.328	2431	2438	2453	rVV	2604010	4464991	73.23%	7.689%
29	17.928	2537	2540	2544	rBV6	6283	8824	0.14%	0.015%
30	18.180	2579	2583	2586	rBV6	7602	14199	0.23%	0.024%
31	19.251	2762	2765	2771	rVB3	33857	49484	0.81%	0.085%
32	19.322	2773	2777	2781	rBV3	37083	54005	0.89%	0.093%
33	19.692	2834	2840	2853	rBV	3955117	5649613	92.65%	9.729%
34	21.674	3171	3177	3184	rVB	1906508	3094950	50.76%	5.330%
35	24.845	3707	3716	3730	rVB	2176637	6097536	100.00%	10.501%
36	25.074	3747	3755	3771	rVB	1226965	3396306	55.70%	5.849%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090324\
Data File : BP021786.D
Acq On : 03 Sep 2024 10:02
Operator : RC/JU
Sample : PB163064BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK064

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 58068901

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090324\
Data File : BP021786.D
Acq On : 03 Sep 2024 10:02
Operator : RC/JU
Sample : PB163064BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK064

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

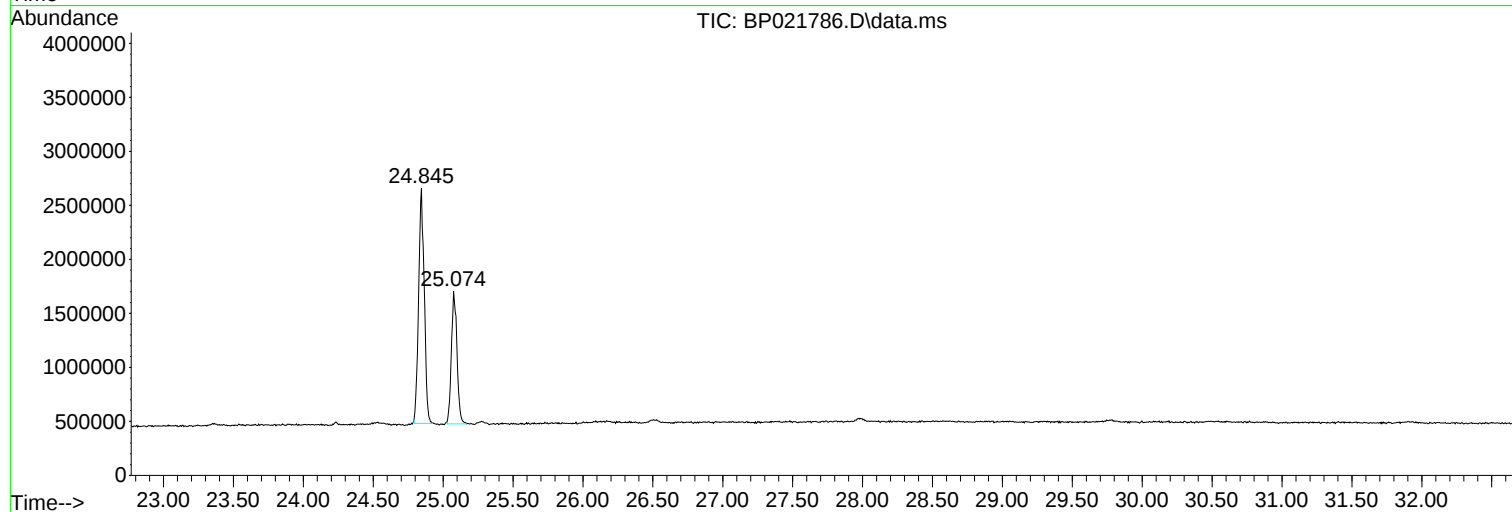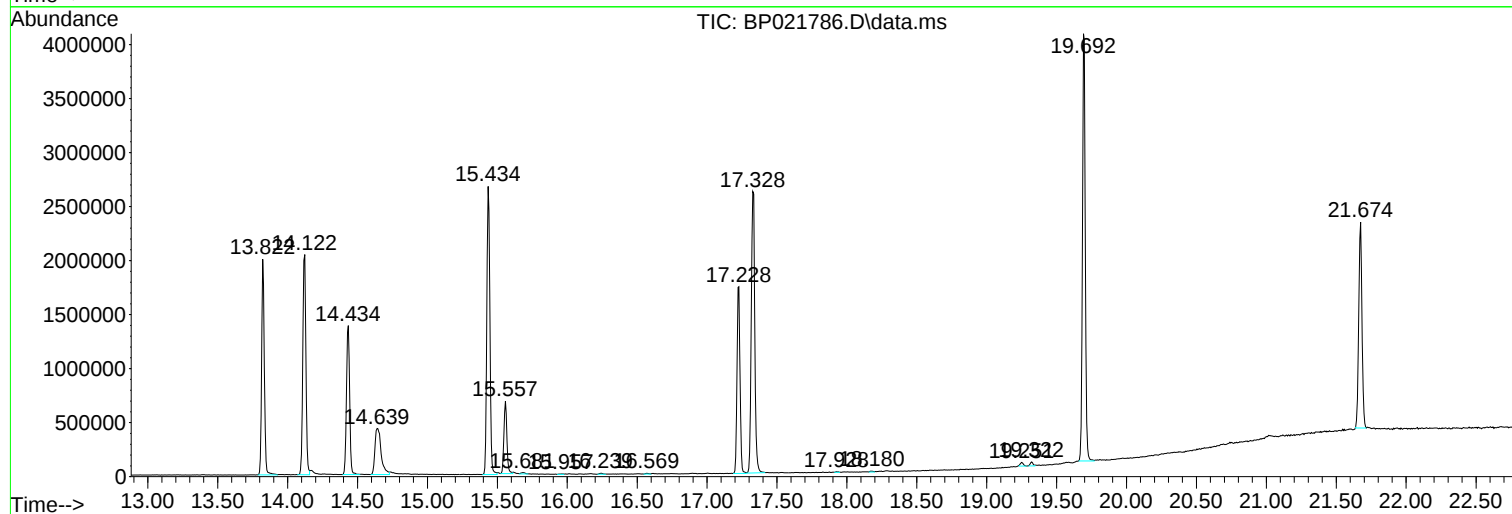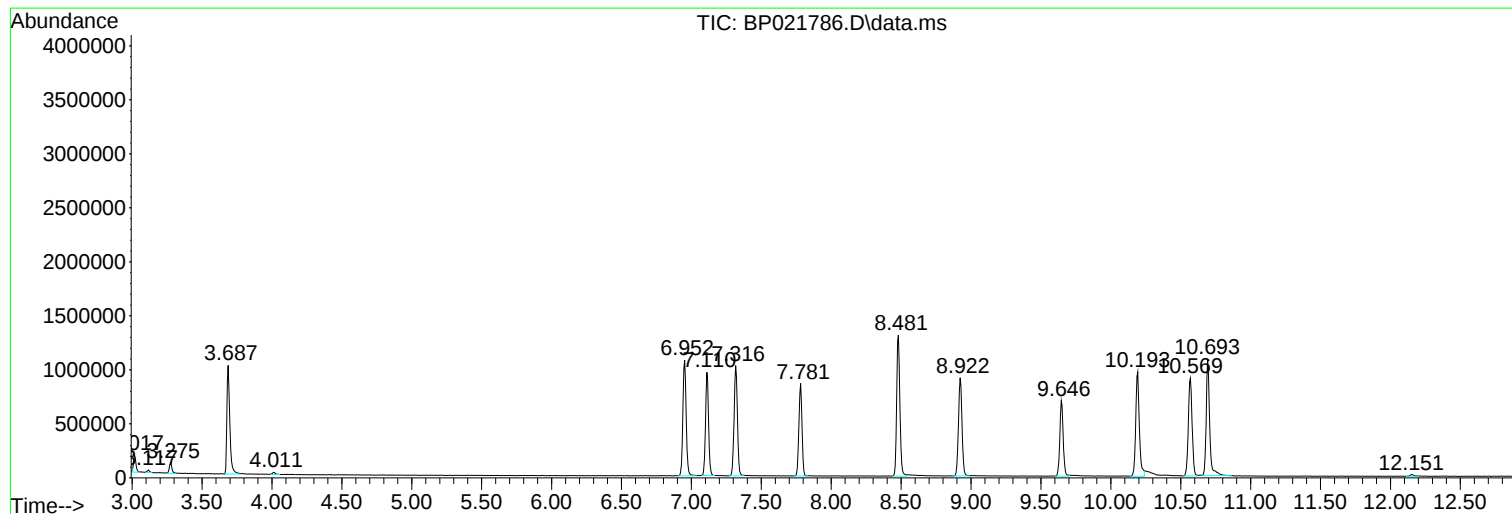

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090324\
Data File : BP021786.D
Acq On : 03 Sep 2024 10:02
Operator : RC/JU
Sample : PB163064BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK064










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.017	2.62 ng/ul	171194	1,4-Dichlorobenzene-d4	7.781

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9

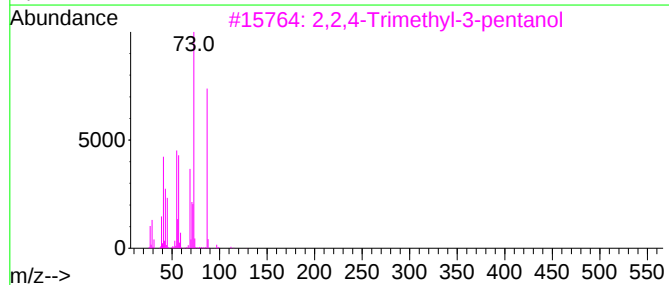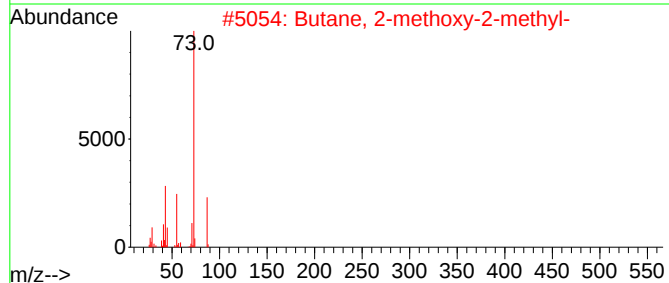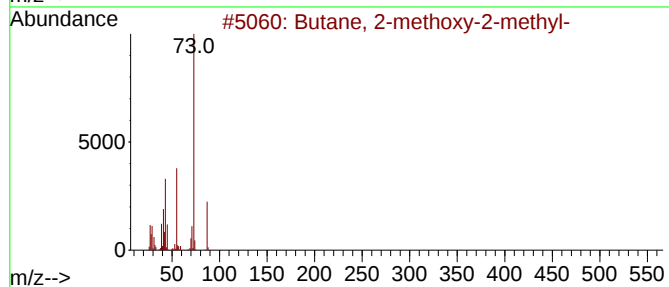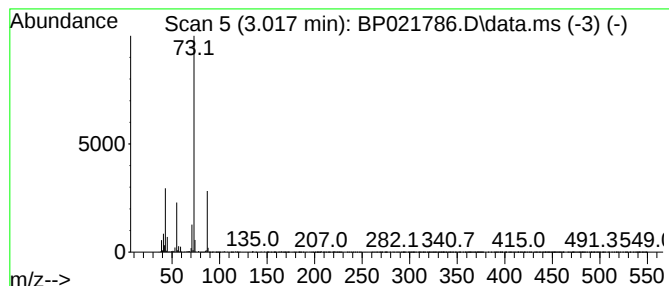

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090324\
Data File : BP021786.D
Acq On : 03 Sep 2024 10:02
Operator : RC/JU
Sample : PB163064BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK064

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.017	2.6	ng/ul	171194	1	7.781	1307860	20.0