




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
 Data File : BP021823.D
 Acq On : 04 Sep 2024 19:14
 Operator : RC/JU
 Sample : P3809-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YE3F1

Manual IntegrationsAPPROVED

Quant Time: Sep 05 05:38:26 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 05 05:03:57 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/05/2024
 Supervised By :mohammad ahmed 09/07/2024

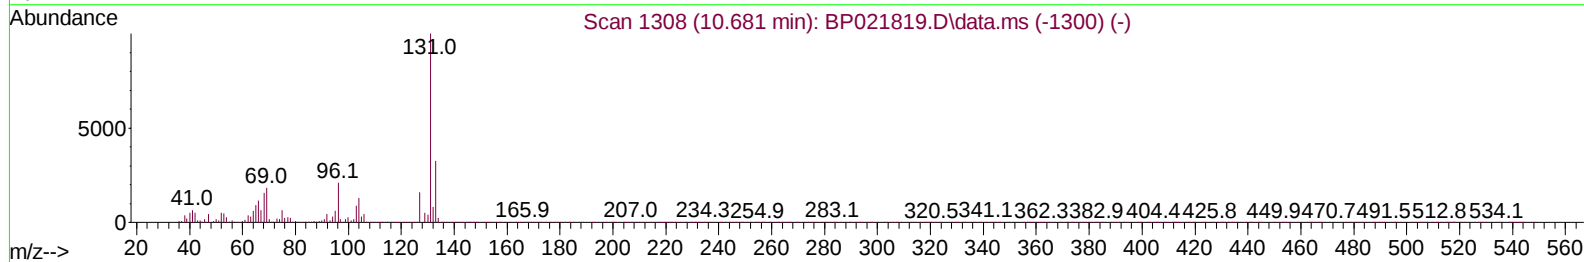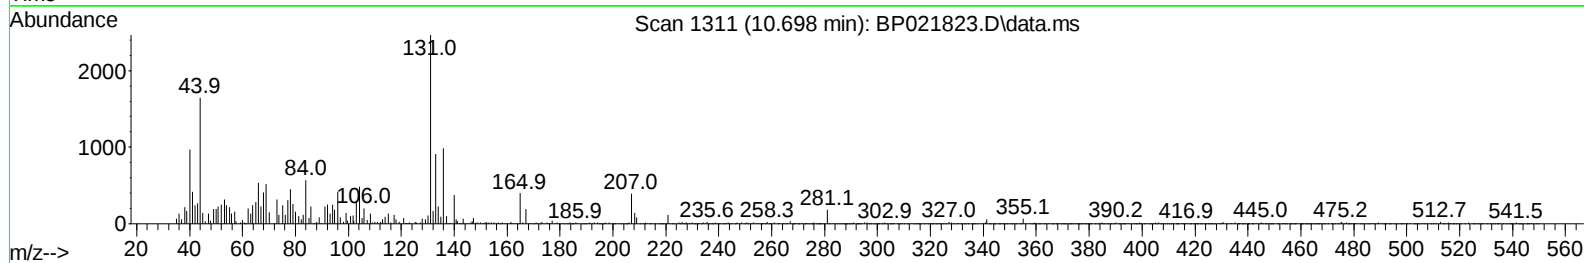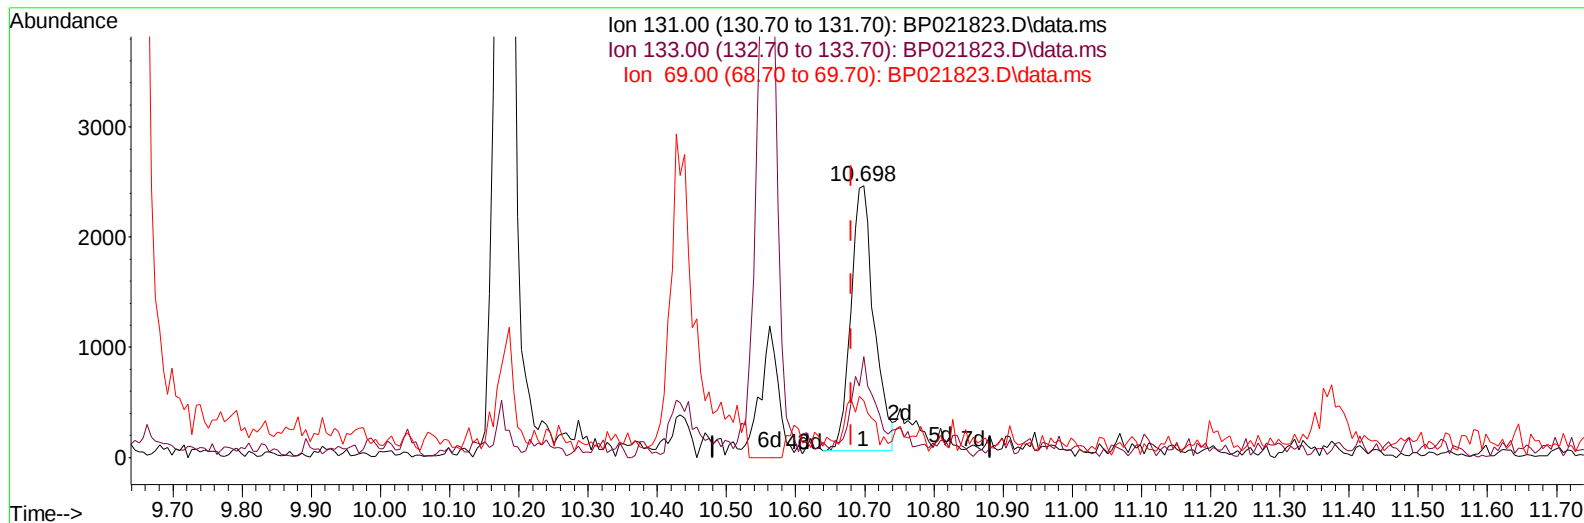

TIC: BP021823.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.698min (+ 0.017) 0.18 ng/u1

response 5570

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.50	37.04
69.00	19.80	20.97
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
Data File : BP021823.D
Acq On : 04 Sep 2024 19:14
Operator : RC/JU
Sample : P3809-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YE3F1

Manual IntegrationsAPPROVED

Quant Time: Sep 05 05:38:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 05 05:03:57 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/05/2024
Supervised By :mohammad ahmed 09/07/2024

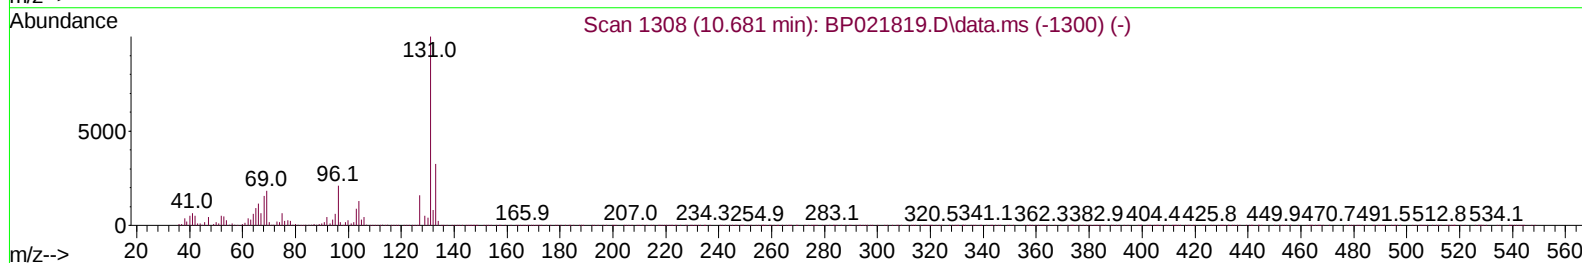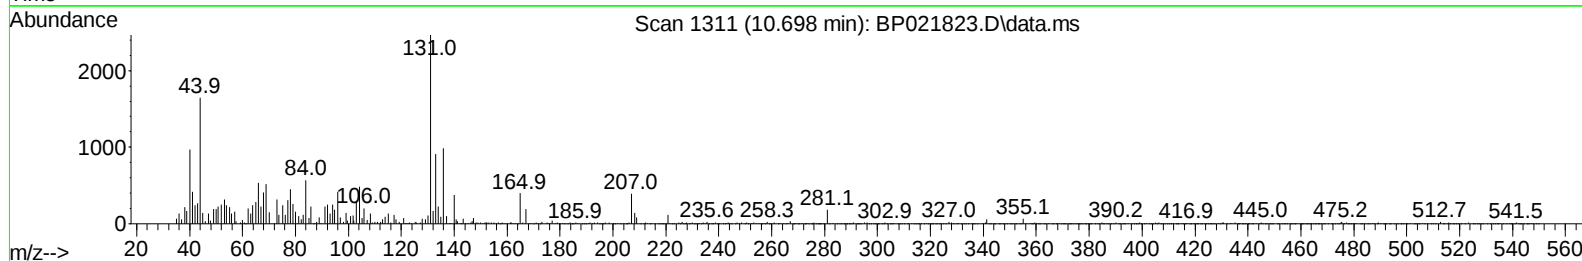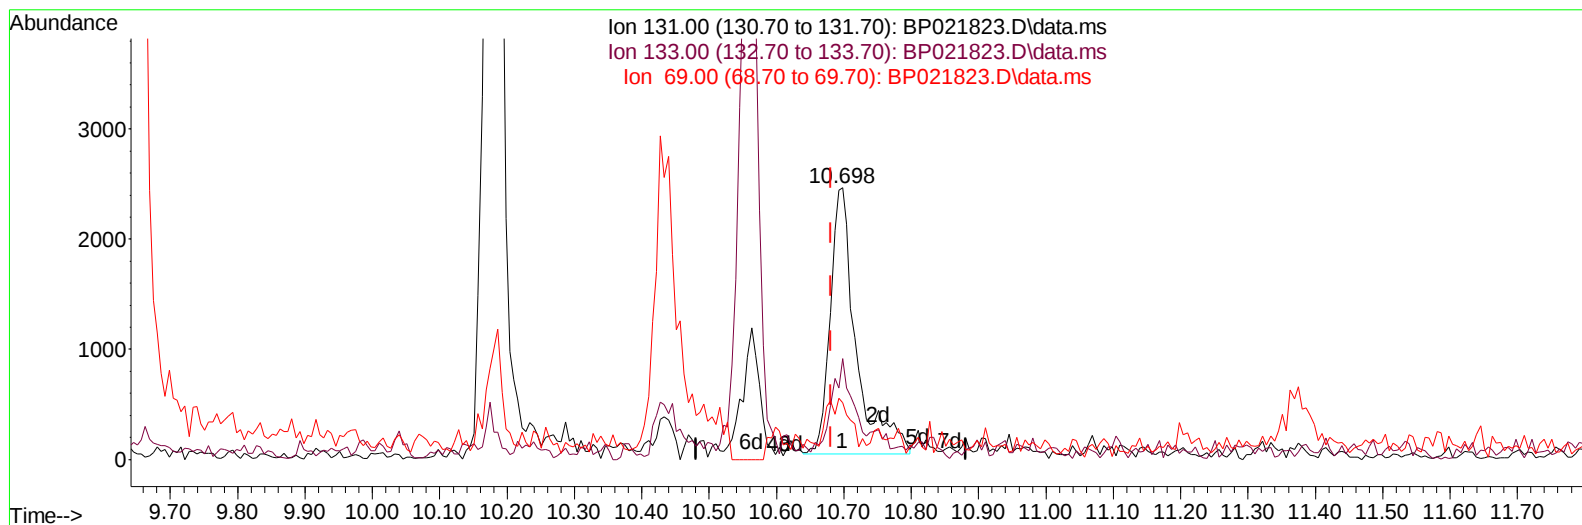

TIC: BP021823.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.698min (+ 0.017) 0.20 ng/ul m

response 6425

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.50	37.04
69.00	19.80	20.97
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
Data File : BP021823.D
Acq On : 04 Sep 2024 19:14
Operator : RC/JU
Sample : P3809-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YE3F1

Manual IntegrationsAPPROVED

Quant Time: Sep 05 05:38:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 05 05:03:57 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/05/2024
Supervised By :mohammad ahmed 09/07/2024

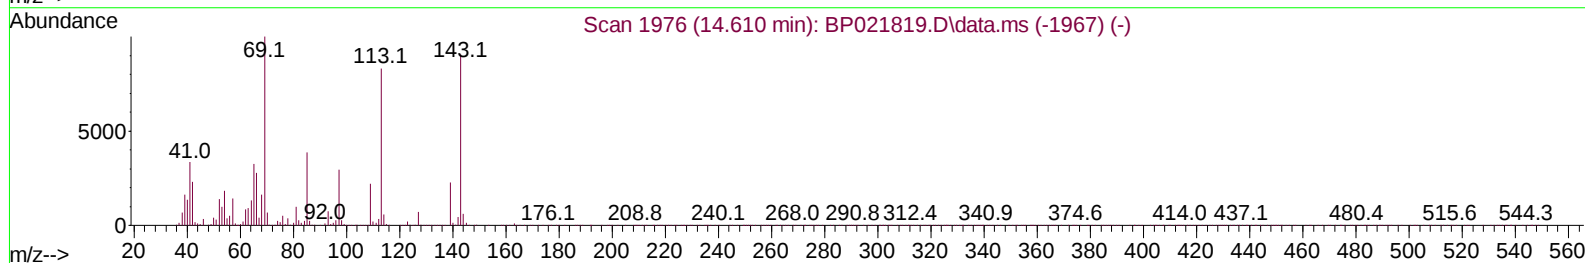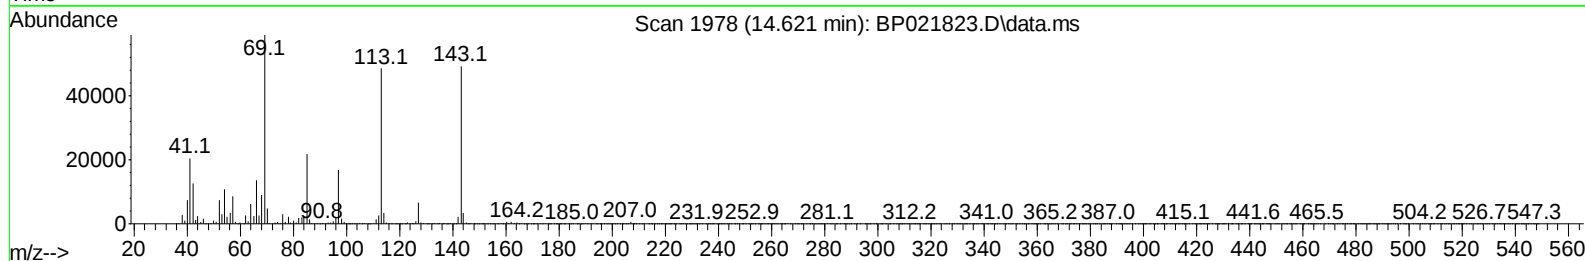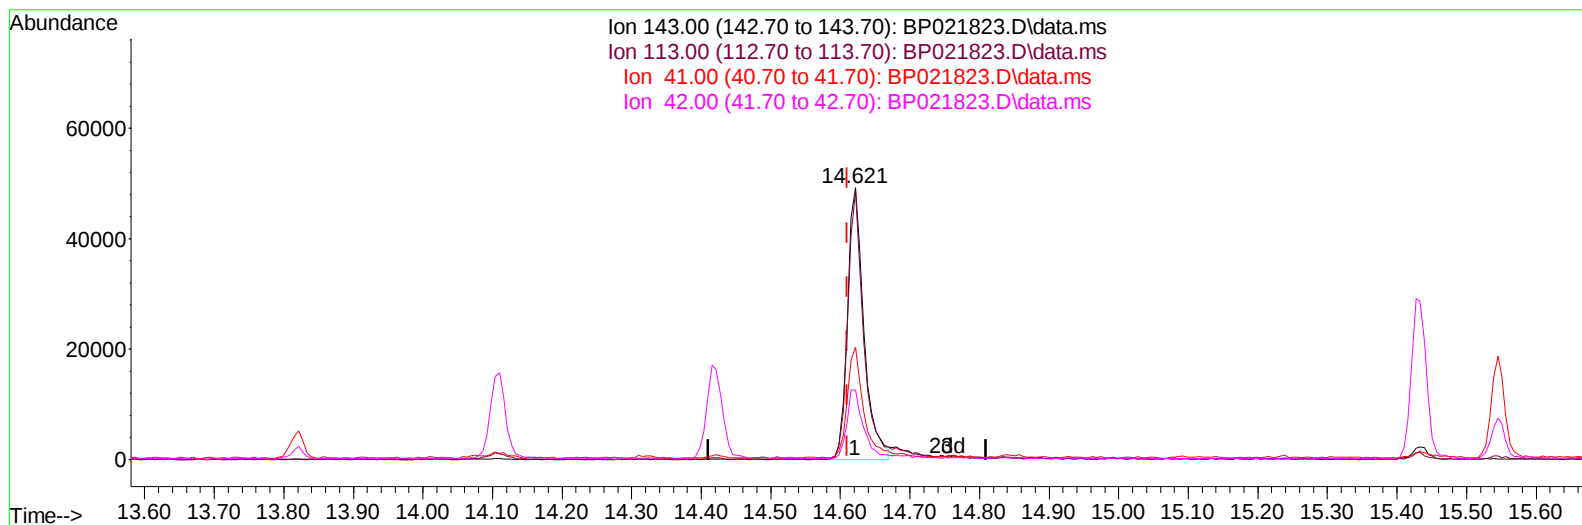

TIC: BP021823.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.621min (+ 0.011) 6.16 ng/u1

response 80677

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	83.10	98.63
41.00	33.90	41.42#
42.00	23.00	25.58




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
Data File : BP021823.D
Acq On : 04 Sep 2024 19:14
Operator : RC/JU
Sample : P3809-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YE3F1

Manual IntegrationsAPPROVED

Quant Time: Sep 05 05:38:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 05 05:03:57 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/05/2024
Supervised By :mohammad ahmed 09/07/2024

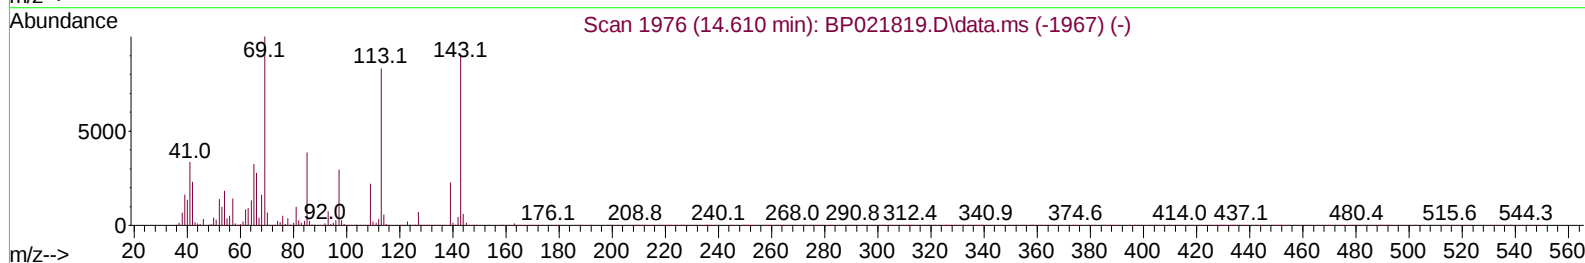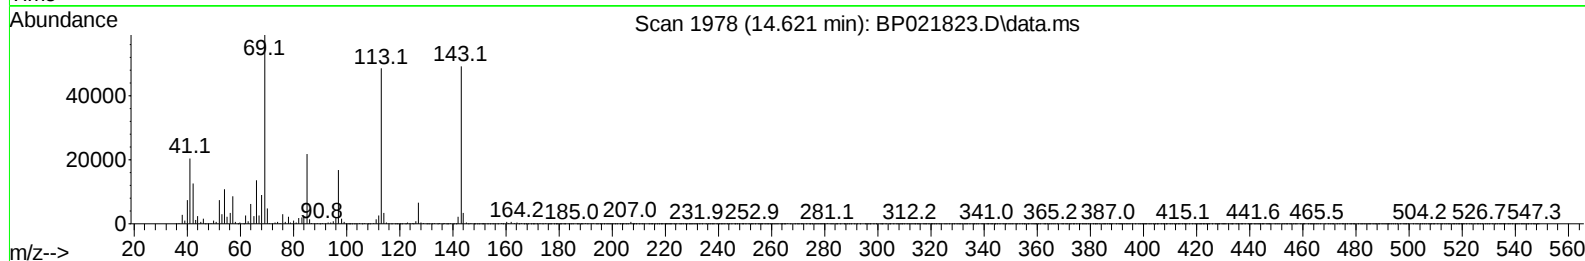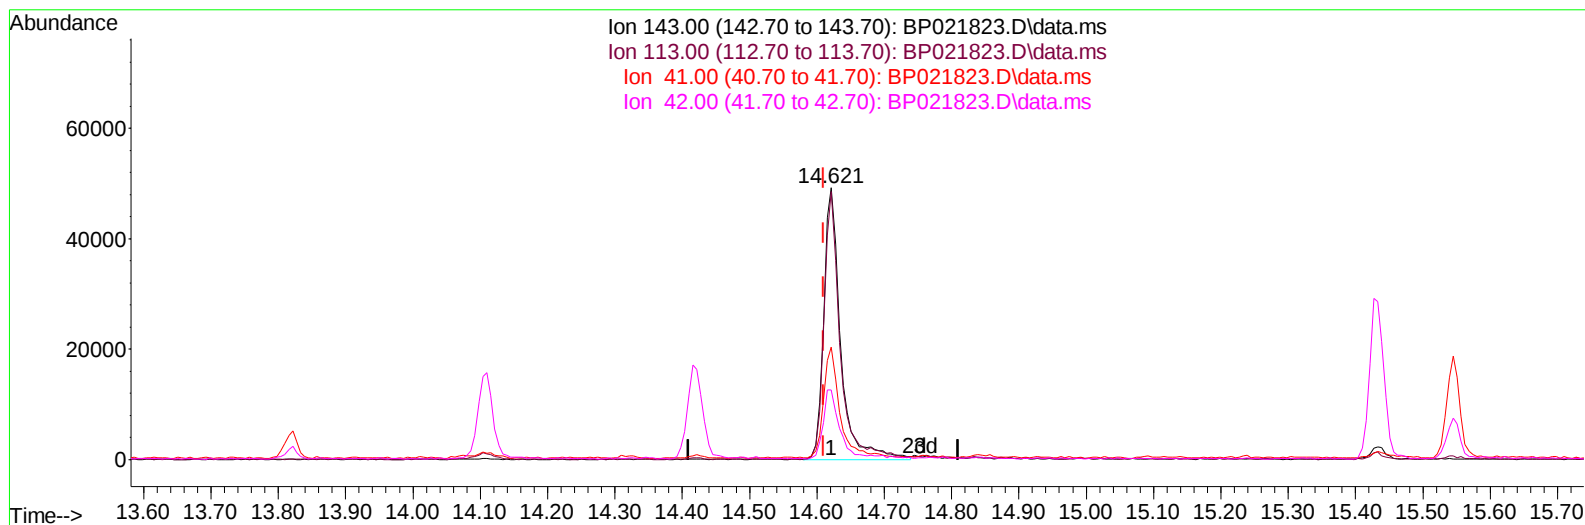

TIC: BP021823.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.621min (+ 0.011) 6.55 ng/ul m

response 85805

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	83.10	98.63
41.00	33.90	41.42#
42.00	23.00	25.58

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
 Data File : BP021823.D
 Acq On : 04 Sep 2024 19:14
 Operator : RC/JU
 Sample : P3809-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YE3F1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/05/2024
 Supervised By :mohammad ahmed 09/07/2024

Quant Time: Sep 05 05:39:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 05 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	329135	20.000	ng/ul	0.01
20) Naphthalene-d8	10.557	136	1343620	20.000	ng/ul	0.01
38) Acenaphthene-d10	14.416	164	899519	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.221	188	1995236	20.000	ng/ul	0.01
79) Chrysene-d12	21.680	240	1978702	20.000	ng/ul	0.00
88) Perylene-d12	25.086	264	2179599	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	35080	3.538	ng/uL	0.00
4) Pyridine-d5	3.687	84	214546	7.482	ng/ul	0.01
7) Phenol-d5	6.945	99	290196	8.262	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.104	67	477235	24.966	ng/ul	0.01
11) 2-Chlorophenol-d4	7.310	132	520217	22.940	ng/ul	0.00
15) 4-Methylphenol-d8	8.469	113	421199	15.518	ng/ul	0.00
21) Nitrobenzene-d5	8.916	128	286113	26.468	ng/ul	0.00
24) 2-Nitrophenol-d4	9.633	143	303779	27.685	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.181	165	545566	25.231	ng/ul	0.01
31) 4-Chloroaniline-d4	10.698	131	6425m	0.204	ng/ul	0.02
46) Dimethylphthalate-d6	13.822	166	2167640	31.493	ng/ul	0.01
49) Acenaphthylene-d8	14.110	160	2123704	27.482	ng/ul	0.02
54) 4-Nitrophenol-d4	14.621	143	85805m	6.553	ng/ul	0.01
60) Fluorene-d10	15.433	176	1784108	30.832	ng/ul	0.02
65) 4,6-Dinitro-2-methylph...	15.545	200	302853	27.597	ng/ul	0.01
73) Anthracene-d10	17.315	188	2735820	28.892	ng/ul	0.00
81) Pyrene-d10	19.698	212	3523754	31.153	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.856	264	3453165	29.711	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
Data File : BP021823.D
Acq On : 04 Sep 2024 19:14
Operator : RC/JU
Sample : P3809-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YE3F1

Manual IntegrationsAPPROVED

Quant Time: Sep 05 05:39:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 05 05:03:57 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/05/2024
Supervised By :mohammad ahmed 09/07/2024

