

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
 Data File : BP021816.D
 Acq On : 04 Sep 2024 12:38
 Operator : RC/JU
 Sample : P3808-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 X0B24

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 09/05/2024
 Supervised By :mohammad ahmed 09/07/2024

Quant Time: Sep 04 13:12:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 29 23:56:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	233611	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.557	136	960661	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.410	164	613761	20.000	ng/u1	-0.02
64) Phenanthrene-d10	17.222	188	1356876	20.000	ng/u1	0.00
79) Chrysene-d12	21.674	240	1459177	20.000	ng/u1	0.00
88) Perylene-d12	25.080	264	1658866	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	35596	5.059	ng/uL	0.00
4) Pyridine-d5	3.681	84	514325	25.270	ng/u1	0.00
7) Phenol-d5	6.952	99	749853	30.077	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.105	67	387542	28.564	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.310	132	496572	30.851	ng/u1	-0.01
15) 4-Methylphenol-d8	8.475	113	576973	29.949	ng/u1	-0.01
21) Nitrobenzene-d5	8.922	128	242056	31.318	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.640	143	254922	32.494	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.187	165	467277	30.225	ng/u1	0.00
31) 4-Chloroaniline-d4	10.687	131	671452	29.853	ng/u1	-0.01
46) Dimethylphthalate-d6	13.810	166	1502819	32.000	ng/u1	-0.03
49) Acenaphthylene-d8	14.098	160	1688869	32.030	ng/u1	-0.02
54) 4-Nitrophenol-d4	14.616	143	275618	30.847	ng/u1	-0.01
60) Fluorene-d10	15.422	176	1305878	33.075	ng/u1	-0.02
65) 4,6-Dinitro-2-methylph...	15.539	200	198068	26.540	ng/u1	-0.02
73) Anthracene-d10	17.328	188	2090240	32.459	ng/u1	-0.01
81) Pyrene-d10	19.698	212	2651651	31.790	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.845	264	2989240	33.793	ng/u1	0.00
Target Compounds						
					Qvalue	
10) Bis(2-Chloroethyl)ether	7.199	93	1312578	64.958	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.575	70	354009	24.289	ng/u1	98
19) Hexachloroethane	8.852	117	404623	53.565	ng/u1	96
22) Nitrobenzene	8.963	77	1272320	59.036	ng/u1	99
23) Isophorone	9.493	82	5163456	119.396	ng/u1	99
27) Bis(2-Chloroethoxy)met...	9.969	93	3398286	125.297	ng/u1	98
30) Naphthalene	10.610	128	5344468	98.710	ng/u1	100
33) Hexachlorobutadiene	10.898	225	1271542	121.987	ng/u1	98
36) 2-Methylnaphthalene	12.216	142	1967704	53.731	ng/u1	100
40) Hexachlorocyclopentadiene	12.569	237	860228	77.498	ng/u1	99
44) 2-Chloronaphthalene	13.275	162	2931068	80.504	ng/u1	98
47) Dimethylphthalate	13.857	163	1974699	41.992	ng/u1	99
48) 2,6-Dinitrotoluene	13.981	165	151089	17.421	ng/u1	99
50) Acenaphthylene	14.128	152	2031238	35.819	ng/u1	99
59) Diethylphthalate	15.245	149	2237686	47.387	ng/u1	99
61) Fluorene	15.475	166	1530722	34.302	ng/u1	99
62) 4-Chlorophenyl-phenyle...	15.475	204	3084345	137.555	ng/u1	95
68) 4-Bromophenyl-phenylether	16.398	248	1092916	72.962	ng/u1	97
69) Hexachlorobenzene	16.510	284	1175966	66.129	ng/u1	95
72) Phenanthrene	17.269	178	2589271	34.759	ng/u1	99
74) Anthracene	17.363	178	3095520	41.018	ng/u1	100
78) Di-n-butylphthalate	18.233	149	4426479	53.576	ng/u1	99
87) Chrysene	21.727	228	3319536	33.982	ng/u1	100
89) Di-n-octyl phthalate	22.904	149	2614416	24.898	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
 Data File : BP021816.D
 Acq On : 04 Sep 2024 12:38
 Operator : RC/JU
 Sample : P3808-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 X0B24

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 09/05/2024
 Supervised By :mohammad ahmed 09/07/2024

Quant Time: Sep 04 13:12:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 29 23:56:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
90) Benzo(b)fluoranthene	24.004	252	2893805	27.879	ng/ul	99
91) Benzo(k)fluoranthene	24.080	252	5340488	52.556	ng/ul	99
93) Benzo(a)pyrene	24.915	252	3314882	34.665	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	28.956	276	5461779	44.297	ng/ul	100
95) Dibenzo(a,h)anthracene	29.033	278	2291040m	23.123	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
 Data File : BP021816.D
 Acq On : 04 Sep 2024 12:38
 Operator : RC/JU
 Sample : P3808-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 X0B24

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 09/05/2024
 Supervised By :mohammad ahmed 09/07/2024


Quant Time: Sep 04 13:12:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 29 23:56:59 2024
 Response via : Initial Calibration

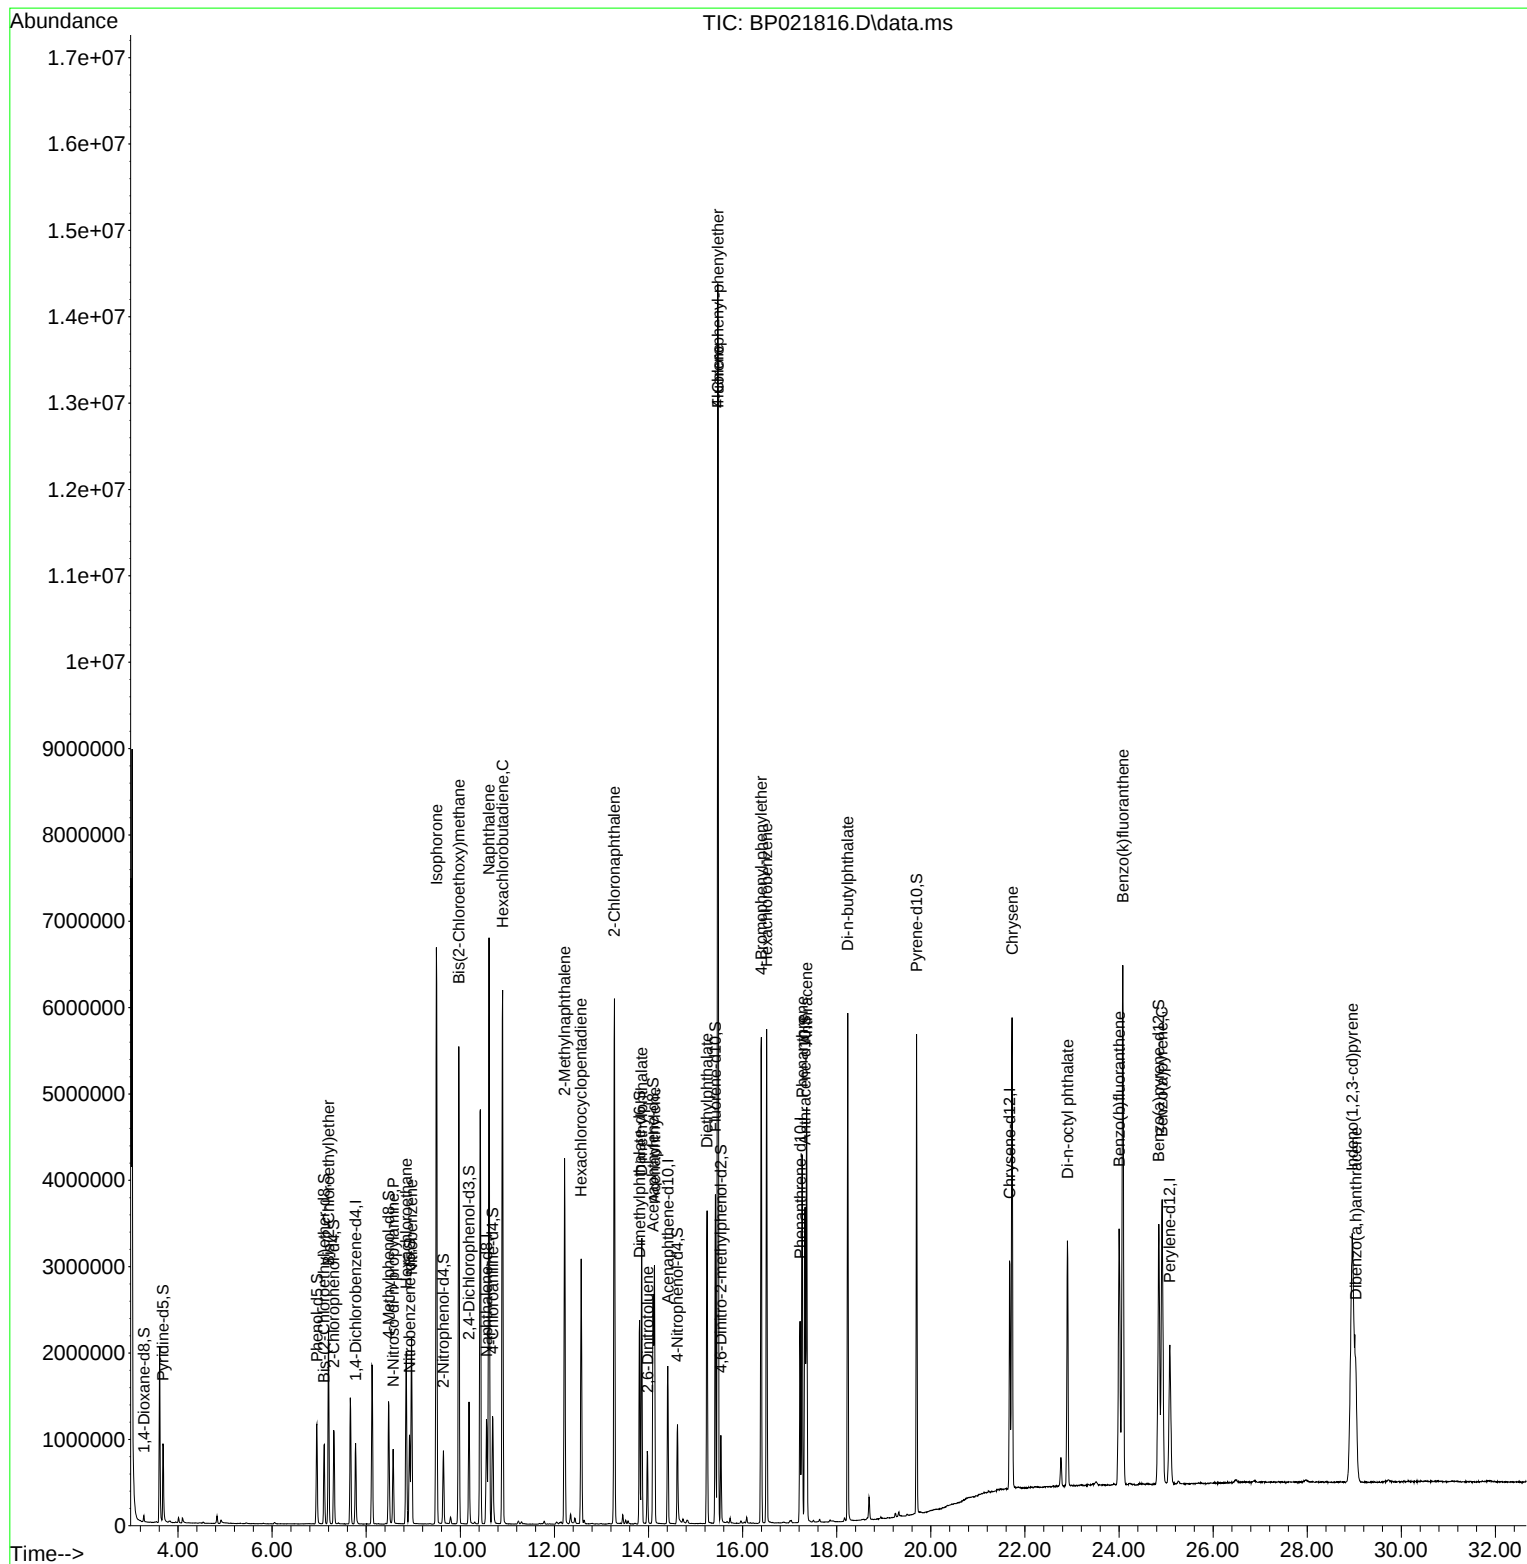



#10
Bis(2-Chloroethyl)ether
Concen: 64.958 ng/ul
RT: 7.199 min Scan# 716
Delta R.T. -0.012 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38




Instrument :
BNA_P
ClientSampleId :
X0B24



Tgt Ion: 93 Resp: 1312578
Ion Ratio Lower Upper
93 100
63 67.1 54.9 82.3
95 32.5 26.0 39.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 09/05/2024
Supervised By :mohammad ahmed 09/07/2024



#17
N-Nitroso-di-n-propylamine
Concen: 24.289 ng/ul
RT: 8.575 min Scan# 950
Delta R.T. -0.012 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38


Tgt Ion: 70 Resp: 354009
Ion Ratio Lower Upper
70 100
42 45.8 35.8 53.6
101 10.5 8.2 12.4
130 20.5 15.1 22.7

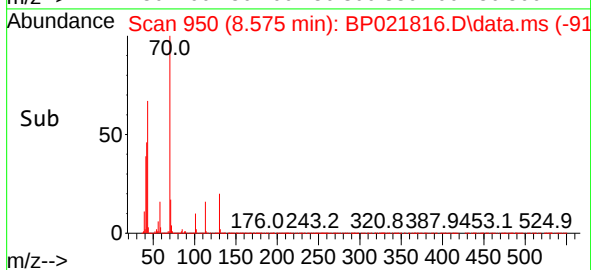



#19
Hexachloroethane
Concen: 53.565 ng/ul
RT: 8.852 min Scan# 997
Delta R.T. -0.012 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38




Instrument :
BNA_P
ClientSampleId :
X0B24

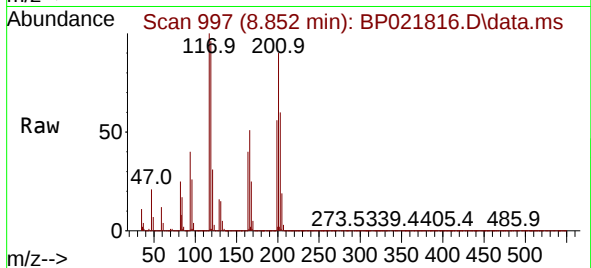


Tgt Ion: 117 Resp: 40462
Ion Ratio Lower Upper
117 100
201 89.8 75.3 112.9
199 56.5 47.4 71.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 09/05/2024
Supervised By :mohammad ahmed 09/07/2024




#22
Nitrobenzene
Concen: 59.036 ng/ul
RT: 8.963 min Scan# 1016
Delta R.T. -0.012 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38




Tgt Ion: 77 Resp: 1272320
Ion Ratio Lower Upper
77 100
123 42.2 33.2 49.8
65 12.7 9.8 14.6

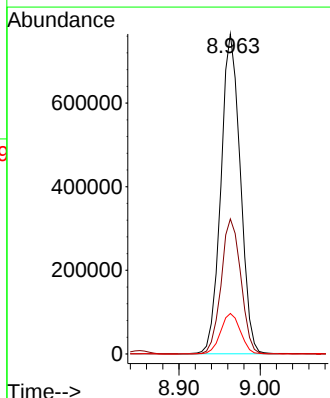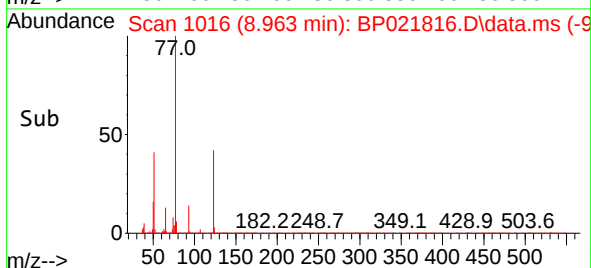



#23
Isophorone
Concen: 119.396 ng/ul
RT: 9.493 min Scan# 1106
Delta R.T. -0.012 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38




Instrument :
BNA_P
ClientSampleId :
X0B24



Tgt Ion: 82 Resp: 5163450
Ion Ratio Lower Upper
82 100
95 7.8 5.8 8.8
138 15.0 11.8 17.8




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 09/05/2024
Supervised By :mohammad ahmed 09/07/2024



#27
Bis(2-Chloroethoxy)methane
Concen: 125.297 ng/ul
RT: 9.969 min Scan# 1187
Delta R.T. -0.012 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38


Tgt Ion: 93 Resp: 3398286
Ion Ratio Lower Upper
93 100
95 32.3 25.3 37.9
123 10.1 7.4 11.0

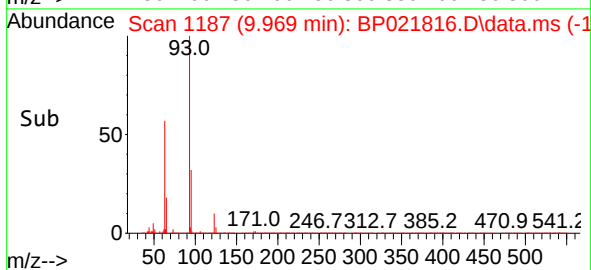



#30
Naphthalene
Concen: 98.710 ng/ul
RT: 10.610 min Scan# 1296
Delta R.T. -0.012 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38




Instrument :
BNA_P
ClientSampleId :
X0B24



Tgt Ion:128 Resp: 5344468
Ion Ratio Lower Upper
128 100
129 10.8 8.6 13.0
127 13.4 10.5 15.7




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 09/05/2024
Supervised By :mohammad ahmed 09/07/2024

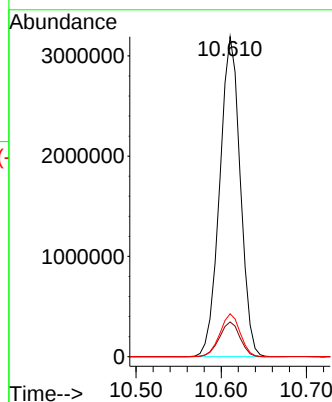

#33
Hexachlorobutadiene
Concen: 121.987 ng/ul
RT: 10.898 min Scan# 1345
Delta R.T. -0.018 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38

Tgt Ion:225 Resp: 1271542
Ion Ratio Lower Upper
225 100
223 62.9 51.5 77.3
227 65.0 51.3 76.9

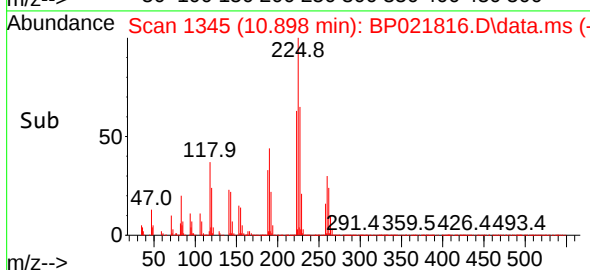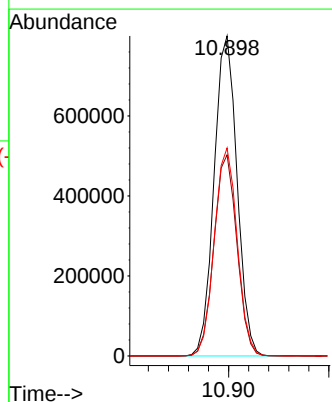







#36
2-Methylnaphthalene
Concen: 53.731 ng/ul
RT: 12.216 min Scan# 1569
Delta R.T. -0.024 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38

Instrument :
BNA_P
ClientSampleId :
X0B24

Tgt Ion:142 Resp: 1967704
Ion Ratio Lower Upper
142 100
141 88.9 71.1 106.7




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 09/05/2024
Supervised By :mohammad ahmed 09/07/2024

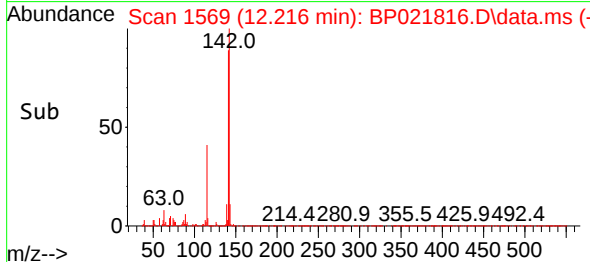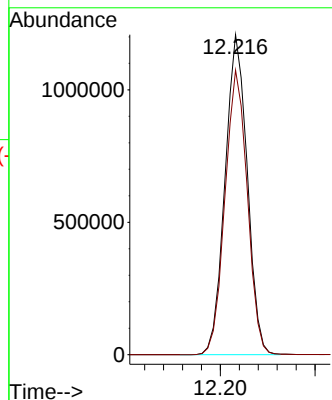

#40
Hexachlorocyclopentadiene
Concen: 77.498 ng/ul
RT: 12.569 min Scan# 1629
Delta R.T. -0.024 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38


Tgt Ion:237 Resp: 860228
Ion Ratio Lower Upper
237 100
235 63.8 50.7 76.1
272 12.7 11.0 16.6

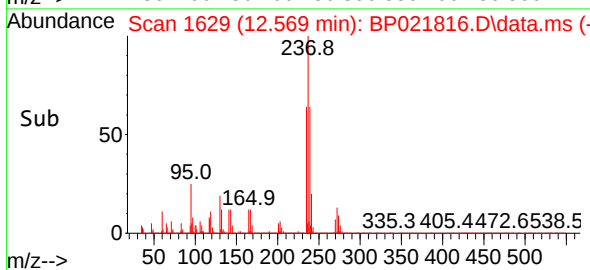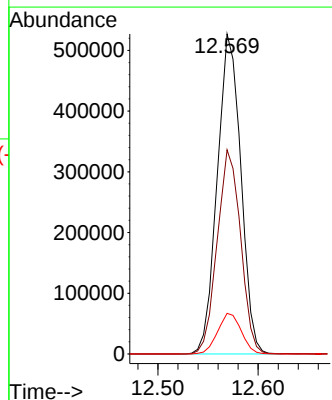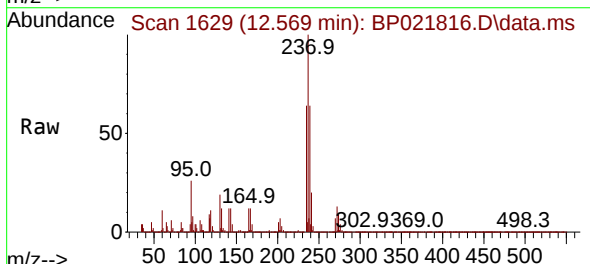



#44
2-Chloronaphthalene
Concen: 80.504 ng/ul
RT: 13.275 min Scan# 11
Delta R.T. -0.018 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38




Instrument :
BNA_P
ClientSampleId :
X0B24

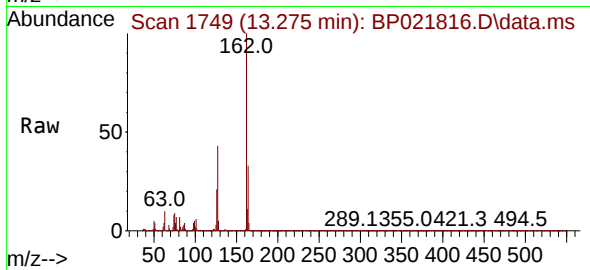


Tgt Ion:162 Resp: 2931068
Ion Ratio Lower Upper
162 100
164 32.9 26.0 39.0
127 42.8 33.1 49.7

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 09/05/2024
Supervised By :mohammad ahmed 09/07/2024

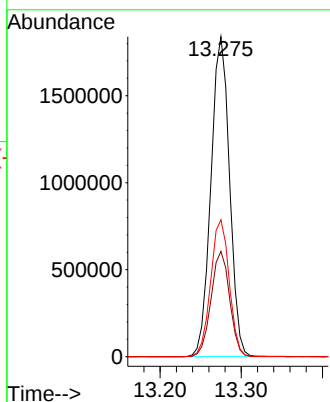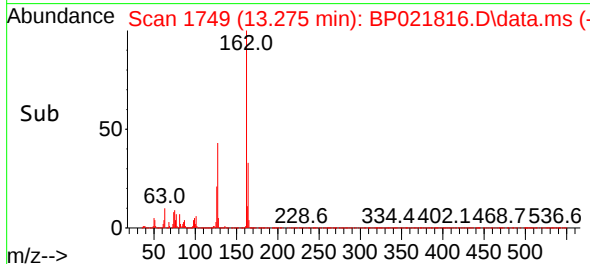


#47
Dimethylphthalate
Concen: 41.992 ng/ul
RT: 13.857 min Scan# 1848
Delta R.T. -0.030 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38




Tgt Ion:163 Resp: 1974699
Ion Ratio Lower Upper
163 100
194 4.1 3.5 5.3
164 10.0 7.8 11.8

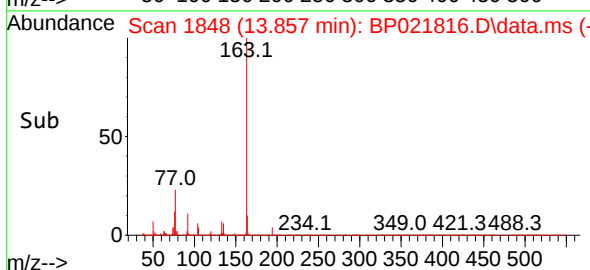



#48
2,6-Dinitrotoluene
Concen: 17.421 ng/ul
RT: 13.981 min Scan# 1869
Delta R.T. -0.018 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38




Instrument :
BNA_P
ClientSampleId :
X0B24




Tgt Ion:165 Resp: 151089
Ion Ratio Lower Upper
165 100
89 68.8 55.7 83.5
121 23.9 18.6 28.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 09/05/2024
Supervised By :mohammad ahmed 09/07/2024

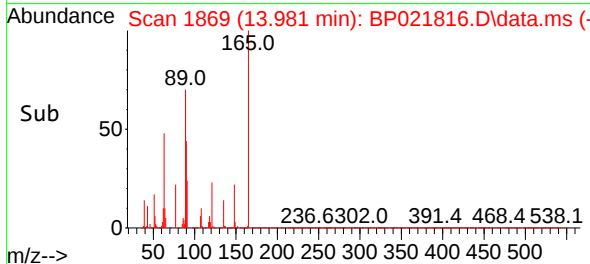


#50
Acenaphthylene
Concen: 35.819 ng/ul
RT: 14.128 min Scan# 1894
Delta R.T. -0.030 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38

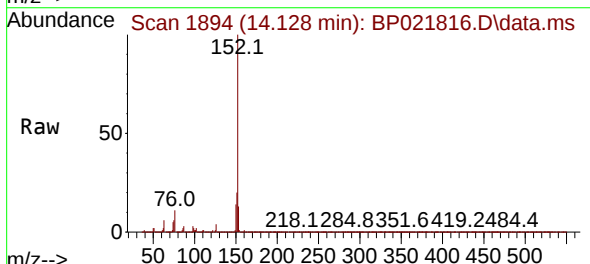


Tgt Ion:152 Resp: 2031238
Ion Ratio Lower Upper
152 100
151 19.9 15.6 23.4
153 13.0 10.2 15.4

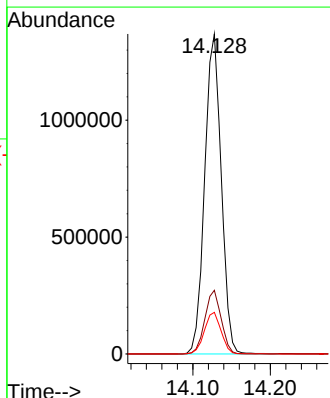



#59
Diethylphthalate
Concen: 47.387 ng/ul
RT: 15.245 min Scan# 2084
Delta R.T. -0.030 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38




Instrument :
BNA_P
ClientSampleId :
X0B24



Tgt Ion:149 Resp: 2237680
Ion Ratio Lower Upper
149 100
177 21.7 18.0 27.0
150 12.6 9.8 14.8




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 09/05/2024
Supervised By :mohammad ahmed 09/07/2024

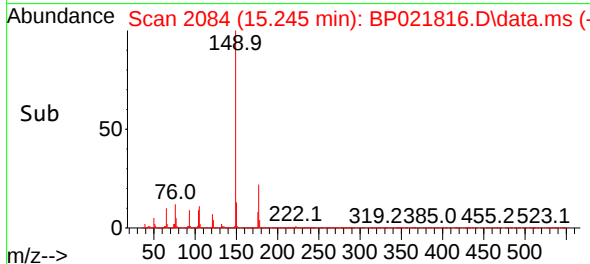

#61
Fluorene
Concen: 34.302 ng/ul
RT: 15.475 min Scan# 2123
Delta R.T. -0.024 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38


Tgt Ion:166 Resp: 1530722
Ion Ratio Lower Upper
166 100
165 99.0 78.2 117.2
167 14.1 10.8 16.2

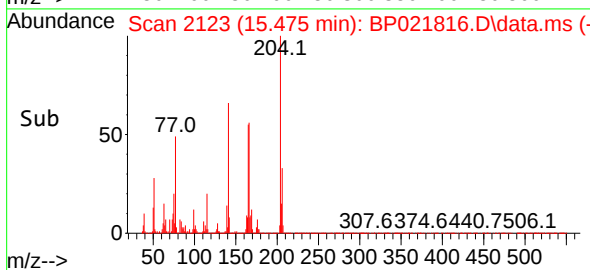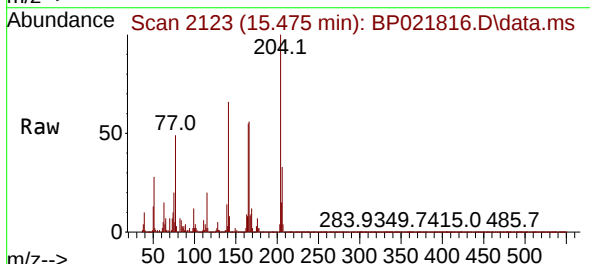

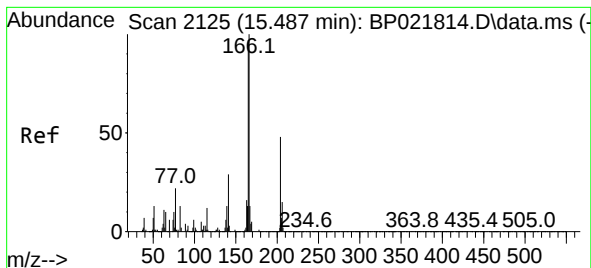

#62
4-Chlorophenyl-phenylether
Concen: 137.555 ng/ul
RT: 15.475 min Scan# 2125
Delta R.T. -0.024 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38




Instrument :
BNA_P
ClientSampleId :
X0B24

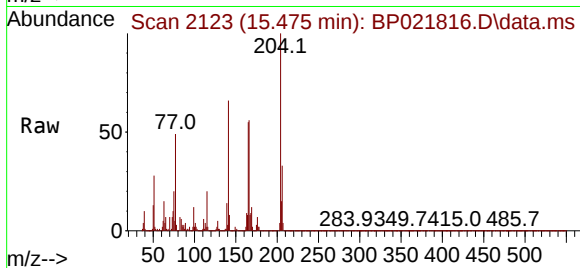

Tgt Ion:204 Resp: 308434
Ion Ratio Lower Upper
204 100
206 33.3 26.2 39.4
141 66.4 48.6 73.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 09/05/2024
Supervised By :mohammad ahmed 09/07/2024

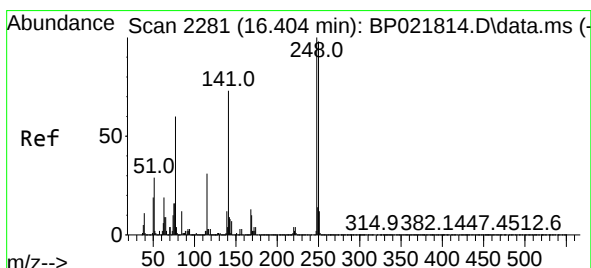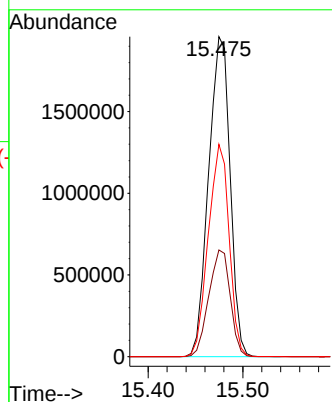

#68
4-Bromophenyl-phenylether
Concen: 72.962 ng/ul
RT: 16.398 min Scan# 2280
Delta R.T. -0.006 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38

Tgt Ion:248 Resp: 1092916
Ion Ratio Lower Upper
248 100
250 98.9 79.6 119.4
141 76.8 57.0 85.4

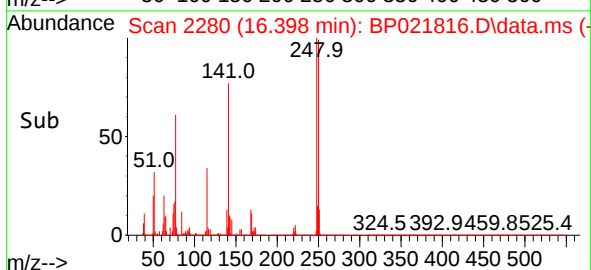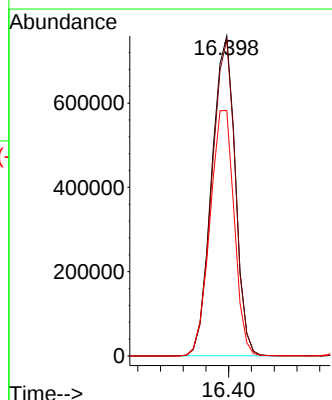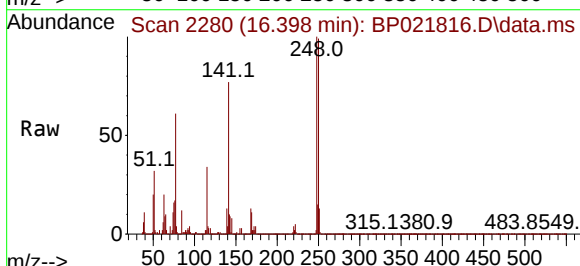



#69

Hexachlorobenzene

Concen: 66.129 ng/ul

RT: 16.510 min Scan# 21

Delta R.T. -0.012 min

Lab File: BP021816.D

Acq: 04 Sep 2024 12:38

Instrument :

BNA_P

ClientSampleId :

X0B24

Tgt Ion:284 Resp: 117596

Ion Ratio Lower Upper

284 100





142 36.4 26.5 39.7

249 33.0 24.2 36.4

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 09/05/2024
Supervised By :mohammad ahmed 09/07/2024

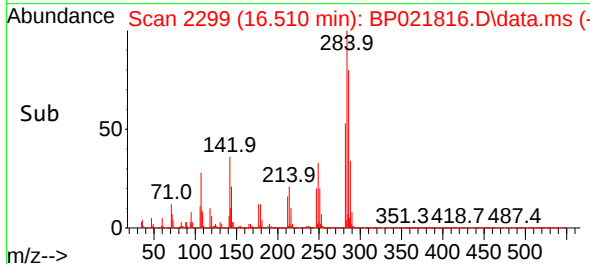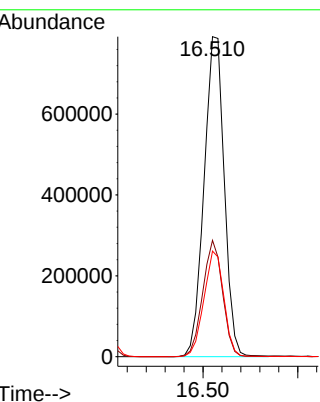

#72

Phenanthrene

Concen: 34.759 ng/ul

RT: 17.269 min Scan# 2428

Delta R.T. -0.006 min

Lab File: BP021816.D

Acq: 04 Sep 2024 12:38




Tgt Ion:178 Resp: 2589271


Ion Ratio Lower Upper

178 100

179 15.2 12.0 18.0

176 18.9 14.8 22.2

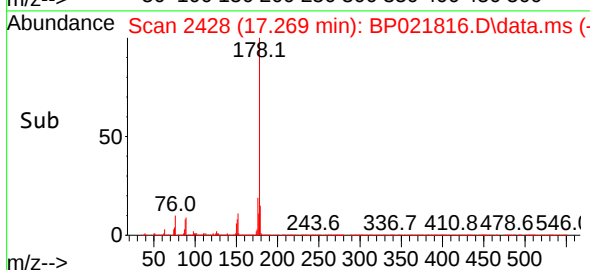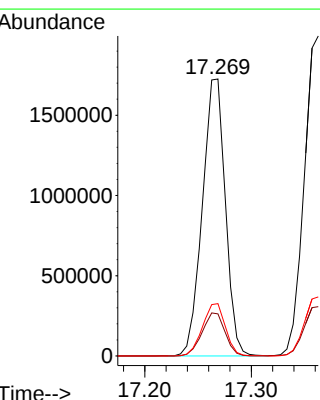

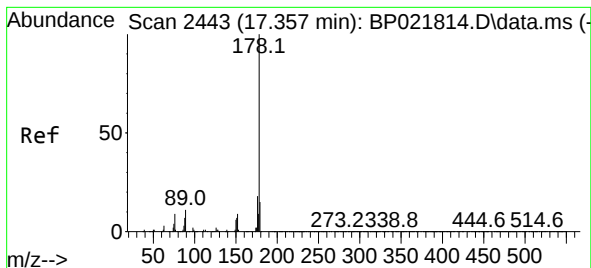

#74

Anthracene

Concen: 41.018 ng/ul

RT: 17.363 min Scan# 2444

Delta R.T. -0.006 min

Lab File: BP021816.D

Acq: 04 Sep 2024 12:38

Instrument :

BNA_P

ClientSampleId :

X0B24

Tgt Ion:178 Resp: 3095520

Ion Ratio Lower Upper

178 100





179 15.4 12.3 18.5

176 18.4 14.6 21.8

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 09/05/2024
Supervised By :mohammad ahmed 09/07/2024

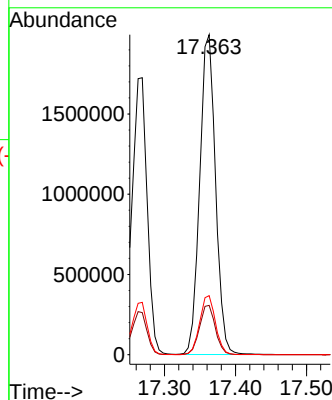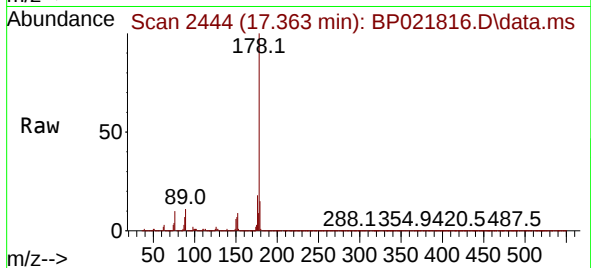

#78

Di-n-butylphthalate

Concen: 53.576 ng/ul

RT: 18.233 min Scan# 2592

Delta R.T. -0.006 min

Lab File: BP021816.D

Acq: 04 Sep 2024 12:38




Tgt Ion:149 Resp: 4426479


Ion Ratio Lower Upper

149 100

150 9.2 7.4 11.0

104 6.4 4.8 7.2

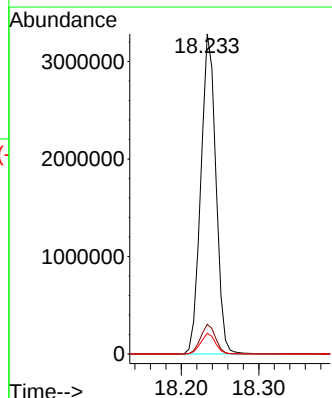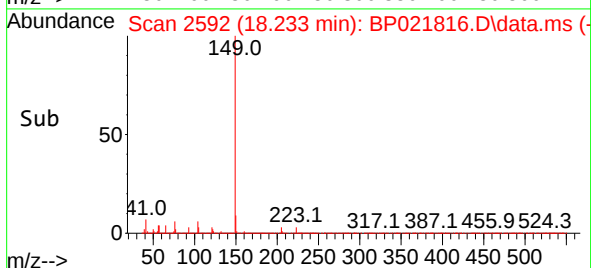



#87

Chrysene

Concen: 33.982 ng/ul

RT: 21.727 min Scan# 3186

Delta R.T. 0.012 min

Lab File: BP021816.D

Acq: 04 Sep 2024 12:38

Instrument :

BNA_P

ClientSampleId :

X0B24

Tgt Ion:228 Resp: 331953

Ion Ratio Lower Upper

228 100





226 29.4 23.5 35.3

229 19.6 15.6 23.4

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 09/05/2024
Supervised By :mohammad ahmed 09/07/2024

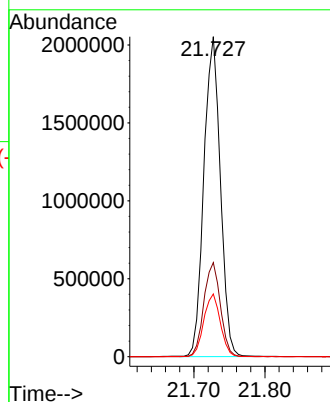

#89

Di-n-octyl phthalate

Concen: 24.898 ng/ul




RT: 22.904 min Scan# 3386


Delta R.T. 0.012 min

Lab File: BP021816.D

Acq: 04 Sep 2024 12:38


Tgt Ion:149 Resp: 2614416

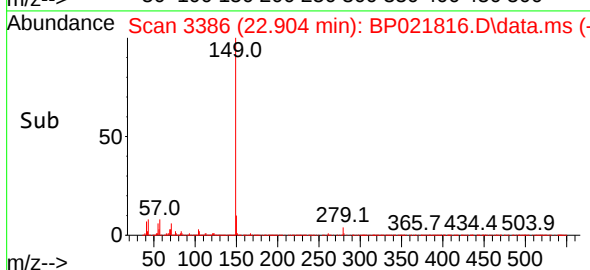



#90
Benzo(b)fluoranthene
Concen: 27.879 ng/u1
RT: 24.004 min Scan# 3573
Delta R.T. 0.012 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38




Instrument :
BNA_P
ClientSampleId :
X0B24



Tgt Ion:252 Resp: 289380
Ion Ratio Lower Upper
252 100
253 21.9 18.1 27.1
125 11.2 8.6 12.8




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 09/05/2024
Supervised By :mohammad ahmed 09/07/2024



#91
Benzo(k)fluoranthene
Concen: 52.556 ng/u1
RT: 24.080 min Scan# 3586
Delta R.T. 0.023 min
Lab File: BP021816.D
Acq: 04 Sep 2024 12:38

Tgt Ion:252 Resp: 5340488
Ion Ratio Lower Upper
252 100
253 22.0 17.8 26.8
125 11.0 8.6 13.0

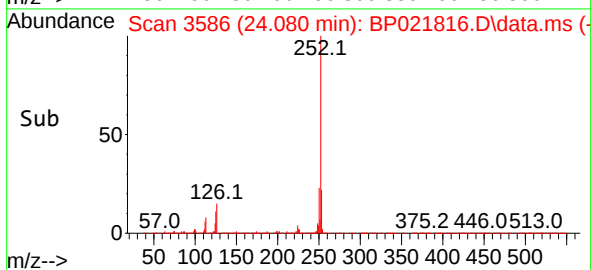



#93

Benzo(a)pyrene

Concen: 34.665 ng/ul

RT: 24.915 min Scan# 31

Delta R.T. 0.006 min

Lab File: BP021816.D

Acq: 04 Sep 2024 12:38

Instrument :

BNA_P

ClientSampleId :

X0B24

Tgt Ion:252 Resp: 331488

Ion Ratio Lower Upper

252 100





253 21.8 17.4 26.0

125 11.7 9.6 14.4

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 09/05/2024
Supervised By :mohammad ahmed 09/07/2024

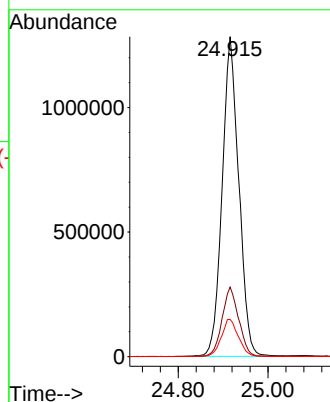

#94

Indeno(1,2,3-cd)pyrene

Concen: 44.297 ng/ul

RT: 28.956 min Scan# 4415

Delta R.T. 0.029 min

Lab File: BP021816.D

Acq: 04 Sep 2024 12:38




Tgt Ion:276 Resp: 5461779


Ion Ratio Lower Upper

276 100

138 18.7 14.9 22.3


277 23.9 19.0 28.6

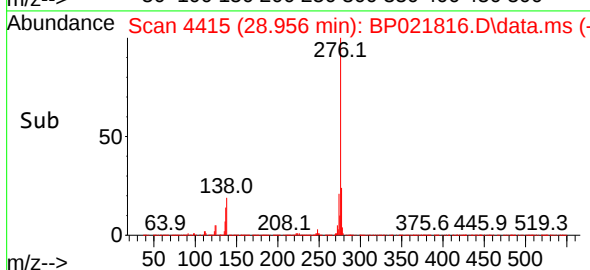

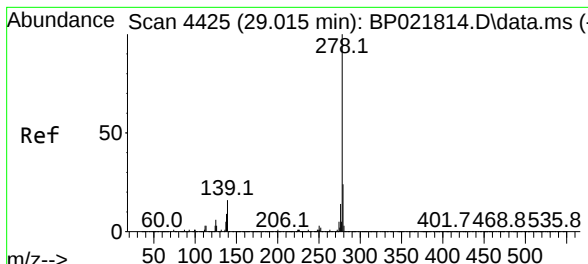

#95
 Dibenzo(a,h)anthracene
 Concen: 23.123 ng/ul m
 RT: 29.033 min Scan# 44
 Delta R.T. 0.017 min
 Lab File: BP021816.D
 Acq: 04 Sep 2024 12:38

Instrument :
 BNA_P
 ClientSampleId :
 X0B24

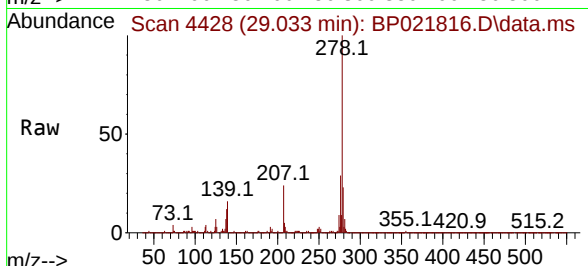

Tgt Ion: 278 Resp: 2291040

Ion	Ratio	Lower	Upper
278	100		
139	15.8	12.7	19.1
279	23.2	18.9	28.3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 09/05/2024
 Supervised By :mohammad ahmed 09/07/2024

