

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
 Data File : BP021824.D
 Acq On : 04 Sep 2024 19:57
 Operator : RC/JU
 Sample : P3809-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YE3E3

Quant Time: Sep 05 05:41:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 05 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	280006	20.000	ng/u1	0.00
20) Naphthalene-d8	10.557	136	1150972	20.000	ng/u1	0.01
38) Acenaphthene-d10	14.410	164	750510	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.216	188	1685500	20.000	ng/u1	0.00
79) Chrysene-d12	21.680	240	1689699	20.000	ng/u1	0.00
88) Perylene-d12	25.080	264	1877237	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	34024	4.034	ng/uL	0.00
4) Pyridine-d5	3.687	84	173829	7.126	ng/u1	0.01
7) Phenol-d5	6.946	99	189210	6.332	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	7.105	67	421711	25.932	ng/u1	0.01
11) 2-Chlorophenol-d4	7.310	132	444763	23.054	ng/u1	0.00
15) 4-Methylphenol-d8	8.469	113	351729	15.232	ng/u1	0.00
21) Nitrobenzene-d5	8.916	128	250862	27.091	ng/u1	0.00
24) 2-Nitrophenol-d4	9.634	143	256036	27.239	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.181	165	459199	24.791	ng/u1	0.01
31) 4-Chloroaniline-d4	10.687	131	551851	20.478	ng/u1	0.00
46) Dimethylphthalate-d6	13.810	166	1709962	29.776	ng/u1	0.00
49) Acenaphthylene-d8	14.098	160	1780722	27.619	ng/u1	0.00
54) 4-Nitrophenol-d4	14.622	143	61338	5.614	ng/u1	0.01
60) Fluorene-d10	15.422	176	1426829	29.553	ng/u1	0.01
65) 4,6-Dinitro-2-methylph...	15.539	200	236767	25.540	ng/u1	0.00
73) Anthracene-d10	17.322	188	2356694	29.462	ng/u1	0.00
81) Pyrene-d10	19.698	212	2963032	30.676	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.851	264	3081047	30.779	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.305	88	50964	5.686	ng/uL	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
Data File : BP021824.D
Acq On : 04 Sep 2024 19:57
Operator : RC/JU
Sample : P3809-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YE3E3

Quant Time: Sep 05 05:41:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 05 05:03:57 2024
Response via : Initial Calibration

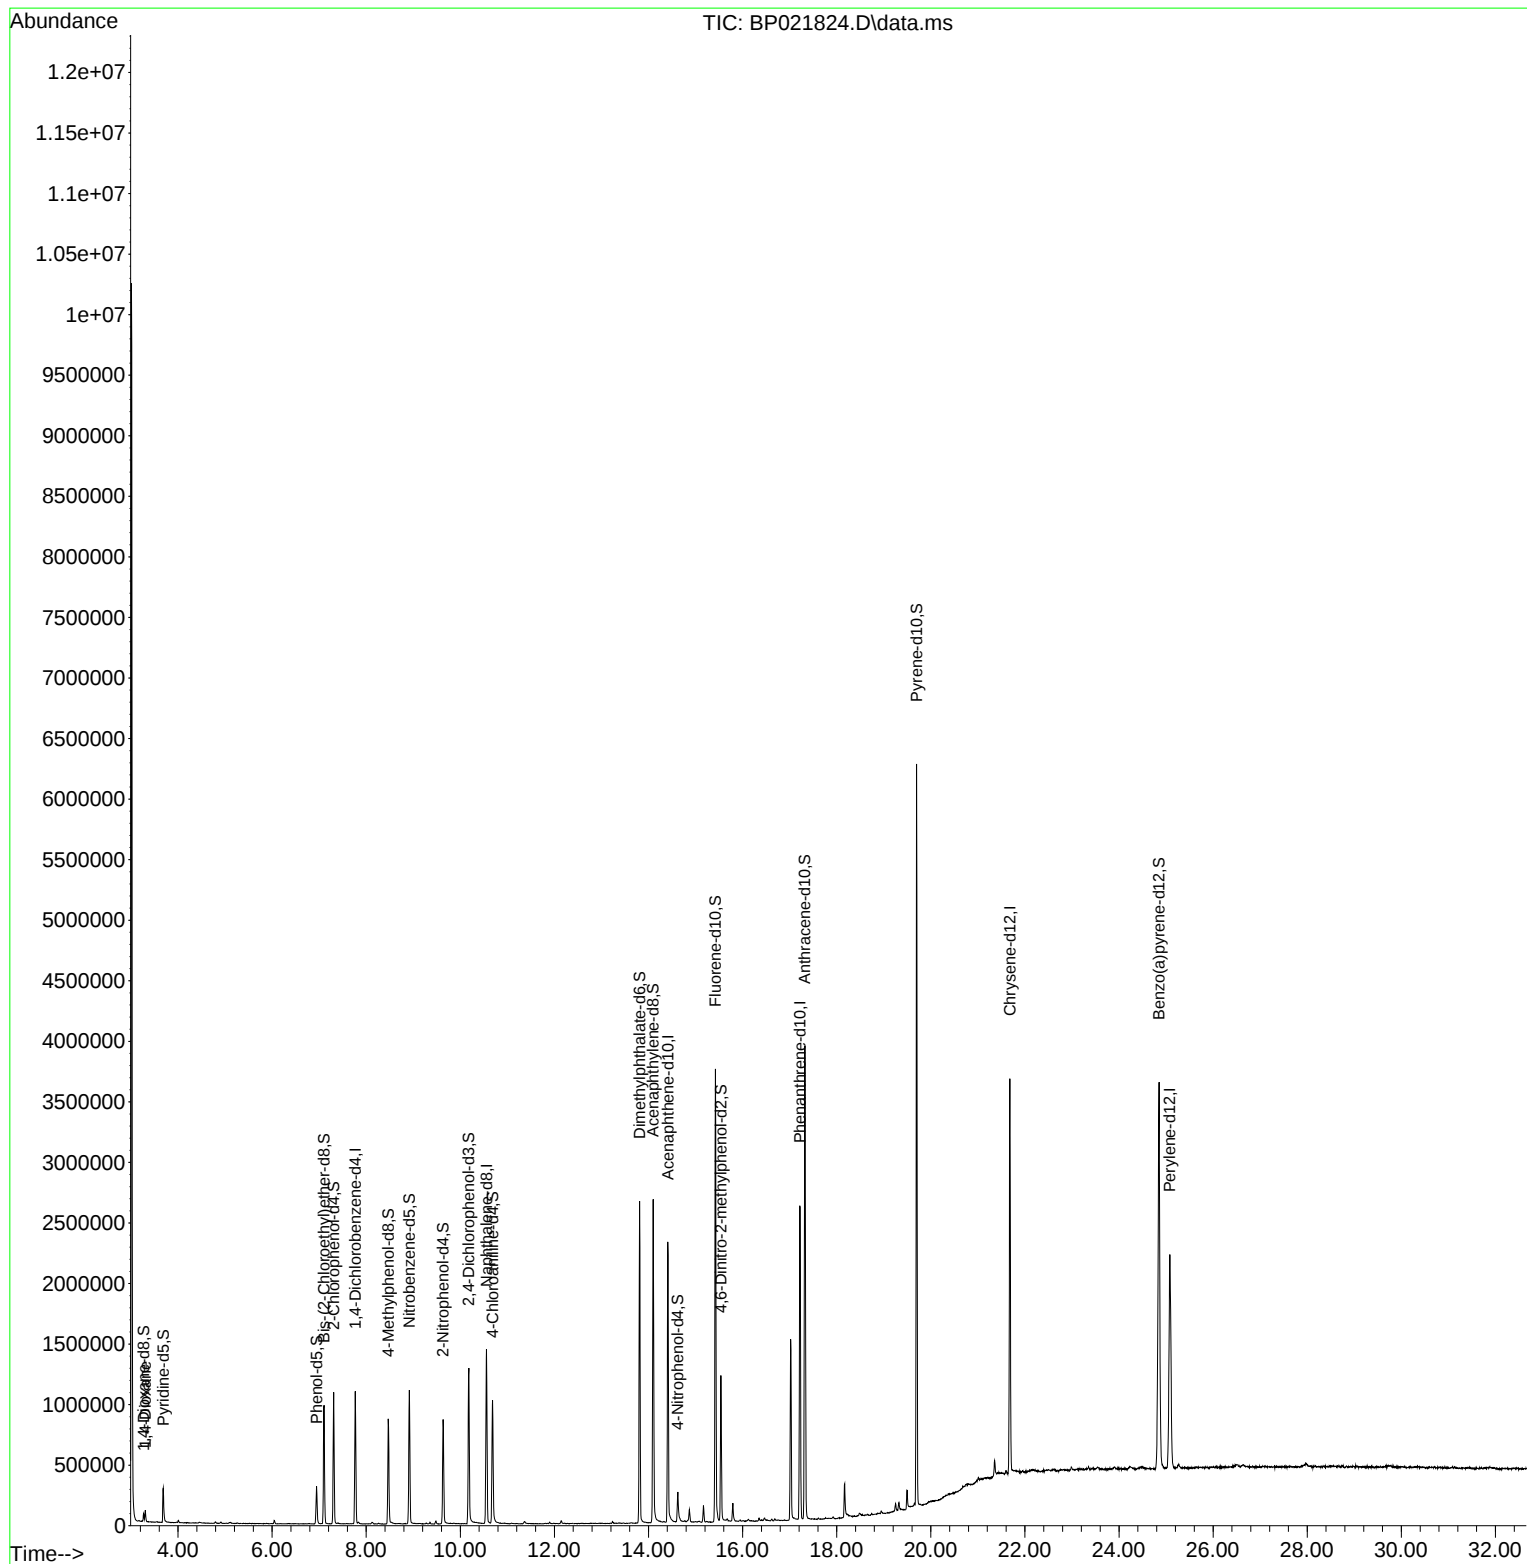

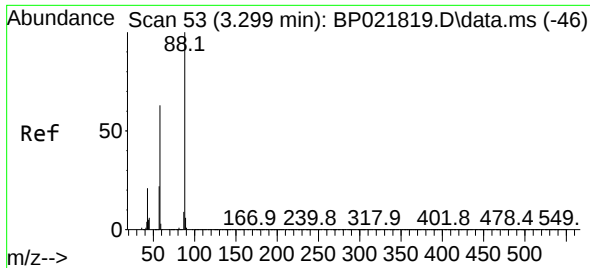

#2
1,4-Dioxane
Concen: 5.686 ng/uL
RT: 3.305 min Scan# 54
Delta R.T. 0.006 min
Lab File: BP021824.D
Acq: 04 Sep 2024 19:57

Instrument :
BNA_P
ClientSampleId :
YE3E3

Tgt Ion: 88 Resp: 50964
Ion Ratio Lower Upper
88 100
43 22.4 15.4 23.2
58 63.9 48.2 72.2

