

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
 Data File : BP021843.D
 Acq On : 05 Sep 2024 15:49
 Operator : RC/JU
 Sample : P3809-11
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YE3E5

Quant Time: Sep 05 16:53:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 05 05:03:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	227715	20.000	ng/u1	0.00
20) Naphthalene-d8	10.552	136	954276	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.404	164	603669	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.210	188	1467293	20.000	ng/u1	0.00
79) Chrysene-d12	21.669	240	1557979	20.000	ng/u1	-0.01
88) Perylene-d12	25.074	264	1735376	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	30157	4.397	ng/uL	0.00
4) Pyridine-d5	3.681	84	195002	9.829	ng/u1	0.00
7) Phenol-d5	6.940	99	155154	6.384	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.099	67	214498	16.219	ng/u1	0.00
11) 2-Chlorophenol-d4	7.305	132	268032	17.084	ng/u1	0.00
15) 4-Methylphenol-d8	8.469	113	260505	13.872	ng/u1	0.00
21) Nitrobenzene-d5	8.916	128	119114	15.515	ng/u1	0.00
24) 2-Nitrophenol-d4	9.634	143	121377	15.575	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.175	165	253275	16.492	ng/u1	0.00
31) 4-Chloroaniline-d4	10.681	131	427679	19.142	ng/u1	0.00
46) Dimethylphthalate-d6	13.810	166	874242	18.927	ng/u1	0.00
49) Acenaphthylene-d8	14.093	160	905174	17.454	ng/u1	0.00
54) 4-Nitrophenol-d4	14.616	143	51192	5.825	ng/u1	0.00
60) Fluorene-d10	15.410	176	745337	19.193	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.534	200	112094	13.890	ng/u1	0.00
73) Anthracene-d10	17.310	188	1319935	18.955	ng/u1	0.00
81) Pyrene-d10	19.686	212	1706664	19.163	ng/u1	-0.01
92) Benzo(a)pyrene-d12	24.845	264	1760513	19.025	ng/u1	-0.01


Target Compounds					Qvalue
2) 1,4-Dioxane	3.299	88	75214	10.318 ng/uL#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
Data File : BP021843.D
Acq On : 05 Sep 2024 15:49
Operator : RC/JU
Sample : P3809-11
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YE3E5

Quant Time: Sep 05 16:53:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 05 05:03:57 2024
Response via : Initial Calibration

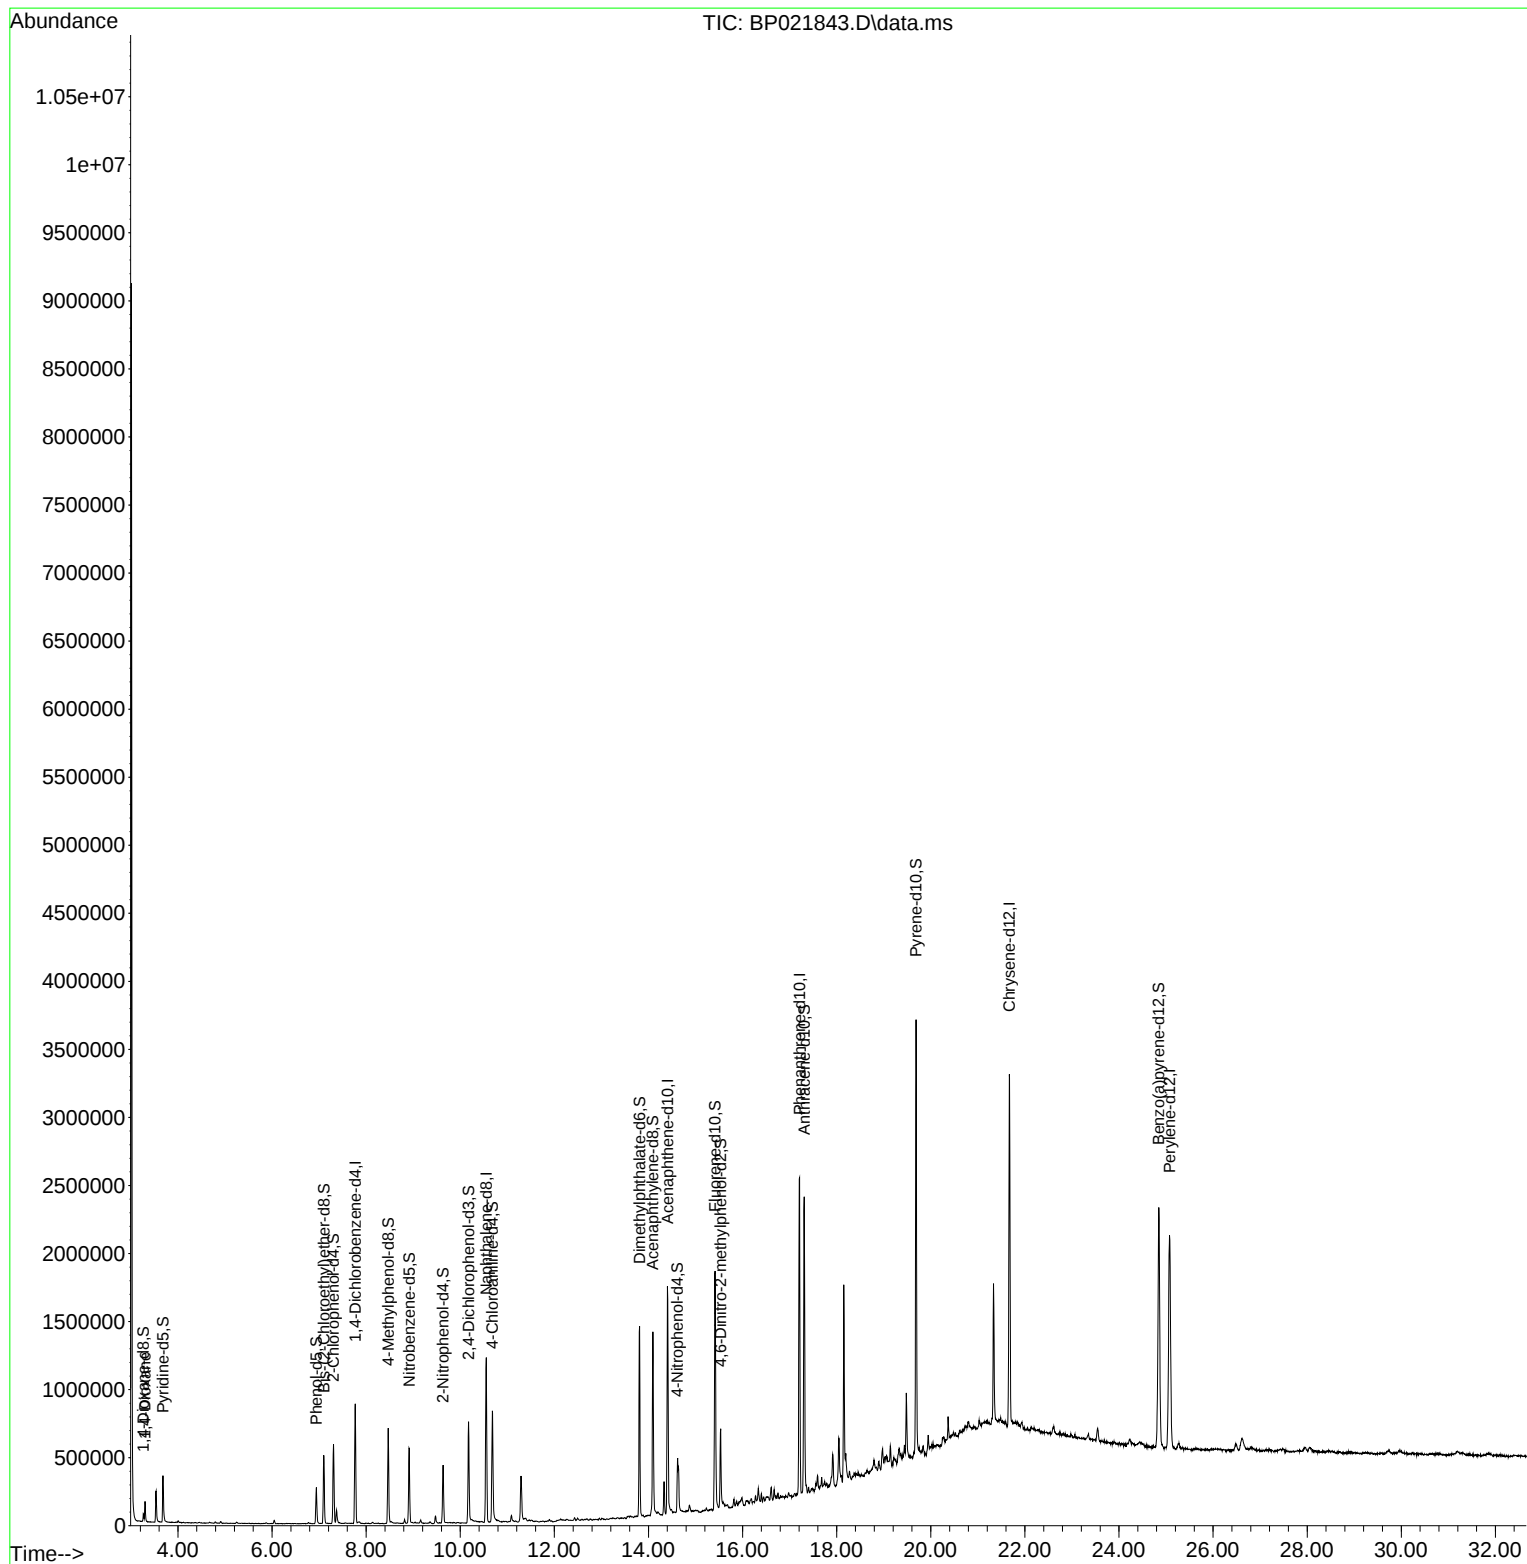

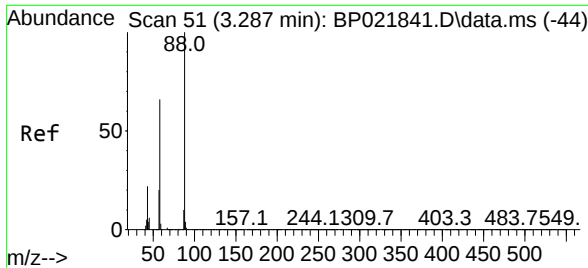

#2
 1,4-Dioxane
 Concen: 10.318 ng/uL
 RT: 3.299 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: BP021843.D
 Acq: 05 Sep 2024 15:49

Instrument :
 BNA_P
 ClientSampleId :
 YE3E5

Tgt Ion: 88 Resp: 75214
 Ion Ratio Lower Upper
 88 100
 43 24.5 15.4 23.2#
 58 63.5 48.2 72.2

