

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
 Data File : BP021815.D
 Acq On : 04 Sep 2024 11:56
 Operator : RC/JU
 Sample : PB163092BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK092

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021815.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	17	rVB	163212	198338	2.21%	0.196%
2	3.111	18	21	29	rVB	21758	35743	0.40%	0.035%
3	3.275	44	49	59	rVB	112879	162998	1.82%	0.161%
4	3.687	114	119	135	rBV	1281031	1990421	22.17%	1.972%
5	4.011	169	174	179	rBV	31971	44256	0.49%	0.044%
6	4.228	209	211	216	rVB5	7237	10151	0.11%	0.010%
7	6.952	666	674	684	rBV	1546129	2590198	28.85%	2.566%
8	7.111	692	701	716	rVB	1369862	2131766	23.75%	2.112%
9	7.316	726	736	745	rBV	1467848	2485778	27.69%	2.462%
10	7.775	806	814	822	rBV	1729581	2667817	29.72%	2.643%
11	8.475	925	933	950	rBV	1939967	3286888	36.61%	3.256%
12	8.922	1001	1009	1018	rBV	1488377	2471531	27.53%	2.448%
13	9.640	1121	1131	1143	rBV	1171088	2014720	22.44%	1.996%
14	10.181	1212	1223	1238	rBV	1736268	3129740	34.86%	3.100%
15	10.557	1278	1287	1302	rBV	2072940	3770468	42.00%	3.735%
16	10.687	1302	1309	1333	rVB	1780248	3036899	33.83%	3.008%
17	11.357	1418	1423	1427	rBV8	5239	10104	0.11%	0.010%
18	12.146	1551	1557	1565	rVB2	33220	60061	0.67%	0.059%
19	13.816	1832	1841	1859	rBV	2905684	4651068	51.81%	4.607%
20	14.104	1881	1890	1908	rBV	3199108	5188734	57.80%	5.140%
21	14.416	1934	1943	1956	rBV	2671461	4824966	53.75%	4.779%
22	14.616	1970	1977	1999	rBV	1292266	2435653	27.13%	2.413%
23	14.845	2012	2016	2022	rVB8	12170	23527	0.26%	0.023%
24	15.422	2107	2114	2128	rBV	3720637	6651713	74.10%	6.589%
25	15.539	2128	2134	2148	rVV	1372053	2119903	23.62%	2.100%
26	15.669	2151	2156	2163	rVB4	21022	43598	0.49%	0.043%
27	15.939	2199	2202	2208	rVV8	7082	9896	0.11%	0.010%
28	16.222	2246	2250	2258	rVB7	13156	24054	0.27%	0.024%
29	16.475	2287	2293	2296	rBV7	4969	10469	0.12%	0.010%
30	16.886	2360	2363	2369	rVB7	7882	12052	0.13%	0.012%
31	17.216	2411	2419	2429	rBV	3904675	6107442	68.04%	6.050%
32	17.322	2429	2437	2450	rVV	4922081	7315799	81.50%	7.247%
33	17.910	2535	2537	2543	rVB6	10749	16843	0.19%	0.017%
34	18.151	2573	2578	2583	rBV3	53450	92175	1.03%	0.091%
35	19.233	2758	2762	2768	rVB2	64263	87987	0.98%	0.087%
36	19.304	2771	2774	2780	rVB	49633	73344	0.82%	0.073%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
Data File : BP021815.D
Acq On : 04 Sep 2024 11:56
Operator : RC/JU
Sample : PB163092BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK092

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Title : SVOA CALIBRATION

37	19.686	2833	2839	2853	rBV	5780563	8976901	100.00%	8.892%
38	21.663	3169	3175	3184	rBV2	4386765	6721930	74.88%	6.658%
39	24.839	3705	3715	3730	rVB	3264333	8703292	96.95%	8.621%
40	25.074	3746	3755	3772	rVB2	2275954	6764768	75.36%	6.701%




Sum of corrected areas: 100953991

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
Data File : BP021815.D
Acq On : 04 Sep 2024 11:56
Operator : RC/JU
Sample : PB163092BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK092

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

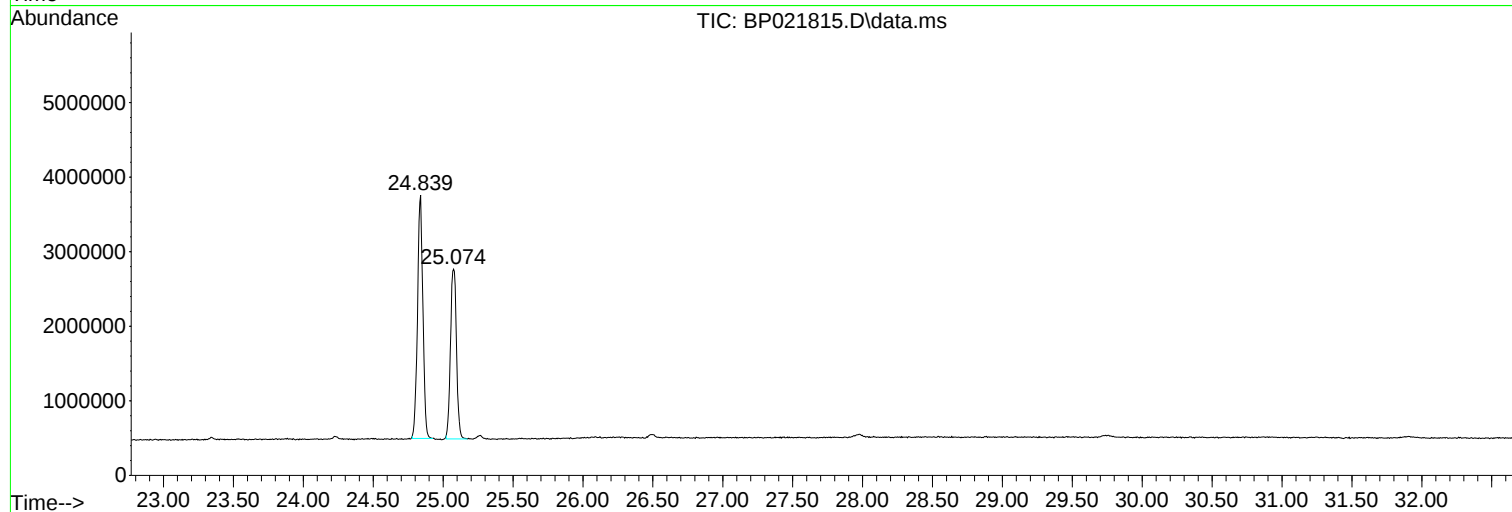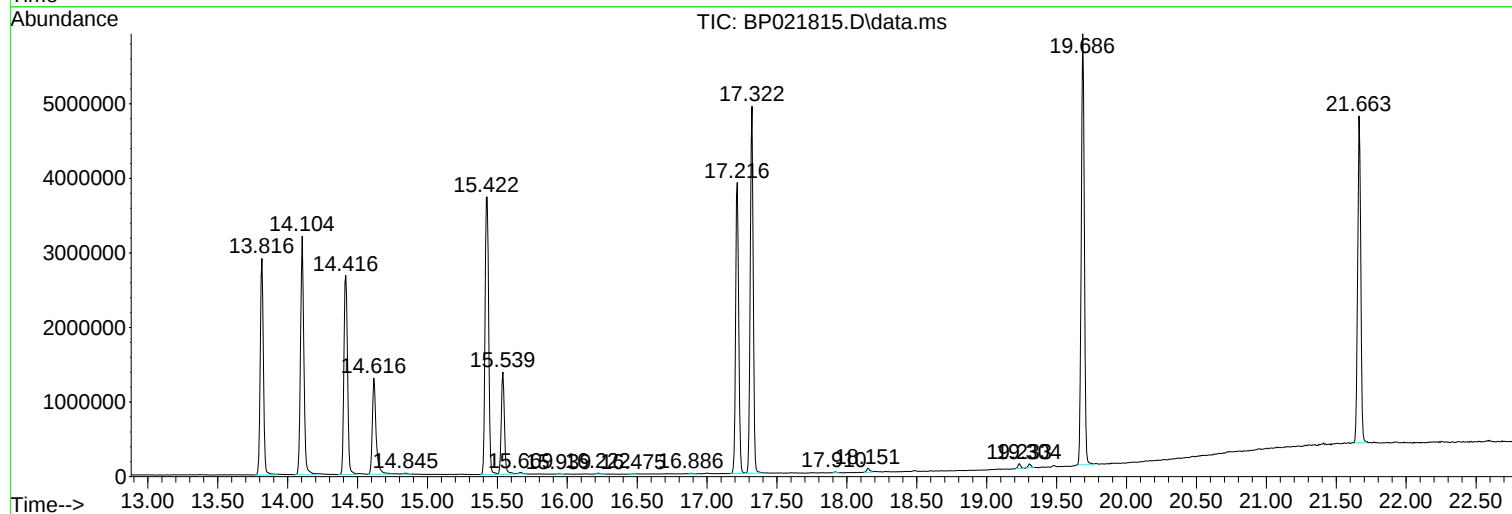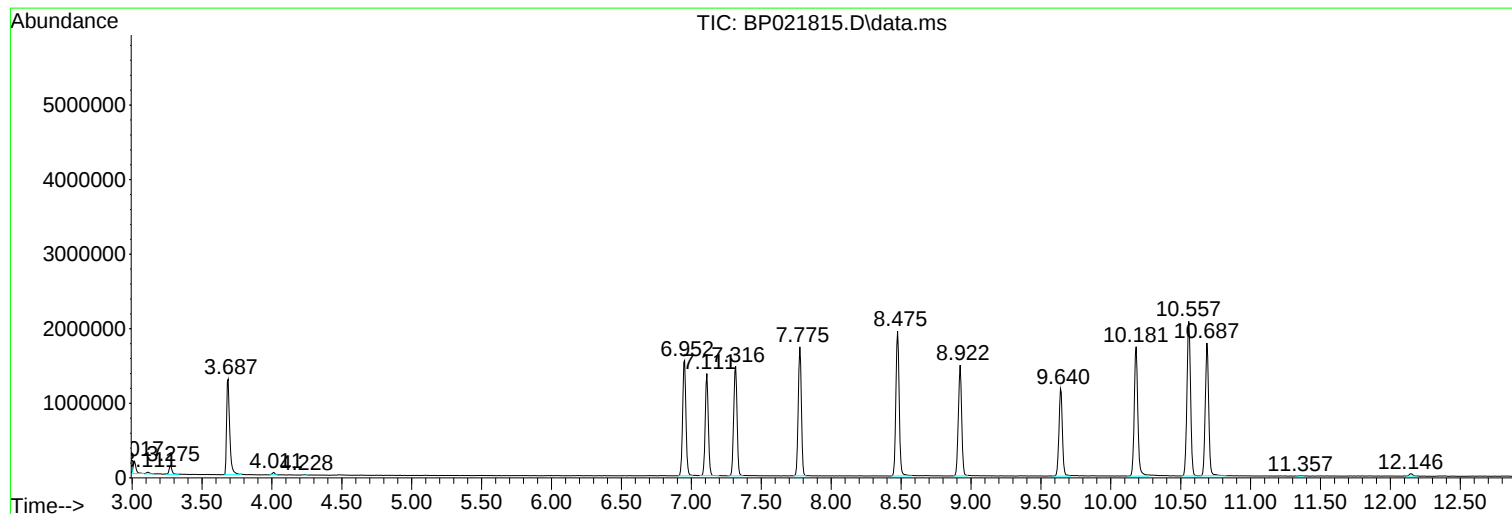

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
Data File : BP021815.D
Acq On : 04 Sep 2024 11:56
Operator : RC/JU
Sample : PB163092BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK092

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
Data File : BP021815.D
Acq On : 04 Sep 2024 11:56
Operator : RC/JU
Sample : PB163092BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK092

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc