

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
 Data File : BP021821.D
 Acq On : 04 Sep 2024 17:47
 Operator : RC/JU
 Sample : P3809-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YE3E9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021821.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.011	3	4	28	rVB	11336608	13344967	100.00%	12.853%
2	3.269	44	48	58	rVB	68272	98440	0.74%	0.095%
3	3.687	115	119	133	rBV	324014	515497	3.86%	0.497%
4	4.011	169	174	182	rVB	23385	36816	0.28%	0.035%
5	4.452	245	249	256	rBV5	6351	13387	0.10%	0.013%
6	4.799	304	308	315	rBV2	12783	21107	0.16%	0.020%
7	4.916	321	328	334	rVB3	13742	26678	0.20%	0.026%
8	5.093	354	358	366	rVB2	8931	15492	0.12%	0.015%
9	6.057	516	522	528	rVB3	38887	76649	0.57%	0.074%
10	6.946	665	673	685	rBV	344666	574517	4.31%	0.553%
11	7.105	693	700	710	rVB	1124497	1701485	12.75%	1.639%
12	7.310	725	735	744	rBV	1141940	1839307	13.78%	1.772%
13	7.769	806	813	821	rBV	1319964	2194073	16.44%	2.113%
14	7.840	821	825	837	rVB5	9392	18852	0.14%	0.018%
15	8.134	870	875	882	rVB6	9398	15853	0.12%	0.015%
16	8.475	926	933	941	rBV	1061436	1686260	12.64%	1.624%
17	8.916	1001	1008	1021	rBV	1216512	2056111	15.41%	1.980%
18	9.363	1078	1084	1088	rBV3	9113	14394	0.11%	0.014%
19	9.481	1099	1104	1111	rBV2	15067	22343	0.17%	0.022%
20	9.569	1113	1119	1124	rBV	15383	30113	0.23%	0.029%
21	9.640	1124	1131	1143	rBV	958015	1624057	12.17%	1.564%
22	10.181	1214	1223	1238	rBV	1390839	2637729	19.77%	2.541%
23	10.557	1278	1287	1298	rBV	1873351	3118929	23.37%	3.004%
24	10.687	1302	1309	1328	rBV	1329461	2294982	17.20%	2.210%
25	10.875	1336	1341	1347	rBV	9304	19371	0.15%	0.019%
26	11.363	1418	1424	1429	rBV9	7499	16912	0.13%	0.016%
27	12.151	1551	1558	1565	rVB2	23346	40133	0.30%	0.039%
28	12.604	1628	1635	1642	rBV	15731	26147	0.20%	0.025%
29	13.245	1739	1744	1751	rVB4	9449	15760	0.12%	0.015%
30	13.816	1834	1841	1857	rBV	2804599	4483636	33.60%	4.318%
31	14.110	1880	1891	1907	rBV	2786393	4746743	35.57%	4.572%
32	14.416	1933	1943	1958	rBV	2508858	4319319	32.37%	4.160%
33	14.628	1972	1979	1995	rBV	302735	599747	4.49%	0.578%
34	14.781	2003	2005	2011	rVB7	11225	14460	0.11%	0.014%
35	14.851	2013	2017	2024	rVB9	14077	23616	0.18%	0.023%
36	15.428	2107	2115	2129	rBV	4549454	6418012	48.09%	6.182%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
 Data File : BP021821.D
 Acq On : 04 Sep 2024 17:47
 Operator : RC/JU
 Sample : P3809-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YE3E9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Title : SVOA CALIBRATION

37	15.551	2129	2136	2152	rVV	1456564	2208251	16.55%	2.127%
38	15.669	2153	2156	2165	rVB3	26017	45559	0.34%	0.044%
39	15.804	2174	2179	2188	rVB	110302	170264	1.28%	0.164%
40	16.380	2274	2277	2282	rVB3	16634	19688	0.15%	0.019%
41	17.222	2413	2420	2431	rBV	3433215	5455518	40.88%	5.255%
42	17.333	2431	2439	2450	rBV2	4745327	7559383	56.65%	7.281%
43	17.927	2537	2540	2544	rBV6	14320	19753	0.15%	0.019%
44	18.169	2576	2581	2587	rBV	222369	338868	2.54%	0.326%
45	18.616	2654	2657	2660	rVB4	20648	27023	0.20%	0.026%
46	19.251	2761	2765	2770	rBV2	87703	116460	0.87%	0.112%
47	19.322	2773	2777	2782	rVV	71061	94162	0.71%	0.091%
48	19.492	2803	2806	2814	rBV3	125727	184397	1.38%	0.178%
49	19.698	2835	2841	2851	rVB	7164901	9476976	71.02%	9.128%
50	21.357	3120	3123	3128	rVB5	109959	158064	1.18%	0.152%
51	21.680	3172	3178	3189	rVB2	3567527	6314207	47.32%	6.082%
52	24.845	3707	3716	3730	rVB2	3474082	9987979	74.84%	9.620%
53	25.086	3748	3757	3773	rVB2	2370762	6946344	52.05%	6.690%




Sum of corrected areas: 103824790

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
Data File : BP021821.D
Acq On : 04 Sep 2024 17:47
Operator : RC/JU
Sample : P3809-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YE3E9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

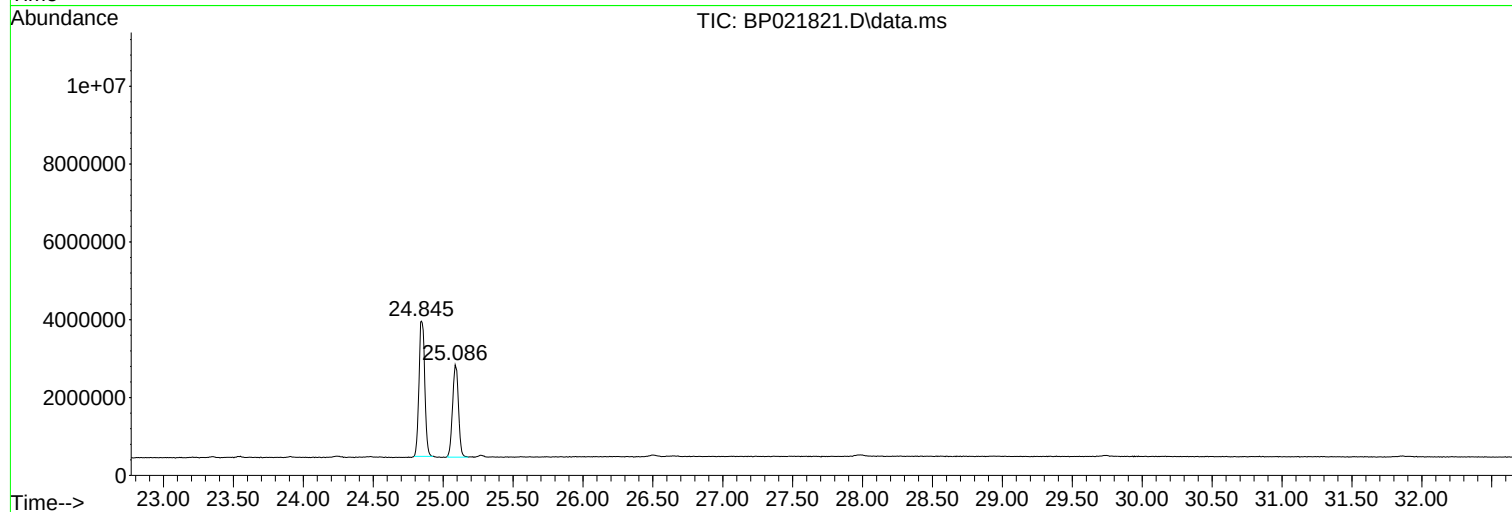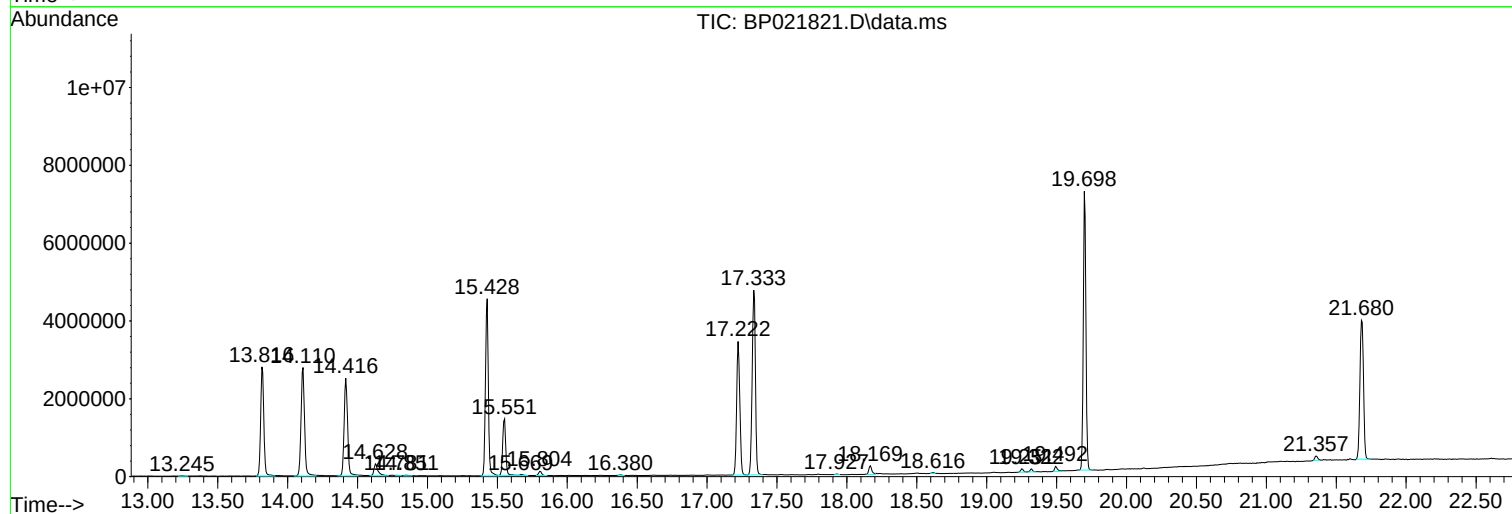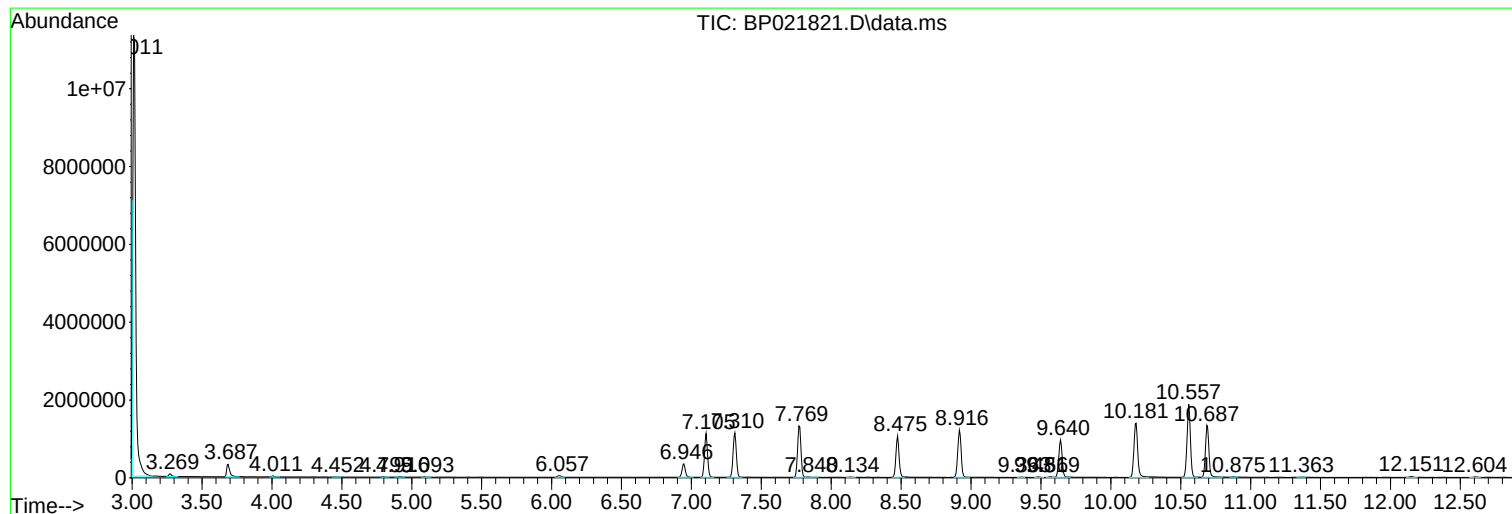

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
Data File : BP021821.D
Acq On : 04 Sep 2024 17:47
Operator : RC/JU
Sample : P3809-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YE3E9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.011	121.65 ng/ul	13345000	1,4-Dichlorobenzene-d4	7.775

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39		
4	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23		
5	Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9		

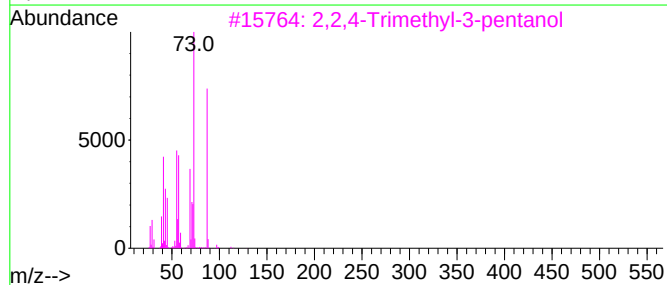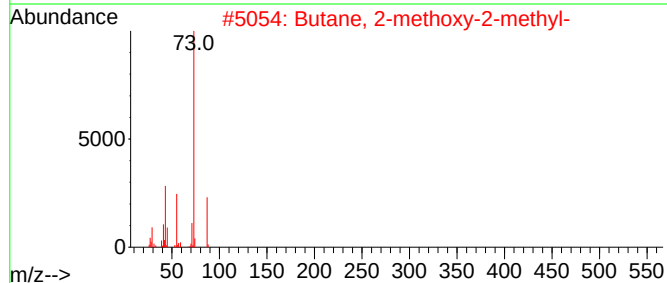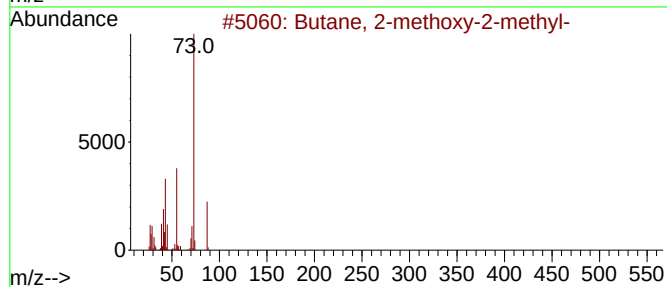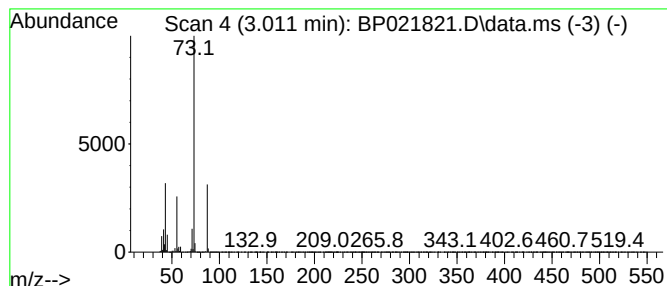

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090424\
Data File : BP021821.D
Acq On : 04 Sep 2024 17:47
Operator : RC/JU
Sample : P3809-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YE3E9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.011	121.7	ng/ul	13345000	1	7.775	2194070	20.0