
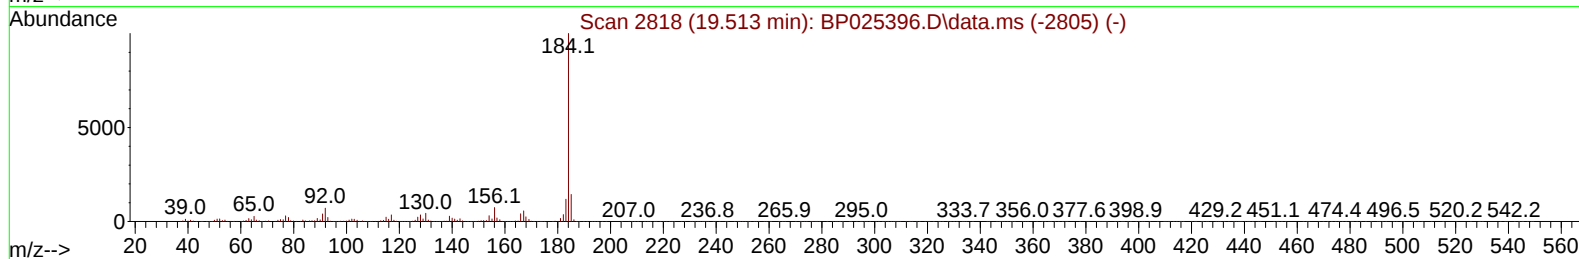
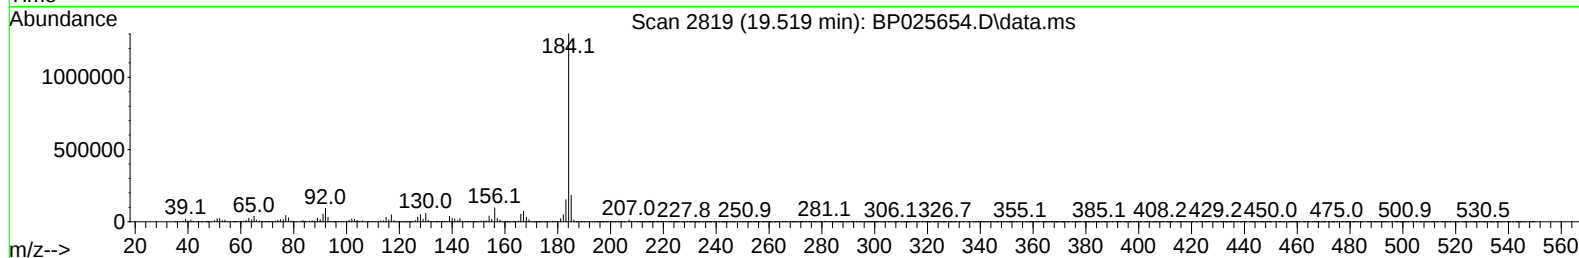


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090425\
Data File : BP025654.D
Acq On : 04 Sep 2025 09:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 12:35:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

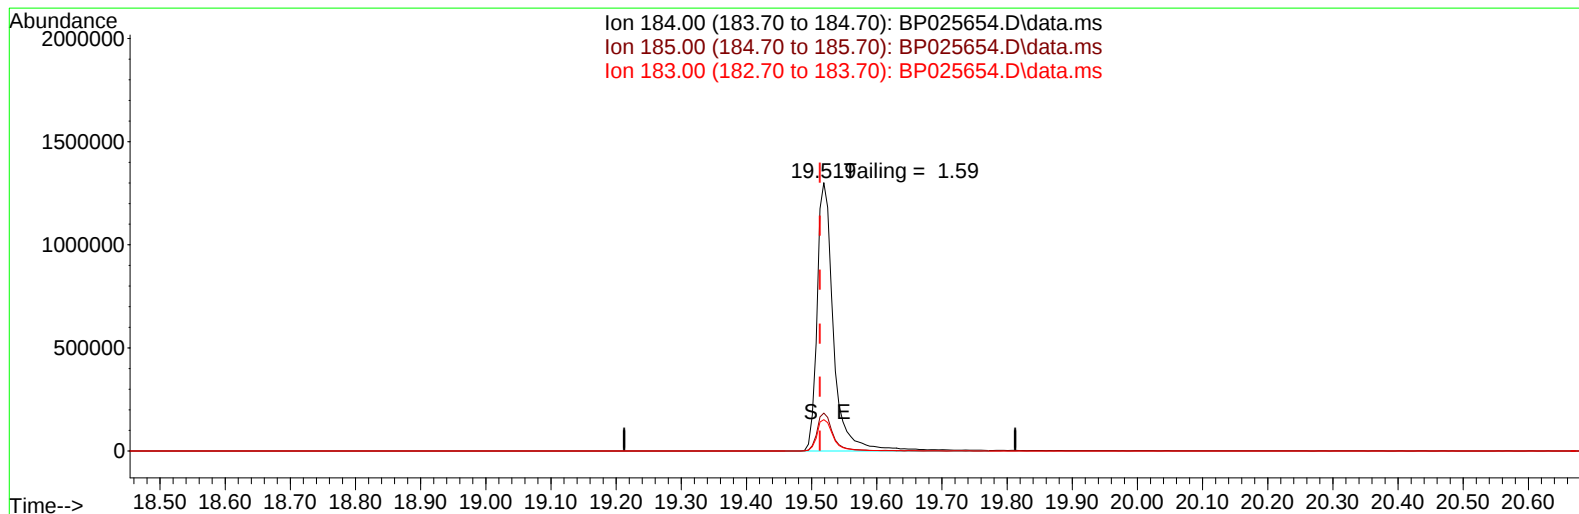

TIC: BP025654.D\data.ms

(77) Benzidine




19.519min (+ 0.006) 37869.50 ng

response 2273343

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.16
183.00	11.80	11.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090425\
Data File : BP025654.D
Acq On : 04 Sep 2025 09:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 12:35:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

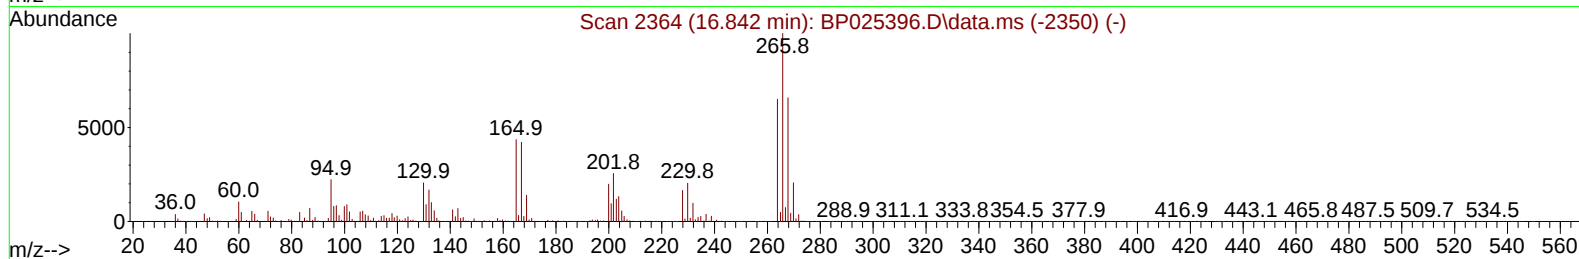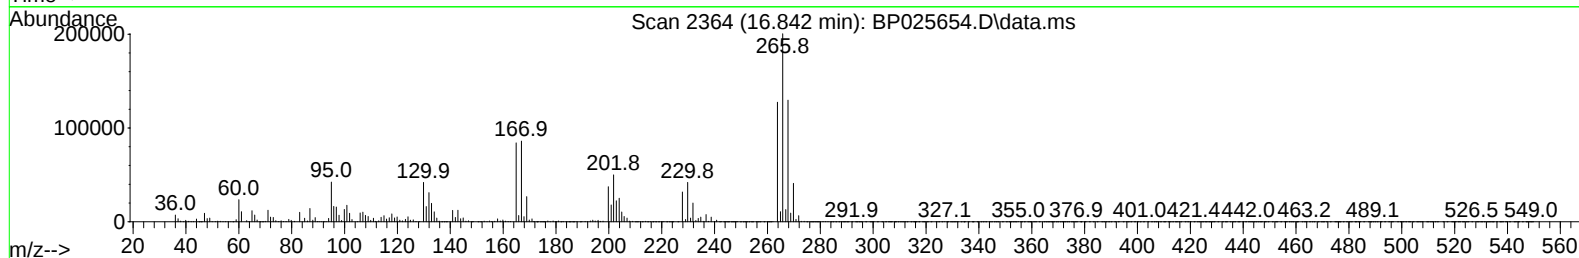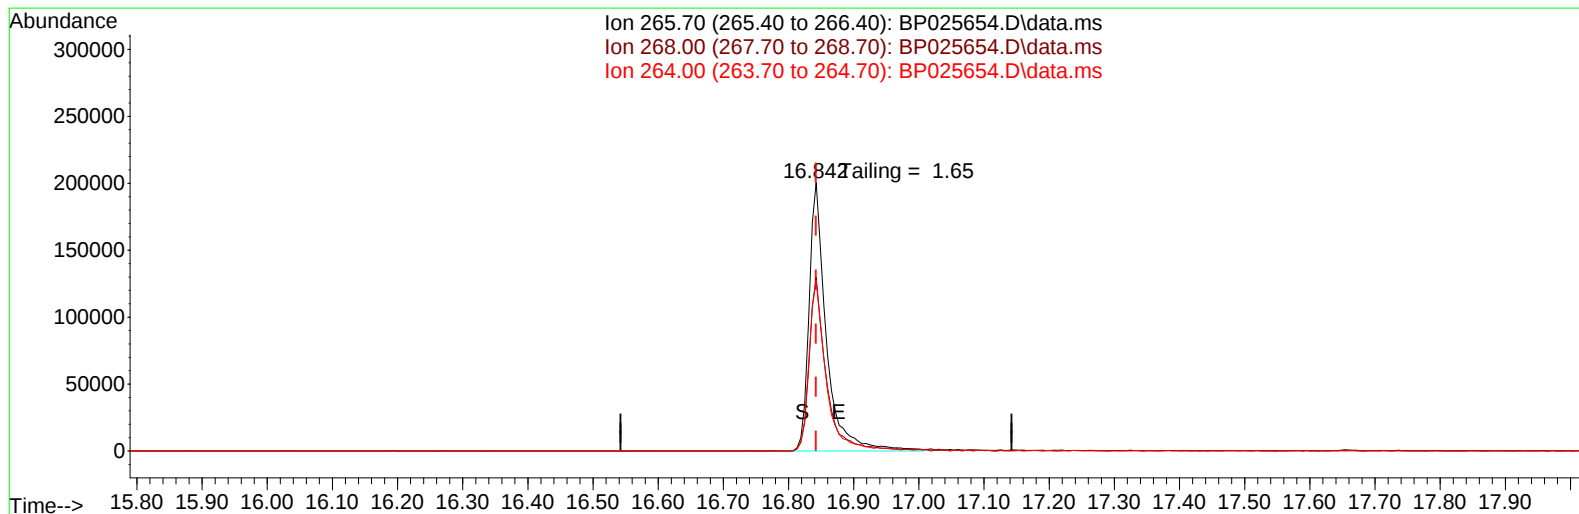

TIC: BP025654.D\data.ms

(70) Pentachlorophenol (C)

16.842min (+ 0.000) 2716934.76 ng

response 371716

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	64.65
264.00	65.00	63.60
0.00	0.00	0.00