


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090425\
Data File : BP025654.D
Acq On : 04 Sep 2025 09:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 14 18:14:31 2025

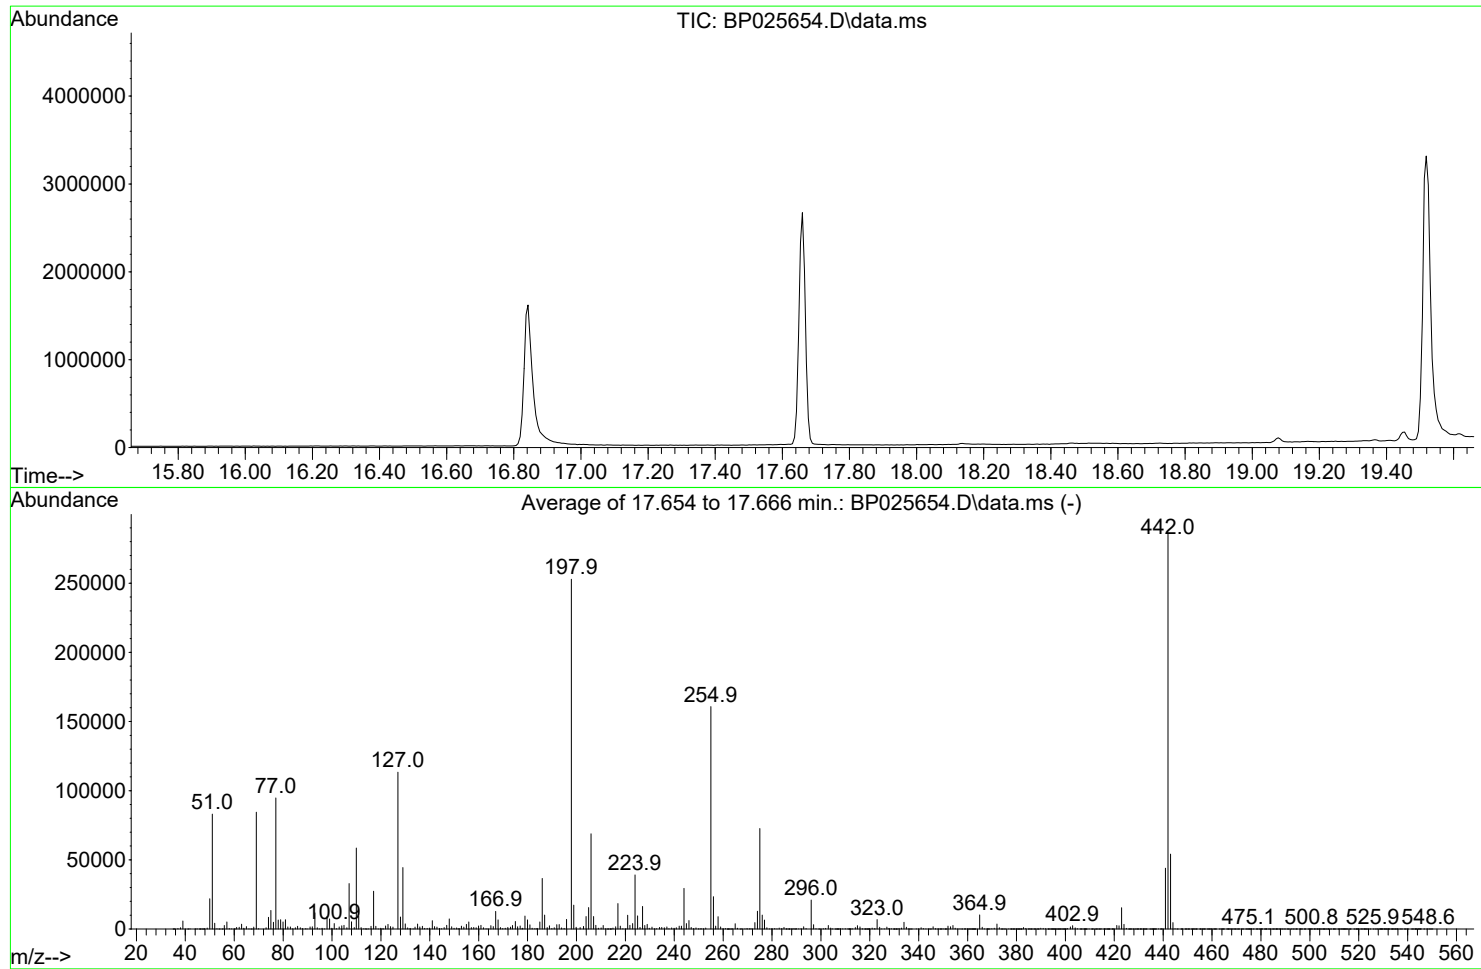

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2495

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	1403	PASS
69	69	100	100	100.0	84491	PASS
70	69	0.00	2	0.3	230	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	252886	PASS
199	198	5	9	6.8	17305	PASS
365	198	1	100	4.1	10252	PASS
441	443	0.01	150	81.1	43934	PASS
442	442	100	100	100.0	285440	PASS
443	442	15	24	19.0	54205	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/4/2025	BNA_P	<u>BP025654.D</u>
Compound Name	Response	Retention Time
DDT	1133989	20.813
DDD	22445	20.36
DDE	6111	19.825
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28556	1162545	2.46

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090425\
Data File : BP025654.D
Acq On : 04 Sep 2025 09:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 04 12:35:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

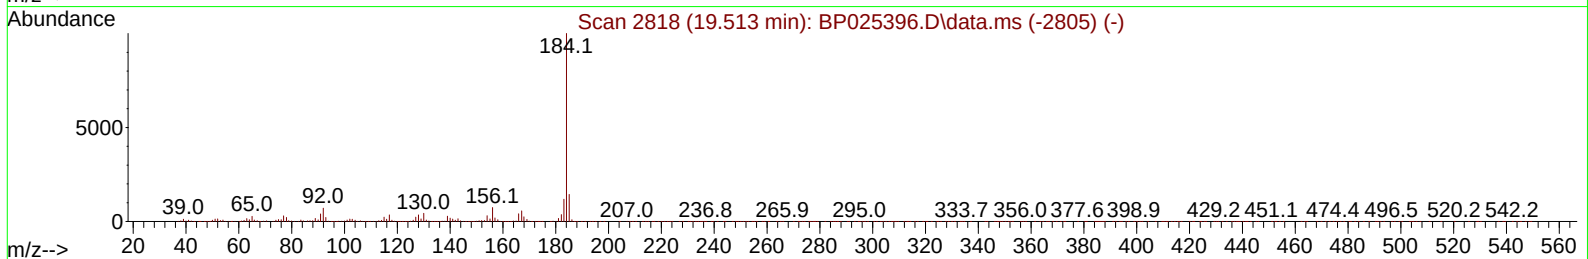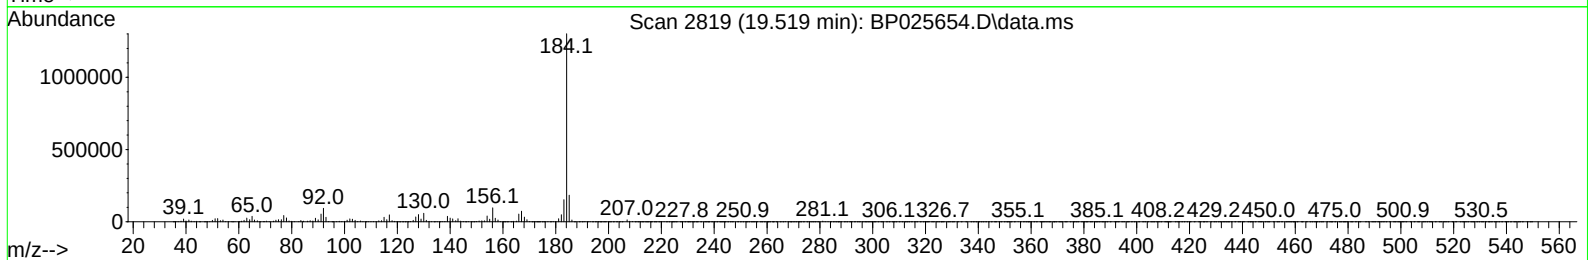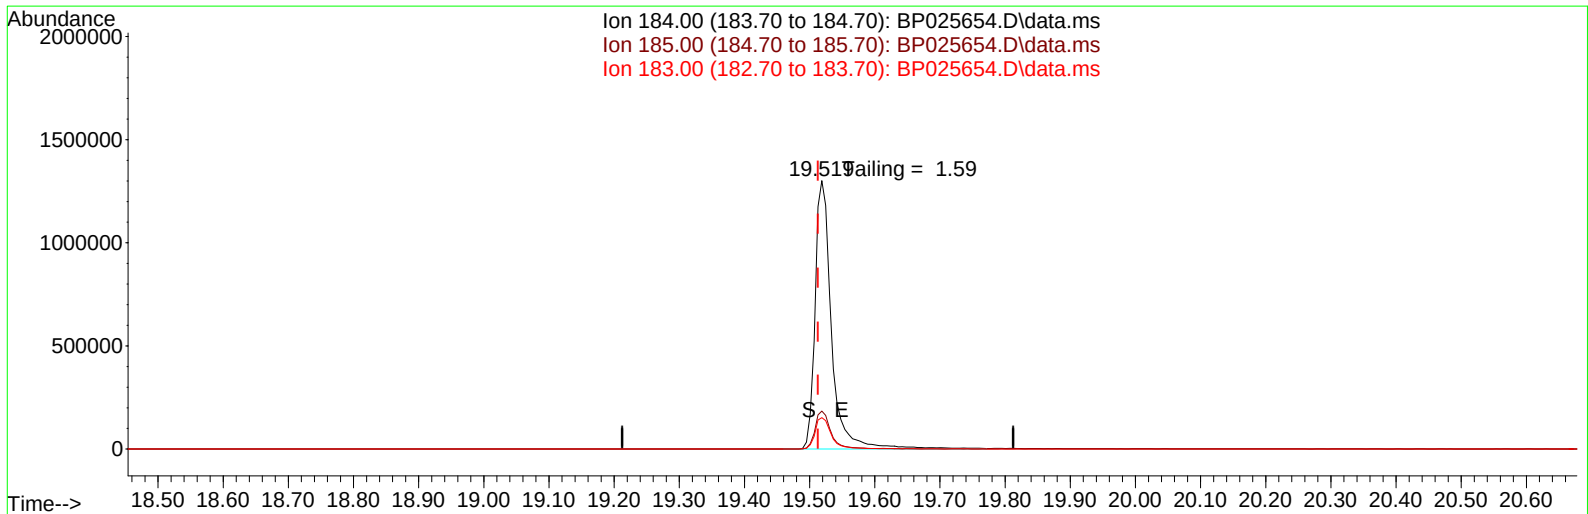

TIC: BP025654.D\data.ms

(77) Benzidine

19.519min (+ 0.006) 37869.50 ng




response 2273343

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.16
183.00	11.80	11.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090425\
Data File : BP025654.D
Acq On : 04 Sep 2025 09:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 04 12:35:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

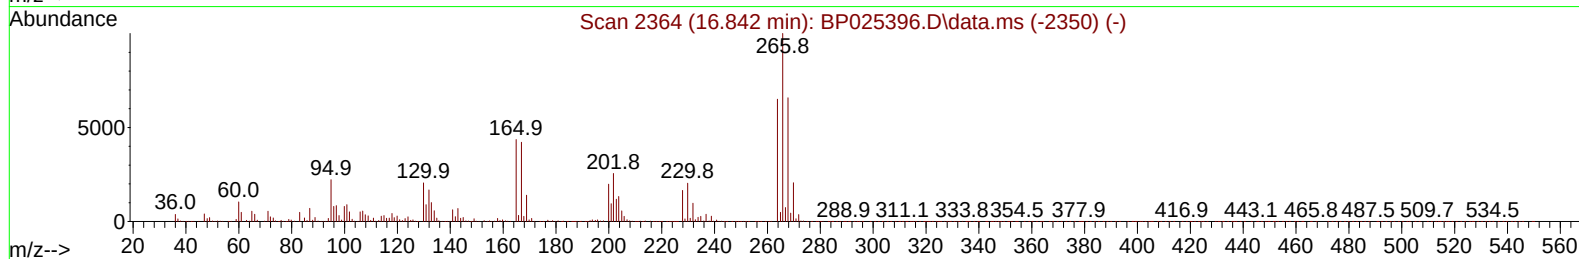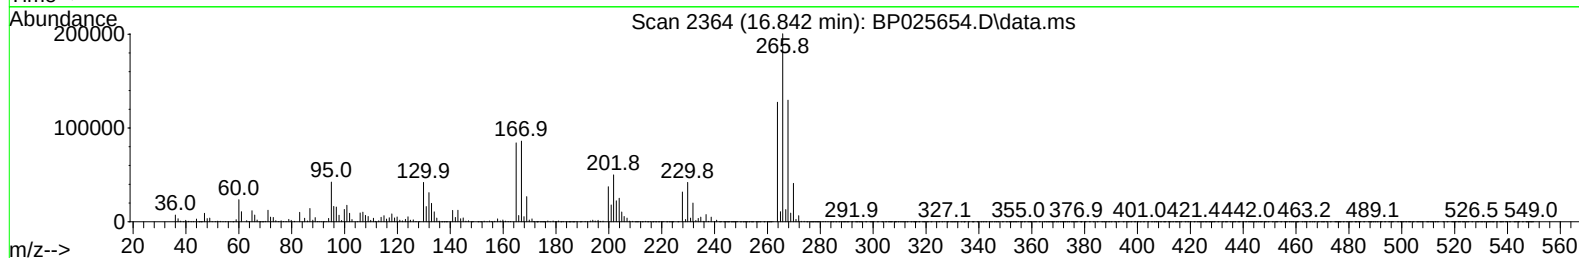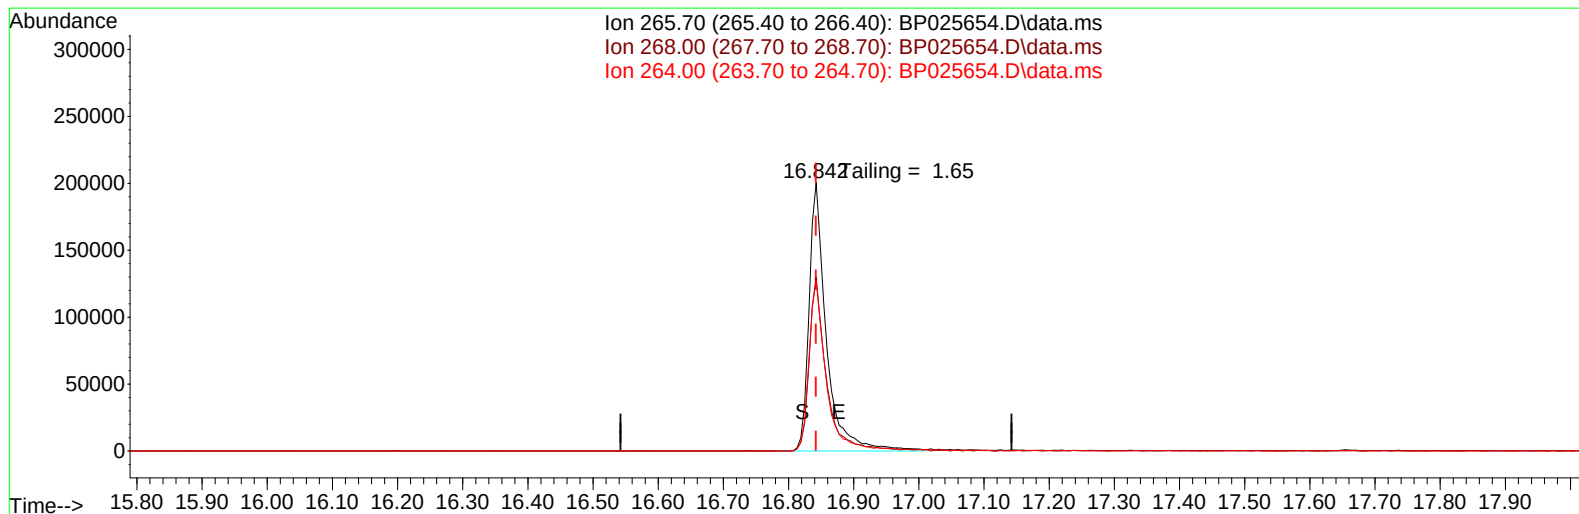

TIC: BP025654.D\data.ms

(70) Pentachlorophenol (C)

16.842min (+ 0.000) 2716934.76 ng

response 371716

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	64.65
264.00	65.00	63.60
0.00	0.00	0.00