
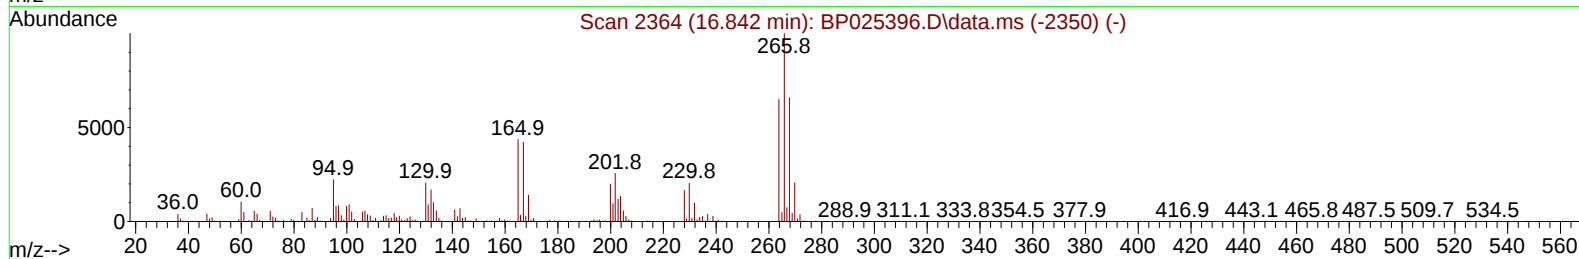
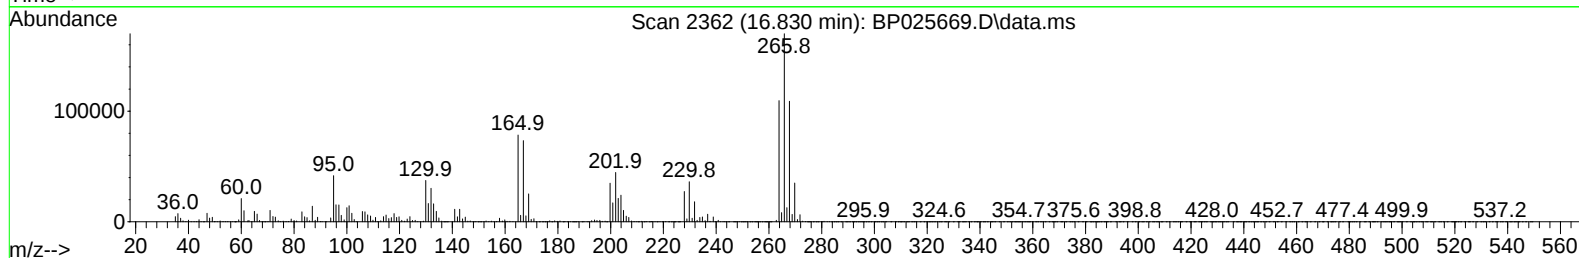


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090525\
Data File : BP025669.D
Acq On : 05 Sep 2025 08:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 12:38:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

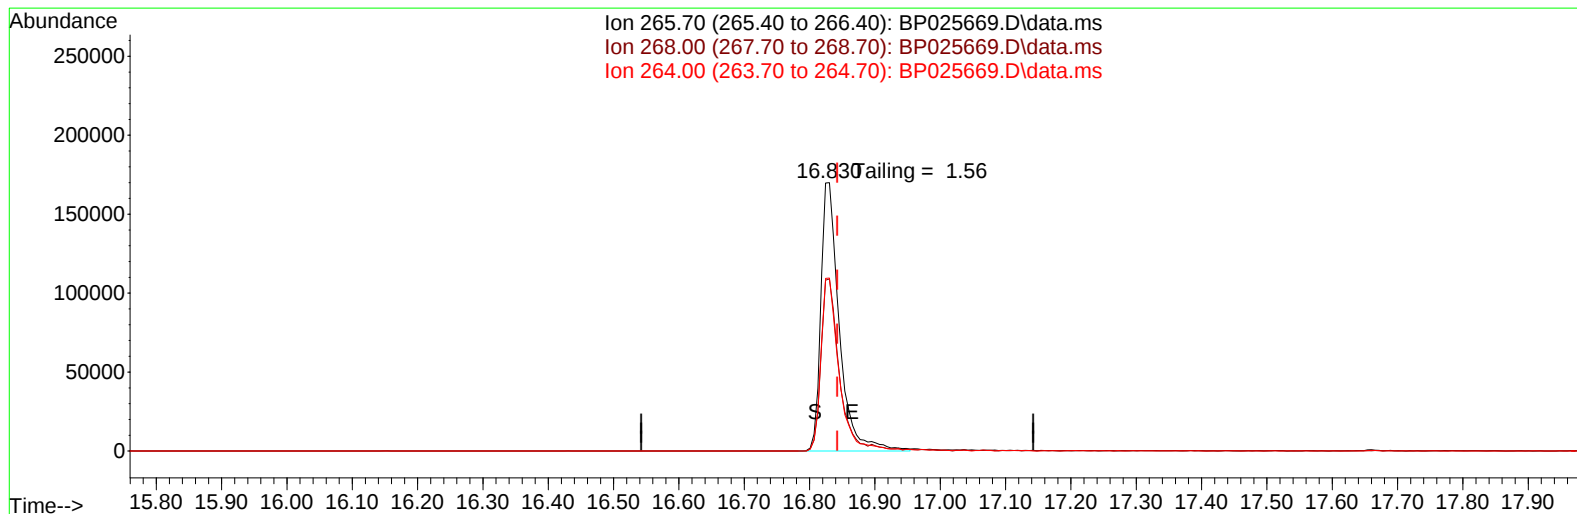

TIC: BP025669.D\data.ms

(70) Pentachlorophenol (C)




16.830min (-0.012) 9764.95 ng

response 336433

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	64.11
264.00	65.00	64.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090525\
Data File : BP025669.D
Acq On : 05 Sep 2025 08:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 12:38:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

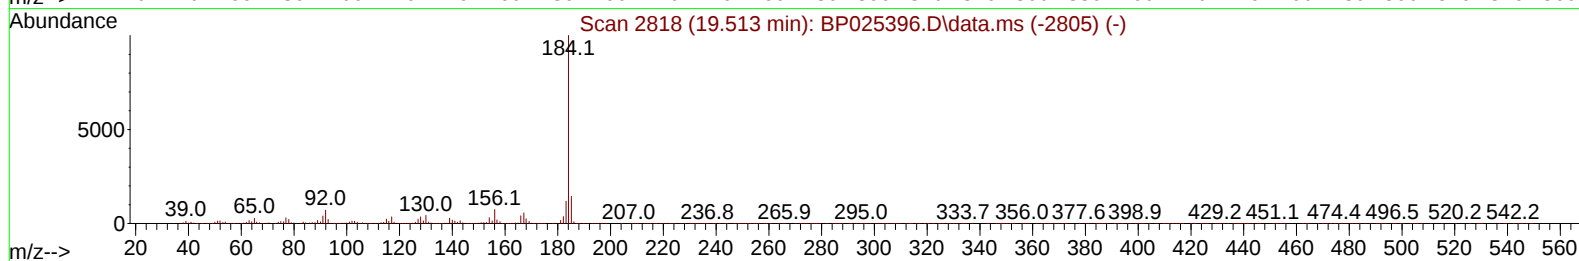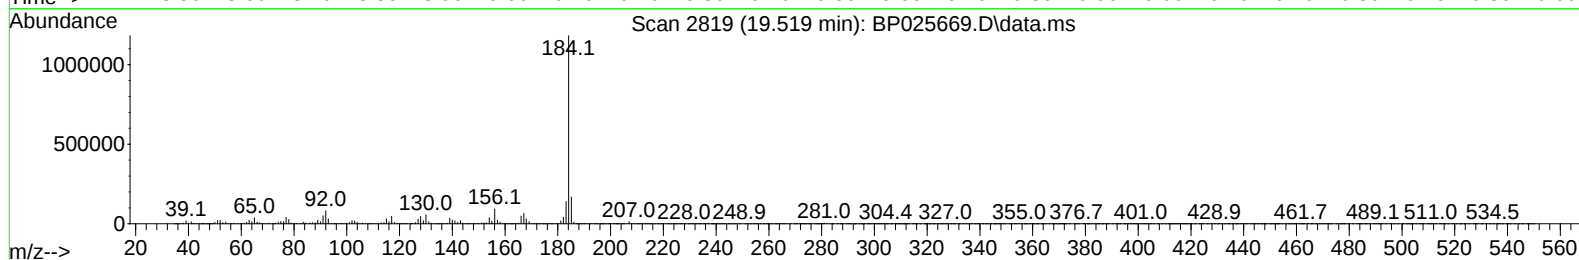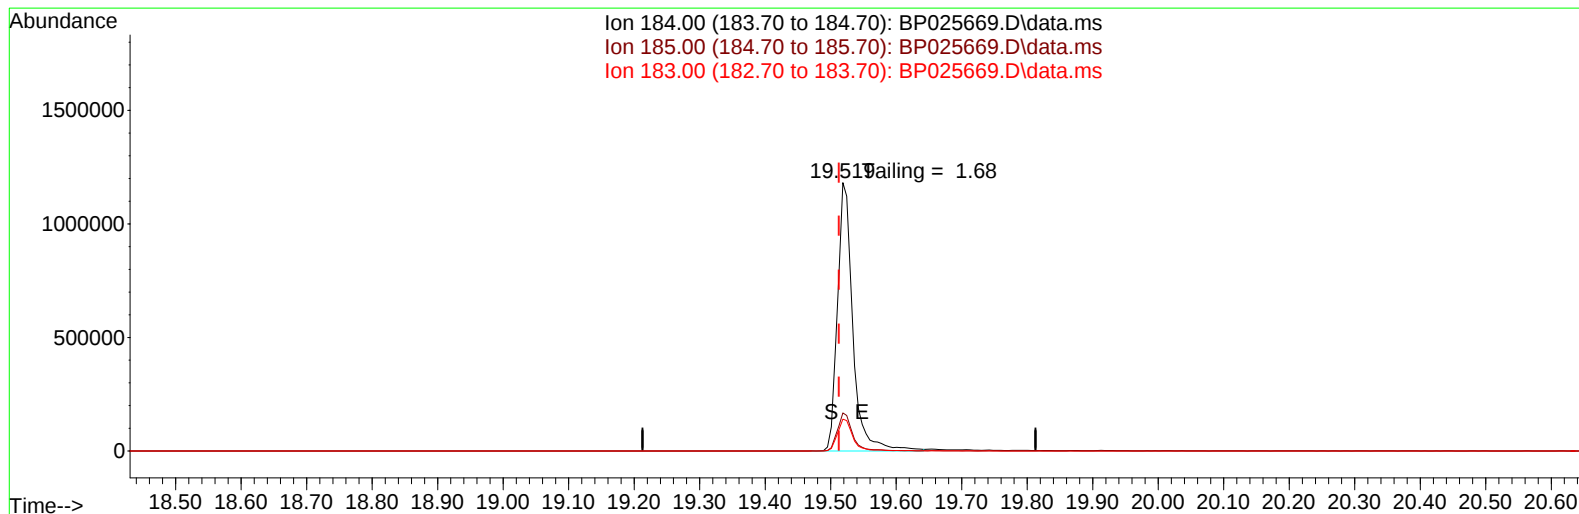

TIC: BP025669.D\data.ms

(77) Benzidine

19.519min (+ 0.006) 1739.01 ng m

response 1928305

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.20
183.00	11.80	11.90
0.00	0.00	0.00