

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090525\
 Data File : BP025680.D
 Acq On : 05 Sep 2025 17:26
 Operator : CG/JU
 Sample : PB169509BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB169509BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP025680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.067	19	22	36	rVB	104354	187359	1.79%	0.380%
2	4.931	333	339	347	rBV	359615	490626	4.67%	0.996%
3	5.396	411	418	435	rBV	2888172	4421826	42.13%	8.976%
4	6.960	675	684	703	rBV	2535725	4458444	42.48%	9.050%
5	7.772	815	822	833	rBV	484121	778201	7.41%	1.580%
6	8.913	1007	1016	1035	rBV	1676488	2990776	28.50%	6.071%
7	10.543	1284	1293	1308	rBV	530679	1044846	9.96%	2.121%
8	13.001	1704	1711	1730	rBV	4030626	6446234	61.42%	13.085%
9	14.395	1941	1948	1967	rVB	923961	1405032	13.39%	2.852%
10	15.913	2198	2206	2217	rBV	3698590	5769666	54.98%	11.712%
11	17.201	2418	2425	2436	rBV2	1124755	1786136	17.02%	3.626%
12	17.689	2500	2508	2514	rBV	244409	697440	6.65%	1.416%
13	17.748	2514	2518	2521	rVB3	68060	140954	1.34%	0.286%
14	18.130	2579	2583	2598	rVB	375395	637236	6.07%	1.294%
15	18.813	2695	2699	2702	rBV6	64993	106408	1.01%	0.216%
16	19.466	2807	2810	2816	rVB	202951	381492	3.63%	0.774%
17	19.789	2860	2865	2869	rVB	761809	1065915	10.16%	2.164%
18	19.919	2882	2887	2893	rVB	8896807	10495072	100.00%	21.304%
19	20.313	2950	2954	2956	rBV2	187755	220270	2.10%	0.447%
20	20.507	2985	2987	2988	rBV	124016	115432	1.10%	0.234%
21	20.936	3058	3060	3061	rBV	337633	257688	2.46%	0.523%
22	21.654	3175	3182	3188	rBV2	1479919	2880777	27.45%	5.848%
23	22.107	3255	3259	3264	rVB	417356	712927	6.79%	1.447%
24	25.030	3750	3756	3767	rBV2	614577	1773026	16.89%	3.599%




Sum of corrected areas: 49263783

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090525\
Data File : BP025680.D
Acq On : 05 Sep 2025 17:26
Operator : CG/JU
Sample : PB169509BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169509BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

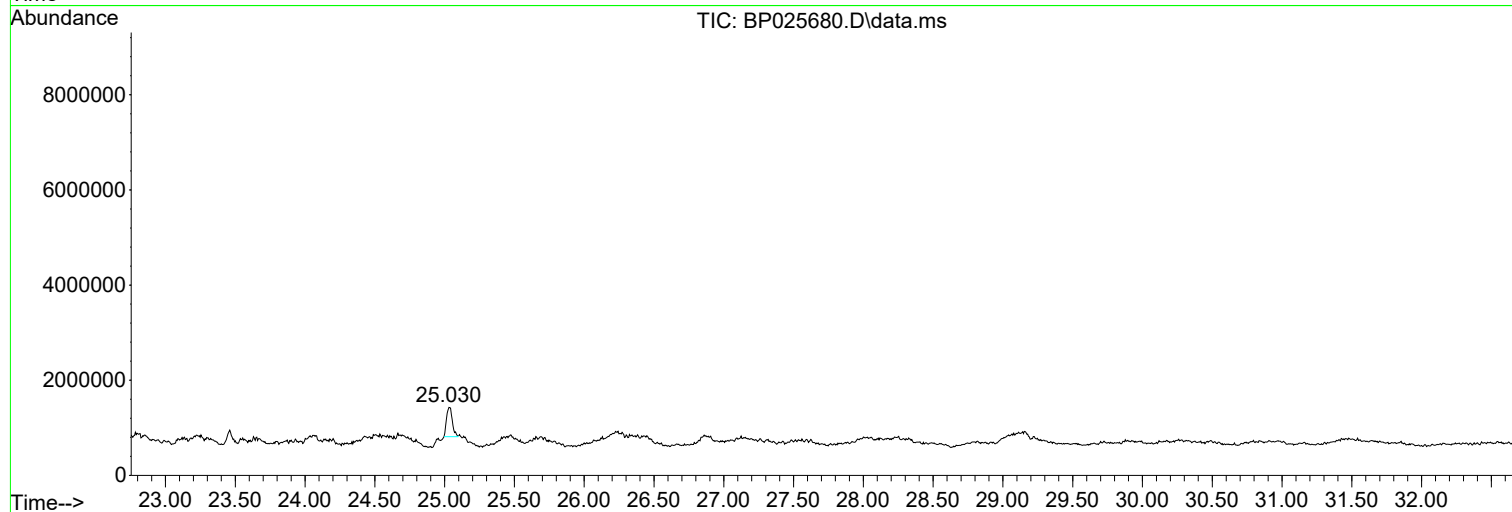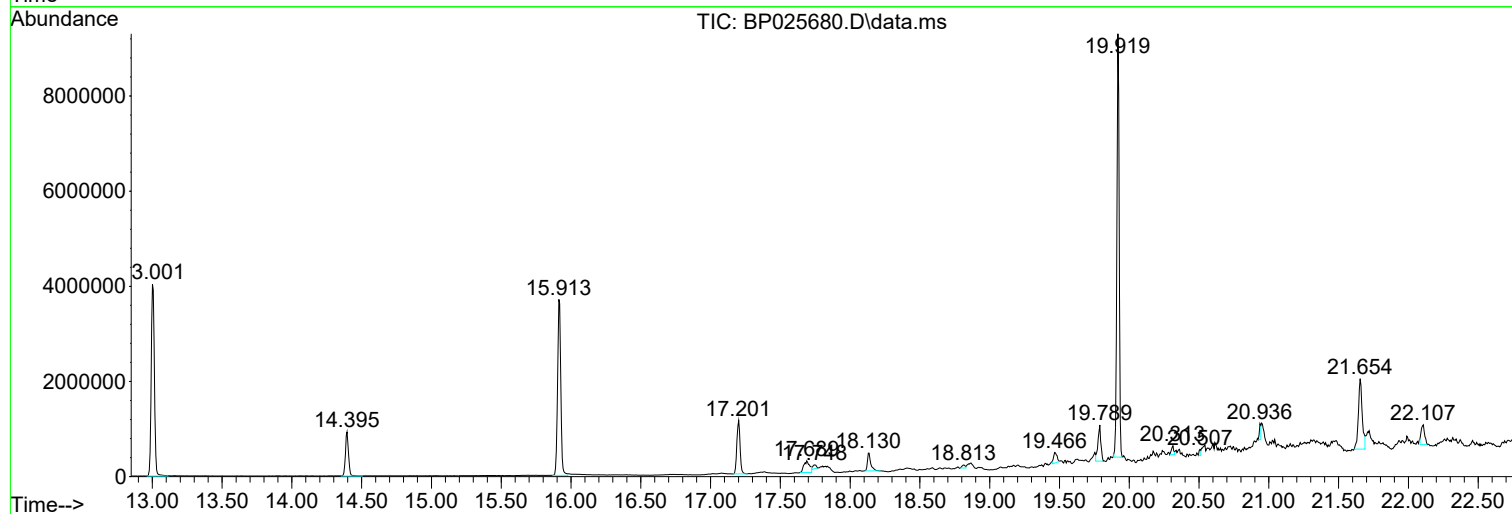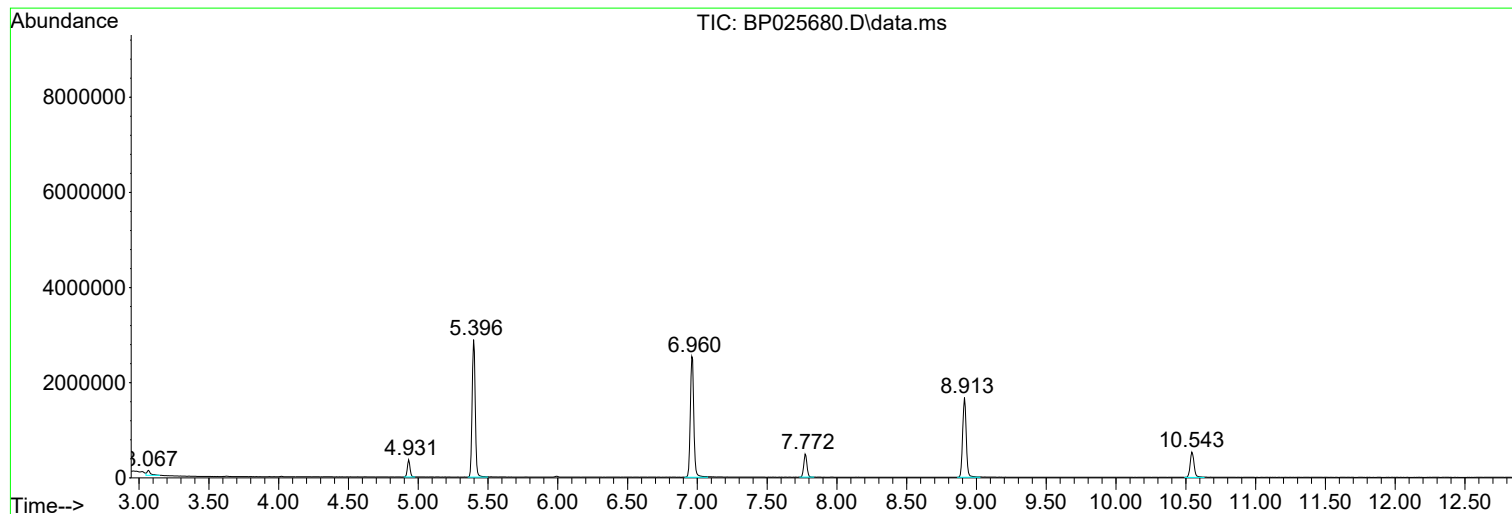

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090525\
Data File : BP025680.D
Acq On : 05 Sep 2025 17:26
Operator : CG/JU
Sample : PB169509BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169509BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090525\
Data File : BP025680.D
Acq On : 05 Sep 2025 17:26
Operator : CG/JU
Sample : PB169509BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB169509BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------