
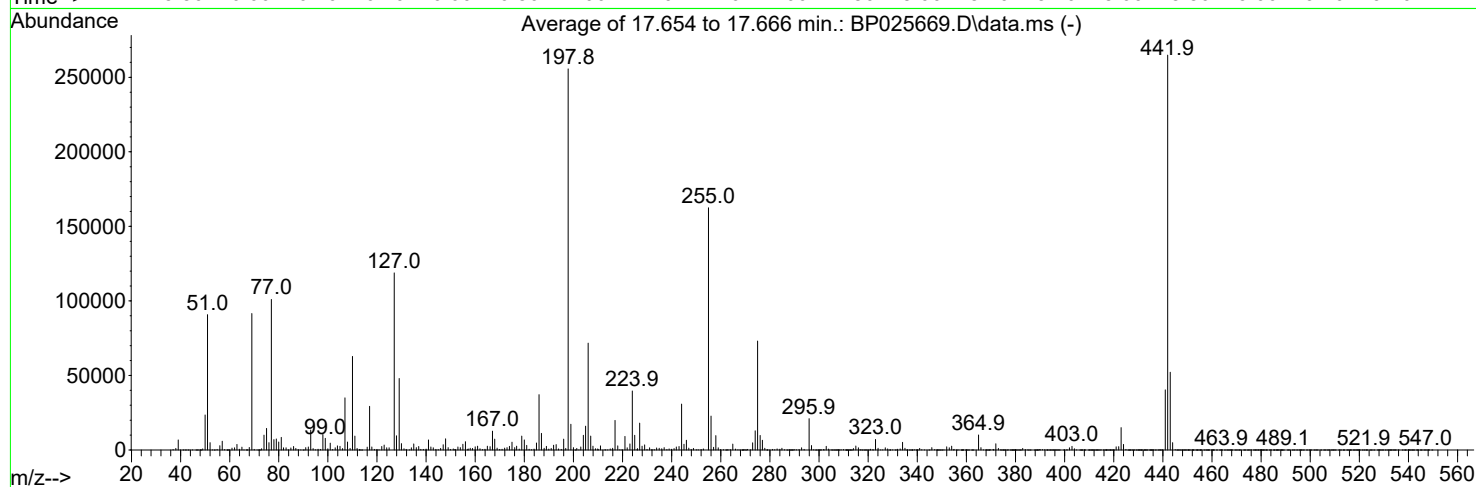


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP090525\  
Data File : BP025669.D  
Acq On : 05 Sep 2025 08:37  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP081425.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Aug 14 18:14:31 2025

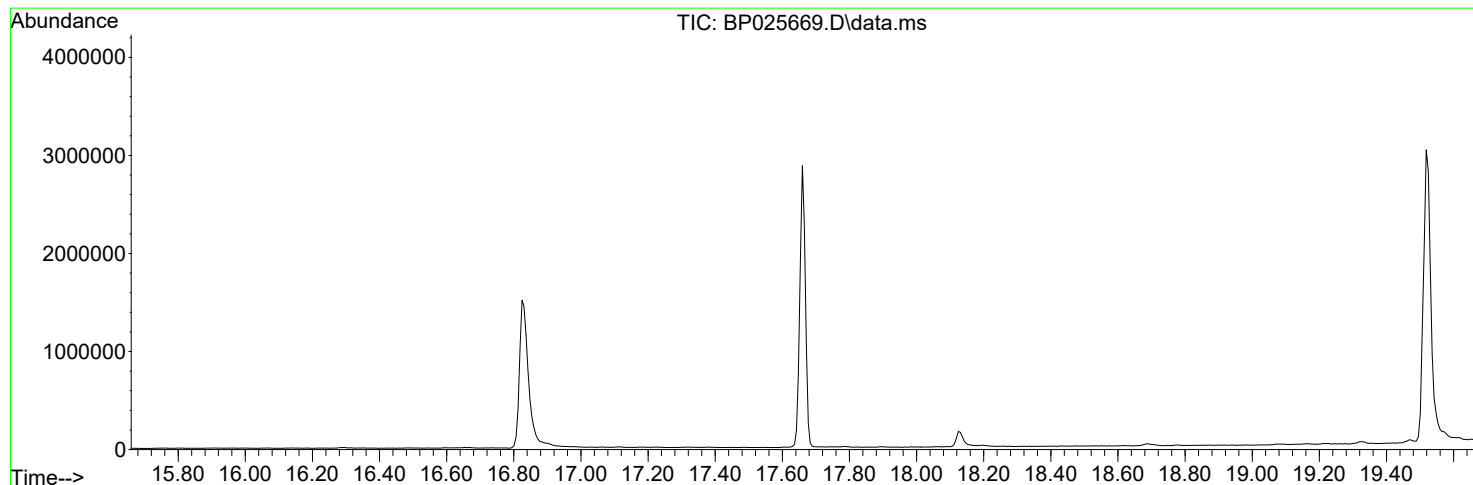

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2494

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 68     | 69      | 0.00   | 2      | 1.9   | 1712   | PASS      |
| 69     | 69      | 100    | 100    | 100.0 | 91557  | PASS      |
| 70     | 69      | 0.00   | 2      | 0.4   | 411    | PASS      |
| 197    | 198     | 0.00   | 2      | 0.4   | 1060   | PASS      |
| 198    | 198     | 100    | 100    | 100.0 | 255636 | PASS      |
| 199    | 198     | 5      | 9      | 6.8   | 17320  | PASS      |
| 365    | 198     | 1      | 100    | 3.9   | 10062  | PASS      |
| 441    | 443     | 0.01   | 150    | 77.4  | 40389  | PASS      |
| 442    | 442     | 100    | 100    | 100.0 | 264827 | PASS      |
| 443    | 442     | 15     | 24     | 19.7  | 52172  | PASS      |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 9/5/2025      | BNA_P            | <u>BP025669.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1003773          | 20.813             |
| DDD           | 14508            | 20.36              |
| DDE           | 4813             | 19.83              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 19321         | 1023094          | 1.89               |
|               |                  |                    |

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP090525\  
Data File : BP025669.D  
Acq On : 05 Sep 2025 08:37  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Sep 05 12:38:00 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP081425.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Aug 14 18:14:31 2025  
Response via : Initial Calibration

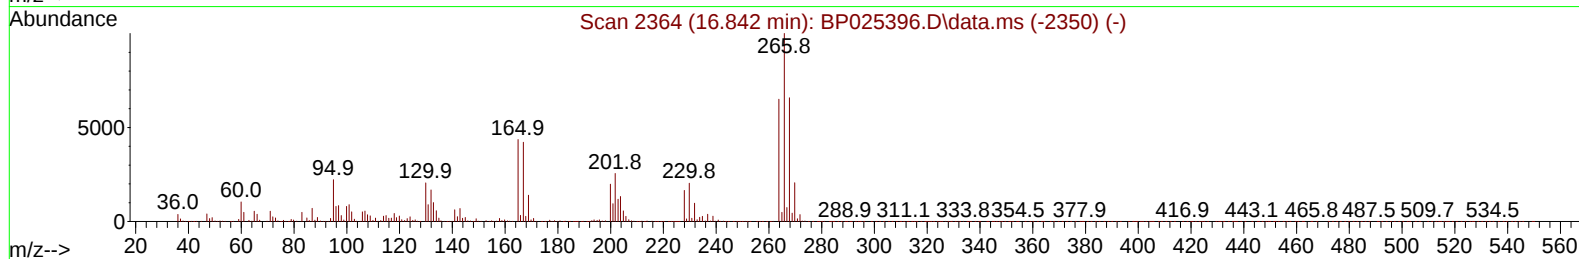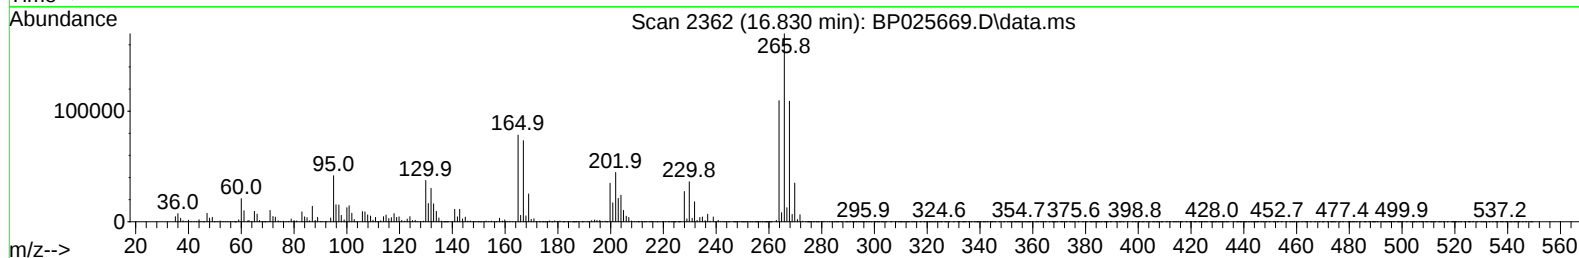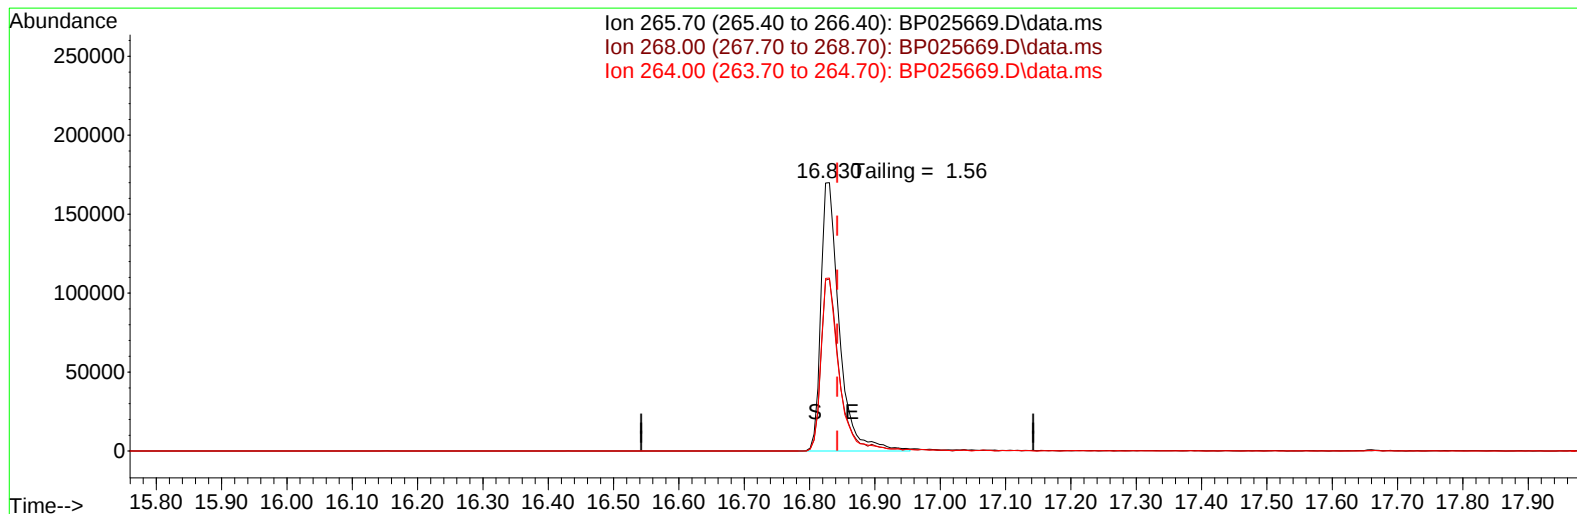

TIC: BP025669.D\data.ms

**(70) Pentachlorophenol (C)**

**16.830min (-0.012) 9764.95 ng**




**response 336433**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.80  | 64.11  |
| 264.00 | 65.00  | 64.46  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP090525\  
Data File : BP025669.D  
Acq On : 05 Sep 2025 08:37  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Sep 05 12:38:00 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP081425.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Aug 14 18:14:31 2025  
Response via : Initial Calibration

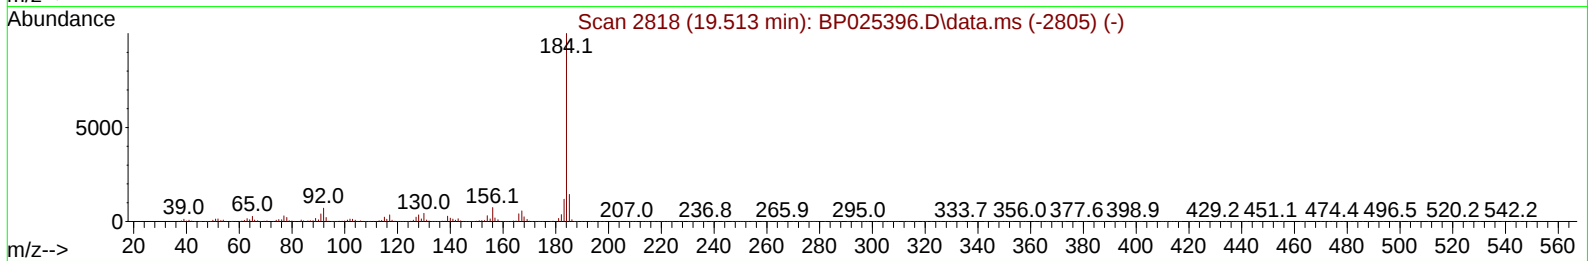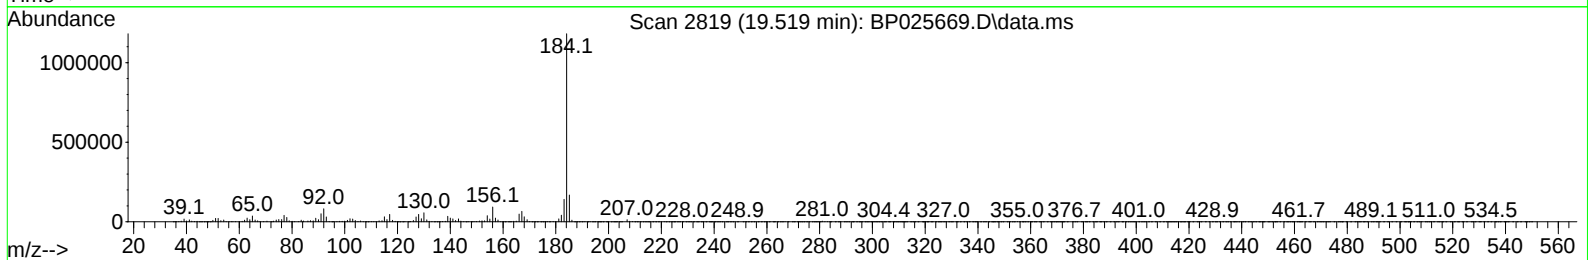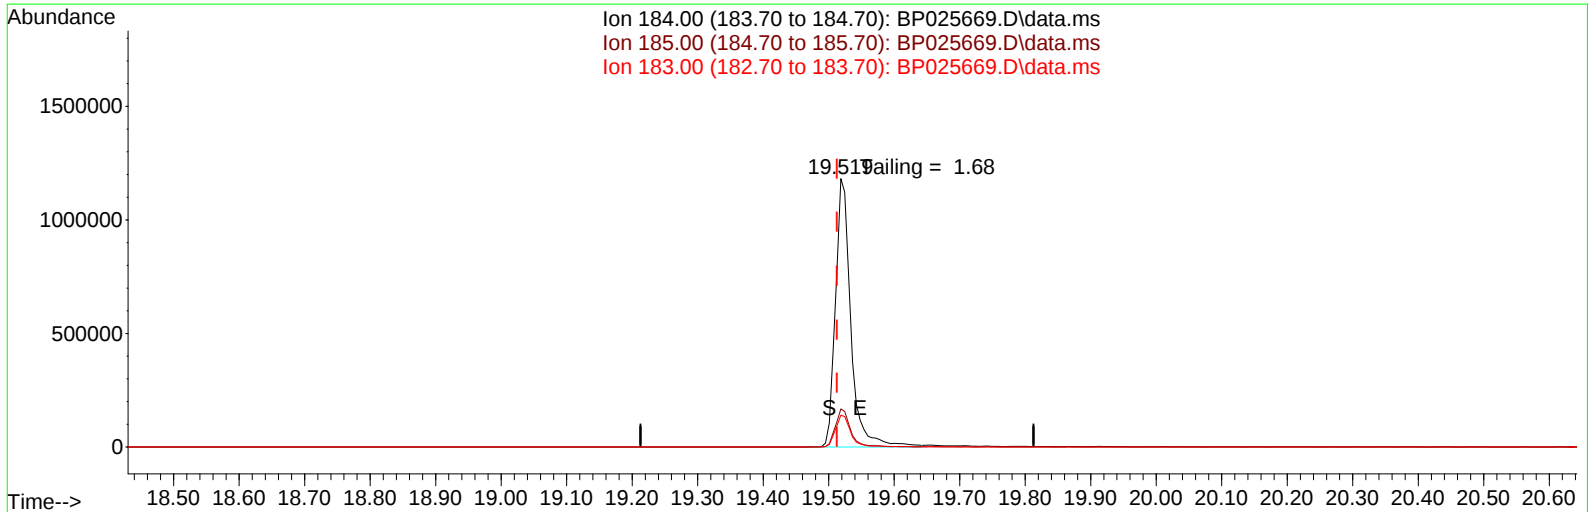

TIC: BP025669.D\data.ms

(77) Benzidine

19.519min (+ 0.006) 1739.01 ng m

response 1928305

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 14.20  |
| 183.00 | 11.80  | 11.90  |
| 0.00   | 0.00   | 0.00   |