
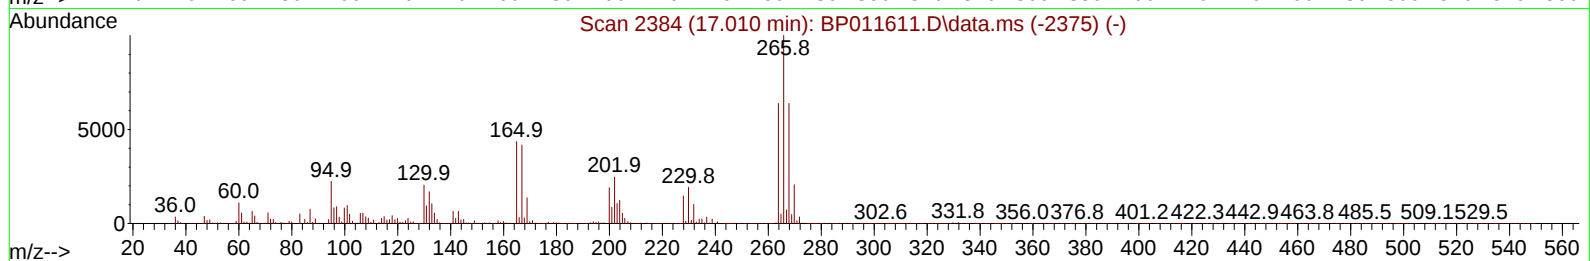
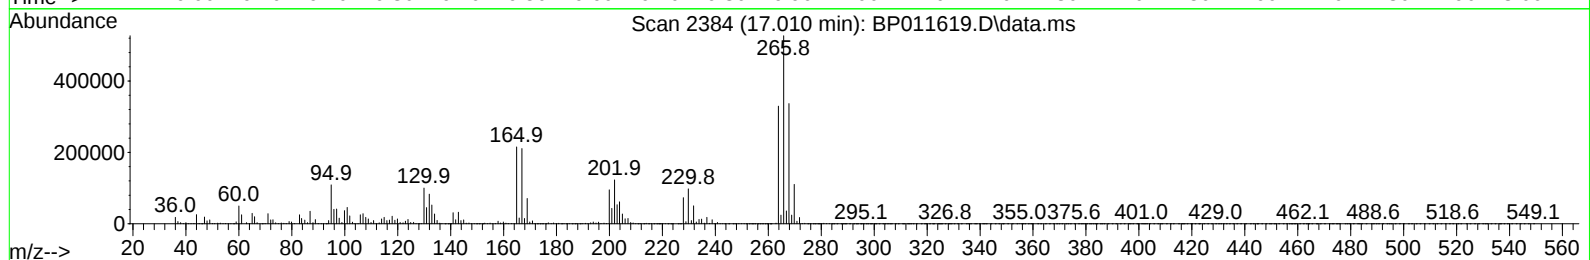


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090622\
Data File : BP011619.D
Acq On : 06 Sep 2022 11:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 07:18:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 03 04:07:09 2022
Response via : Initial Calibration

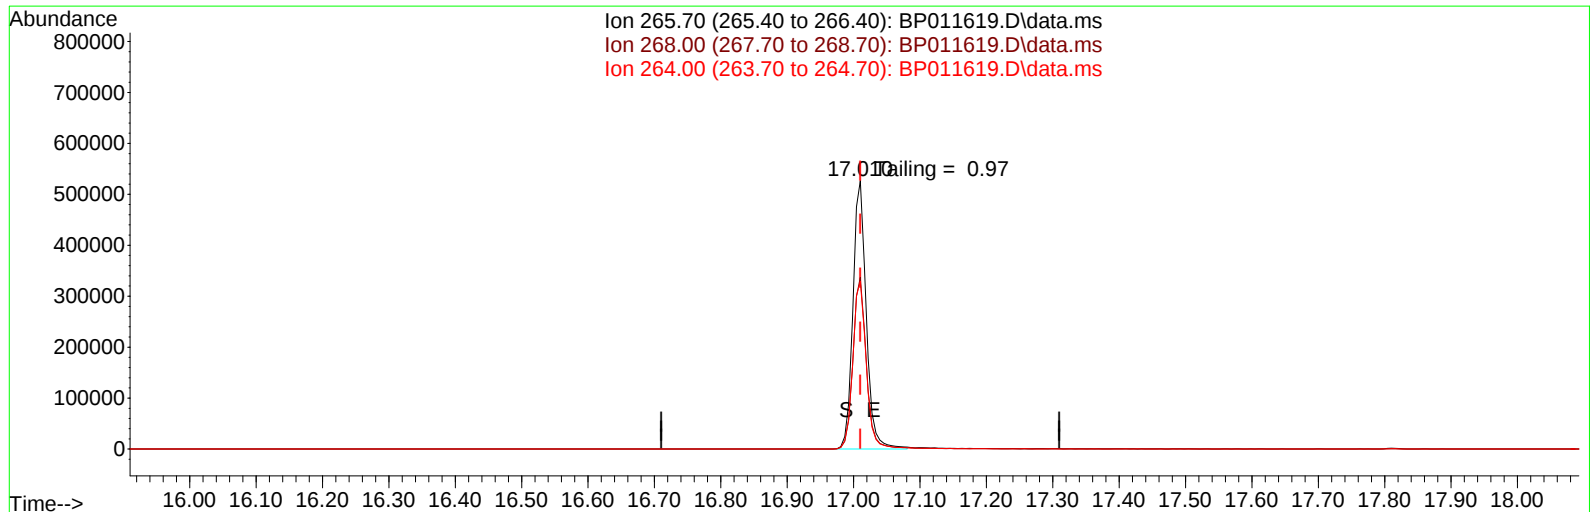

TIC: BP011619.D\data.ms

(70) Pentachlorophenol (C)




17.010min (-0.000) 4399478.32 ng

response 736156

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.91
264.00	63.00	62.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090622\
Data File : BP011619.D
Acq On : 06 Sep 2022 11:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 07:18:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 03 04:07:09 2022
Response via : Initial Calibration

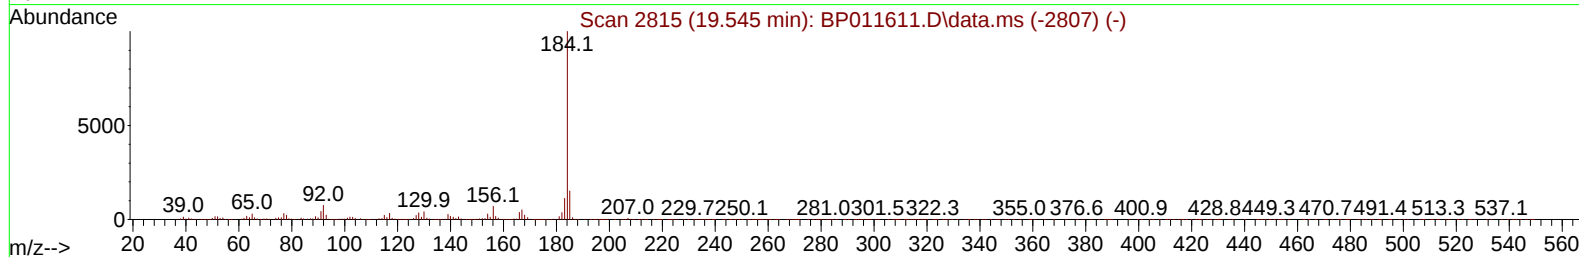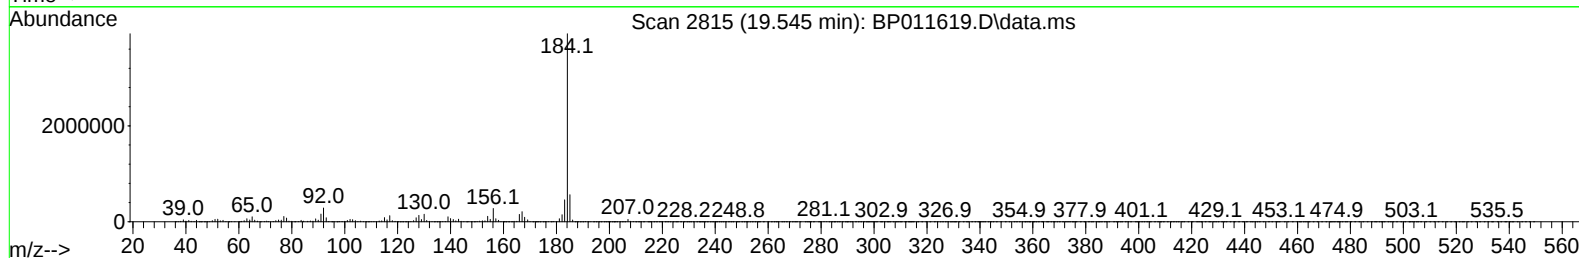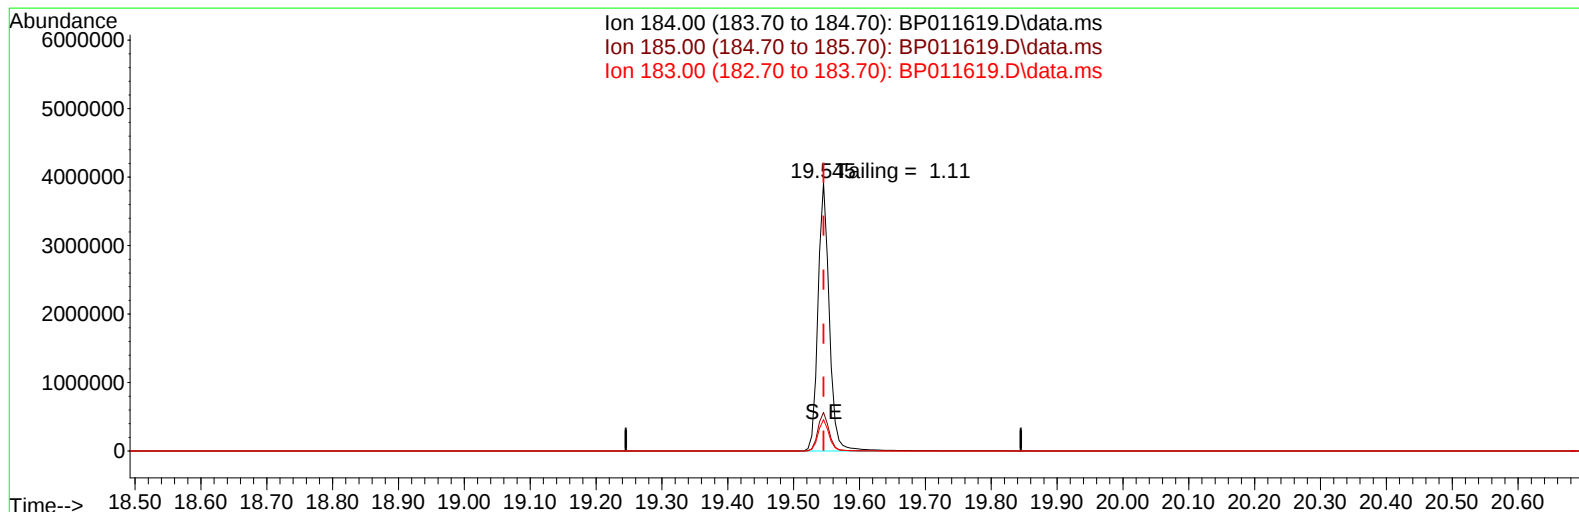

TIC: BP011619.D\data.ms

(77) Benzidine**19.545min (-0.000) 17422148.74 ng****response 4662117**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.38
183.00	11.30	11.69
0.00	0.00	0.00