

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090622\
 Data File : BP011623.D
 Acq On : 06 Sep 2022 13:46
 Operator : CG/JU
 Sample : N4446-06RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MW-06RE

Quant Time: Sep 07 03:41:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 03 04:07:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	65270	20.000	ng	0.00
21) Naphthalene-d8	10.787	136	294847	20.000	ng	# 0.00
39) Acenaphthene-d10	14.610	164	222400	20.000	ng	0.00
64) Phenanthrene-d10	17.363	188	639091	20.000	ng	0.00
76) Chrysene-d12	21.439	240	983595	20.000	ng	-0.01
86) Perylene-d12	23.910	264	1220138	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.522	112	285074	77.245	ng	0.00
7) Phenol-d6	7.116	99	248670	50.923	ng	-0.01
23) Nitrobenzene-d5	9.134	82	464312	96.664	ng	0.00
42) 2,4,6-Tribromophenol	16.098	330	474785	188.949	ng	0.00
45) 2-Fluorobiphenyl	13.240	172	1361922	87.570	ng	0.00
79) Terphenyl-d14	19.916	244	4228145	90.035	ng	0.00
Target Compounds						Qvalue
60) Diethylphthalate	15.428	149	139770	8.878	ng	98
74) Di-n-butylphthalate	18.322	149	449324	12.735	ng	99
80) Butylbenzylphthalate	20.586	149	9314	4.040	ng	85
84) Bis(2-ethylhexyl)phtha...	21.357	149	98183	4.344	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090622\
Data File : BP011623.D
Acq On : 06 Sep 2022 13:46
Operator : CG/JU
Sample : N4446-06RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW-06RE

Quant Time: Sep 07 03:41:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 03 04:07:09 2022
Response via : Initial Calibration




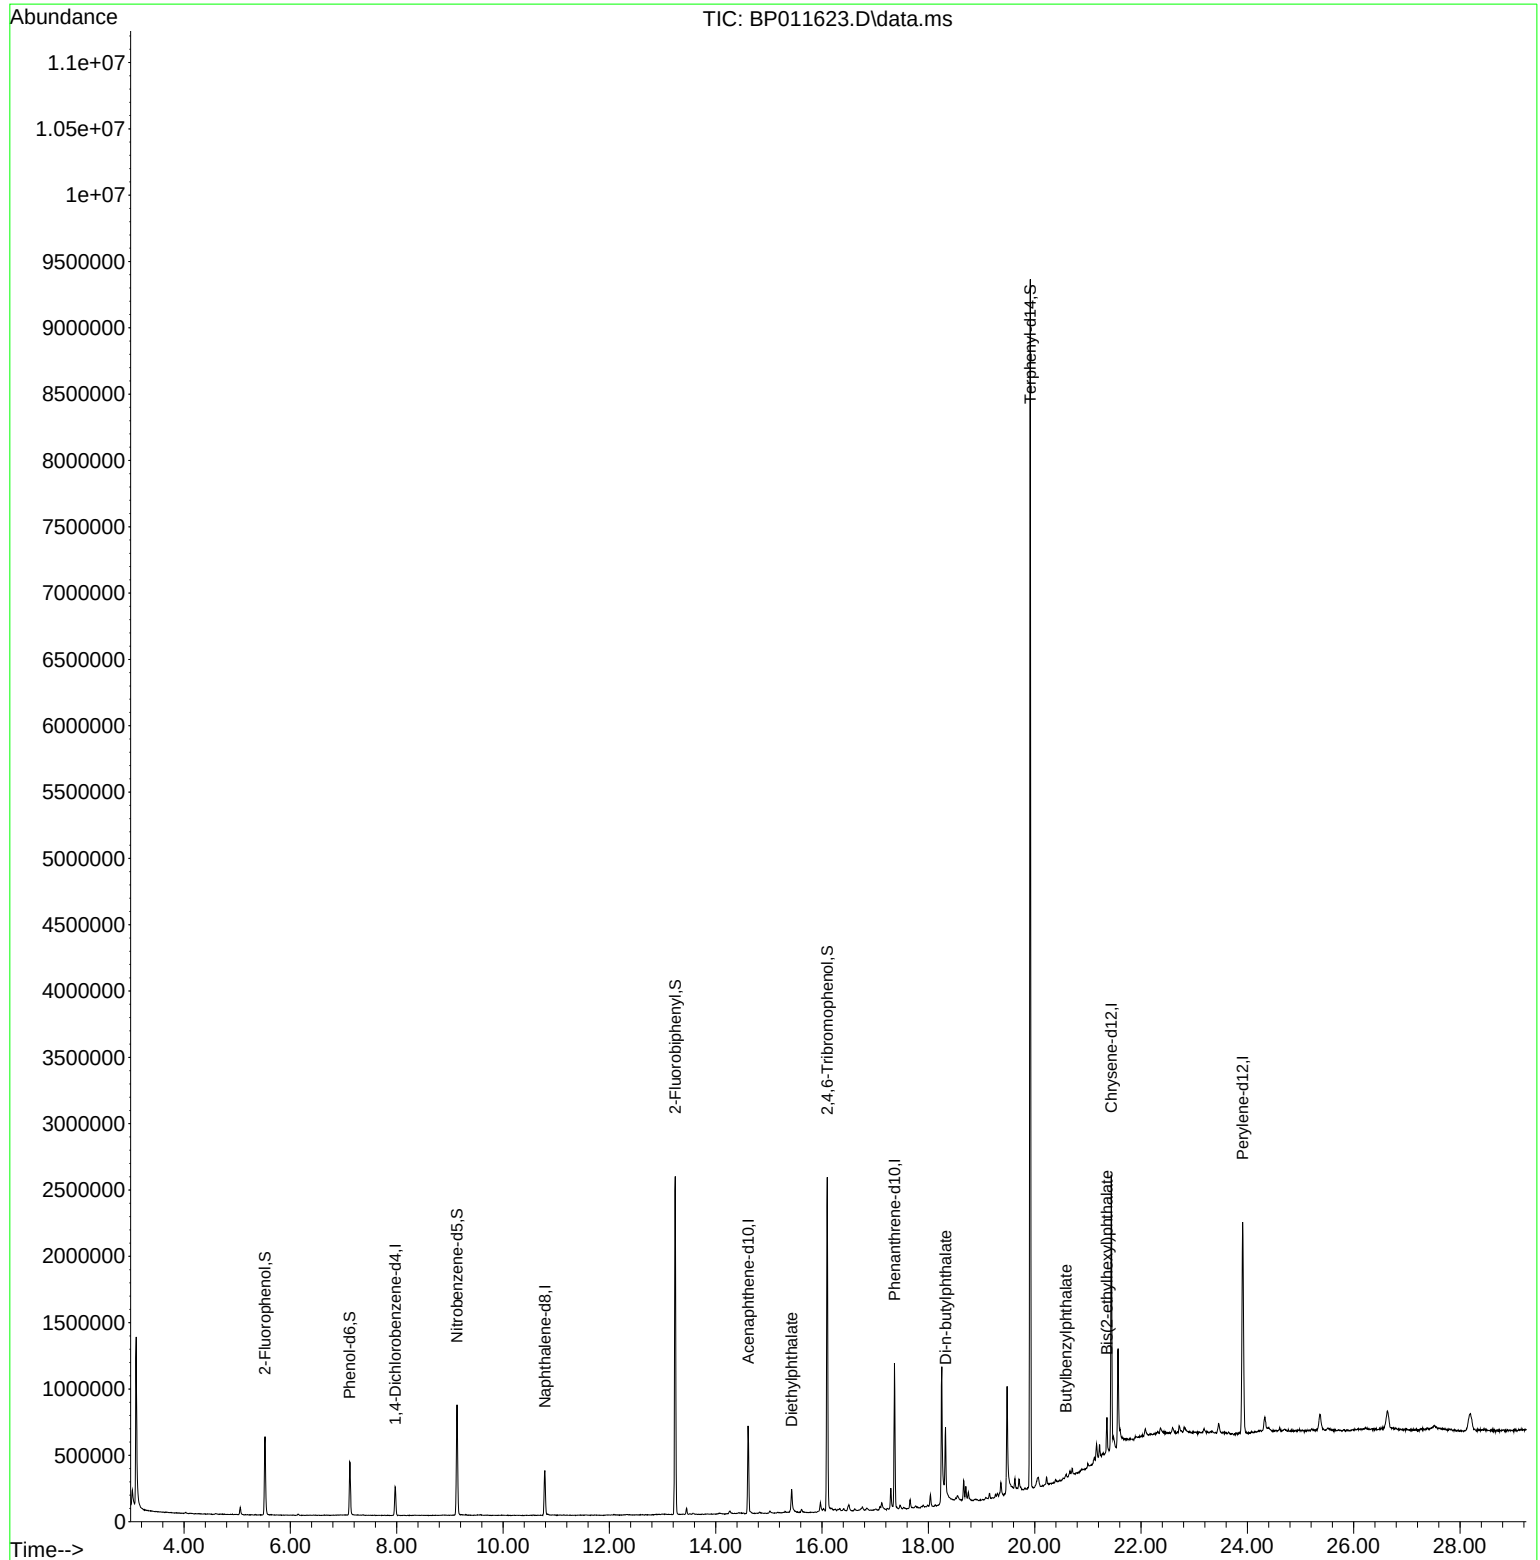




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.969 min Scan# 848
Delta R.T. -0.006 min
Lab File: BP011623.D
Acq: 06 Sep 2022 13:46




Instrument :
BNA_P
ClientSampleId :
MW-06RE


Tgt Ion:152 Resp: 65270
Ion Ratio Lower Upper
152 100
150 143.7 123.4 185.2
115 52.0 51.3 76.9

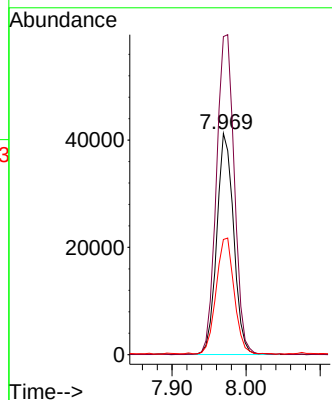

#5
2-Fluorophenol
Concen: 77.245 ng
RT: 5.522 min Scan# 431
Delta R.T. -0.000 min
Lab File: BP011623.D
Acq: 06 Sep 2022 13:46

Tgt Ion:112 Resp: 285074
Ion Ratio Lower Upper
112 100
64 55.8 56.9 85.3#
63 28.5 31.2 46.8#


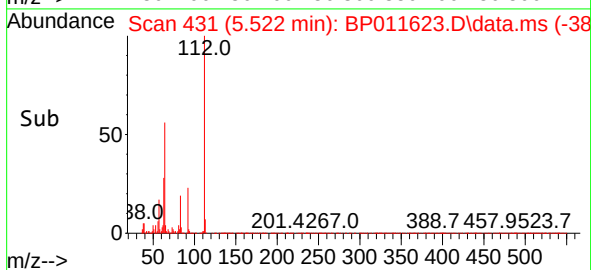
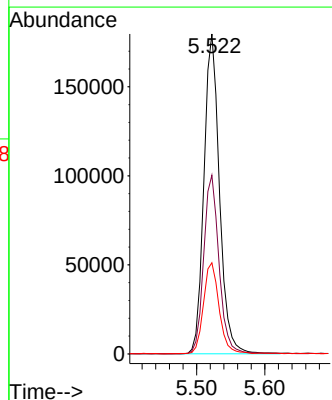





#7
Phenol-d6
Concen: 50.923 ng
RT: 7.116 min Scan# 704
Delta R.T. -0.012 min
Lab File: BP011623.D
Acq: 06 Sep 2022 13:46




Instrument :
BNA_P
ClientSampleId :
MW-06RE


Tgt Ion: 99 Resp: 248670
Ion Ratio Lower Upper
99 100
42 16.3 20.3 30.5#
71 30.8 33.9 50.9#

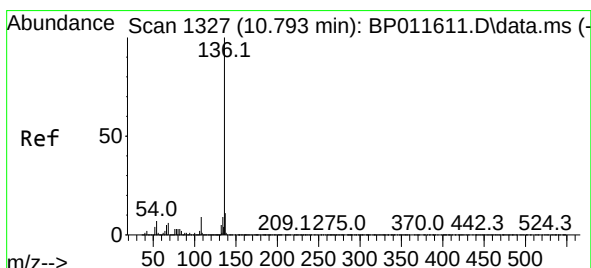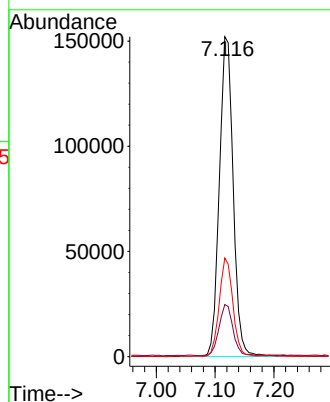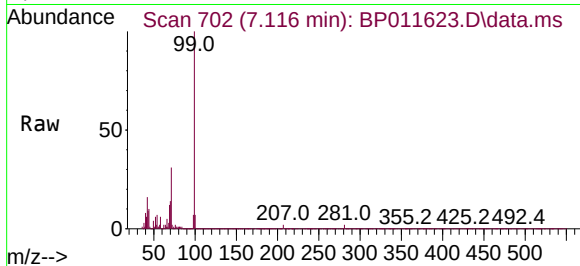

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.787 min Scan# 1326
Delta R.T. -0.006 min
Lab File: BP011623.D
Acq: 06 Sep 2022 13:46

Tgt Ion:136 Resp: 294847
Ion Ratio Lower Upper
136 100
137 11.1 9.0 13.4
54 7.4 8.7 13.1#
68 5.6 4.8 7.2


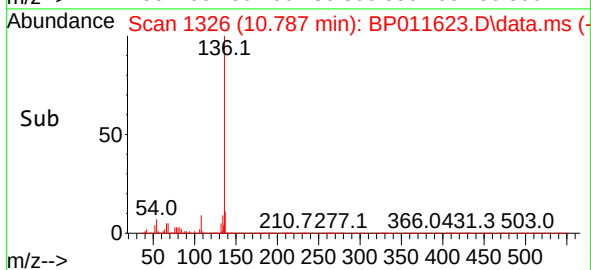
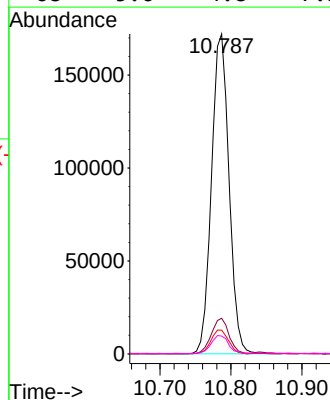
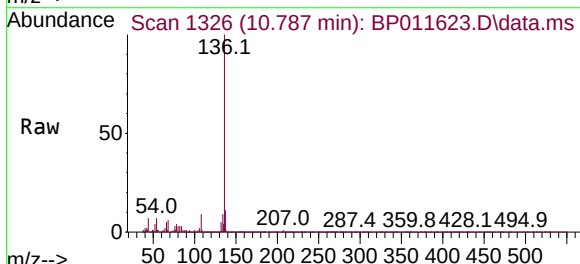




#23
Nitrobenzene-d5
Concen: 96.664 ng
RT: 9.134 min Scan# 1045
Delta R.T. -0.006 min
Lab File: BP011623.D
Acq: 06 Sep 2022 13:46




Instrument :
BNA_P
ClientSampleId :
MW-06RE


Tgt Ion: 82 Resp: 464312
Ion Ratio Lower Upper
82 100
128 43.8 31.3 46.9
54 49.4 49.8 74.8#

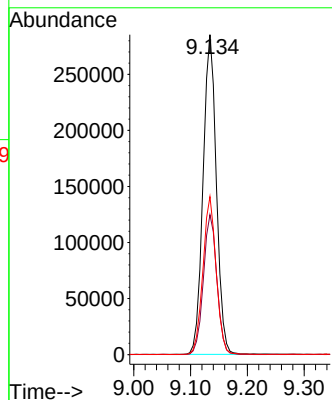

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.610 min Scan# 1976
Delta R.T. -0.006 min
Lab File: BP011623.D
Acq: 06 Sep 2022 13:46

Tgt Ion: 164 Resp: 222400
Ion Ratio Lower Upper
164 100
162 102.4 81.9 122.9
160 46.5 34.6 51.8

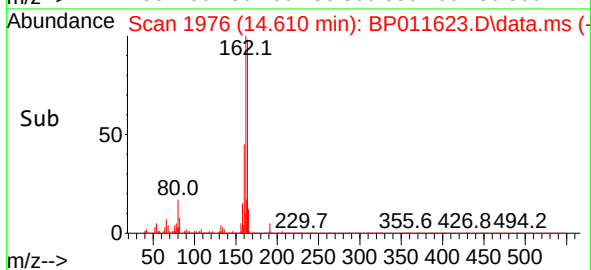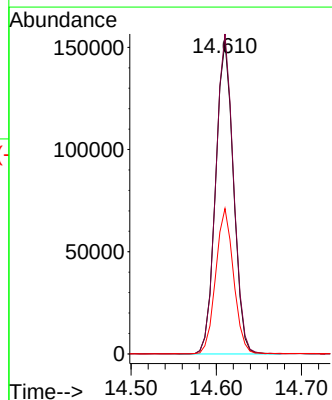

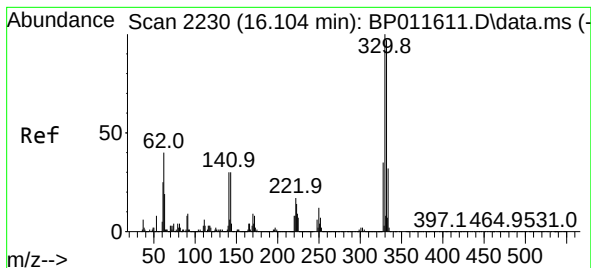

#42

2,4,6-Tribromophenol

Concen: 188.949 ng

RT: 16.098 min Scan# 21

Delta R.T. -0.006 min

Lab File: BP011623.D

Acq: 06 Sep 2022 13:46

Instrument :

BNA_P

ClientSampleId :

MW-06RE





Tgt Ion:330 Resp: 474785

Ion Ratio Lower Upper

330 100

332 97.0 78.1 117.1

141 34.2 31.4 47.2

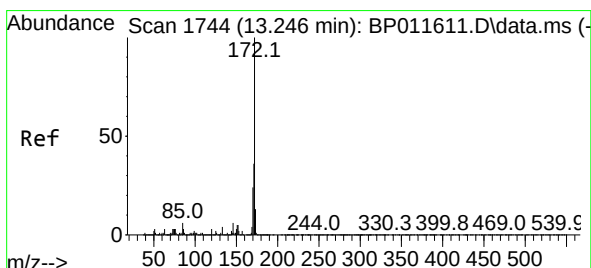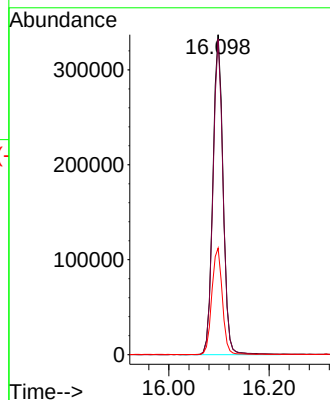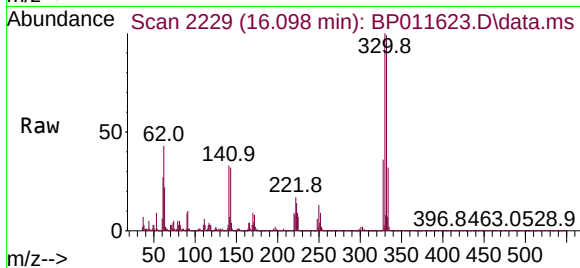

#45

2-Fluorobiphenyl

Concen: 87.570 ng

RT: 13.240 min Scan# 1743

Delta R.T. -0.006 min

Lab File: BP011623.D

Acq: 06 Sep 2022 13:46




Tgt Ion:172 Resp: 1361922


Ion Ratio Lower Upper

172 100

171 34.0 27.9 41.9

170 23.0 18.2 27.2


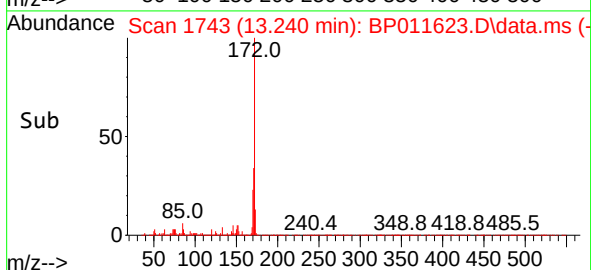
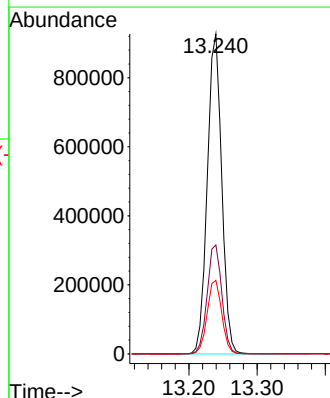
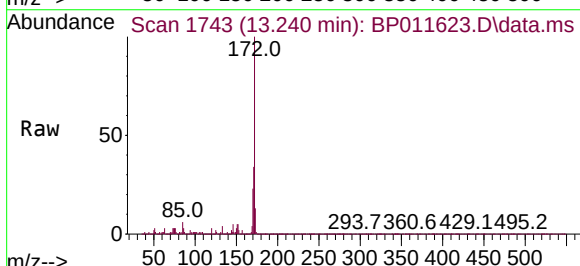




#60
Diethylphthalate
Concen: 8.878 ng
RT: 15.428 min Scan# 2115
Delta R.T. -0.012 min
Lab File: BP011623.D
Acq: 06 Sep 2022 13:46




Instrument :
BNA_P
ClientSampleId :
MW-06RE


Tgt Ion:149 Resp: 139770
Ion Ratio Lower Upper
149 100
177 23.4 17.8 26.8
150 12.2 9.9 14.9

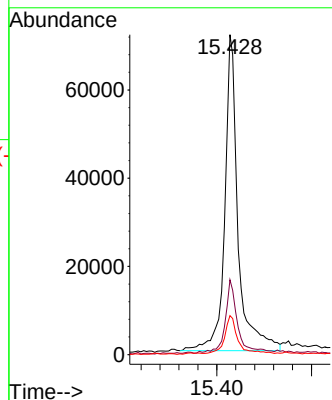

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.363 min Scan# 2444
Delta R.T. -0.006 min
Lab File: BP011623.D
Acq: 06 Sep 2022 13:46

Tgt Ion:188 Resp: 639091
Ion Ratio Lower Upper
188 100
94 8.6 6.6 10.0
80 9.6 8.0 12.0


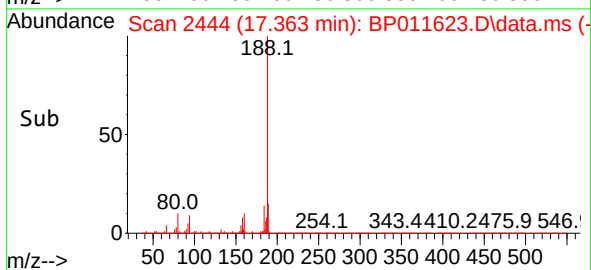
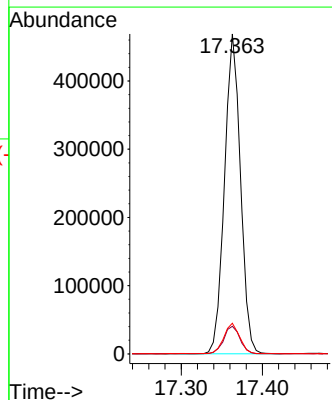





#74
Di-n-butylphthalate
Concen: 12.735 ng
RT: 18.322 min Scan# 2608
Delta R.T. -0.006 min
Lab File: BP011623.D
Acq: 06 Sep 2022 13:46




Instrument :
BNA_P
ClientSampleId :
MW-06RE


Tgt Ion:149 Resp: 449324
Ion Ratio Lower Upper
149 100
150 9.2 7.5 11.3
104 5.0 4.8 7.2

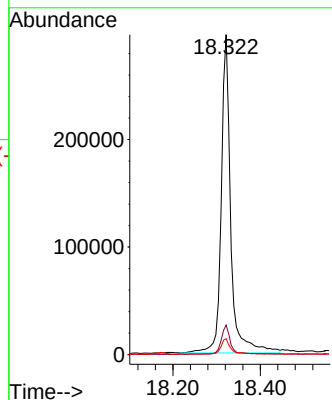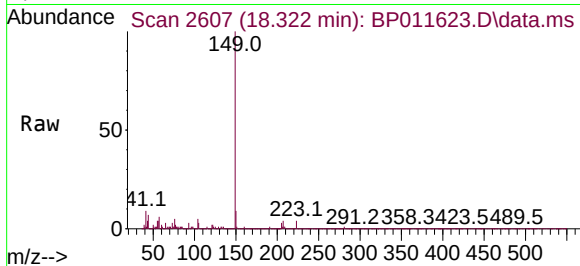

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.439 min Scan# 3137
Delta R.T. -0.012 min
Lab File: BP011623.D
Acq: 06 Sep 2022 13:46

Tgt Ion:240 Resp: 983595
Ion Ratio Lower Upper
240 100
120 10.4 8.6 12.8
236 26.2 19.8 29.6


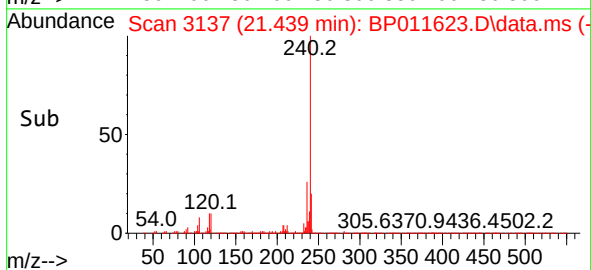
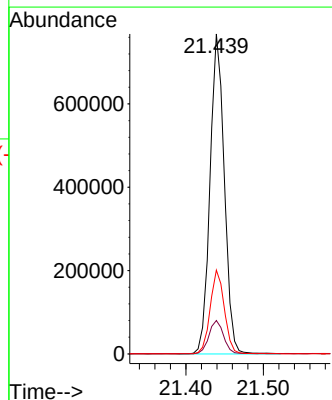
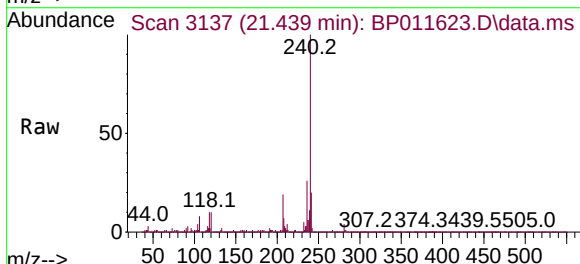




#79
 Terphenyl-d14
 Concen: 90.035 ng
 RT: 19.916 min Scan# 2878
 Delta R.T. -0.006 min
 Lab File: BP011623.D
 Acq: 06 Sep 2022 13:46




Instrument :
 BNA_P
 ClientSampleId :
 MW-06RE


Tgt Ion:244 Resp: 4228145
 Ion Ratio Lower Upper
 244 100
 212 6.6 5.8 8.8
 122 9.8 7.6 11.4

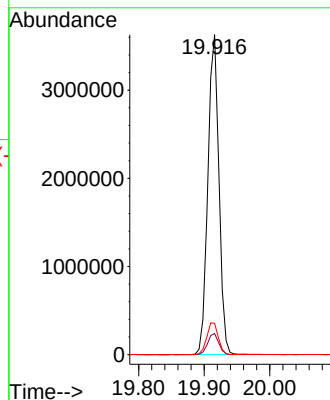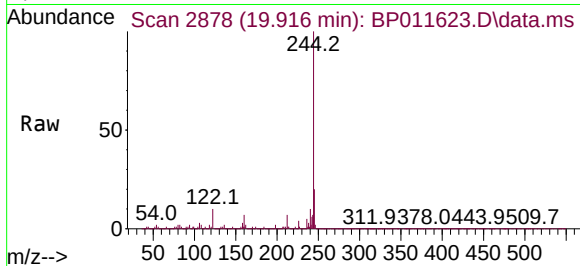

#80
 Butylbenzylphthalate
 Concen: 4.040 ng
 RT: 20.586 min Scan# 2992
 Delta R.T. -0.012 min
 Lab File: BP011623.D
 Acq: 06 Sep 2022 13:46

Tgt Ion:149 Resp: 9314
 Ion Ratio Lower Upper
 149 100
 91 62.8 62.5 93.7
 206 17.5 17.0 25.4


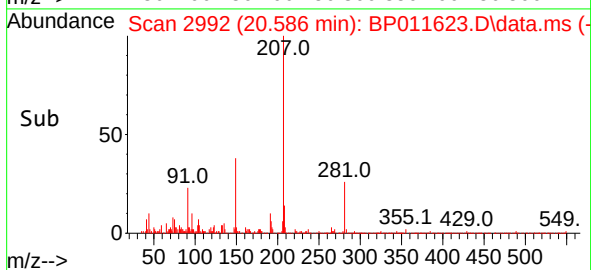
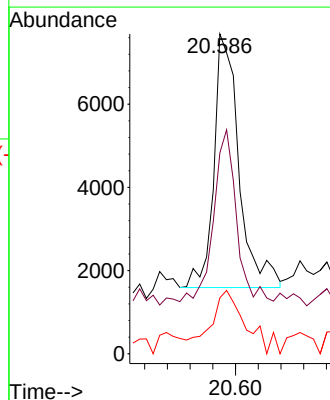
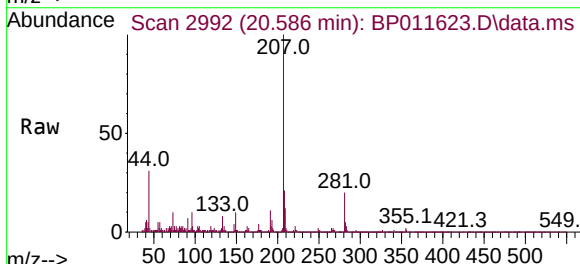


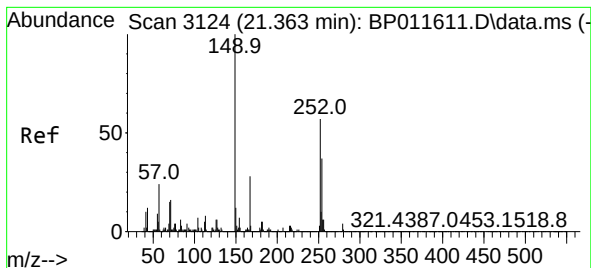

#84
Bis(2-ethylhexyl)phthalate
Concen: 4.344 ng
RT: 21.357 min Scan# 3124
Delta R.T. -0.006 min
Lab File: BP011623.D
Acq: 06 Sep 2022 13:46

Instrument :
BNA_P
ClientSampleId :
MW-06RE

Tgt Ion:149 Resp: 98183
Ion Ratio Lower Upper
149 100
167 26.9 21.8 32.8
279 4.8 3.7 5.5

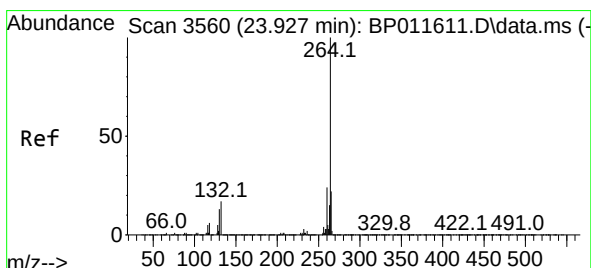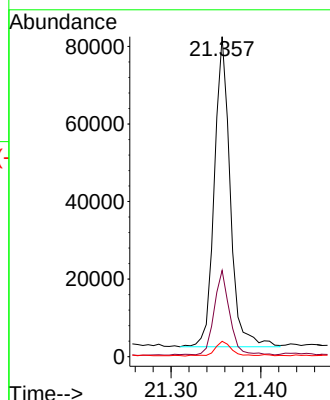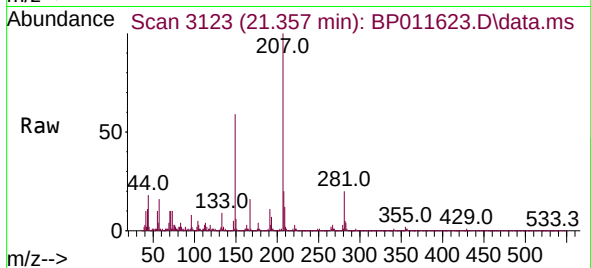

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.910 min Scan# 3557
Delta R.T. -0.018 min
Lab File: BP011623.D
Acq: 06 Sep 2022 13:46

Tgt Ion:264 Resp: 1220138
Ion Ratio Lower Upper
264 100
260 24.3 19.3 28.9
265 21.8 18.0 27.0

