
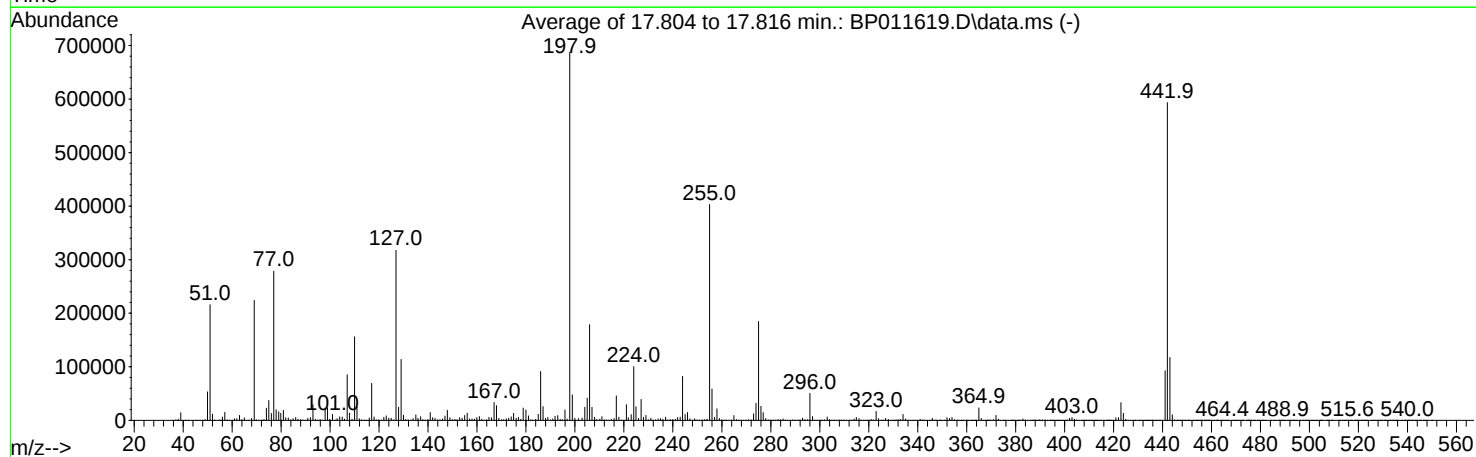


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090622\
 Data File : BP011619.D
 Acq On : 06 Sep 2022 11:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 03 04:07:09 2022

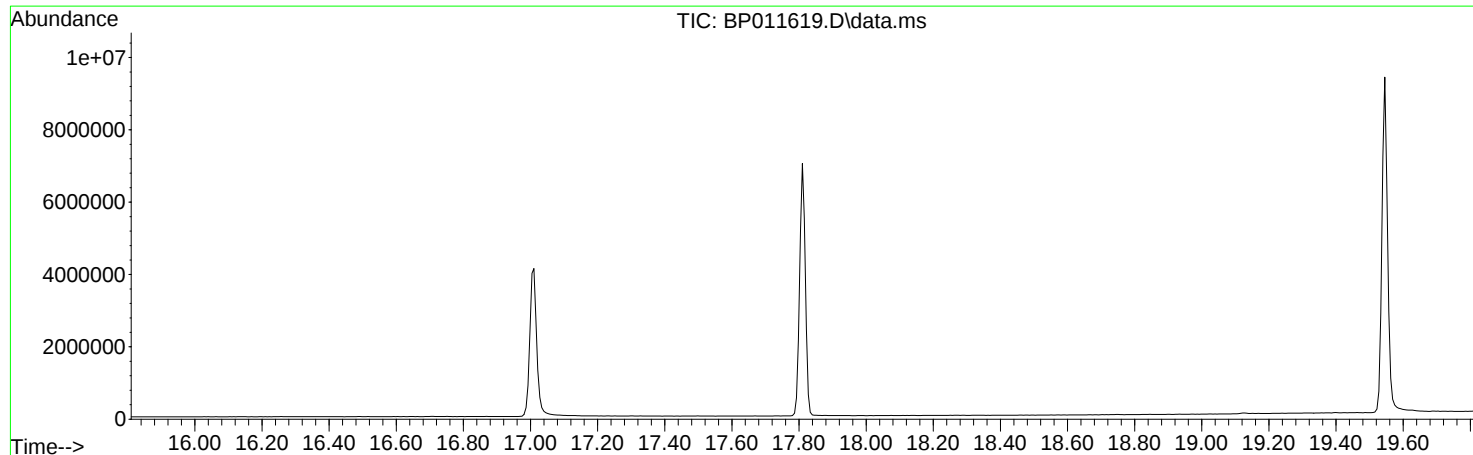

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	215909	PASS
68	69	0.00	2	1.6	3599	PASS
69	198	0.00	100	32.6	224000	PASS
70	69	0.00	2	0.5	1107	PASS
127	198	10	80	46.2	317712	PASS
197	198	0.00	2	0.3	2203	PASS
198	198	100	100	100.0	687143	PASS
199	198	5	9	6.9	47551	PASS
275	198	10	60	26.9	184704	PASS
365	198	1	100	3.4	23262	PASS
441	198	0.01	100	13.5	92427	PASS
442	442	100	100	100.0	593388	PASS
443	442	15	24	19.8	117467	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/6/2022	BNA_P	<u>BP011619.D</u>
Compound Name	Response	Retention Time
DDT	2180160	20.751
DDD	16263	20.316
DDE	1745	19.828
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18008	2198168	0.82

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090622\
Data File : BP011619.D
Acq On : 06 Sep 2022 11:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 07 07:18:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 03 04:07:09 2022
Response via : Initial Calibration

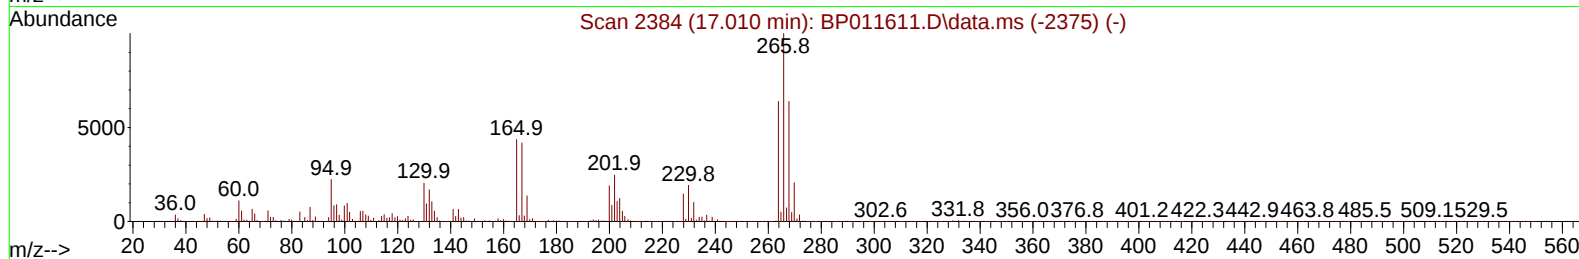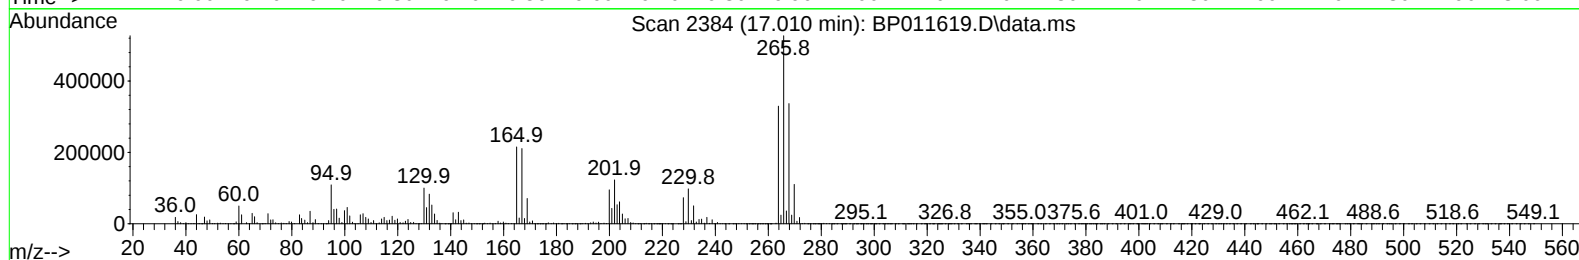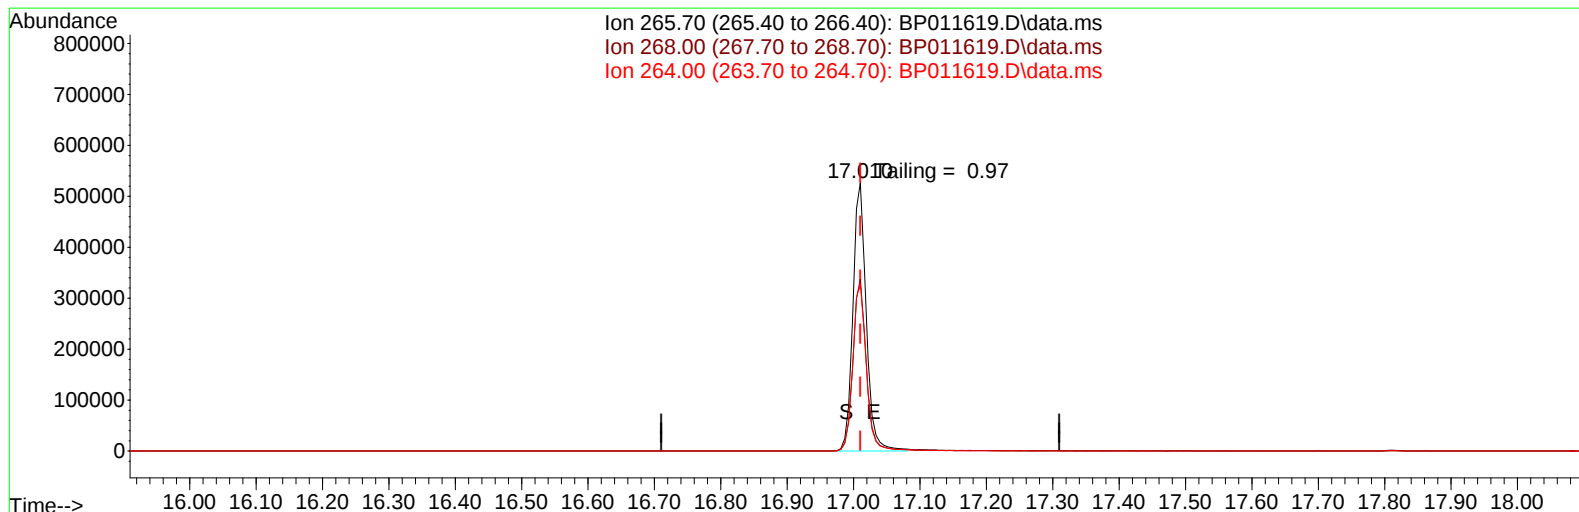

TIC: BP011619.D\data.ms

(70) Pentachlorophenol (C)

17.010min (-0.000) 4399478.32 ng




response 736156

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.91
264.00	63.00	62.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090622\
Data File : BP011619.D
Acq On : 06 Sep 2022 11:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 07 07:18:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 03 04:07:09 2022
Response via : Initial Calibration

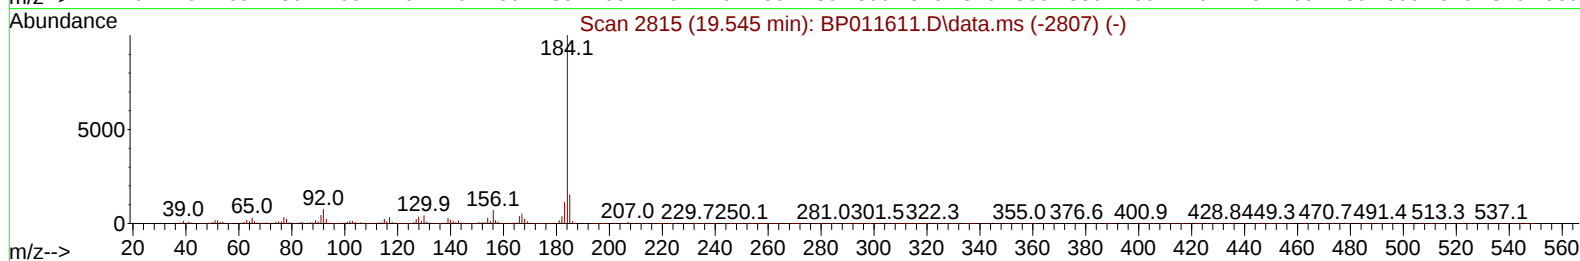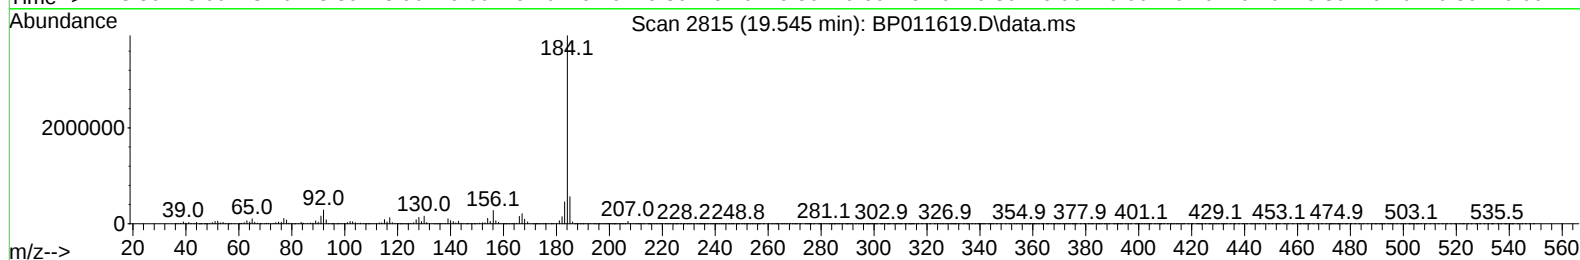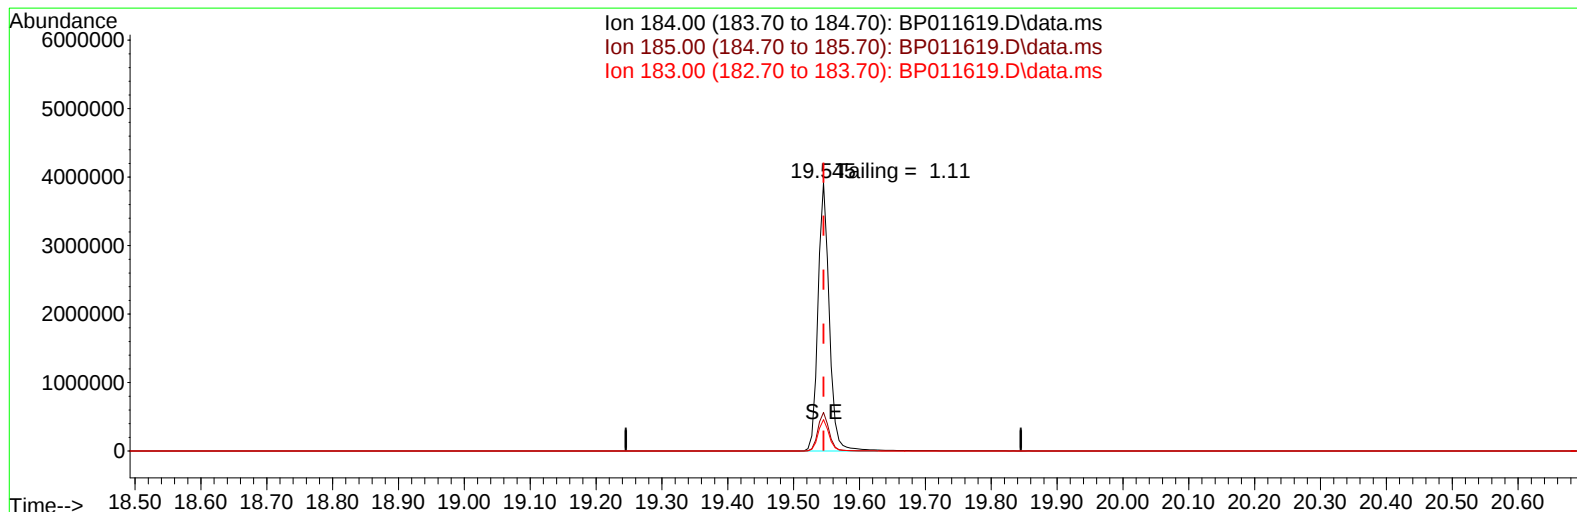

TIC: BP011619.D\data.ms

(77) Benzidine

19.545min (-0.000) 17422148.74 ng

response 4662117

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.38
183.00	11.30	11.69
0.00	0.00	0.00