
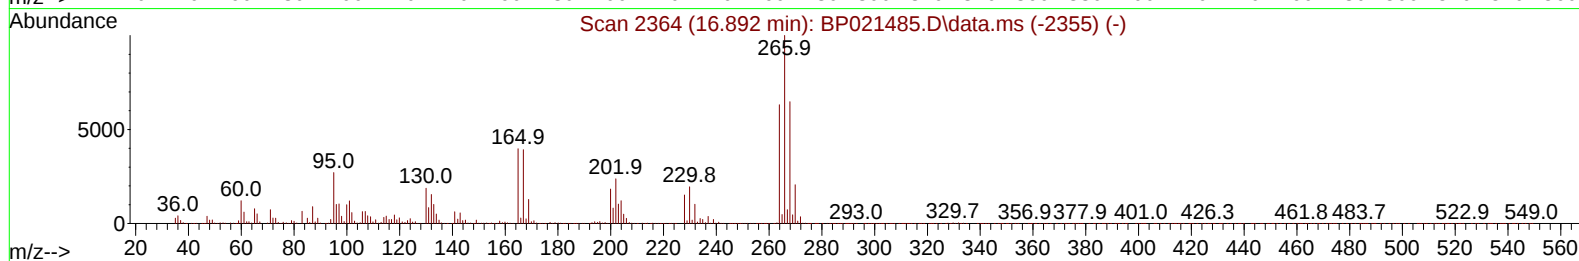
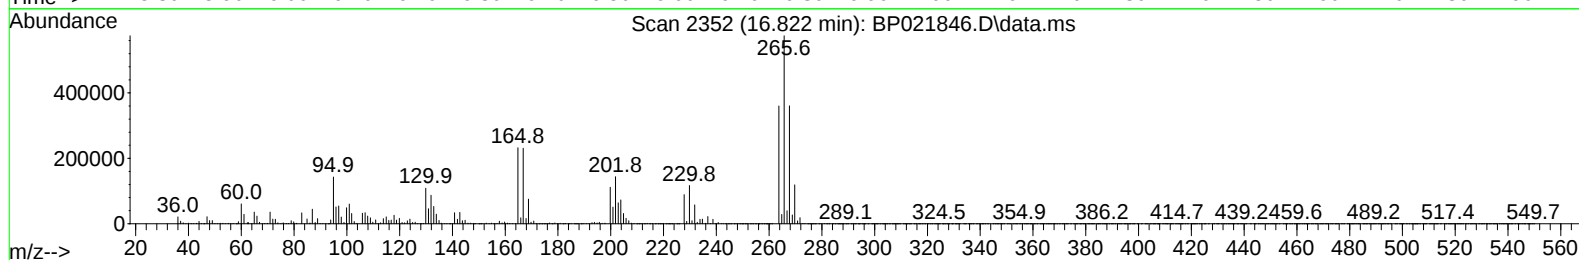


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090624\
Data File : BP021846.D
Acq On : 06 Sep 2024 10:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 12:30:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 11:12:31 2024
Response via : Initial Calibration

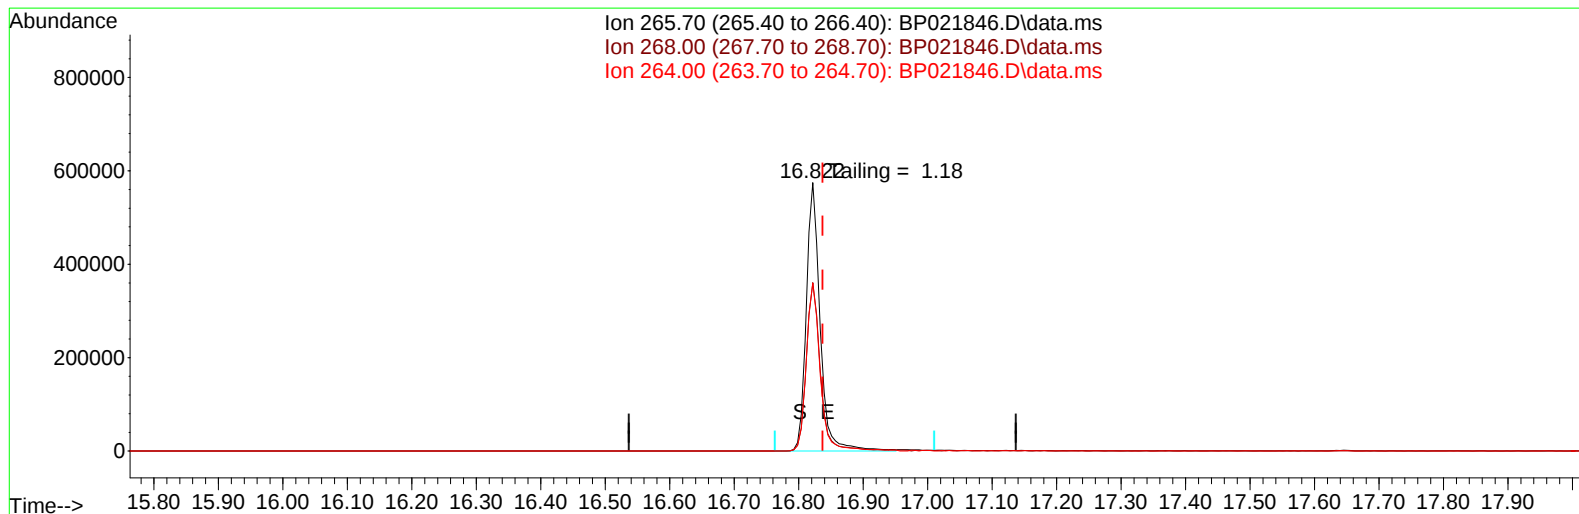

TIC: BP021846.D\data.ms

(70) Pentachlorophenol (C)




16.822min (-0.015) 2944199.61 ng

response 864239

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	62.73
264.00	63.10	62.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090624\
Data File : BP021846.D
Acq On : 06 Sep 2024 10:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 12:30:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 11:12:31 2024
Response via : Initial Calibration

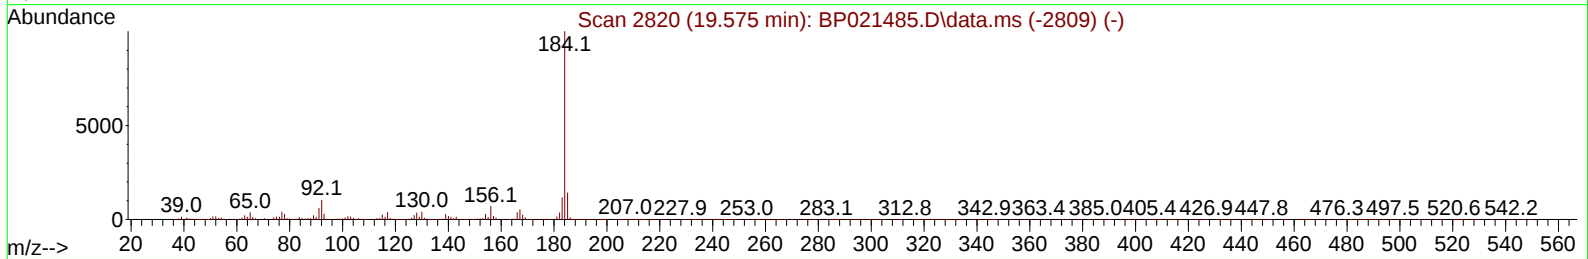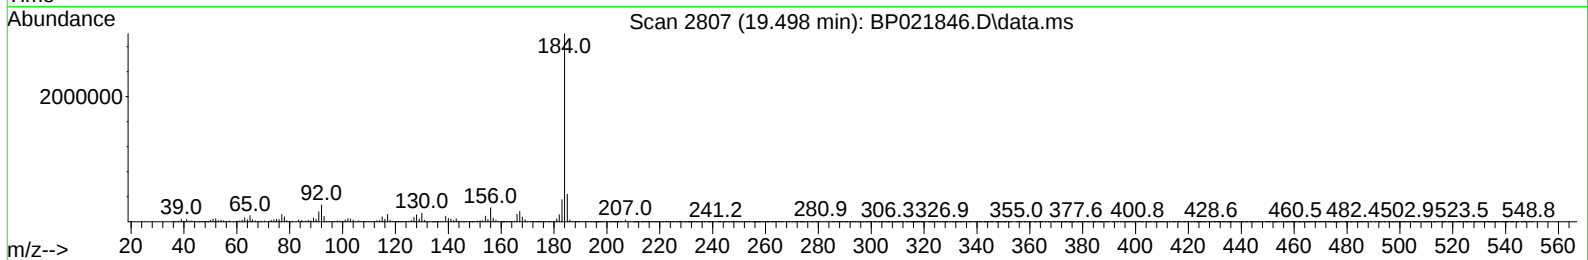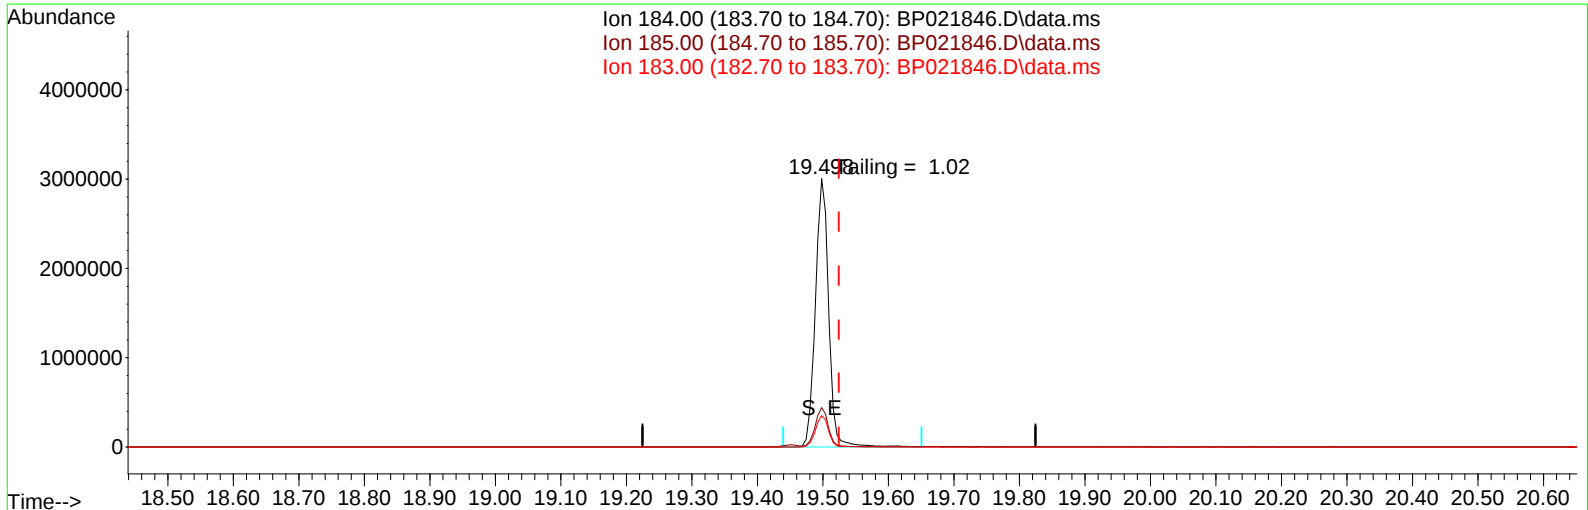

TIC: BP021846.D\data.ms

(77) Benzidine**19.498min (-0.027) -20.00 ng****response 4238129**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.67
183.00	11.60	11.73
0.00	0.00	0.00