


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090624\
Data File : BP021846.D
Acq On : 06 Sep 2024 10:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 06 23:52:54 2024

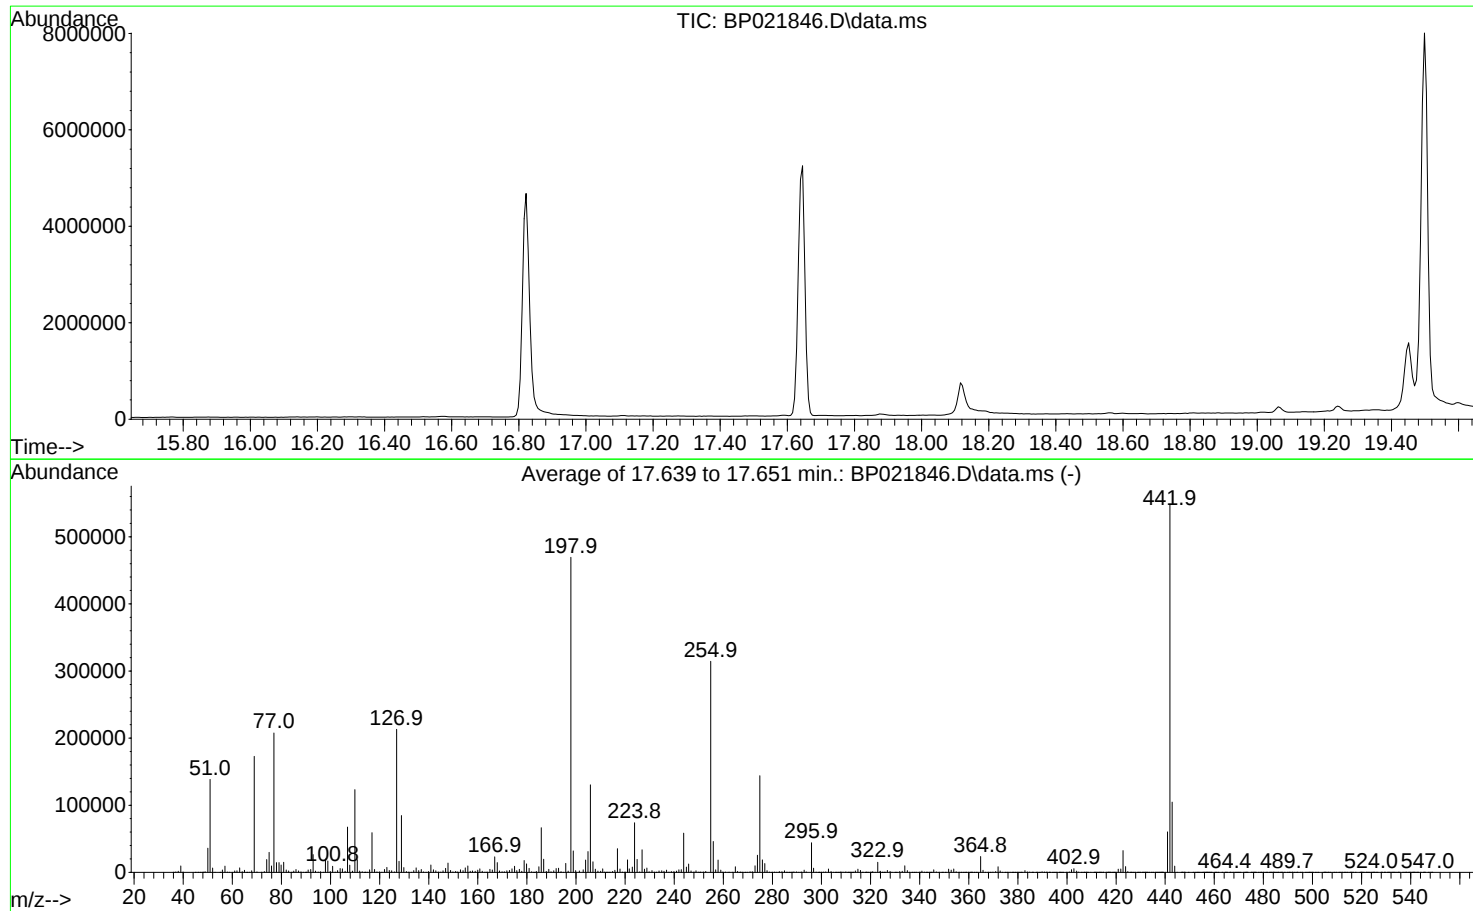

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2482

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	29.5	138480	PASS
68	69	0.00	2	1.4	2384	PASS
69	198	0.00	100	36.8	172925	PASS
70	69	0.00	2	0.4	627	PASS
127	198	10	80	45.4	213077	PASS
197	198	0.00	2	0.4	1824	PASS
198	198	100	100	100.0	469368	PASS
199	198	5	9	6.8	32082	PASS
275	198	10	60	30.7	143963	PASS
365	198	1	100	5.1	23712	PASS
441	198	0.01	100	12.9	60419	PASS
442	442	100	100	100.0	548139	PASS
443	442	15	24	19.1	104586	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
9/6/2024	BNA_P	<u>BP021846.D</u>
Compound Name	Response	Retention Time
DDT	1647204	20.792
DDD	143664	20.327
DDE	4463	19.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
148127	1795331	8.25

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090624\
Data File : BP021846.D
Acq On : 06 Sep 2024 10:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 06 12:30:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 11:12:31 2024
Response via : Initial Calibration

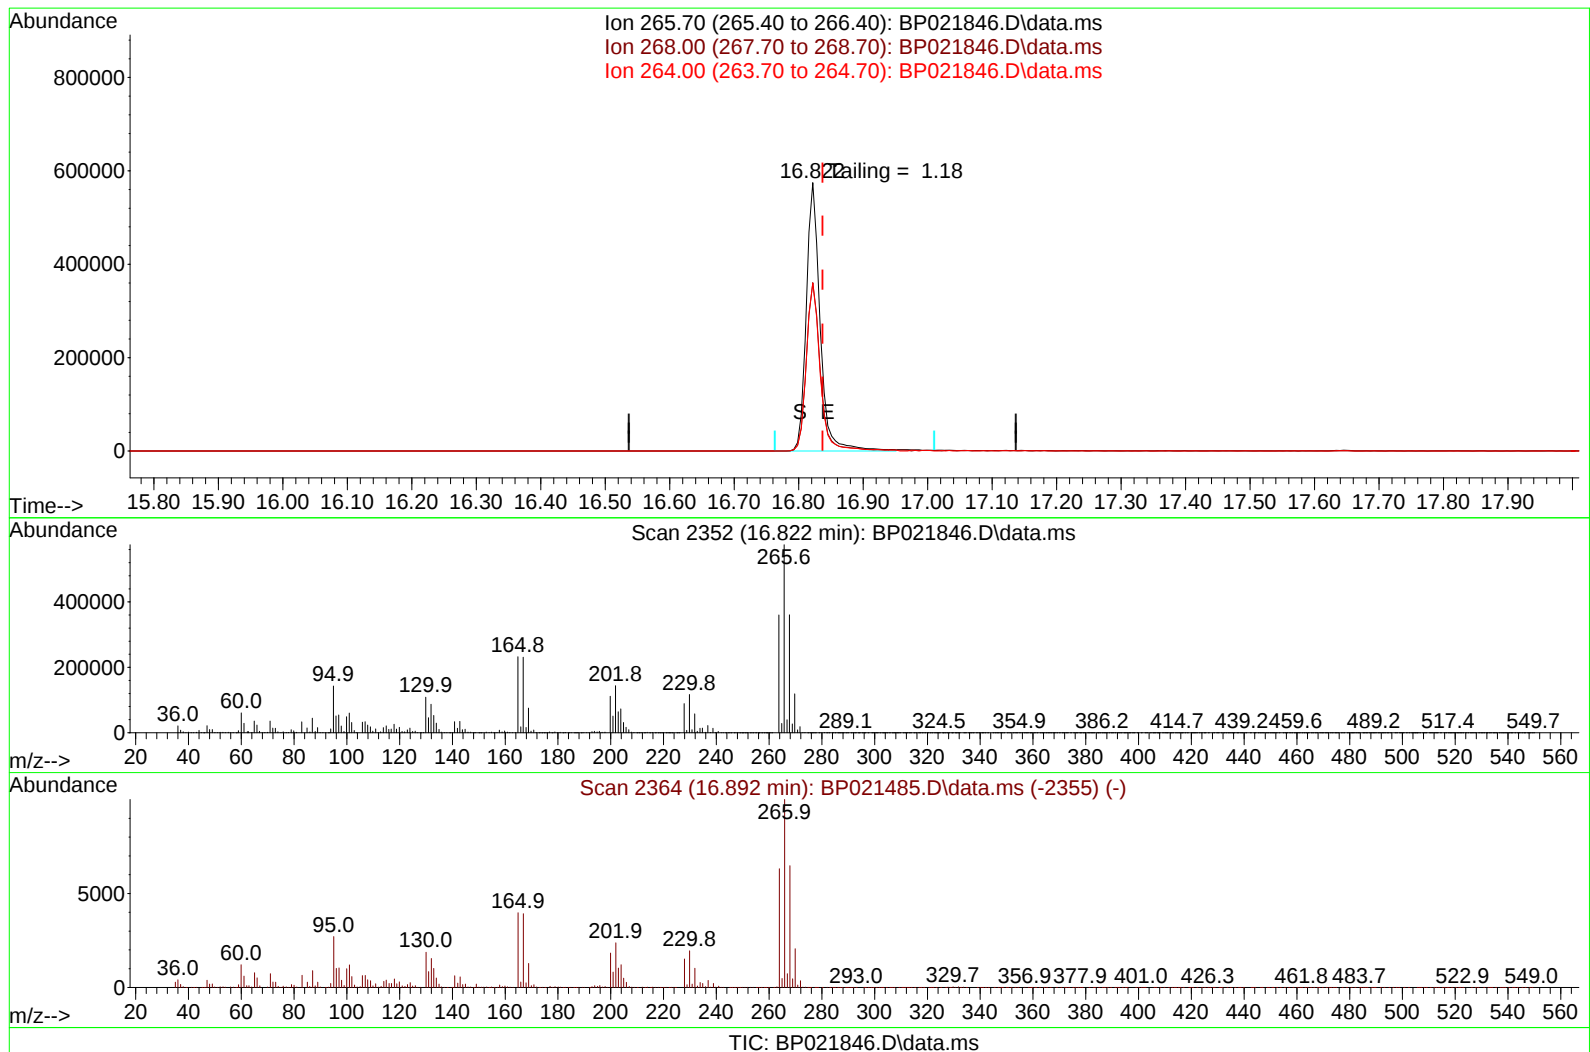

(70) Pentachlorophenol (C)

16.822min (-0.015) 2944199.61 ng




response 864239

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	62.73
264.00	63.10	62.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090624\
Data File : BP021846.D
Acq On : 06 Sep 2024 10:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 06 12:30:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 11:12:31 2024
Response via : Initial Calibration

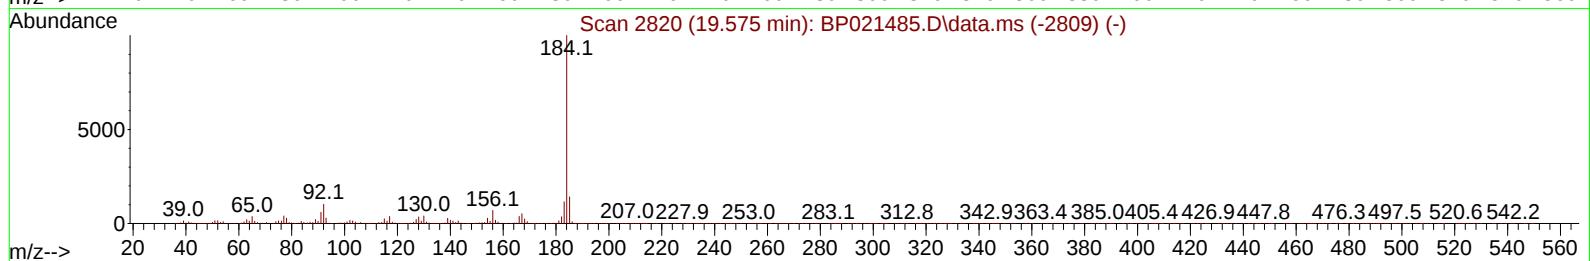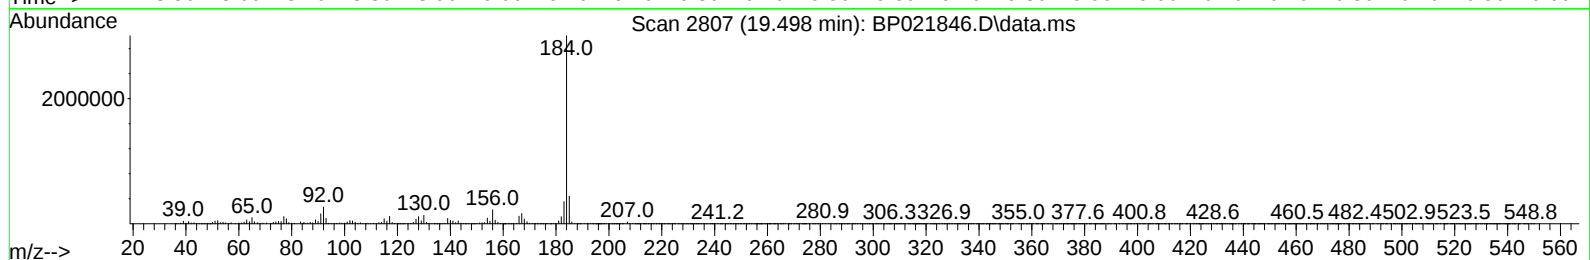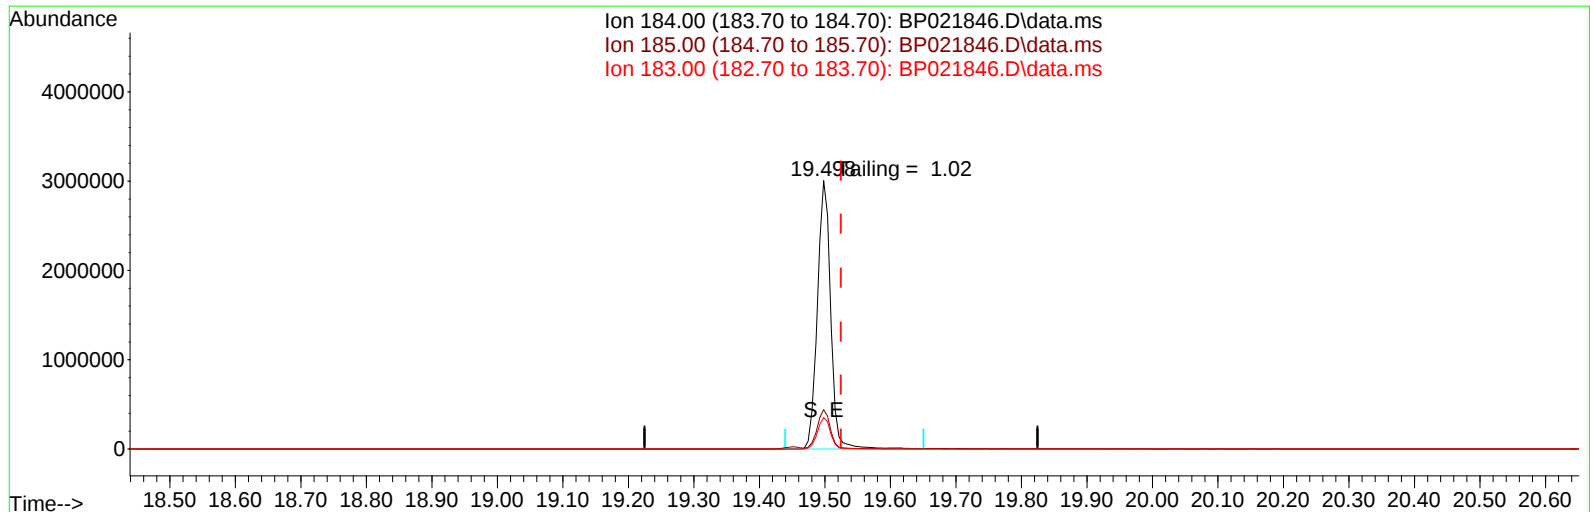

TIC: BP021846.D\data.ms

(77) Benzidine

19.498min (-0.027) -20.00 ng

response 4238129

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.67
183.00	11.60	11.73
0.00	0.00	0.00