
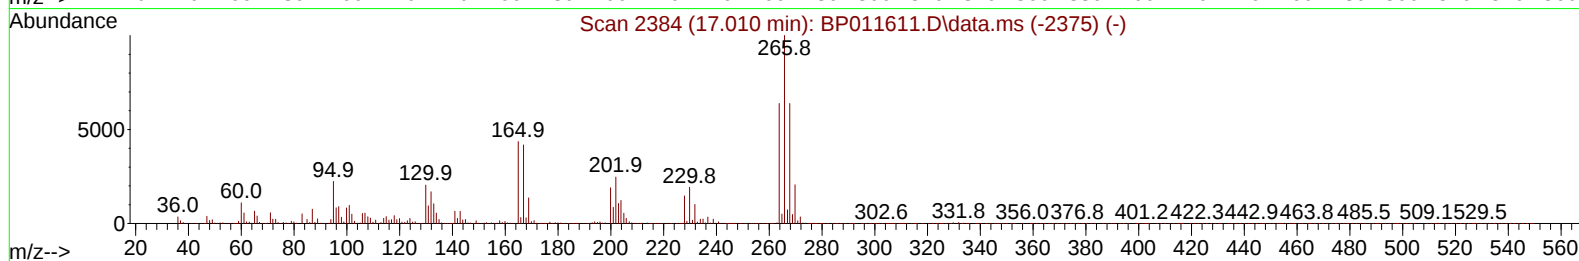
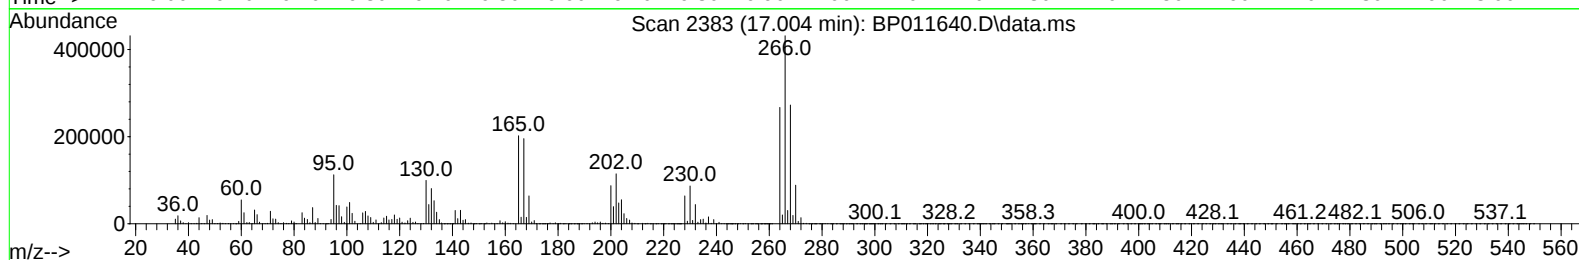


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090722\
 Data File : BP011640.D
 Acq On : 07 Sep 2022 10:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 06:14:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 03 04:07:09 2022
 Response via : Initial Calibration

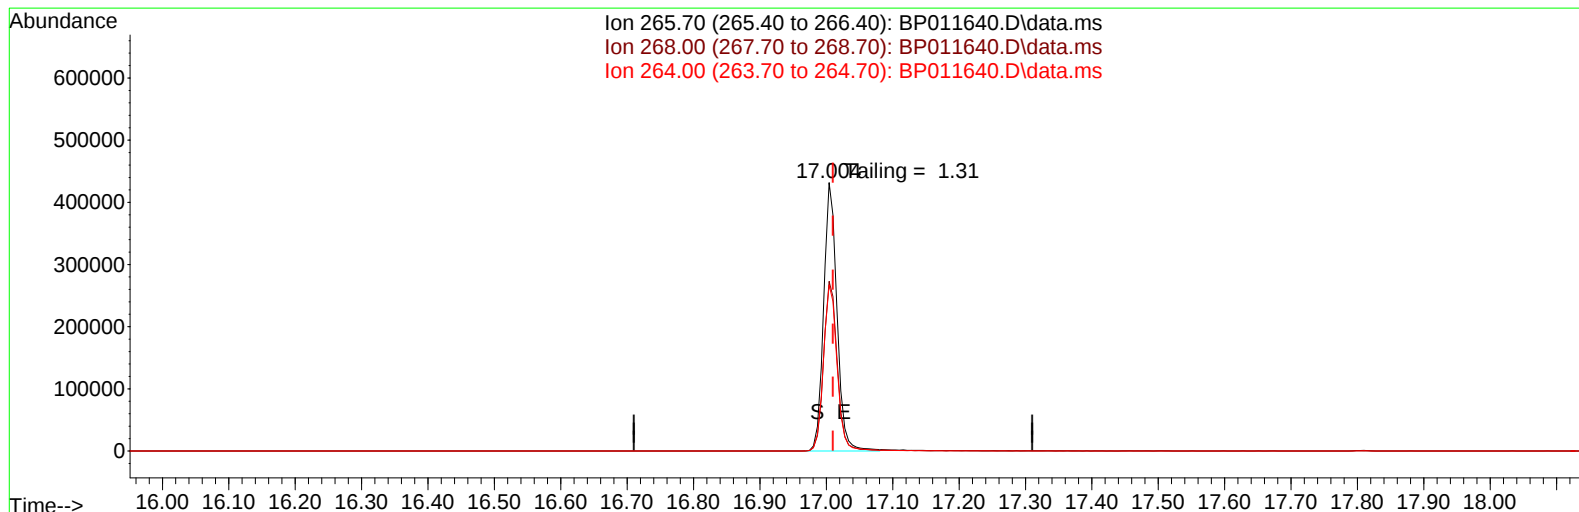

TIC: BP011640.D\data.ms

(70) Pentachlorophenol (C)




17.004min (-0.006) 917188.94 ng

response 607491

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.19
264.00	63.00	61.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090722\
 Data File : BP011640.D
 Acq On : 07 Sep 2022 10:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 06:14:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 03 04:07:09 2022
 Response via : Initial Calibration

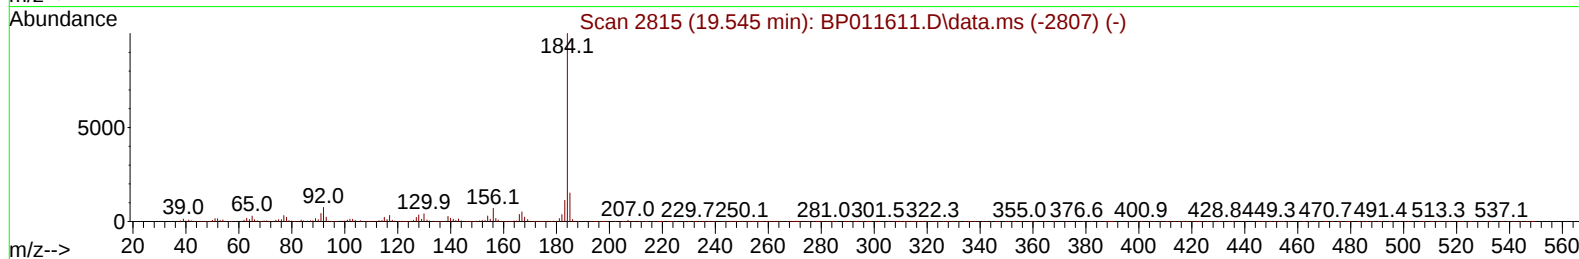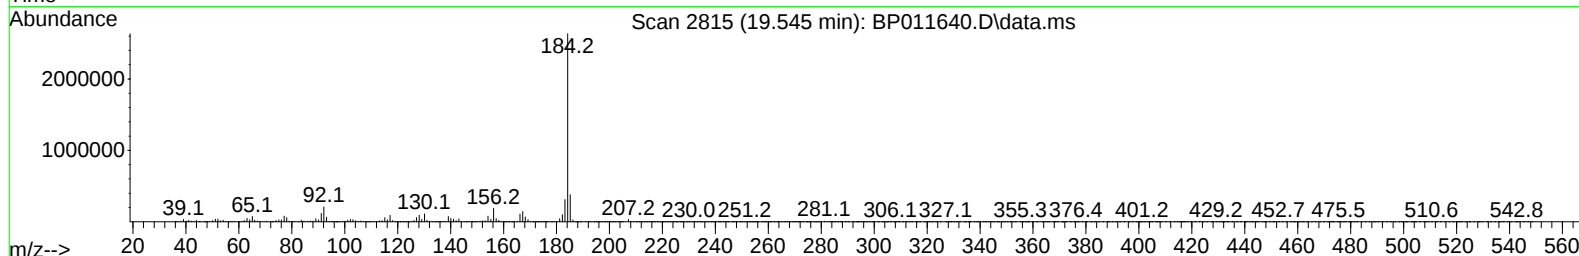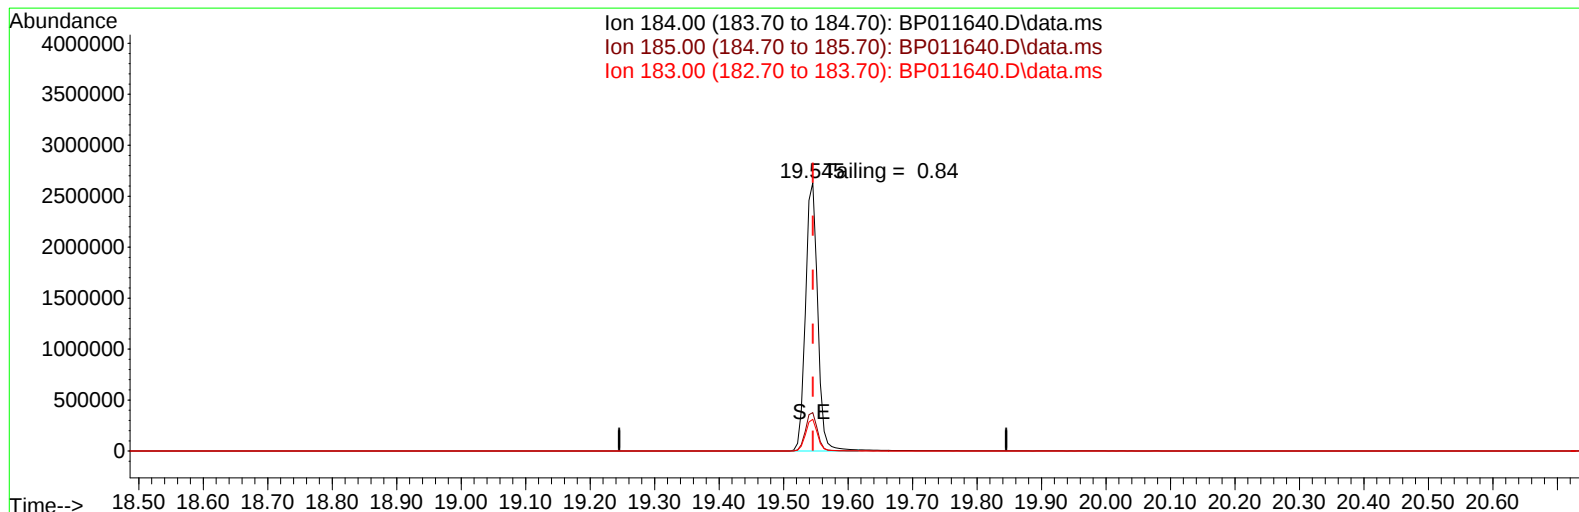

TIC: BP011640.D\data.ms

(77) Benzidine**19.545min (-0.000) 2504131.12 ng****response 3494084**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.35
183.00	11.30	11.80
0.00	0.00	0.00