

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090722\
 Data File : BP011642.D
 Acq On : 07 Sep 2022 11:42
 Operator : CG/JU
 Sample : PB147377BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB147377BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP011642.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	15	rVB	181895	273310	1.12%	0.223%
2	3.099	15	19	26	rVB	348788	439061	1.80%	0.358%
3	5.522	423	431	445	rBV	9794900	14516896	59.65%	11.845%
4	7.122	695	703	720	rBV	8767048	14407485	59.20%	11.755%
5	7.969	839	847	859	rBV	1742666	2832603	11.64%	2.311%
6	9.134	1036	1045	1059	rBV	5477119	9064755	37.25%	7.396%
7	10.781	1318	1325	1337	rBV	2273016	3904683	16.04%	3.186%
8	13.240	1735	1743	1755	rBV	13031286	20110705	82.63%	16.409%
9	14.610	1969	1976	1991	rBV	3176507	4718622	19.39%	3.850%
10	16.098	2222	2229	2249	rBV	8931433	12946698	53.20%	10.563%
11	17.363	2438	2444	2455	rBV	3685950	5161819	21.21%	4.212%
12	19.916	2872	2878	2883	rBV	20117573	24338125	100.00%	19.858%
13	21.445	3132	3138	3149	rBV	3560249	4903912	20.15%	4.001%
14	23.915	3551	3558	3572	rVB2	2333224	4943005	20.31%	4.033%




Sum of corrected areas: 122561679

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090722\
Data File : BP011642.D
Acq On : 07 Sep 2022 11:42
Operator : CG/JU
Sample : PB147377BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB147377BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

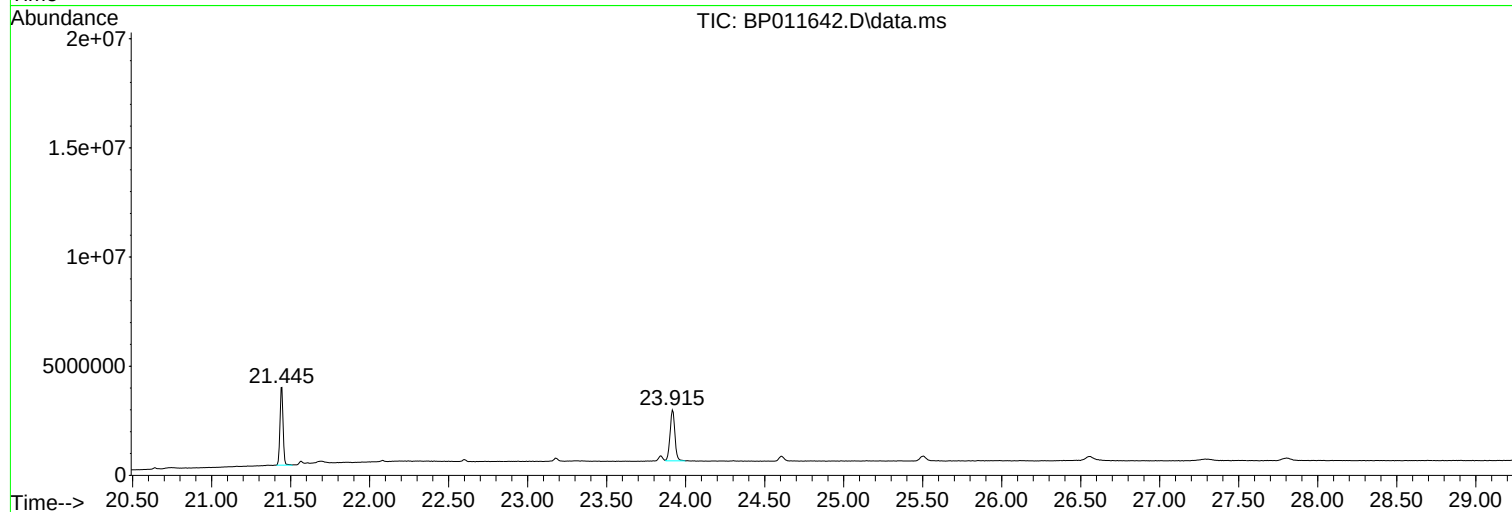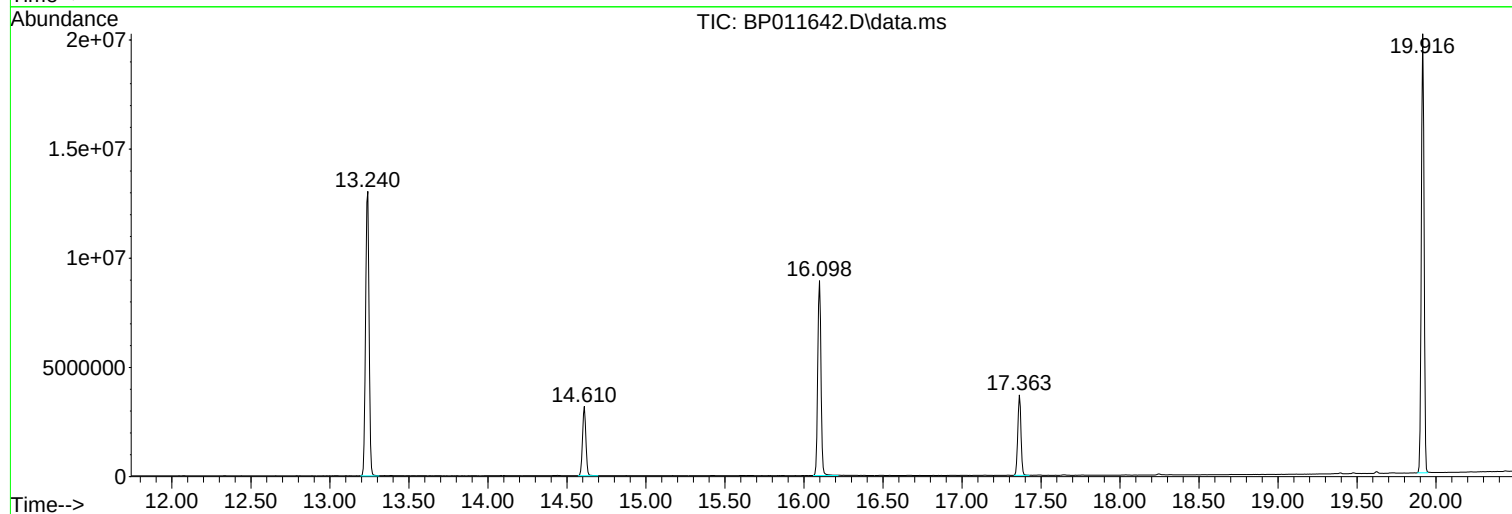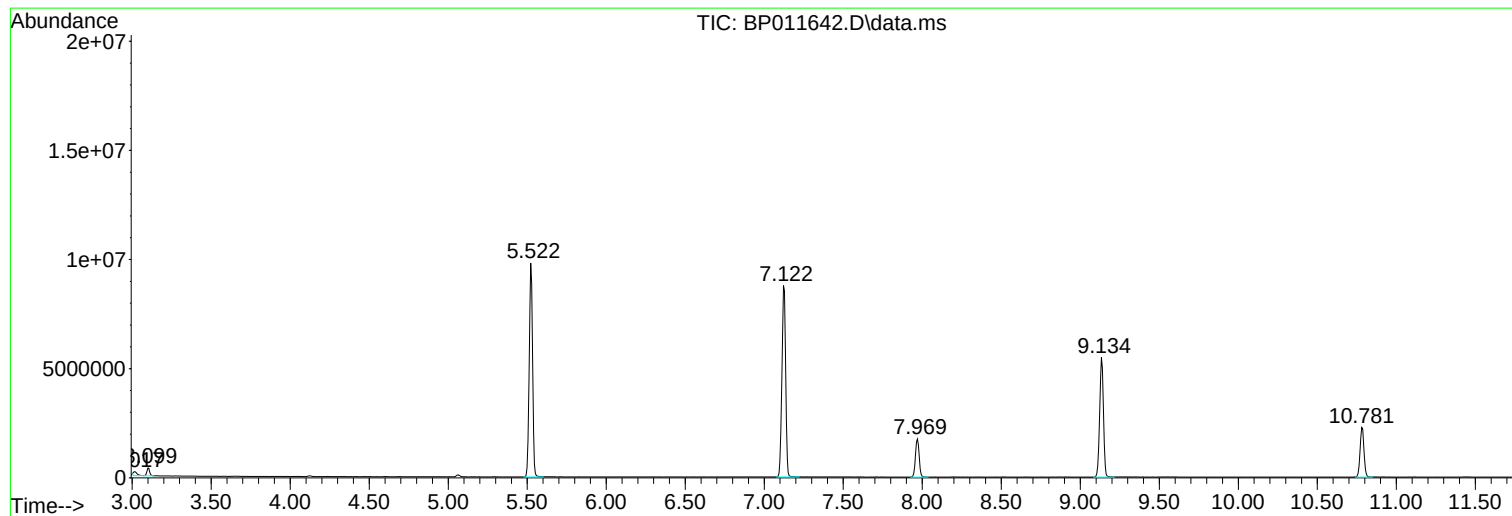

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090722\
Data File : BP011642.D
Acq On : 07 Sep 2022 11:42
Operator : CG/JU
Sample : PB147377BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB147377BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.099	3.10 ng	439061	1,4-Dichlorobenzene-d4	7.969

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	33
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	27
5			Octanal, 7-methoxy-3,7-dimethyl-	186	C11H22O2	003613-30-7	23

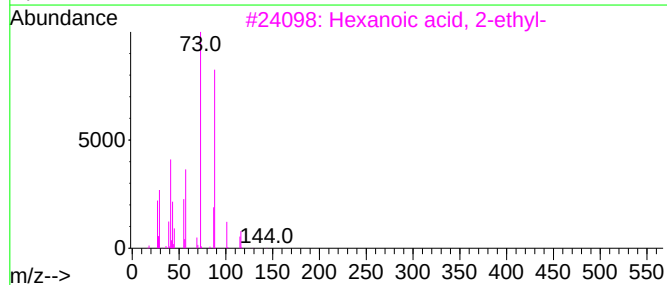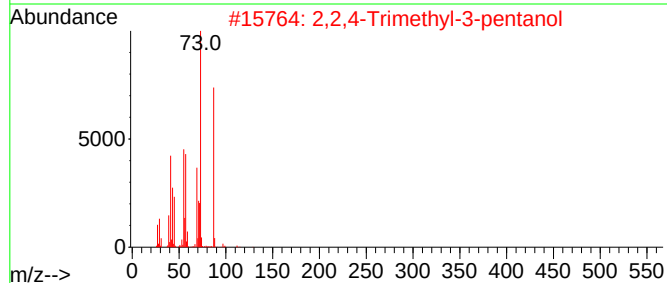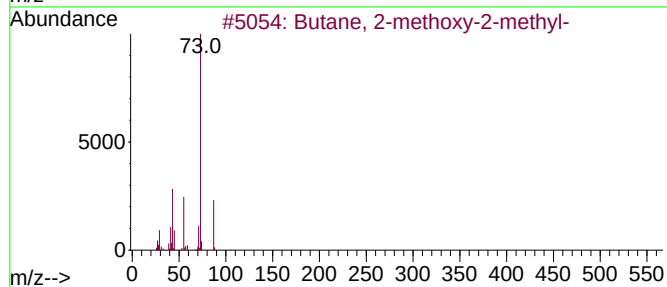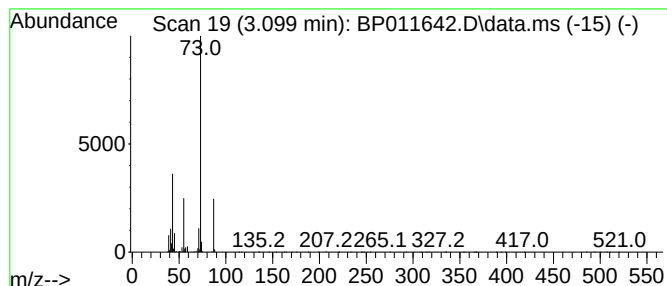

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090722\
Data File : BP011642.D
Acq On : 07 Sep 2022 11:42
Operator : CG/JU
Sample : PB147377BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB147377BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.099	3.1	ng	439061	1	7.969	2832600	20.0