
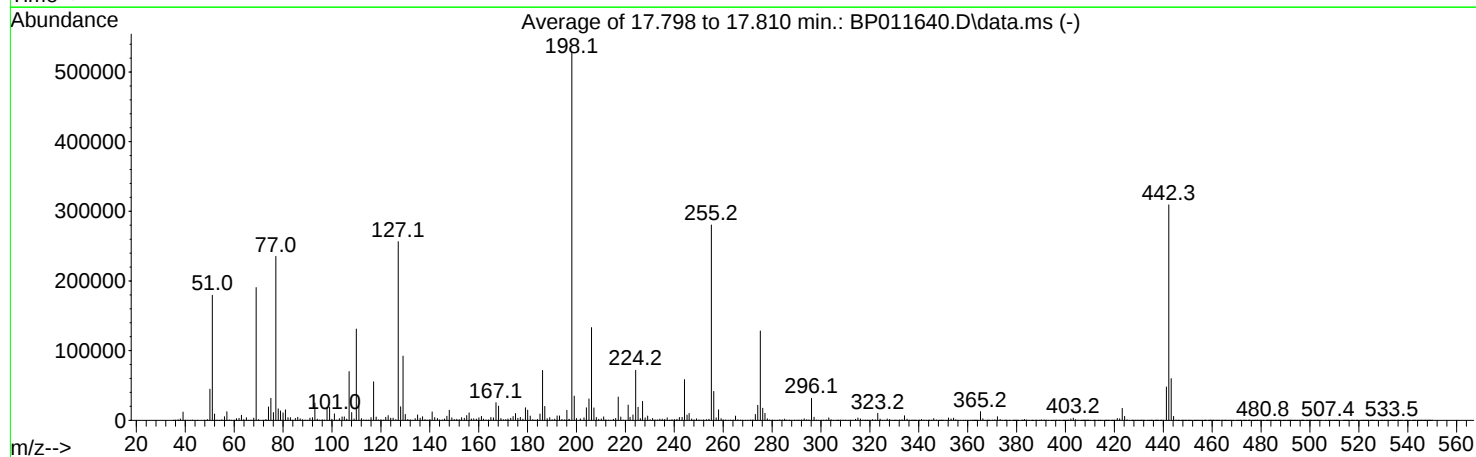


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090722\
 Data File : BP011640.D
 Acq On : 07 Sep 2022 10:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 03 04:07:09 2022

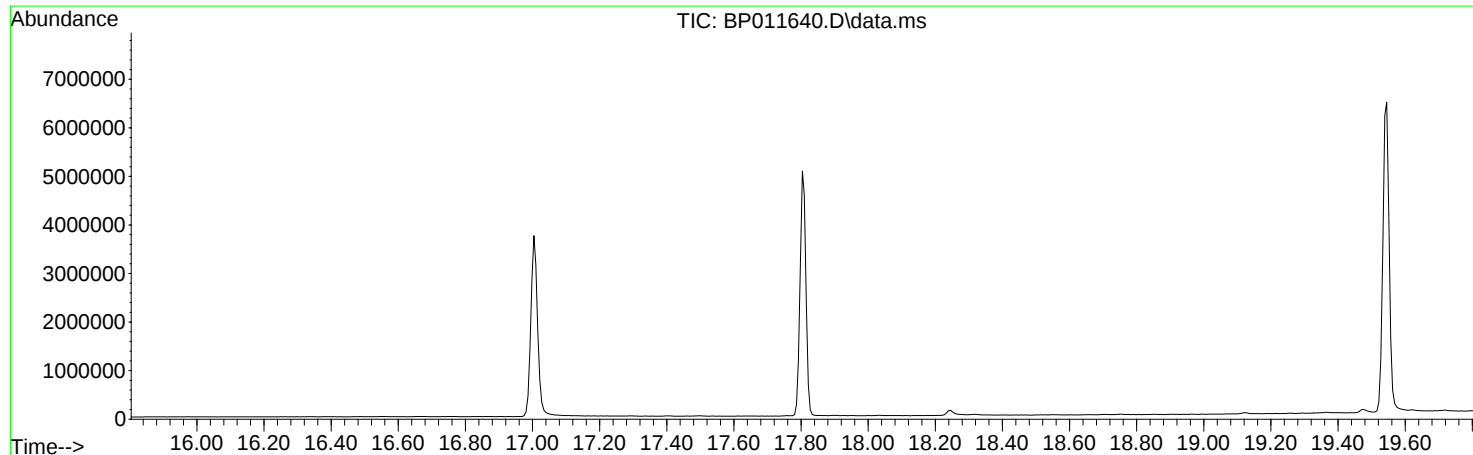




AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	179516	PASS
68	69	0.00	2	1.7	3213	PASS
69	198	0.00	100	36.1	190643	PASS
70	69	0.00	2	0.5	1005	PASS
127	198	10	80	48.6	256512	PASS
197	198	0.00	2	0.3	1491	PASS
198	198	100	100	100.0	528085	PASS
199	198	5	9	6.6	34880	PASS
275	198	10	60	24.3	128312	PASS
365	198	1	100	2.4	12504	PASS
441	198	0.01	100	9.1	47896	PASS
442	442	100	100	100.0	309269	PASS
443	442	15	24	19.4	59891	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090722\
Data File : BP011640.D
Acq On : 07 Sep 2022 10:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 08 06:14:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 03 04:07:09 2022
Response via : Initial Calibration

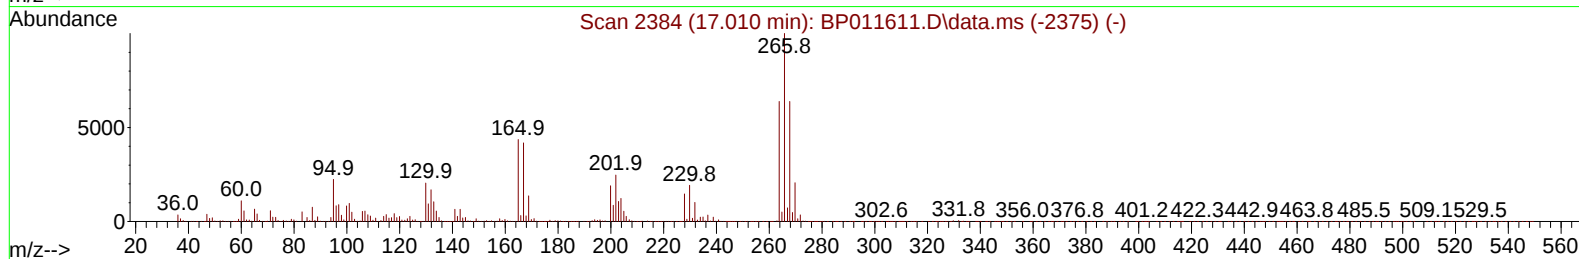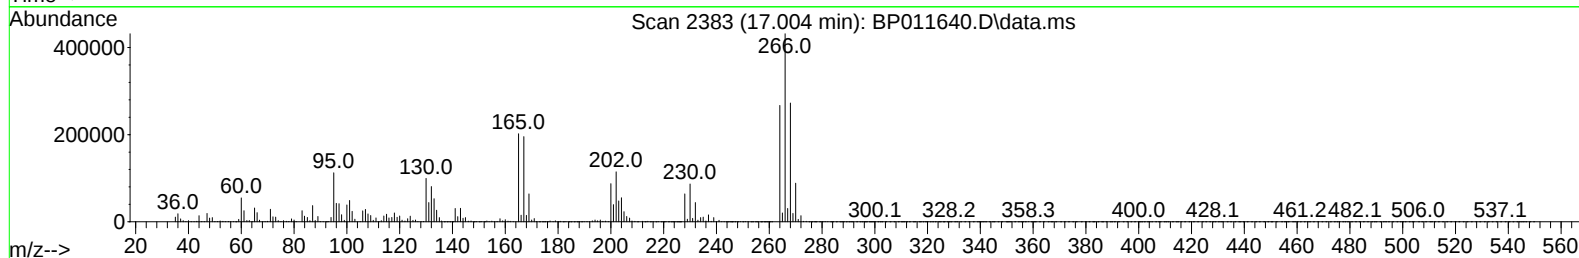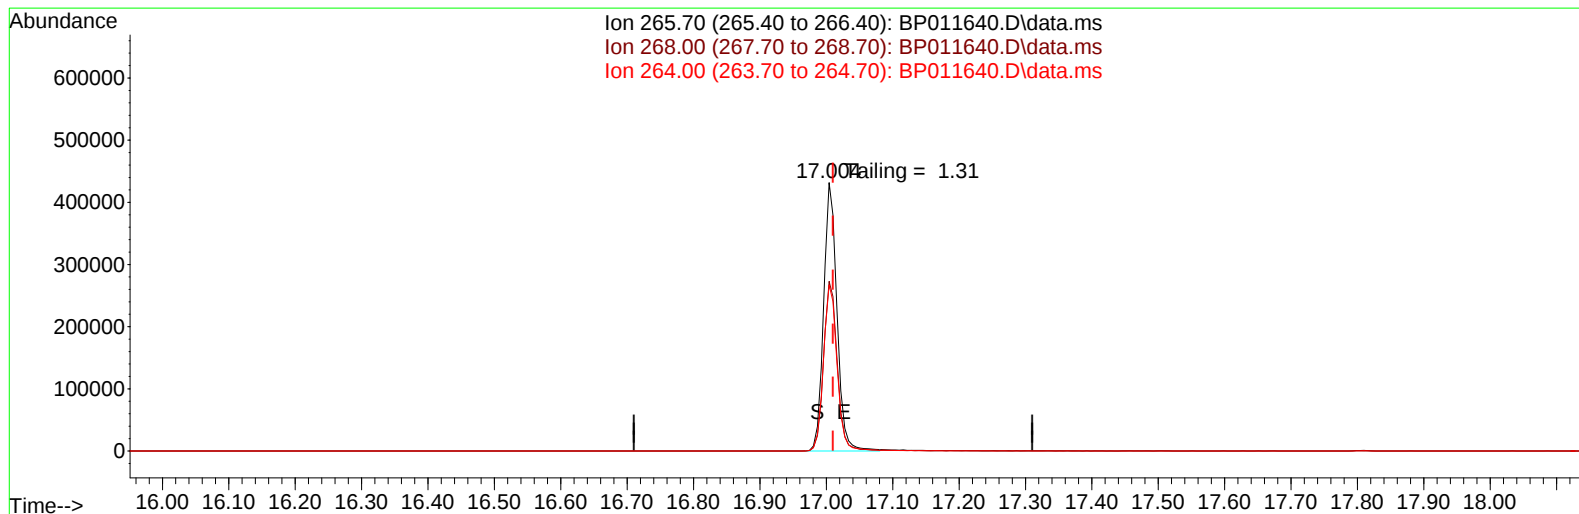

TIC: BP011640.D\data.ms

(70) Pentachlorophenol (C)

17.004min (-0.006) 917188.94 ng




response 607491

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.19
264.00	63.00	61.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090722\
Data File : BP011640.D
Acq On : 07 Sep 2022 10:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 08 06:14:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 03 04:07:09 2022
Response via : Initial Calibration

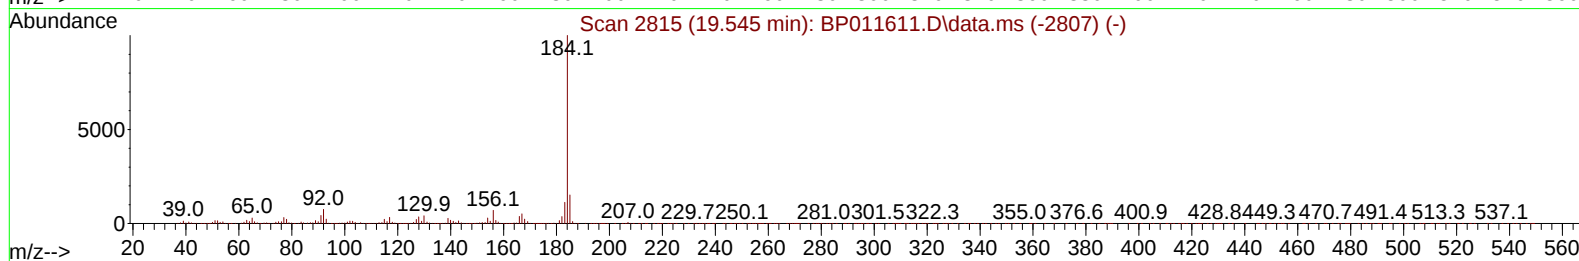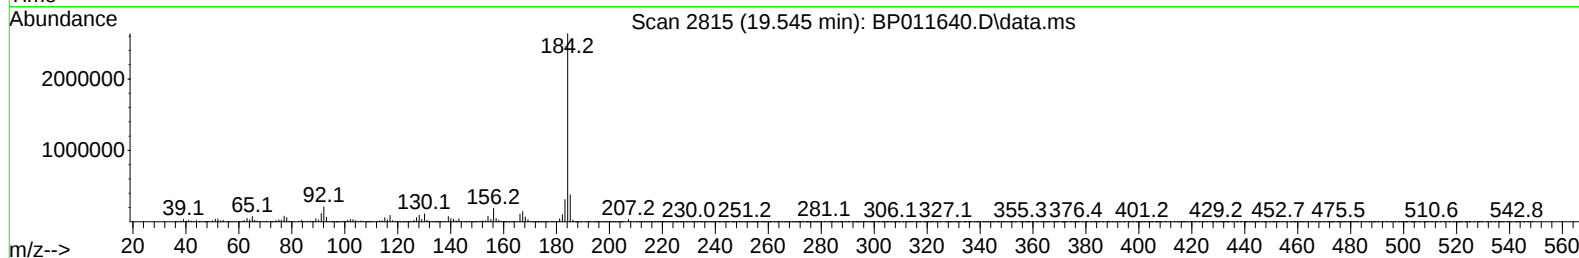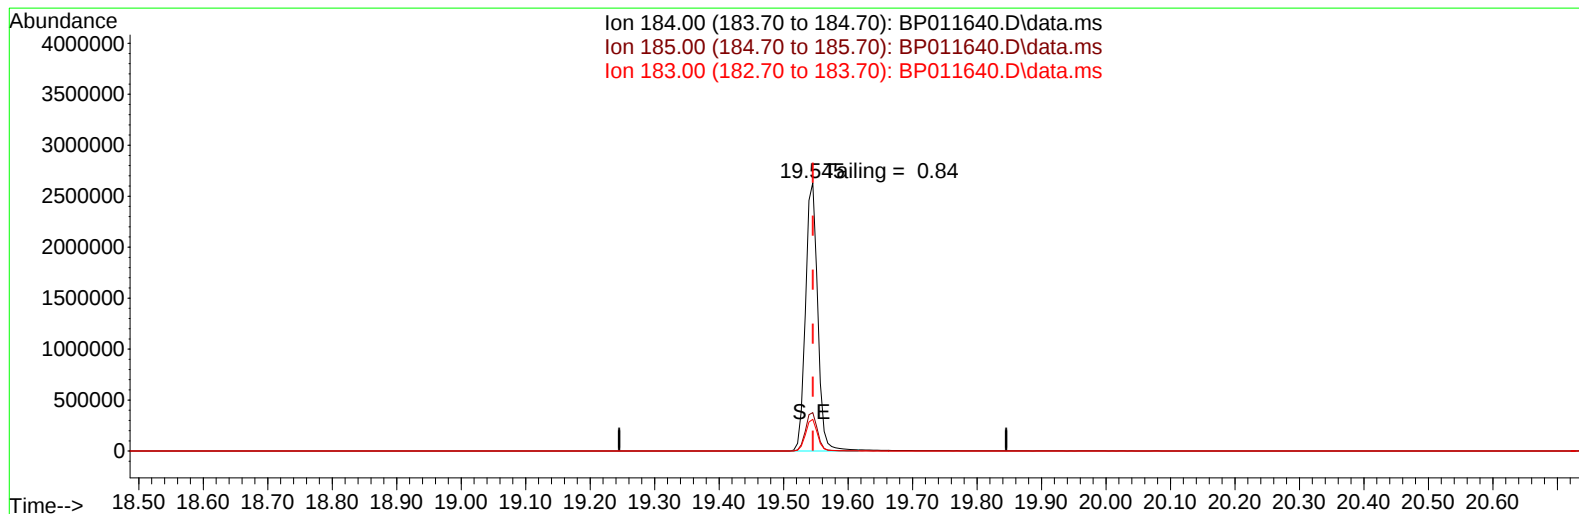

TIC: BP011640.D\data.ms

(77) Benzidine

19.545min (-0.000) 2504131.12 ng

response 3494084

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.35
183.00	11.30	11.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/7/2022	BNA_P	BP011640.D
Compound Name	Response	Retention Time
DDT	1702089	20.751
DDD	10819	20.369
DDE	832	19.822
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11651	1713740	0.68

Instrument :
BNA_P
ClientSampleId :
DFTPP