


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP090819\
 Data File : BP000103.D
 Acq On : 08 Sep 2019 21:00
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 30 17:47:17 2019

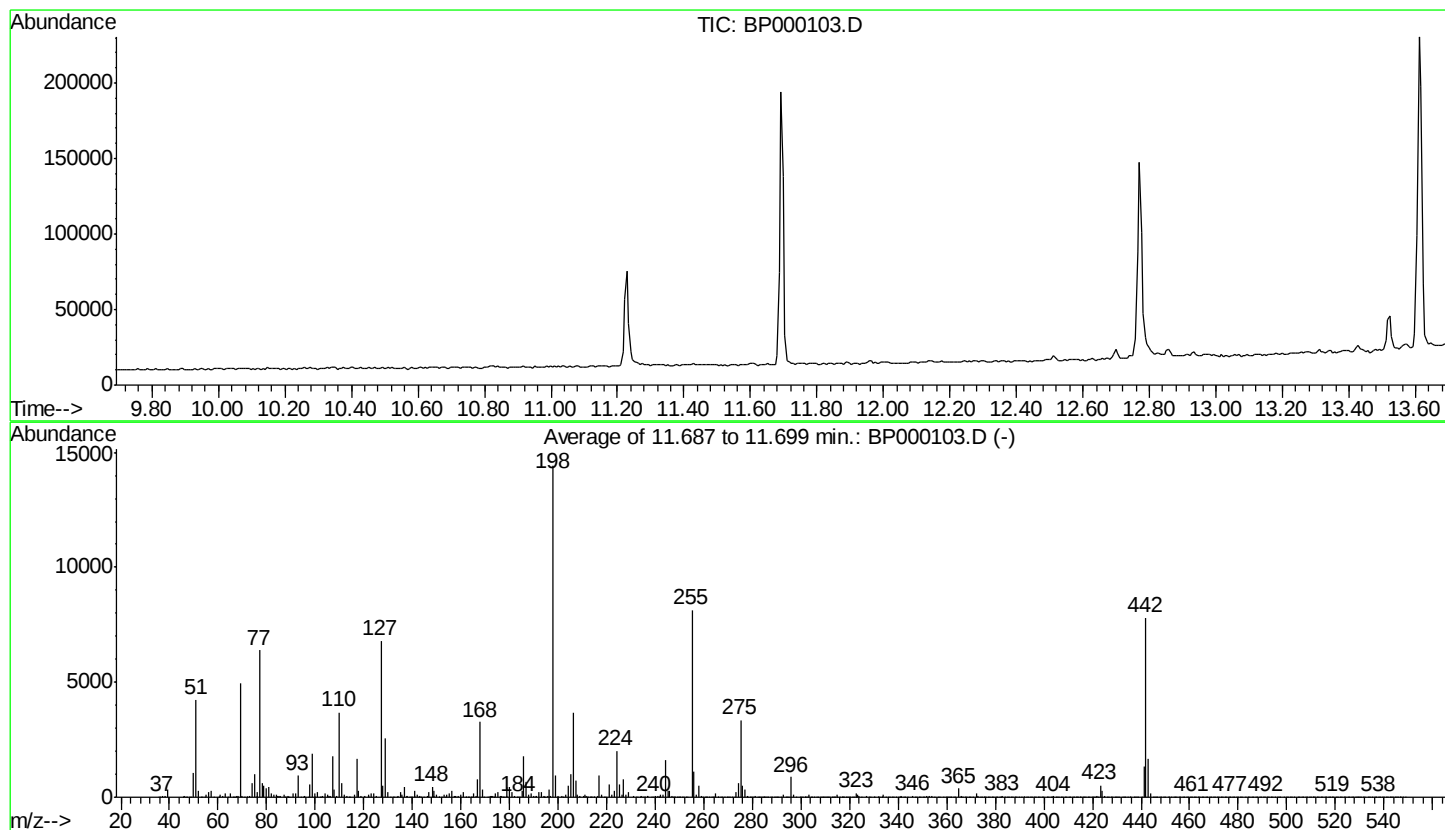

AutoFind: Scans 1632, 1633, 1634; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	4236	PASS
68	69	0.00	2	1.6	79	PASS
69	198	0.00	100	34.2	4933	PASS
70	69	0.00	2	1.0	48	PASS
127	198	10	80	47.2	6808	PASS
197	198	0.00	2	0.3	42	PASS
198	198	100	100	100.0	14424	PASS
199	198	5	9	6.6	946	PASS
275	198	10	60	23.3	3365	PASS
365	198	1	100	2.7	384	PASS
441	198	0.01	100	9.4	1359	PASS
442	198	50	100	54.1	7800	PASS
443	442	15	24	21.4	1670	PASS