

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP090820\
 Data File : BP003226.D
 Acq On : 08 Sep 2020 14:29
 Operator : CG/JU
 Sample : PB131465BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB131465BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.263	397	404	420	rBV	2404932	3516566	41.42%	9.003%
2	6.840	664	672	698	rBV	2083943	3375854	39.77%	8.643%
3	7.652	801	810	821	rBV	635915	975694	11.49%	2.498%
4	8.799	996	1005	1025	rBV	1453578	2464791	29.03%	6.311%
5	10.434	1275	1283	1300	rBV	709873	1340113	15.79%	3.431%
6	12.916	1697	1705	1731	rBV	3931397	6571263	77.41%	16.824%
7	14.298	1933	1940	1959	rBV2	988585	1788346	21.07%	4.579%
8	15.798	2186	2195	2241	rBV	2029702	4149857	48.88%	10.625%
9	17.051	2401	2408	2423	rBV	1189117	2010584	23.68%	5.148%
10	19.627	2840	2846	2866	rBV	6550213	8489321	100.00%	21.735%
11	21.145	3099	3104	3119	rBV	1502157	2236020	26.34%	5.725%
12	23.386	3478	3485	3504	rBV2	883359	2139990	25.21%	5.479%


Sum of corrected areas: 39058399

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP090820\
Data File : BP003226.D
Acq On : 08 Sep 2020 14:29
Operator : CG/JU
Sample : PB131465BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131465BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

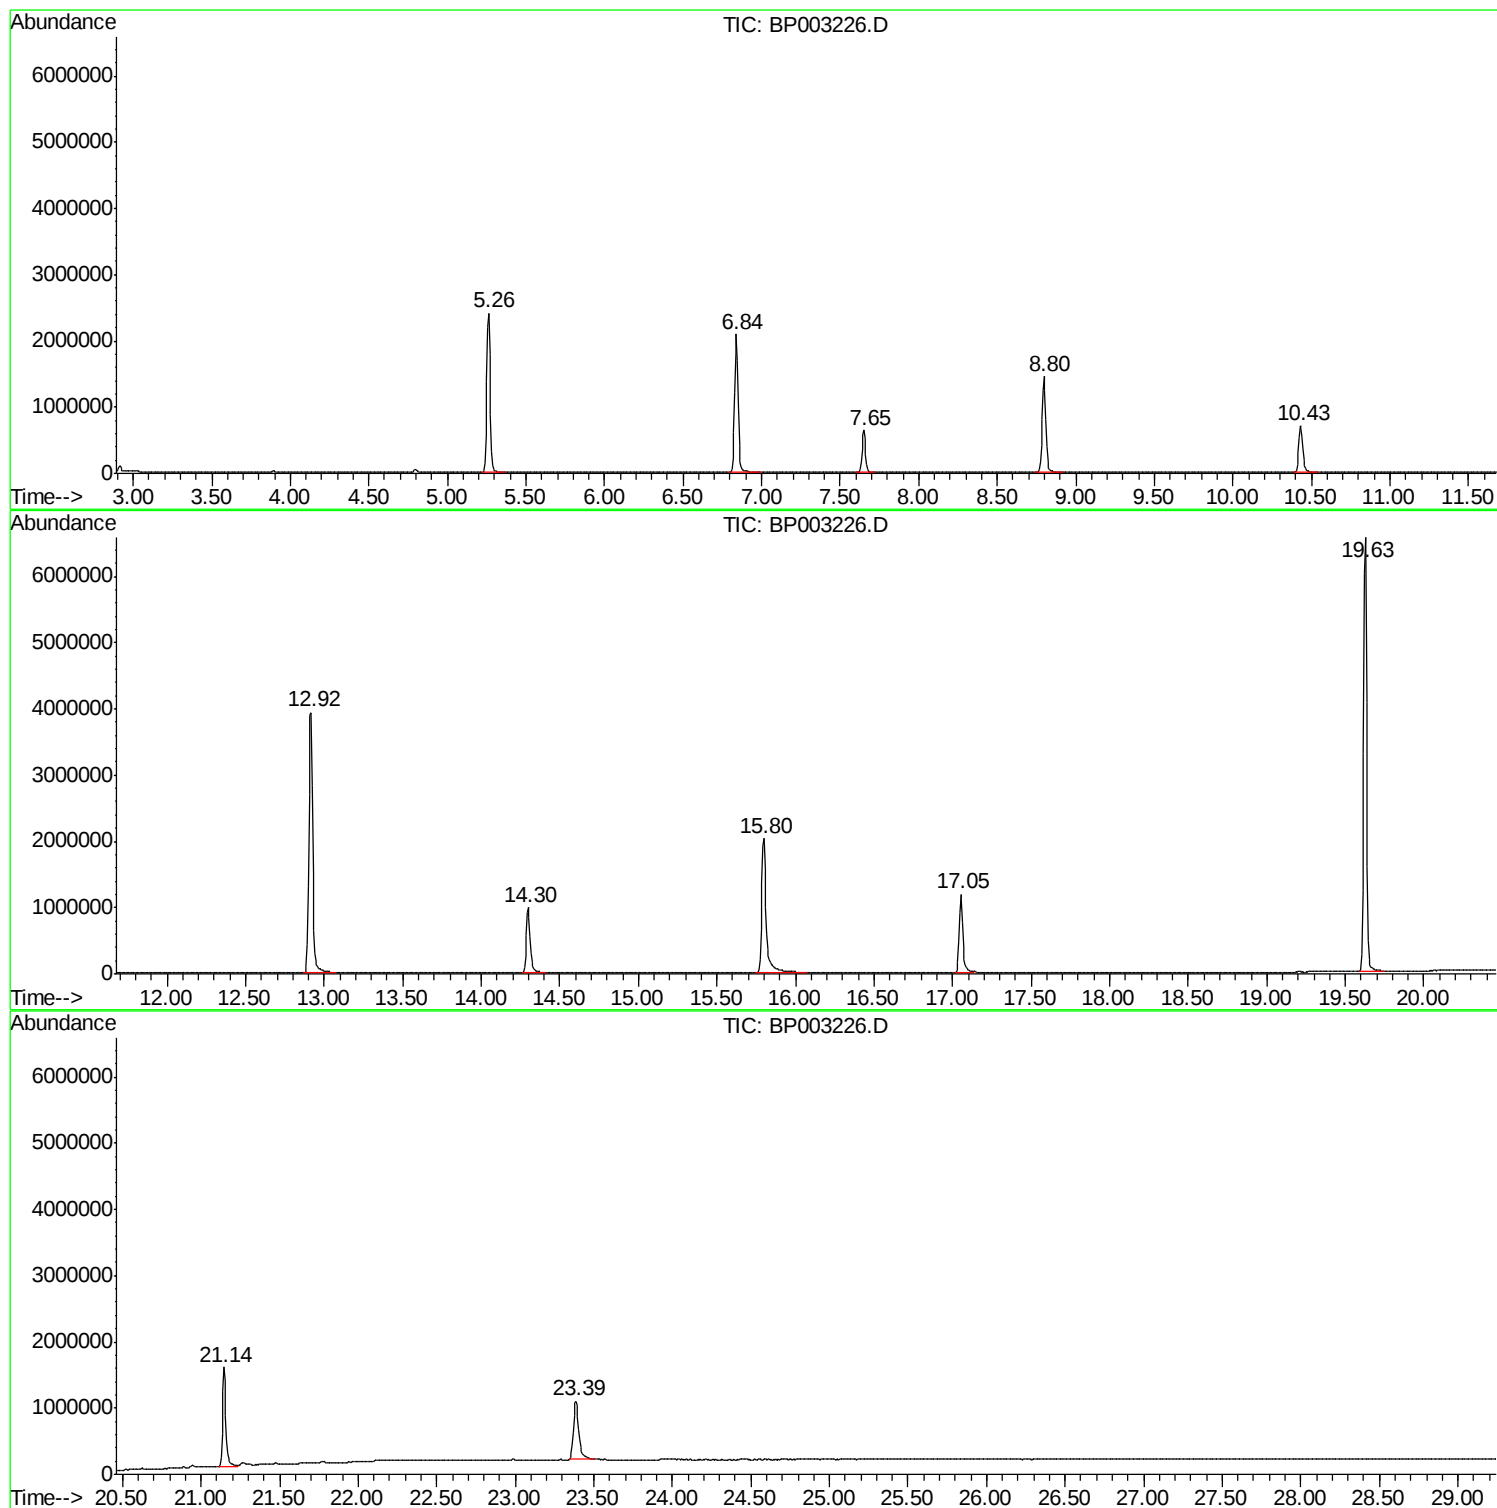

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP090820\
Data File : BP003226.D
Acq On : 08 Sep 2020 14:29
Operator : CG/JU
Sample : PB131465BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131465BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP090820\
Data File : BP003226.D
Acq On : 08 Sep 2020 14:29
Operator : CG/JU
Sample : PB131465BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131465BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc