


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP090820\
 Data File : BP003221.D
 Acq On : 08 Sep 2020 09:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 01 14:37:05 2020

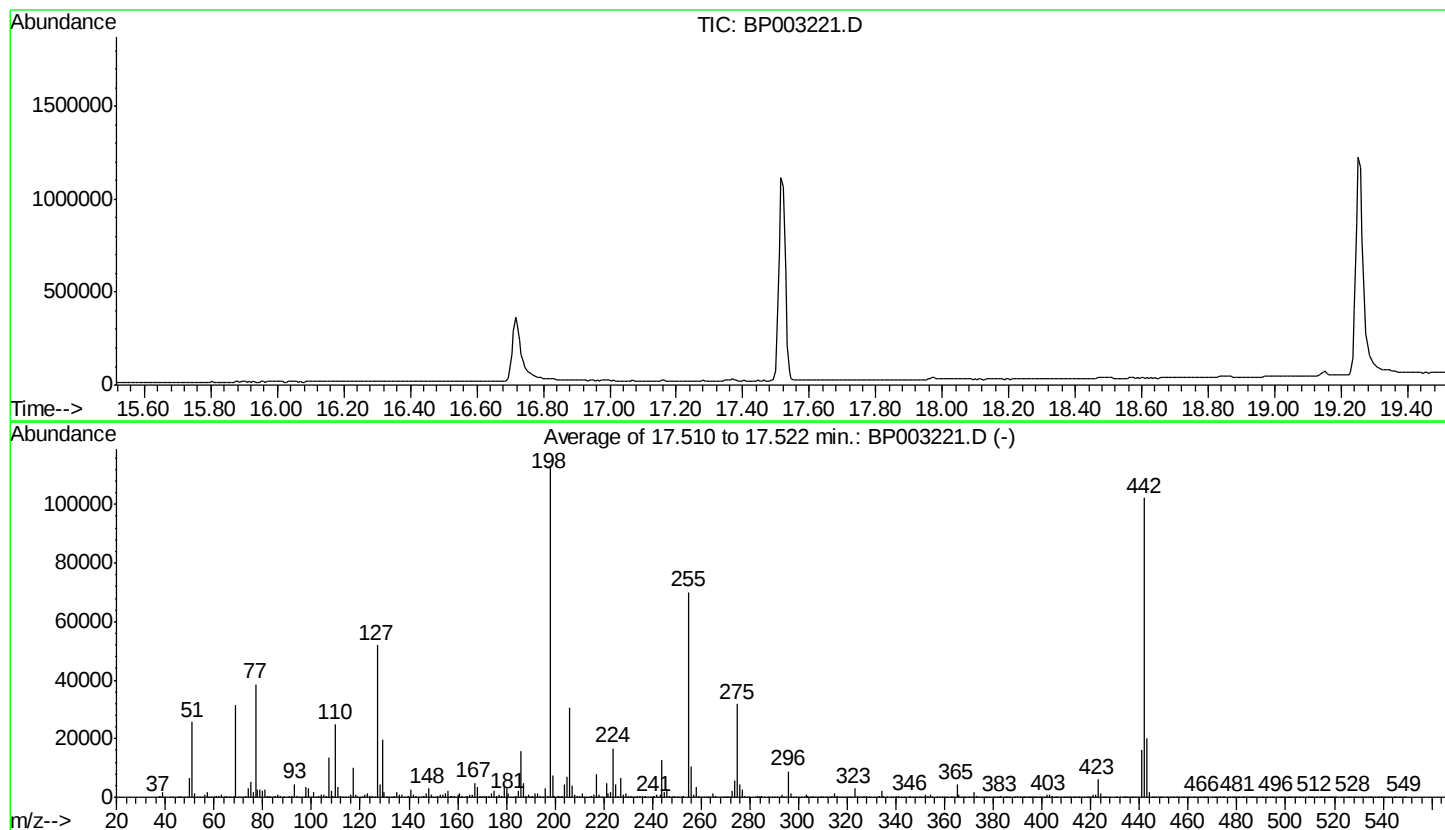

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.6	25613	PASS
68	69	0.00	2	2.0	647	PASS
69	198	0.00	100	28.0	31680	PASS
70	69	0.00	2	0.4	132	PASS
127	198	10	80	45.8	51920	PASS
197	198	0.00	2	0.4	508	PASS
198	198	100	100	100.0	113264	PASS
199	198	5	9	6.7	7596	PASS
275	198	10	60	28.1	31832	PASS
365	198	1	100	3.7	4185	PASS
441	198	0.01	100	14.2	16122	PASS
442	198	50	100	90.2	102205	PASS
443	442	15	24	19.5	19921	PASS