

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090821\
 Data File : BP006884.D
 Acq On : 08 Sep 2021 15:50
 Operator : CG/JU
 Sample : SSTD00515
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD005615

Quant Time: Sep 09 01:59:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 09 01:57:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	257603	20.000	ng/u1	0.00
20) Naphthalene-d8	10.740	136	1053616	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.563	164	661480	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.316	188	1409355	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.398	240	1438342	20.000	ng/u1	0.00
88) Perylene-d12	23.839	264	1491830	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	13115	1.722	ng/uL	0.00
4) Pyridine-d5	3.793	84	76667	3.502	ng/u1	0.01
7) Phenol-d5	7.087	99	81343	3.141	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	54485	3.423	ng/u1	0.00
11) 2-Chlorophenol-d4	7.463	132	71835	3.725	ng/u1	0.00
15) 4-Methylphenol-d8	8.634	113	64558	3.120	ng/u1	0.00
21) Nitrobenzene-d5	9.099	128	27813	3.110	ng/u1	0.00
24) 2-Nitrophenol-d4	9.822	143	24908	2.662	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.440	165	256	0.016	ng/u1	0.08
31) 4-Chloroaniline-d4	10.875	131	90964	3.540	ng/u1	0.00
46) Dimethylphthalate-d6	13.975	166	205808	4.057	ng/u1	0.00
49) Acenaphthylene-d8	14.257	160	254020	4.082	ng/u1	0.00
54) 4-Nitrophenol-d4	14.745	143	22798	2.152	ng/u1	0.00
60) Fluorene-d10	15.557	176	188160	4.561	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.669	200	16242	1.744	ng/u1	0.00
73) Anthracene-d10	17.416	188	282120	4.231	ng/u1	0.00
81) Pyrene-d10	19.645	212	328650	4.351	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.680	264	334904	4.163	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.399	88	15103	1.952	ng/uL#	76
5) Pyridine	3.811	79	80337	3.545	ng/u1#	81
6) Benzaldehyde	7.075	77	59204	4.650	ng/u1	90
8) Phenol	7.116	94	89397	3.380	ng/u1	92
10) Bis(2-Chloroethyl)ether	7.358	93	76537	3.755	ng/u1	97
12) 2-Chlorophenol	7.493	128	73972	3.804	ng/u1	91
13) 2-Methylphenol	8.375	108	64783	3.329	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.463	45	95335	4.003	ng/u1	97
16) Acetophenone	8.757	105	111671	3.429	ng/u1	92
17) N-Nitroso-di-n-propyla...	8.746	70	49859	2.846	ng/u1	97
18) 4-Methylphenol	8.699	108	68797	3.252	ng/u1	94
19) Hexachloroethane	9.022	117	32097	3.793	ng/u1	83
22) Nitrobenzene	9.134	77	70884	3.027	ng/u1	95
23) Isophorone	9.663	82	138552	3.173	ng/u1	95
25) 2-Nitrophenol	9.852	139	27097	2.745	ng/u1#	86
26) 2,4-Dimethylphenol	9.904	107	77884	3.673	ng/u1	91
27) Bis(2-Chloroethoxy)met...	10.152	93	96832	3.826	ng/u1	98
29) 2,4-Dichlorophenol	10.493	162	73	0.005	ng/u1	89
30) Naphthalene	10.787	128	253762	4.438	ng/u1	99
32) 4-Chloroaniline	10.899	127	92884	3.683	ng/u1	98
33) Hexachlorobutadiene	11.081	225	49599	5.484	ng/u1	98
34) Caprolactam	11.675	113	5149	0.838	ng/u1	92
35) 4-Chloro-3-methylphenol	12.010	107	65355	3.331	ng/u1	91
36) 2-Methylnaphthalene	12.398	142	167004	4.250	ng/u1	97

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090821\
 Data File : BP006884.D
 Acq On : 08 Sep 2021 15:50
 Operator : CG/JU
 Sample : SSTD00515
 Misc :
 ALS Vial : 2 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 SSTD005615


Quant Time: Sep 09 01:59:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 09 01:57:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.616	142	171742	4.392	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.763	216	93401	5.240	ng/ul#	92
40) Hexachlorocyclopentadiene	12.746	237	53449	4.570	ng/ul	99
41) 2,4,6-Trichlorophenol	12.998	196	46843	3.826	ng/ul	97
42) 2,4,5-Trichlorophenol	13.063	196	53850	4.131	ng/ul	96
43) 1,1'-Biphenyl	13.404	154	229116	4.455	ng/ul#	97
44) 2-Chloronaphthalene	13.445	162	175570	4.500	ng/ul	92
45) 2-Nitroaniline	13.640	65	28339	2.014	ng/ul#	80
47) Dimethylphthalate	14.022	163	210902	4.203	ng/ul	98
48) 2,6-Dinitrotoluene	14.140	165	27620	2.852	ng/ul#	83
50) Acenaphthylene	14.287	152	266837	4.387	ng/ul	100
51) 3-Nitroaniline	14.463	138	26237	2.366	ng/ul#	89
52) Acenaphthene	14.628	153	187282	4.318	ng/ul	98
53) 2,4-Dinitrophenol	14.669	184	8647	1.380	ng/ul#	75
55) 4-Nitrophenol	14.757	109	18538	1.951	ng/ul#	88
56) Dibenzofuran	14.963	168	268217	4.625	ng/ul#	85
57) 2,4-Dinitrotoluene	14.922	165	38325	2.690	ng/ul#	77
58) 2,3,4,6-Tetrachlorophenol	15.187	232	43159	3.989	ng/ul#	78
59) Diethylphthalate	15.387	149	203051	3.807	ng/ul	95
61) Fluorene	15.610	166	216849	4.485	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.610	204	110371	5.042	ng/ul#	82
63) 4-Nitroaniline	15.622	138	23589	2.271	ng/ul	87
66) 4,6-Dinitro-2-methylph...	15.681	198	17201	1.847	ng/ul#	92
67) N-Nitrosodiphenylamine	15.822	169	179365	4.143	ng/ul	98
68) 4-Bromophenyl-phenylether	16.504	248	63335	4.557	ng/ul#	86
69) Hexachlorobenzene	16.581	284	114	0.007	ng/ul	93
70) Atrazine	16.775	200	60391	3.932	ng/ul	93
71) Pentachlorophenol	16.963	266	30016	2.917	ng/ul	97
72) Phenanthrene	17.357	178	354325	4.450	ng/ul	99
74) Anthracene	17.445	178	342021	4.230	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.369	216	96240	5.022	ng/ul	99
76) Pentachlorobenzene	14.887	250	94894	5.026	ng/ul	98
77) Carbazole	17.716	167	291693	3.863	ng/ul	97
78) Di-n-butylphthalate	18.275	149	329071	3.370	ng/ul	98
80) Fluoranthene	19.322	202	410745	4.327	ng/ul	94
82) Pyrene	19.675	202	432043	4.406	ng/ul	94
83) Butylbenzylphthalate	20.551	149	125348	2.586	ng/ul#	87
84) 3,3'-Dichlorobenzidine	21.316	252	104292	3.177	ng/ul	99
85) Benzo(a)anthracene	21.386	228	407204	4.346	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.316	149	195159	2.613	ng/ul#	96
87) Chrysene	21.439	228	418068	4.628	ng/ul	98
89) Di-n-octyl phthalate	22.251	149	312302	2.422	ng/ul	100
90) Benzo(b)fluoranthene	23.092	252	415390	4.286	ng/ul	97
91) Benzo(k)fluoranthene	23.139	252	398421	4.246	ng/ul	99
93) Benzo(a)pyrene	23.727	252	393544	4.483	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.392	276	445465	3.881	ng/ul	97
95) Dibenzo(a,h)anthracene	26.415	278	386747	4.011	ng/ul	97
96) Benzo(g,h,i)perylene	27.174	276	386211	4.052	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Sep 09 01:59:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 09 01:57:53 2021
Response via : Initial Calibration







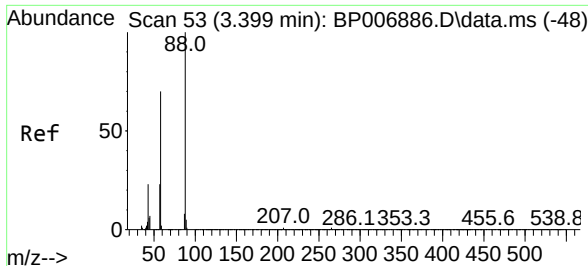

#2
1,4-Dioxane
Concen: 1.952 ng/uL
RT: 3.399 min Scan# 53
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion: 88 Resp: 15103
Ion Ratio Lower Upper
88 100
43 34.0 20.1 30.1#
58 80.3 48.4 72.6#

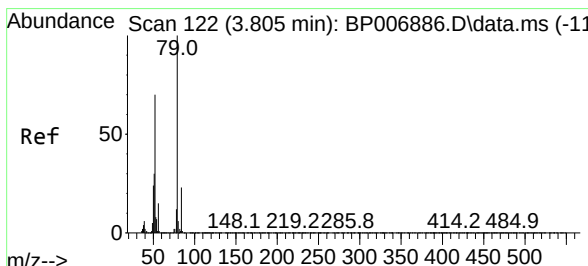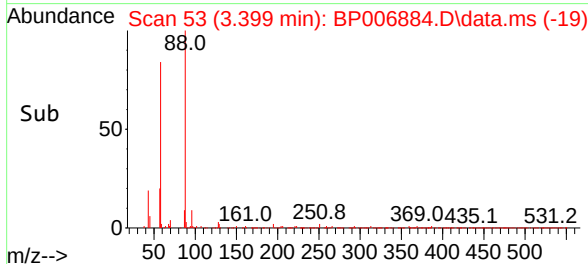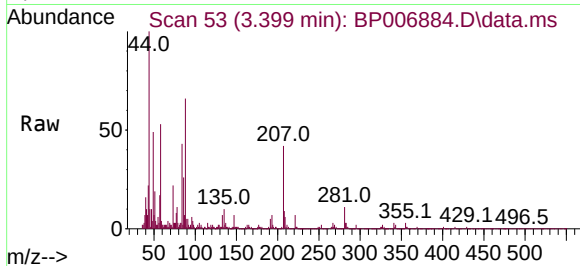

#5
Pyridine
Concen: 3.545 ng/uL
RT: 3.811 min Scan# 123
Delta R.T. 0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion: 79 Resp: 80337
Ion Ratio Lower Upper
79 100
52 75.3 49.2 73.8#
51 39.0 22.7 34.1#


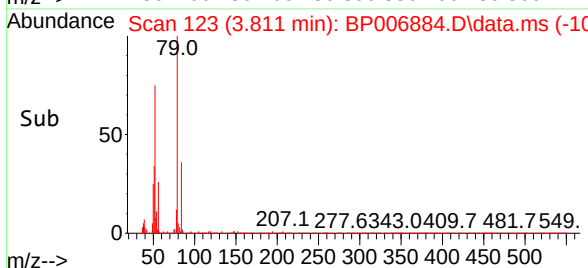
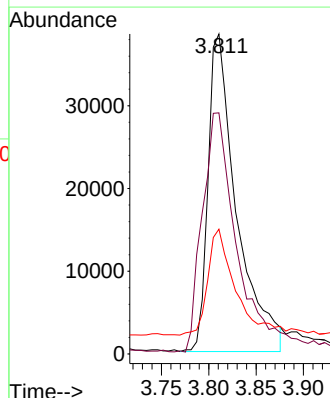
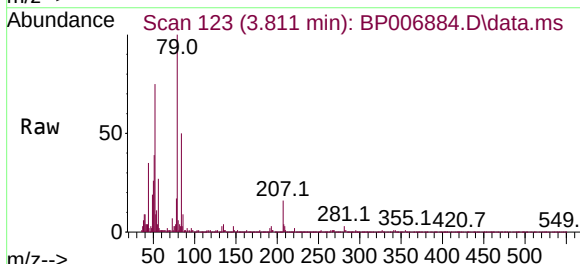




#6
Benzaldehyde
Concen: 4.650 ng/ul
RT: 7.075 min Scan# 678
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion: 77 Resp: 59204
Ion Ratio Lower Upper
77 100
105 101.8 74.4 111.6
106 97.9 70.3 105.5

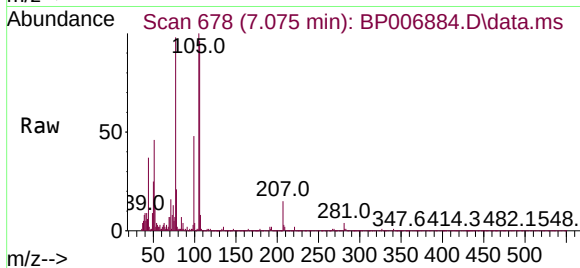

#8
Phenol
Concen: 3.380 ng/ul
RT: 7.116 min Scan# 685
Delta R.T. -0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion: 94 Resp: 89397
Ion Ratio Lower Upper
94 100
65 26.0 24.4 36.6
66 35.0 31.8 47.6


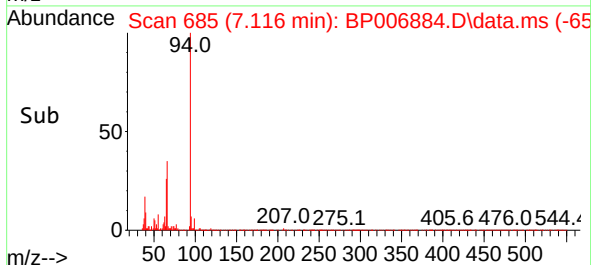
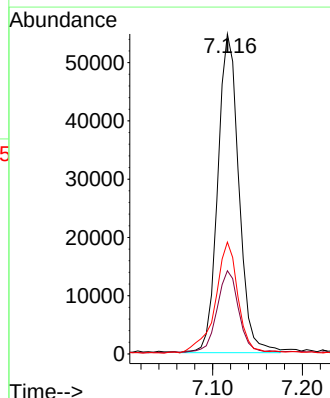
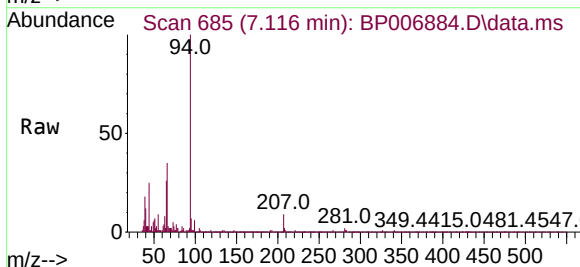




#10
 Bis(2-Chloroethyl)ether
 Concen: 3.755 ng/ul
 RT: 7.358 min Scan# 726
 Delta R.T. -0.006 min
 Lab File: BP006884.D
 Acq: 08 Sep 2021 15:50




Instrument :
 BNA_P
 ClientSampleId :
 SSTD005615


Tgt Ion:	93	Resp:	76537
Ion	Ratio	Lower	Upper
93	100		
63	72.3	59.7	89.5
95	29.7	25.3	37.9

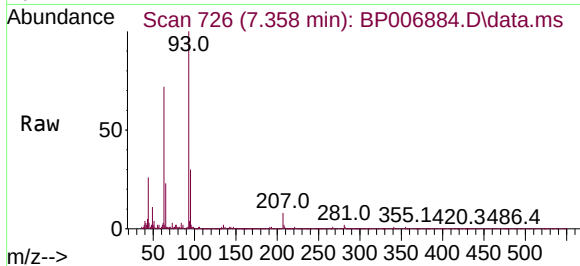

#12
 2-Chlorophenol
 Concen: 3.804 ng/ul
 RT: 7.493 min Scan# 749
 Delta R.T. -0.006 min
 Lab File: BP006884.D
 Acq: 08 Sep 2021 15:50

Tgt Ion:	128	Resp:	73972
Ion	Ratio	Lower	Upper
128	100		
64	42.4	40.6	60.8
130	29.9	26.4	39.6




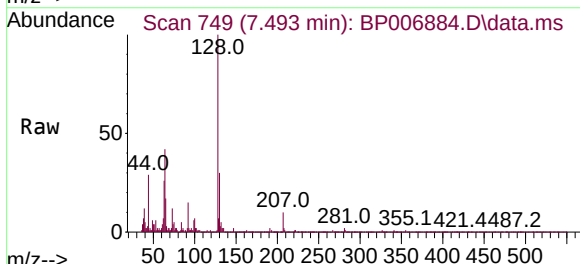




#13
2-Methylphenol
Concen: 3.329 ng/ul
RT: 8.375 min Scan# 899
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:108 Resp: 64783
Ion Ratio Lower Upper
108 100
107 92.1 72.2 108.2

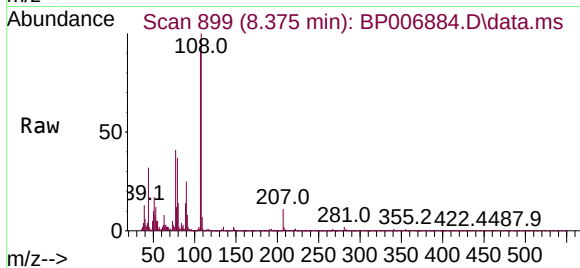

#14
2,2'-oxybis(1-Chloropropane)
Concen: 4.003 ng/ul
RT: 8.463 min Scan# 914
Delta R.T. -0.012 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion: 45 Resp: 95335
Ion Ratio Lower Upper
45 100
77 16.9 13.8 20.8
79 11.6 10.9 16.3




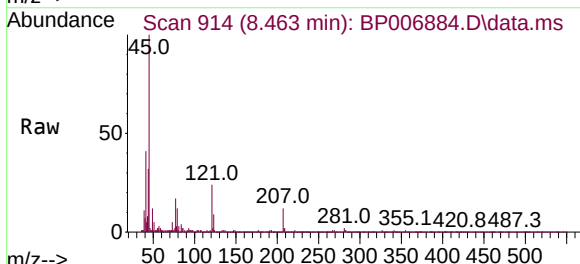




#16
Acetophenone
Concen: 3.429 ng/ul
RT: 8.757 min Scan# 964
Delta R.T. -0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:	105	Resp:	111671
Ion	Ratio	Lower	Upper
105	100		
77	74.5	67.0	100.4
51	24.7	19.0	28.6



#17
N-Nitroso-di-n-propylamine
Concen: 2.846 ng/ul
RT: 8.746 min Scan# 962
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:	70	Resp:	49859
Ion	Ratio	Lower	Upper
70	100		
42	51.1	40.4	60.6
101	9.4	7.2	10.8
130	22.1	14.9	22.3









#18
4-Methylphenol
Concen: 3.252 ng/ul
RT: 8.699 min Scan# 954
Delta R.T. -0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:108 Resp: 68797
Ion Ratio Lower Upper
108 100
107 117.5 88.6 133.0



#19
Hexachloroethane
Concen: 3.793 ng/ul
RT: 9.022 min Scan# 1009
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:117 Resp: 32097
Ion Ratio Lower Upper
117 100
201 102.0 68.2 102.2
199 65.1 43.5 65.3



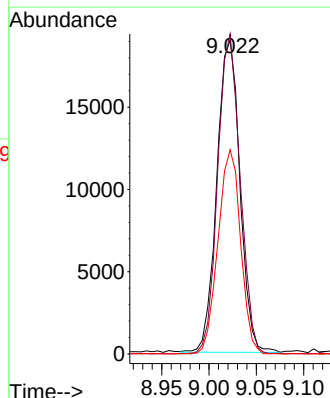



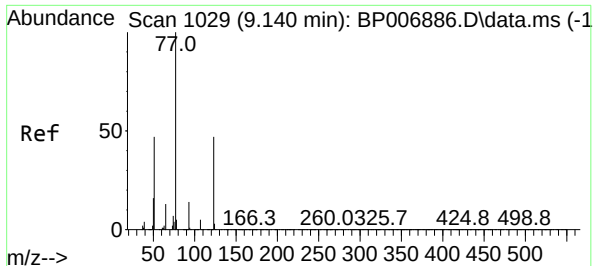

#22
Nitrobenzene
Concen: 3.027 ng/ul
RT: 9.134 min Scan# 1028
Delta R.T. -0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion: 77	Resp: 70884
Ion Ratio	Lower Upper
77 100	
123 42.6	31.1 46.7
65 12.1	10.6 16.0

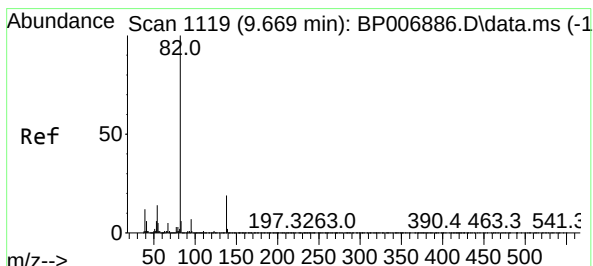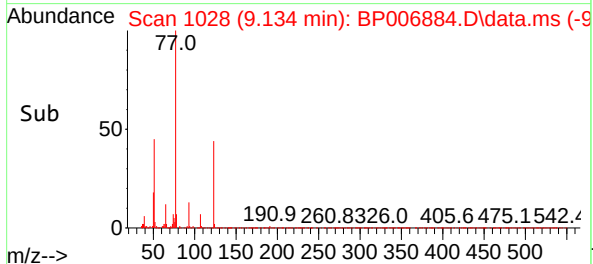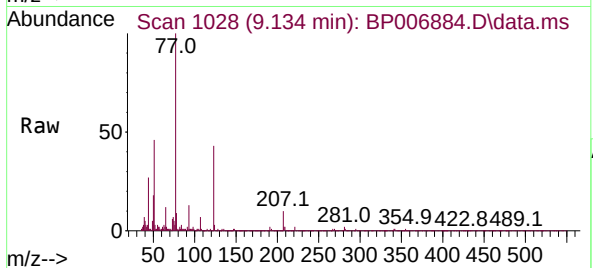

#23
Isophorone
Concen: 3.173 ng/ul
RT: 9.663 min Scan# 1118
Delta R.T. -0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion: 82	Resp: 138552
Ion Ratio	Lower Upper
82 100	
95 6.6	5.8 8.8
138 18.1	12.5 18.7


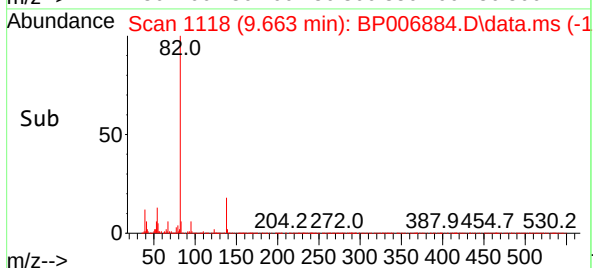
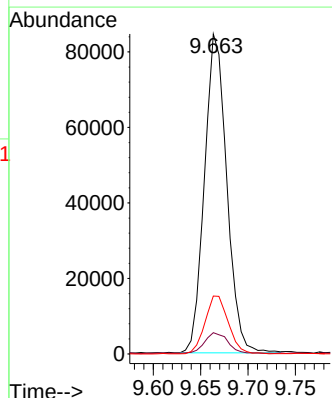
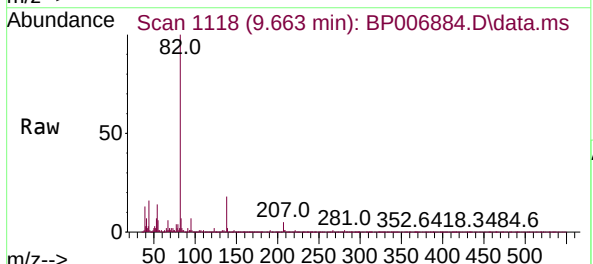




#25
2-Nitrophenol
Concen: 2.745 ng/ul
RT: 9.852 min Scan# 1150
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampled :
SSTD005615


Tgt Ion:139 Resp: 27097
Ion Ratio Lower Upper
139 100
65 50.0 48.4 72.6
109 27.6 28.2 42.2#



#26
2,4-Dimethylphenol
Concen: 3.673 ng/ul
RT: 9.904 min Scan# 1159
Delta R.T. -0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:107 Resp: 77884
Ion Ratio Lower Upper
107 100
121 51.6 38.1 57.1
122 89.2 64.2 96.4



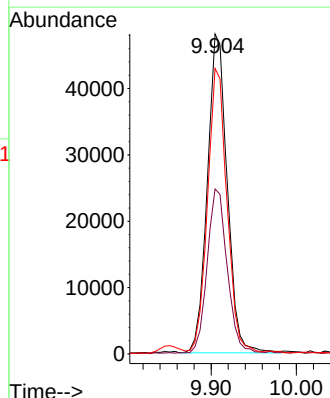





#27
 Bis(2-Chloroethoxy)methane
 Concen: 3.826 ng/ul
 RT: 10.152 min Scan# 1201
 Delta R.T. 0.000 min
 Lab File: BP006884.D
 Acq: 08 Sep 2021 15:50




Instrument :
 BNA_P
 ClientSampleID :
 SST005615


Tgt Ion: 93	Resp: 96832
Ion Ratio	Lower Upper
93 100	
95 31.1	25.6 38.4
123 11.8	8.2 12.4

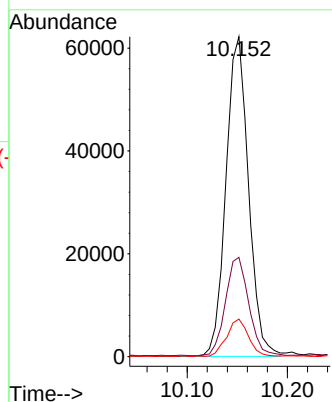

#29
 2,4-Dichlorophenol
 Concen: 0.005 ng/ul
 RT: 10.493 min Scan# 1259
 Delta R.T. 0.112 min
 Lab File: BP006884.D
 Acq: 08 Sep 2021 15:50

Tgt Ion: 162	Resp: 73
Ion Ratio	Lower Upper
162 100	
164 55.9	52.0 78.0
98 49.8	34.3 51.5









#30
Naphthalene
Concen: 4.438 ng/ul
RT: 10.787 min Scan# 1309
Delta R.T. -0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:128 Resp: 253762
Ion Ratio Lower Upper
128 100
129 11.5 8.8 13.2
127 12.9 10.6 15.8

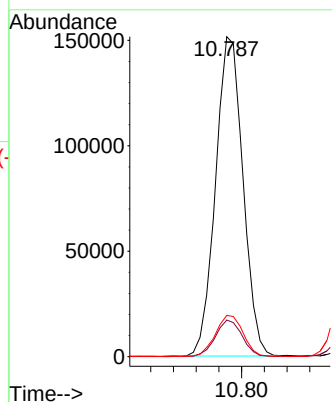

#32
4-Chloroaniline
Concen: 3.683 ng/ul
RT: 10.899 min Scan# 1328
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:127 Resp: 92884
Ion Ratio Lower Upper
127 100
129 33.1 25.7 38.5









#33
Hexachlorobutadiene
Concen: 5.484 ng/ul
RT: 11.081 min Scan# 1359
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampled :
SSTD005615


Tgt Ion:225 Resp: 49599
Ion Ratio Lower Upper
225 100
223 59.8 48.2 72.2
227 64.6 49.6 74.4



#34
Caprolactam
Concen: 0.838 ng/ul
RT: 11.675 min Scan# 1460
Delta R.T. 0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:113 Resp: 5149
Ion Ratio Lower Upper
113 100
55 174.2 125.8 188.6
56 123.5 98.2 147.2









#35
4-Chloro-3-methylphenol
Concen: 3.331 ng/ul
RT: 12.010 min Scan# 1517
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:	107	Resp:	65355
Ion Ratio	Lower	Upper	
107	100		
144	27.4	18.8	28.2
142	80.4	58.4	87.6

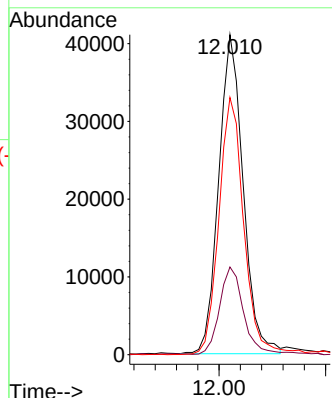

#36
2-Methylnaphthalene
Concen: 4.250 ng/ul
RT: 12.398 min Scan# 1583
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:	142	Resp:	167004
Ion Ratio	Lower	Upper	
142	100		
141	87.9	72.3	108.5



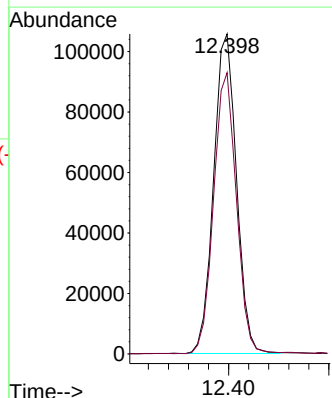



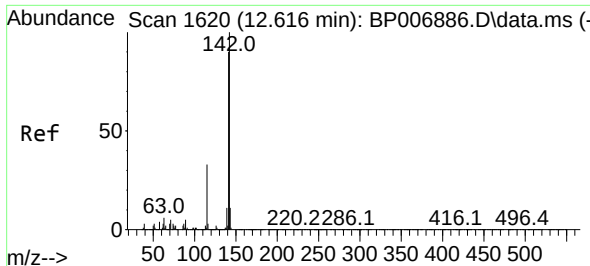

#37
1-Methylnaphthalene
Concen: 4.392 ng/ul
RT: 12.616 min Scan# 1620
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:	142	Resp:	171742
Ion Ratio	Lower	Upper	
142	100		
141	92.7	74.9	112.3
116	3.6	3.3	4.9

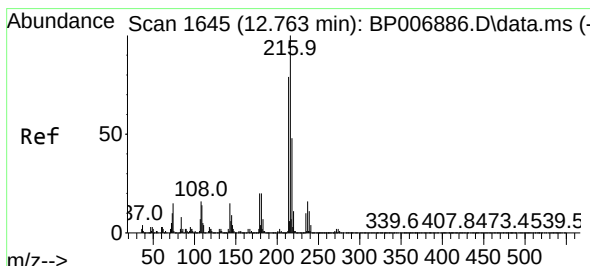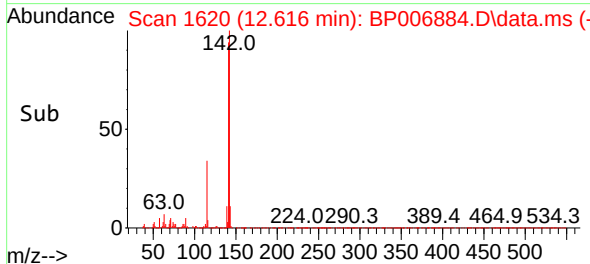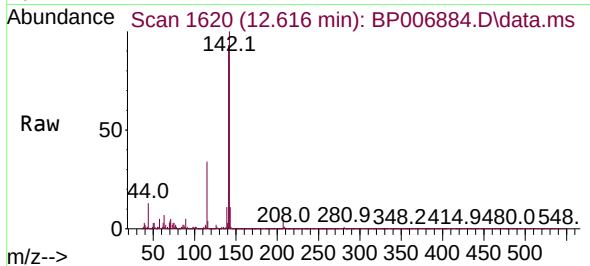

#39
1,2,4,5-Tetrachlorobenzene
Concen: 5.240 ng/ul
RT: 12.763 min Scan# 1645
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:	216	Resp:	93401
Ion Ratio	Lower	Upper	
216	100		
214	75.2	64.3	96.5
179	20.5	19.3	28.9
108	15.9	19.8	29.6#


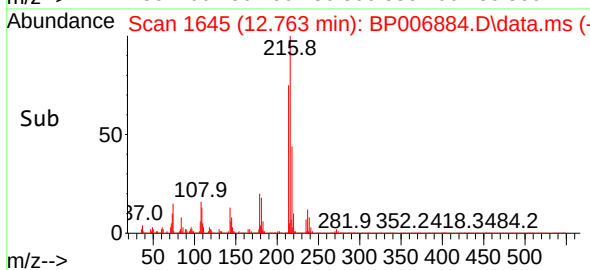
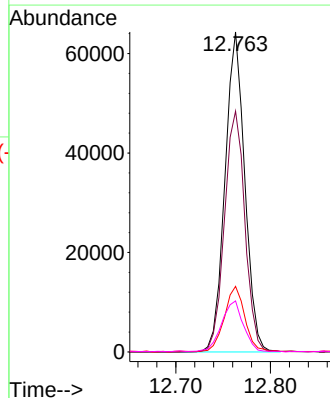
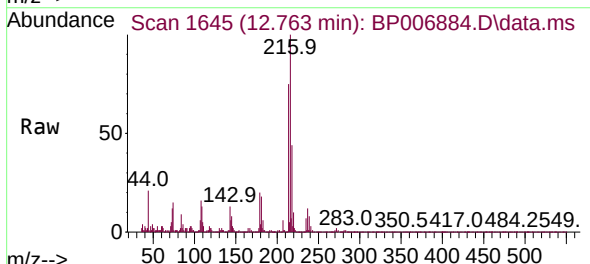




#40
Hexachlorocyclopentadiene
Concen: 4.570 ng/ul
RT: 12.746 min Scan# 1642
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:237 Resp: 53449
Ion Ratio Lower Upper
237 100
235 62.9 50.4 75.6
272 13.8 9.7 14.5

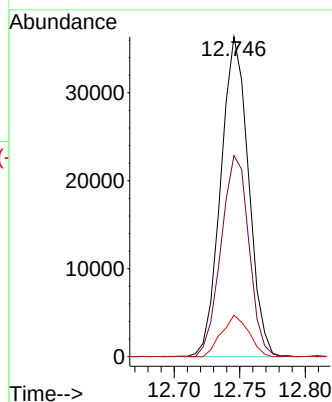

#41
2,4,6-Trichlorophenol
Concen: 3.826 ng/ul
RT: 12.998 min Scan# 1685
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:196 Resp: 46843
Ion Ratio Lower Upper
196 100
198 99.7 76.2 114.4
200 30.5 24.6 36.8









#42
2,4,5-Trichlorophenol
Concen: 4.131 ng/ul
RT: 13.063 min Scan# 1696
Delta R.T. -0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:196 Resp: 53850
Ion Ratio Lower Upper
196 100
198 95.9 79.3 118.9
200 29.7 25.8 38.8

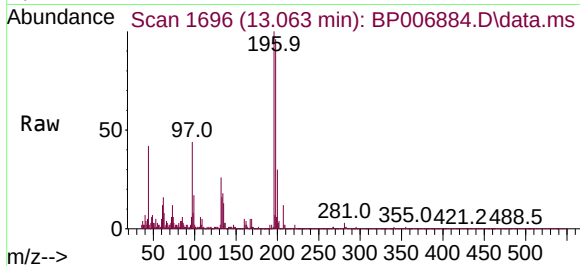

#43
1,1'-Biphenyl
Concen: 4.455 ng/ul
RT: 13.404 min Scan# 1754
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:154 Resp: 229116
Ion Ratio Lower Upper
154 100
153 39.7 32.4 48.6
76 12.4 12.9 19.3#




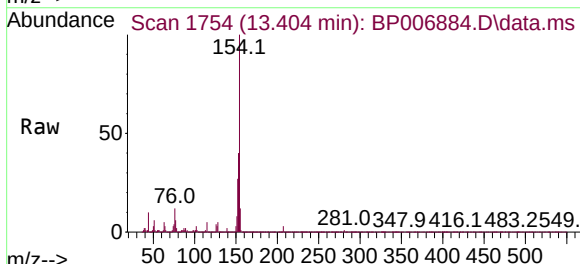




#44
2-Chloronaphthalene
Concen: 4.500 ng/ul
RT: 13.445 min Scan# 1761
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:162 Resp: 175570
Ion Ratio Lower Upper
162 100
164 32.4 25.6 38.4
127 36.7 36.2 54.2



#45
2-Nitroaniline
Concen: 2.014 ng/ul
RT: 13.640 min Scan# 1794
Delta R.T. -0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion: 65 Resp: 28339
Ion Ratio Lower Upper
65 100
92 77.8 53.7 80.5
138 112.5 71.4 107.2#


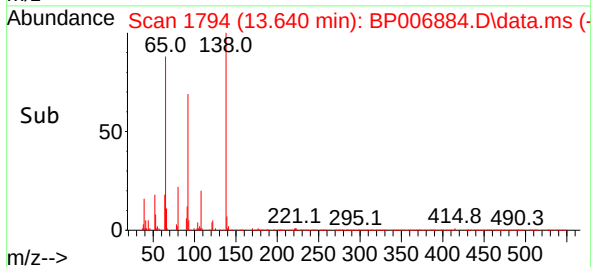

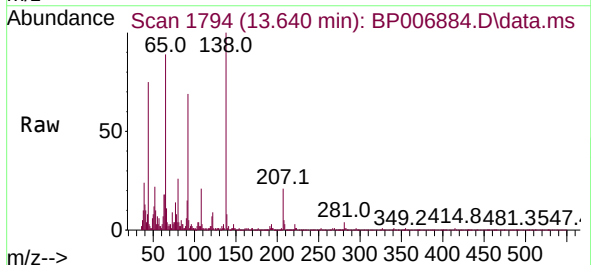




#47
Dimethylphthalate
Concen: 4.203 ng/ul
RT: 14.022 min Scan# 1859
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:163 Resp: 210902
Ion Ratio Lower Upper
163 100
194 4.4 3.0 4.4
164 10.3 7.8 11.8



#48
2,6-Dinitrotoluene
Concen: 2.852 ng/ul
RT: 14.140 min Scan# 1879
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:165 Resp: 27620
Ion Ratio Lower Upper
165 100
89 58.9 62.2 93.2#
121 25.1 22.1 33.1









#50
Acenaphthylene
Concen: 4.387 ng/ul
RT: 14.287 min Scan# 1904
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:152 Resp: 266837
Ion Ratio Lower Upper
152 100
151 19.9 15.9 23.9
153 13.1 10.4 15.6

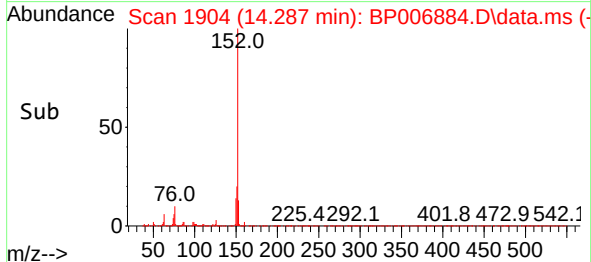

#51
3-Nitroaniline
Concen: 2.366 ng/ul
RT: 14.463 min Scan# 1934
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:138 Resp: 26237
Ion Ratio Lower Upper
138 100
108 19.5 9.7 14.5#
92 121.7 106.7 160.1


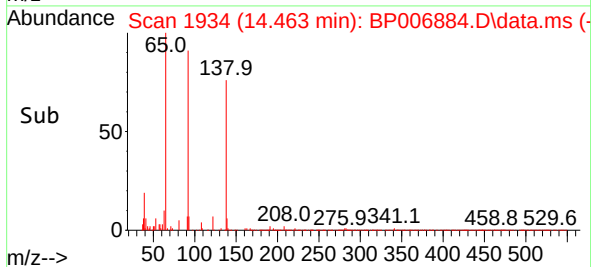

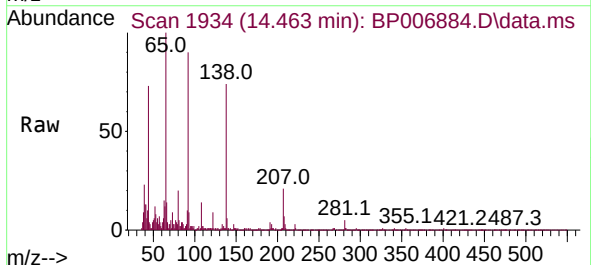




#52
Acenaphthene
Concen: 4.318 ng/ul
RT: 14.628 min Scan# 1962
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:153 Resp: 187282
Ion Ratio Lower Upper
153 100
152 47.4 38.6 57.8
154 88.3 69.0 103.6



#53
2,4-Dinitrophenol
Concen: 1.380 ng/ul
RT: 14.669 min Scan# 1969
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:184 Resp: 8647
Ion Ratio Lower Upper
184 100
63 66.1 73.4 110.2#
154 55.9 59.4 89.0#



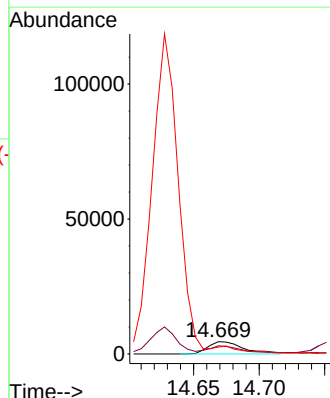



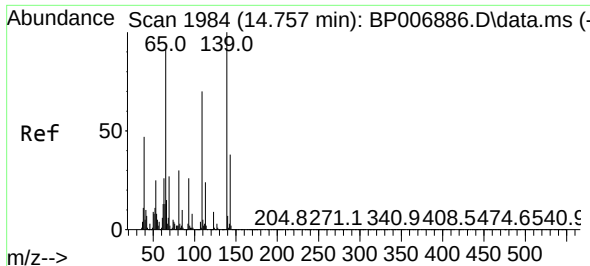

#55
4-Nitrophenol
Concen: 1.951 ng/ul
RT: 14.757 min Scan# 1984
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:109 Resp: 18538
Ion Ratio Lower Upper
109 100
139 137.6 90.3 135.5#
65 125.6 102.2 153.2

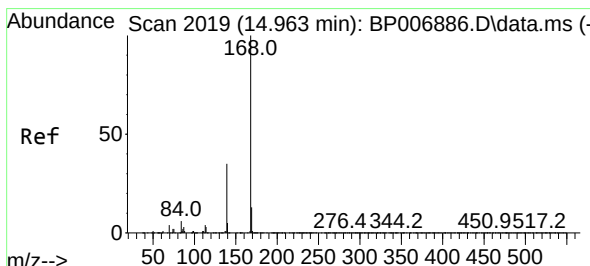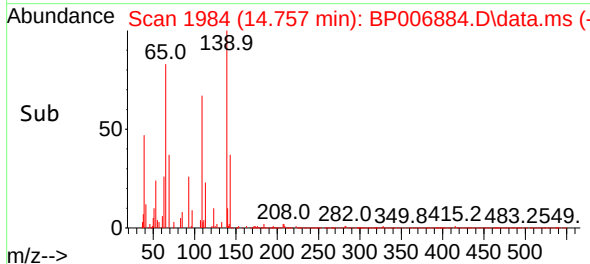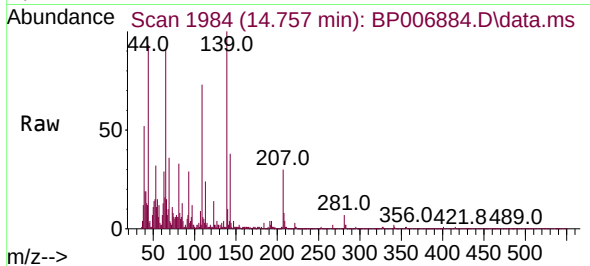

#56
Dibenzofuran
Concen: 4.625 ng/ul
RT: 14.963 min Scan# 2019
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:168 Resp: 268217
Ion Ratio Lower Upper
168 100
139 34.6 35.3 52.9#


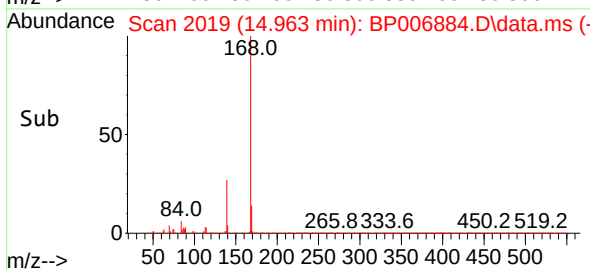

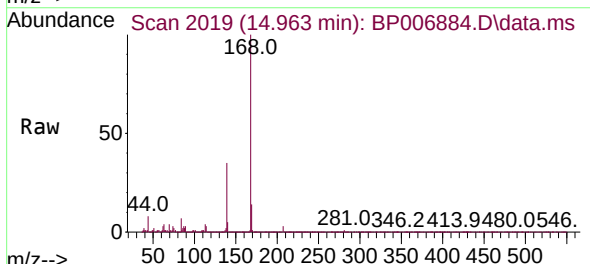




#57
2,4-Dinitrotoluene
Concen: 2.690 ng/ul
RT: 14.922 min Scan# 2012
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:165 Resp: 38325
Ion Ratio Lower Upper
165 100
63 38.8 45.2 67.8#
182 1.9 1.9 2.9#



#58
2,3,4,6-Tetrachlorophenol
Concen: 3.989 ng/ul
RT: 15.187 min Scan# 2057
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:232 Resp: 43159
Ion Ratio Lower Upper
232 100
131 43.3 51.8 77.6#
130 1.8 3.1 4.7#
166 29.4 31.0 46.4#









#59
Diethylphthalate
Concen: 3.807 ng/ul
RT: 15.387 min Scan# 2091
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:149 Resp: 203051
Ion Ratio Lower Upper
149 100
177 22.7 15.5 23.3
150 12.3 9.9 14.9



#61
Fluorene
Concen: 4.485 ng/ul
RT: 15.610 min Scan# 2129
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:166 Resp: 216849
Ion Ratio Lower Upper
166 100
165 97.4 79.6 119.4
167 13.7 10.7 16.1









#62
4-Chlorophenyl-phenylether
Concen: 5.042 ng/ul
RT: 15.610 min Scan# 2129
Delta R.T. 0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:204 Resp: 110371
Ion Ratio Lower Upper
204 100
206 32.8 26.3 39.5
141 55.5 62.0 93.0#



#63
4-Nitroaniline
Concen: 2.271 ng/ul
RT: 15.622 min Scan# 2131
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:138 Resp: 23589
Ion Ratio Lower Upper
138 100
92 50.9 47.1 70.7
108 79.2 73.8 110.8



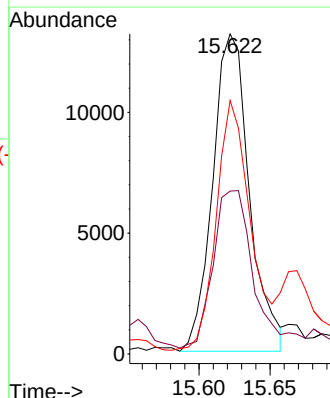





#66
4,6-Dinitro-2-methylphenol
Concen: 1.847 ng/ul
RT: 15.681 min Scan# 2141
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:198 Resp: 17201
Ion Ratio Lower Upper
198 100
182 8.7 4.5 6.7#
77 34.8 31.7 47.5

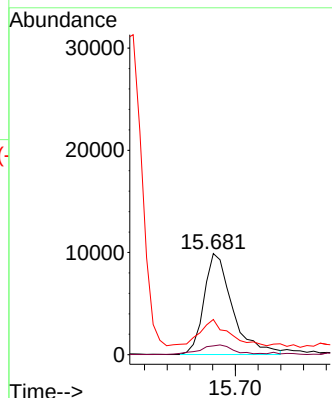

#67
N-Nitrosodiphenylamine
Concen: 4.143 ng/ul
RT: 15.822 min Scan# 2165
Delta R.T. 0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:169 Resp: 179365
Ion Ratio Lower Upper
169 100
168 66.8 53.9 80.9
167 35.7 30.0 45.0



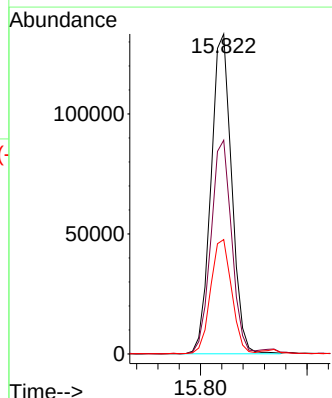



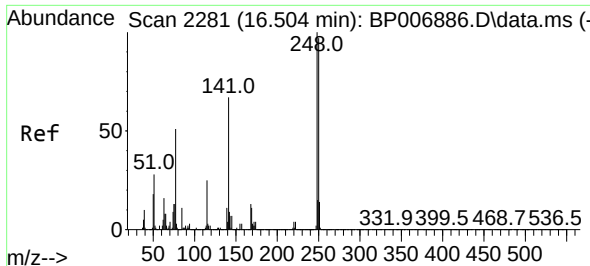

#68
4-Bromophenyl-phenylether
Concen: 4.557 ng/ul
RT: 16.504 min Scan# 2281
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:248 Resp: 63335
Ion Ratio Lower Upper
248 100
250 97.6 78.4 117.6
141 73.1 80.6 121.0#

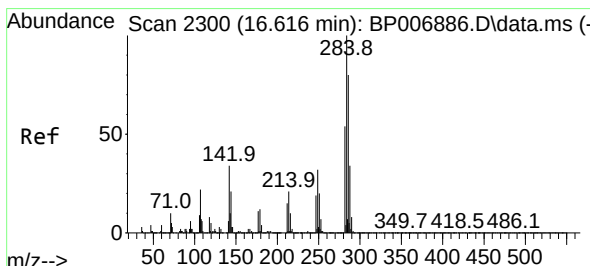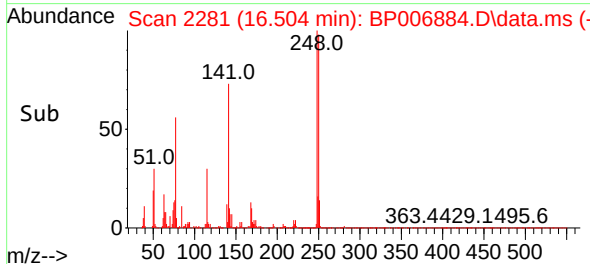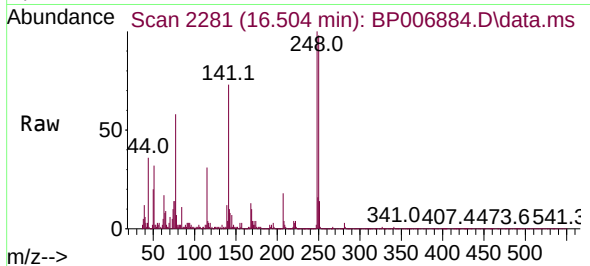

#69
Hexachlorobenzene
Concen: 0.007 ng/ul
RT: 16.581 min Scan# 2294
Delta R.T. -0.035 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:284 Resp: 114
Ion Ratio Lower Upper
284 100
142 53.8 37.8 56.6
249 35.3 27.1 40.7


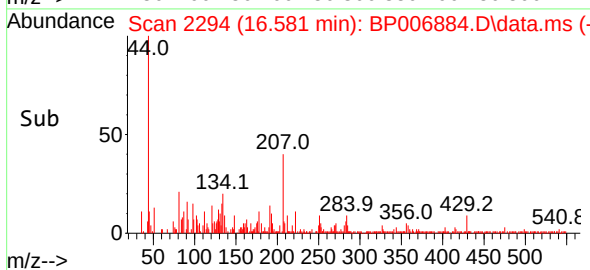

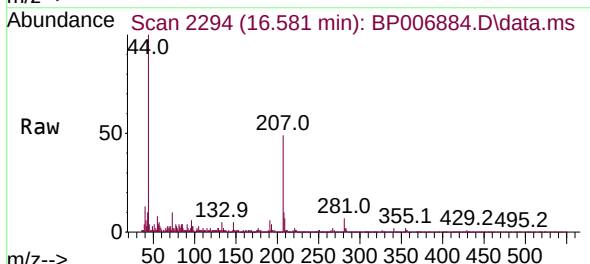




#70
Atrazine
Concen: 3.932 ng/ul
RT: 16.775 min Scan# 2327
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:200 Resp: 60391
Ion Ratio Lower Upper
200 100
173 24.6 22.2 33.4
215 48.8 35.4 53.0

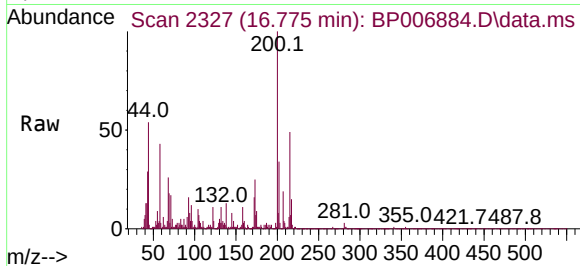

#71
Pentachlorophenol
Concen: 2.917 ng/ul
RT: 16.963 min Scan# 2359
Delta R.T. 0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:266 Resp: 30016
Ion Ratio Lower Upper
266 100
264 61.8 51.0 76.4
268 59.5 49.4 74.2




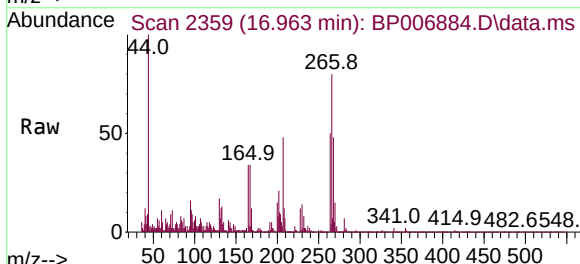


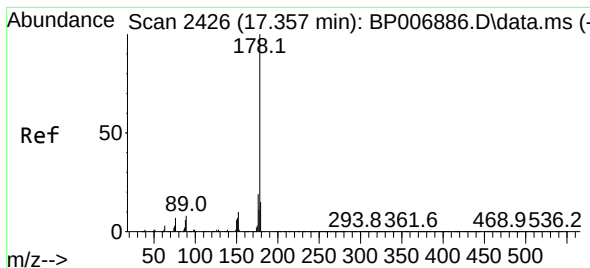

#72
Phenanthrene
Concen: 4.450 ng/ul
RT: 17.357 min Scan# 2426
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:178 Resp: 354325
Ion Ratio Lower Upper
178 100
179 14.6 12.0 18.0
176 19.6 15.6 23.4

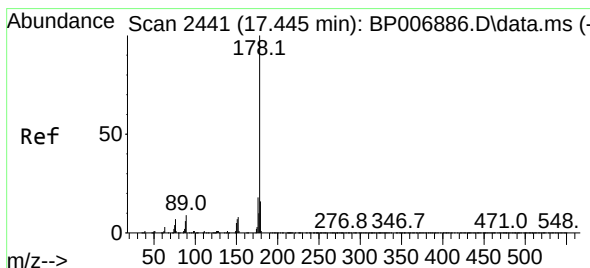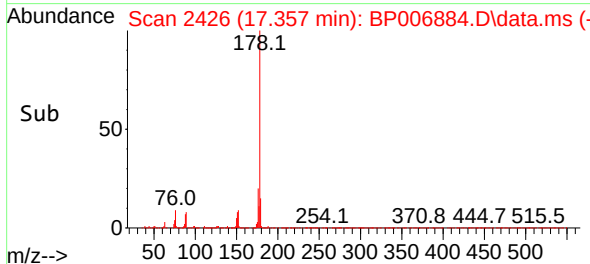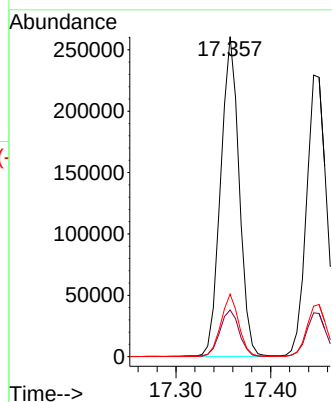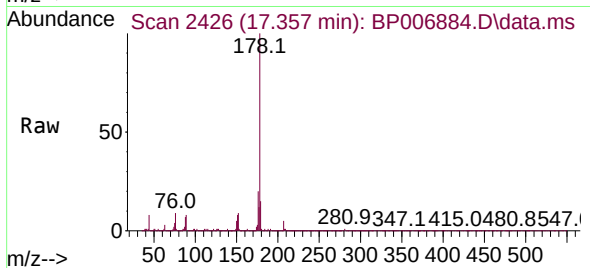

#74
Anthracene
Concen: 4.230 ng/ul
RT: 17.445 min Scan# 2441
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:178 Resp: 342021
Ion Ratio Lower Upper
178 100
179 15.6 12.1 18.1
176 17.9 14.9 22.3


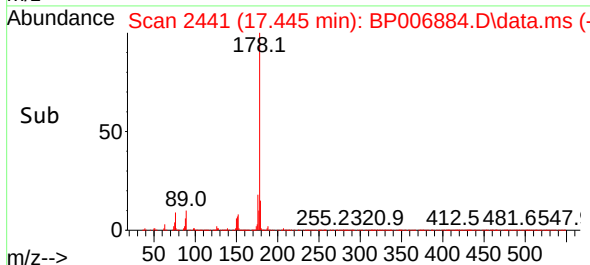

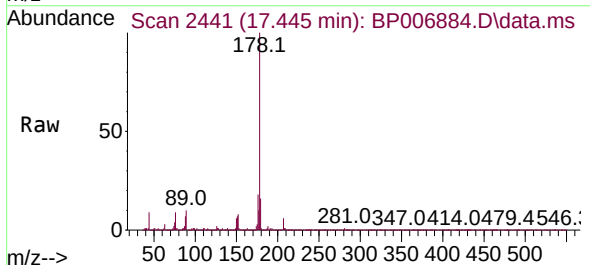




#75
1,2,3,4-Tetrachlorobenzene
Concen: 5.022 ng/uL
RT: 13.369 min Scan# 1748
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:216 Resp: 96240
Ion Ratio Lower Upper
216 100
214 77.3 62.9 94.3
218 47.9 37.8 56.8



#76
Pentachlorobenzene
Concen: 5.026 ng/uL
RT: 14.887 min Scan# 2006
Delta R.T. 0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:250 Resp: 94894
Ion Ratio Lower Upper
250 100
248 63.8 51.0 76.6
252 61.4 51.0 76.4



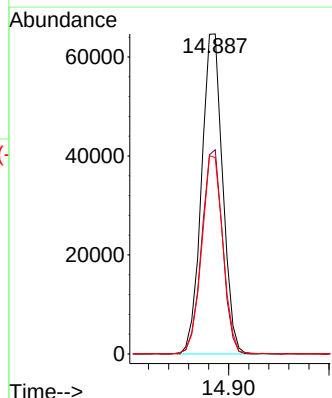





#77
 Carbazole
 Concen: 3.863 ng/ul
 RT: 17.716 min Scan# 2487
 Delta R.T. 0.000 min
 Lab File: BP006884.D
 Acq: 08 Sep 2021 15:50




Instrument :
 BNA_P
 ClientSampleId :
 SST005615


Tgt Ion:	167	Resp:	291693
Ion Ratio	Lower	Upper	
167	100		
166	21.5	17.6	26.4
139	12.8	11.9	17.9



#78
 Di-n-butylphthalate
 Concen: 3.370 ng/ul
 RT: 18.275 min Scan# 2582
 Delta R.T. 0.006 min
 Lab File: BP006884.D
 Acq: 08 Sep 2021 15:50

Tgt Ion:	149	Resp:	329071
Ion Ratio	Lower	Upper	
149	100		
150	8.9	7.3	10.9
104	5.0	4.8	7.2









#80
Fluoranthene
Concen: 4.327 ng/ul
RT: 19.322 min Scan# 2760
Delta R.T. 0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:202 Resp: 410745
Ion Ratio Lower Upper
202 100
101 11.3 11.0 16.4
100 8.6 8.3 12.5

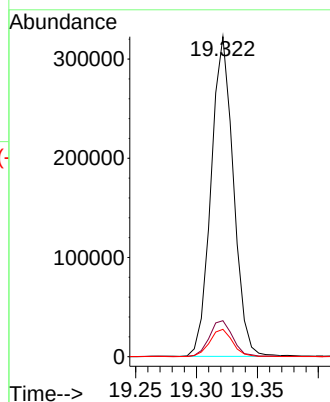

#82
Pyrene
Concen: 4.406 ng/ul
RT: 19.675 min Scan# 2820
Delta R.T. 0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:202 Resp: 432043
Ion Ratio Lower Upper
202 100
101 13.1 12.6 19.0
100 10.9 10.6 15.8









#83
Butylbenzylphthalate
Concen: 2.586 ng/ul
RT: 20.551 min Scan# 2969
Delta R.T. 0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:149 Resp: 125348
Ion Ratio Lower Upper
149 100
91 67.0 63.0 94.6
206 22.8 14.1 21.1#

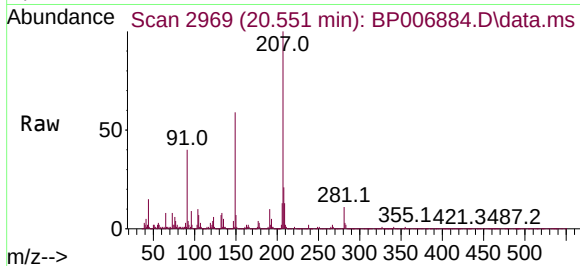

#84
3,3'-Dichlorobenzidine
Concen: 3.177 ng/ul
RT: 21.316 min Scan# 3099
Delta R.T. 0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:252 Resp: 104292
Ion Ratio Lower Upper
252 100
254 64.0 51.6 77.4
126 12.3 10.7 16.1



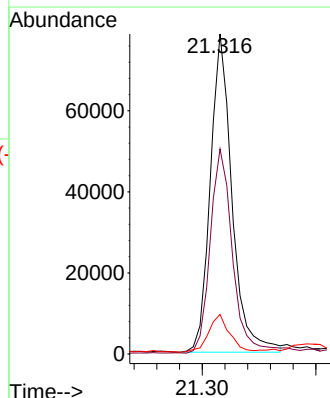
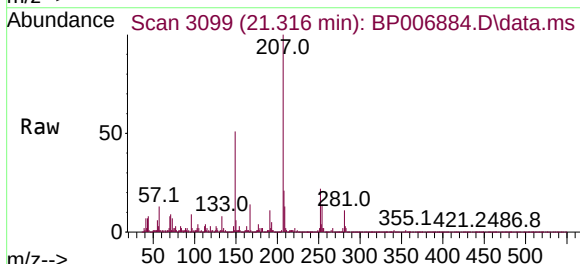




#85
Benzo(a)anthracene
Concen: 4.346 ng/ul
RT: 21.386 min Scan# 3111
Delta R.T. 0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:228 Resp: 407204
Ion Ratio Lower Upper
228 100
229 18.8 15.8 23.8
226 26.3 21.6 32.4

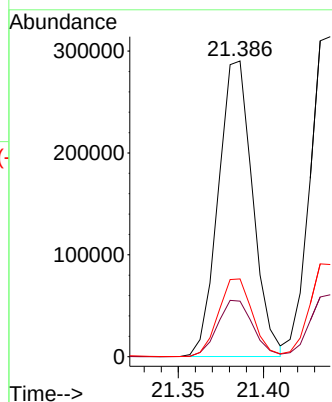

#86
Bis(2-ethylhexyl)phthalate
Concen: 2.613 ng/ul
RT: 21.316 min Scan# 3099
Delta R.T. 0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:149 Resp: 195159
Ion Ratio Lower Upper
149 100
167 27.4 20.2 30.2
279 4.5 2.7 4.1#









#87
Chrysene
Concen: 4.628 ng/ul
RT: 21.439 min Scan# 3120
Delta R.T. 0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:228 Resp: 418068
Ion Ratio Lower Upper
228 100
226 28.8 24.5 36.7
229 19.4 15.9 23.9

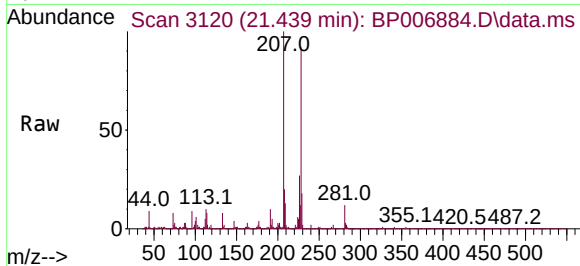

#89
Di-n-octyl phthalate
Concen: 2.422 ng/ul
RT: 22.251 min Scan# 3258
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:149 Resp: 312302




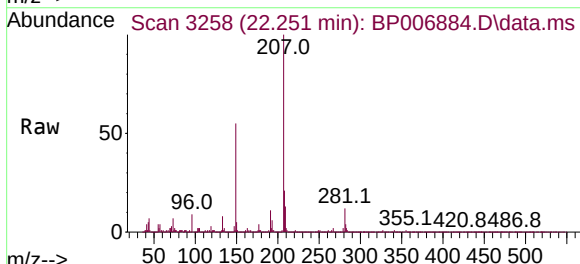




#90
Benzo(b)fluoranthene
Concen: 4.286 ng/ul
RT: 23.092 min Scan# 3401
Delta R.T. 0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:252 Resp: 415390
Ion Ratio Lower Upper
252 100
253 22.9 17.7 26.5
125 10.7 10.1 15.1



#91
Benzo(k)fluoranthene
Concen: 4.246 ng/ul
RT: 23.139 min Scan# 3409
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:252 Resp: 398421
Ion Ratio Lower Upper
252 100
253 21.3 17.2 25.8
125 11.2 9.4 14.0









#93
Benzo(a)pyrene
Concen: 4.483 ng/ul
RT: 23.727 min Scan# 3509
Delta R.T. 0.000 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50




Instrument :
BNA_P
ClientSampleId :
SSTD005615


Tgt Ion:252 Resp: 393544
Ion Ratio Lower Upper
252 100
253 22.4 17.6 26.4
125 12.2 11.3 16.9



#94
Indeno(1,2,3-cd)pyrene
Concen: 3.881 ng/ul
RT: 26.392 min Scan# 3962
Delta R.T. 0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:276 Resp: 445465
Ion Ratio Lower Upper
276 100
138 24.5 21.8 32.8
277 24.5 19.9 29.9









#95
Dibenzo(a,h)anthracene
Concen: 4.011 ng/ul
RT: 26.415 min Scan# 3966
Delta R.T. 0.012 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Instrument :
BNA_P
ClientSampleId :
SSTD005615

Tgt Ion:278 Resp: 386747
Ion Ratio Lower Upper
278 100
139 16.3 15.4 23.2
279 23.5 19.0 28.4

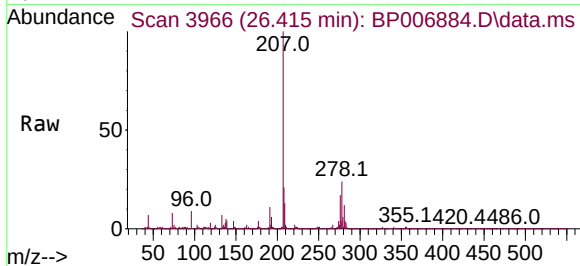

#96
Benzo(g,h,i)perylene
Concen: 4.052 ng/ul
RT: 27.174 min Scan# 4095
Delta R.T. 0.006 min
Lab File: BP006884.D
Acq: 08 Sep 2021 15:50

Tgt Ion:276 Resp: 386211
Ion Ratio Lower Upper
276 100
138 23.2 20.7 31.1
277 24.2 19.0 28.4

