
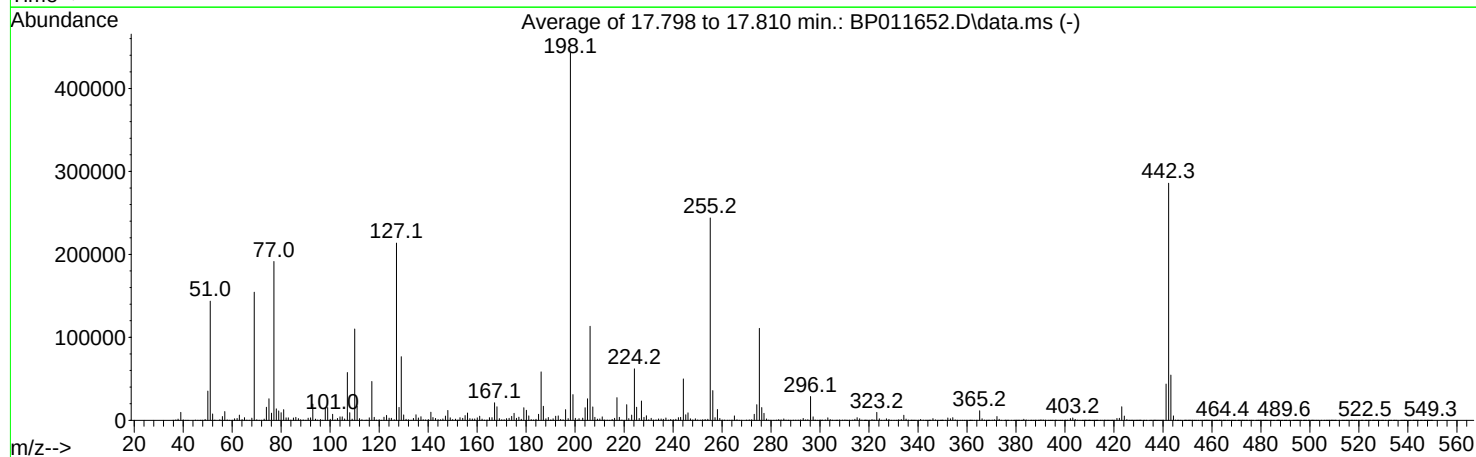


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090822\
 Data File : BP011652.D
 Acq On : 08 Sep 2022 10:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 03 04:07:09 2022

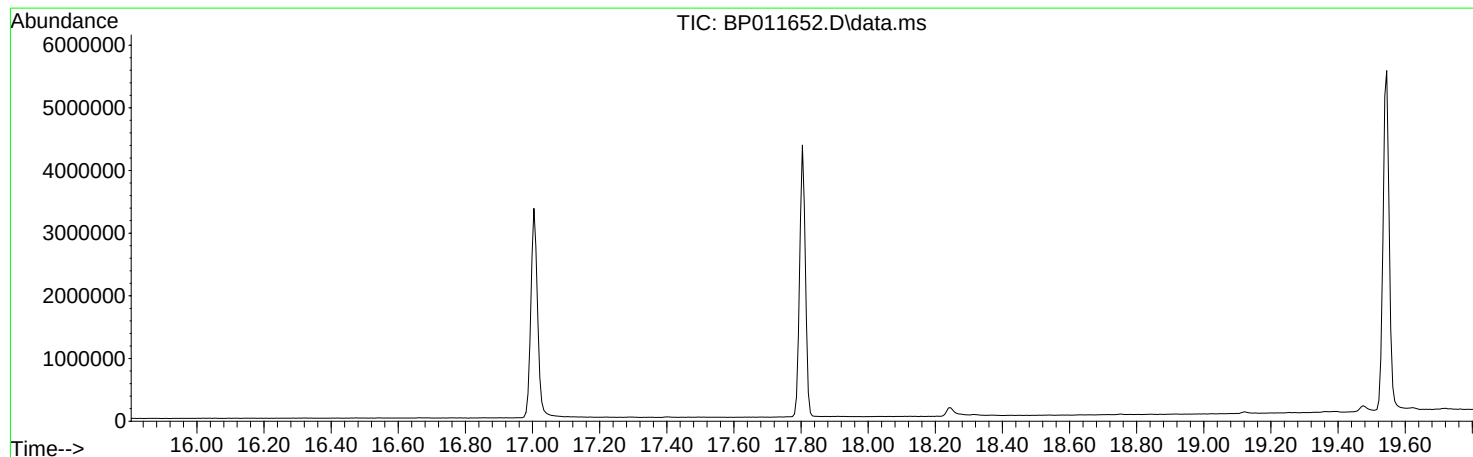




AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	143645	PASS
68	69	0.00	2	1.7	2604	PASS
69	198	0.00	100	34.8	154402	PASS
70	69	0.00	2	0.5	766	PASS
127	198	10	80	48.2	213589	PASS
197	198	0.00	2	0.5	2030	PASS
198	198	100	100	100.0	443413	PASS
199	198	5	9	7.0	30912	PASS
275	198	10	60	25.0	110856	PASS
365	198	1	100	2.6	11463	PASS
441	198	0.01	100	9.9	43789	PASS
442	442	100	100	100.0	285824	PASS
443	442	15	24	19.1	54589	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090822\
 Data File : BP011652.D
 Acq On : 08 Sep 2022 10:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 09 06:02:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 03 04:07:09 2022
 Response via : Initial Calibration

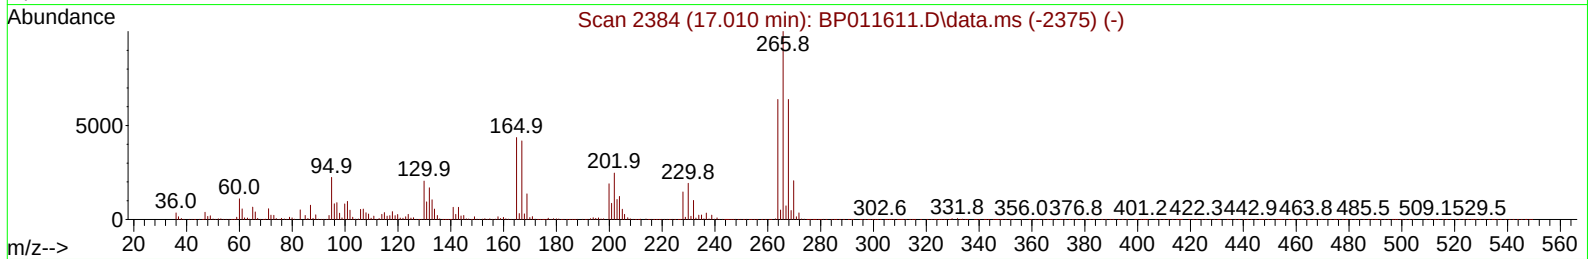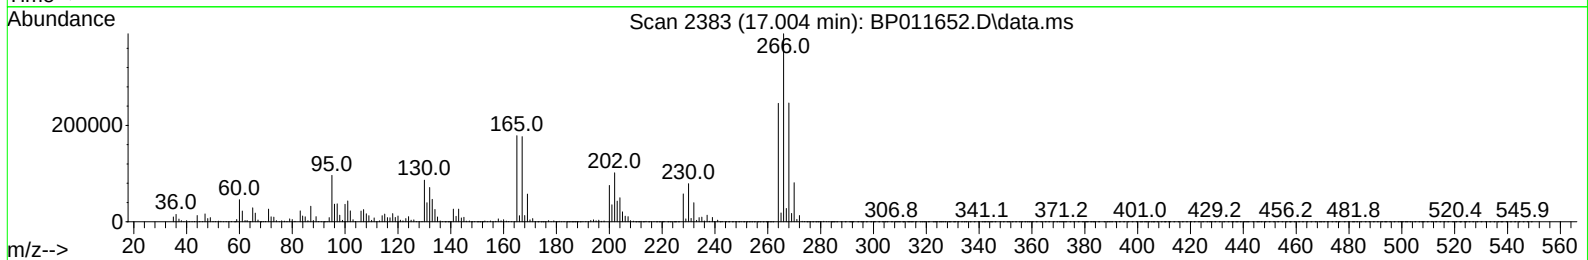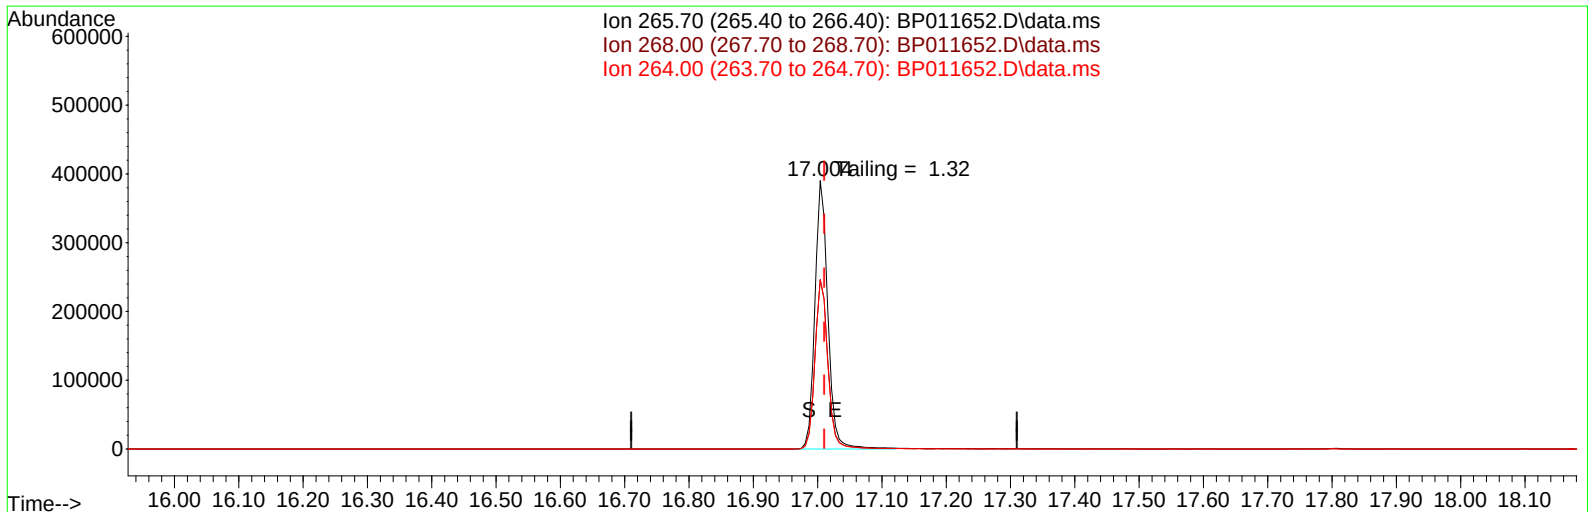

TIC: BP011652.D\data.ms

(70) Pentachlorophenol (C)

17.004min (-0.006) 204262.90 ng




response 552559

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.13
264.00	63.00	63.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090822\
Data File : BP011652.D
Acq On : 08 Sep 2022 10:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 09 06:02:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 03 04:07:09 2022
Response via : Initial Calibration

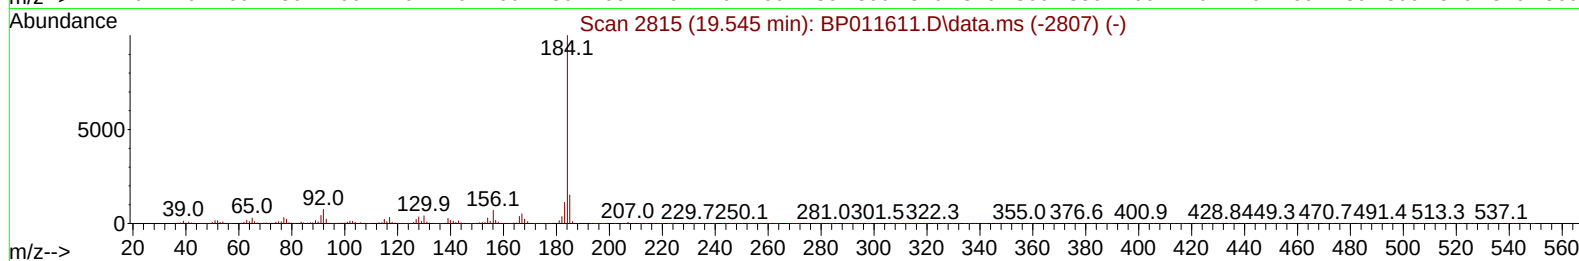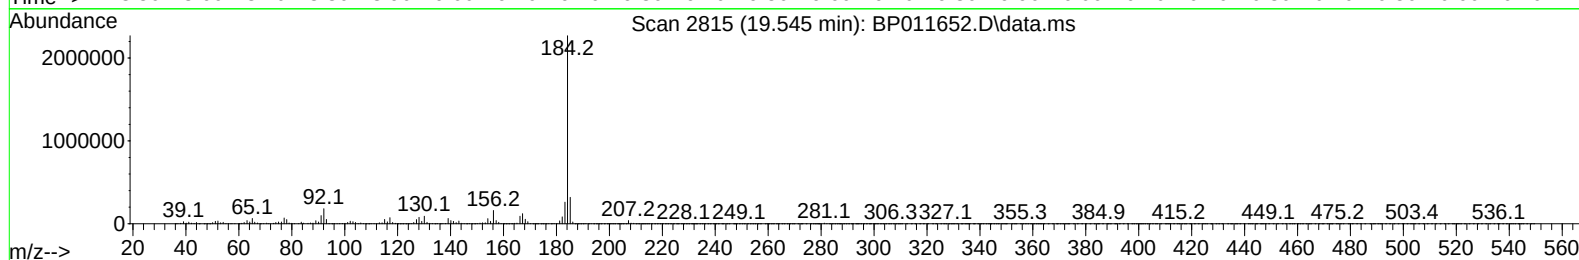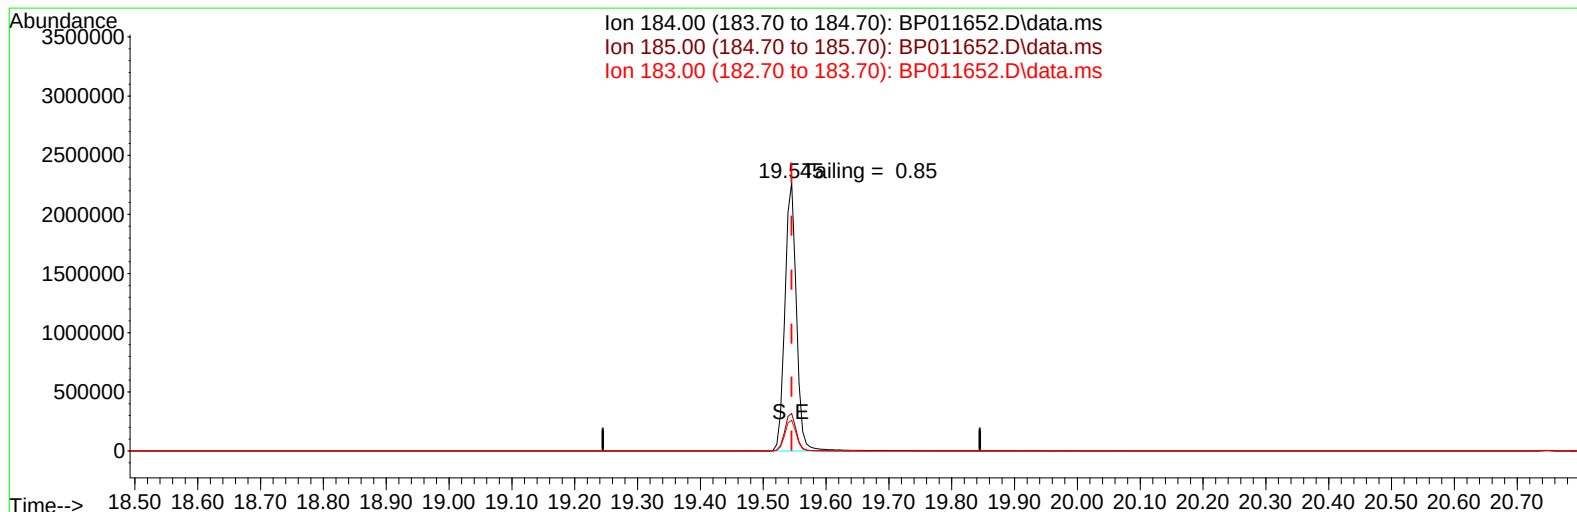

TIC: BP011652.D\data.ms

(77) Benzidine

19.545min (-0.000) 756843.26 ng

response 2907739

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.03
183.00	11.30	11.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/8/2022	BNA_P	<u>BP011652.D</u>
Compound Name	Response	Retention Time
DDT	1323534	20.751
DDD	10948	20.316
DDE	725	19.828
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11673	1335207	0.87

Instrument :
BNA_P
ClientSampleId :
DFTPP