
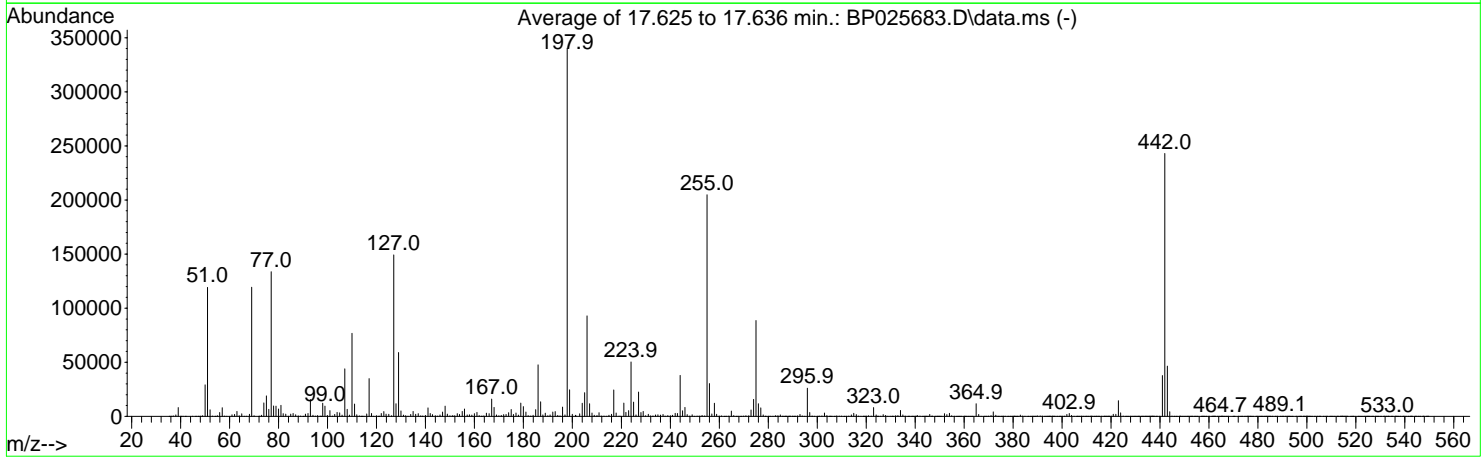


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090825\
 Data File : BP025683.D
 Acq On : 08 Sep 2025 14:01
 Operator : CG/JU
 Sample : DFTPP627
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
ClientSampleId :
 DFTPP627

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090825.MA.M
 Title : SVOA CALIBRATION
 Last Update : Tue Sep 09 09:26:50 2025

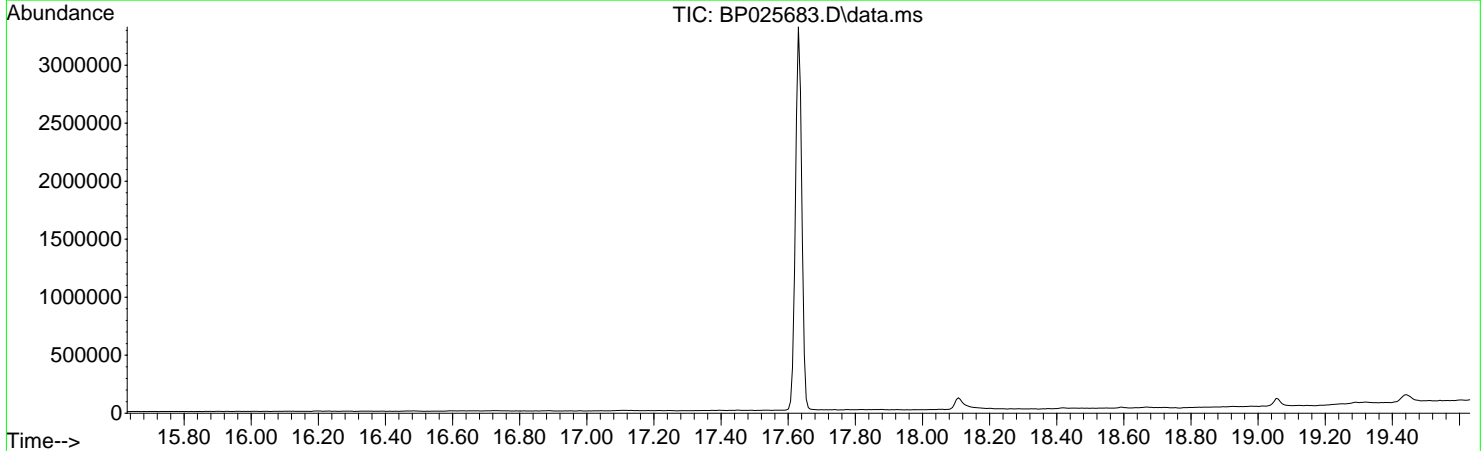

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	119217	PASS
68	69	0.00	2	1.6	1892	PASS
69	198	0.00	100	35.1	119407	PASS
70	69	0.00	2	0.5	643	PASS
127	198	10	80	43.9	149256	PASS
197	198	0.00	2	0.4	1421	PASS
198	198	100	100	100.0	340037	PASS
199	198	5	9	7.2	24504	PASS
275	198	10	60	26.0	88570	PASS
365	198	1	100	3.5	11763	PASS
441	198	0.01	100	11.1	37697	PASS
442	198	50	100	71.4	242944	PASS
443	442	15	24	19.1	46485	PASS