
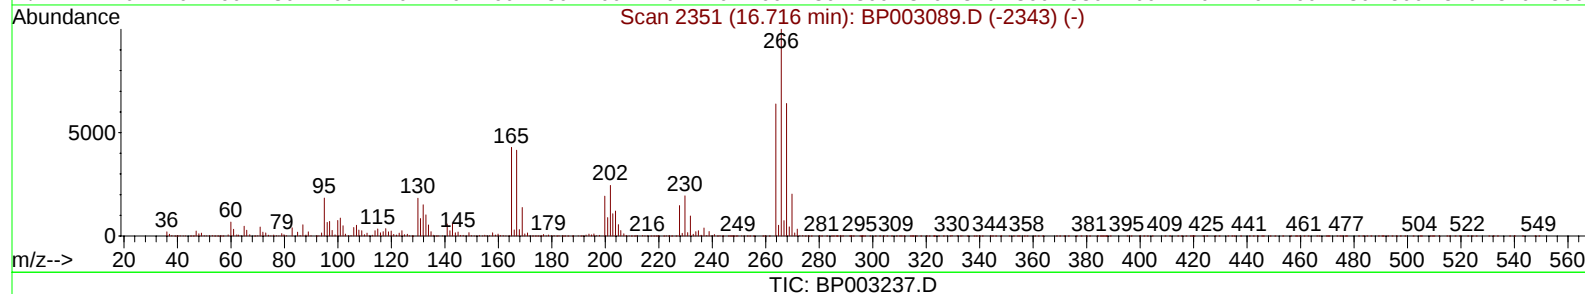
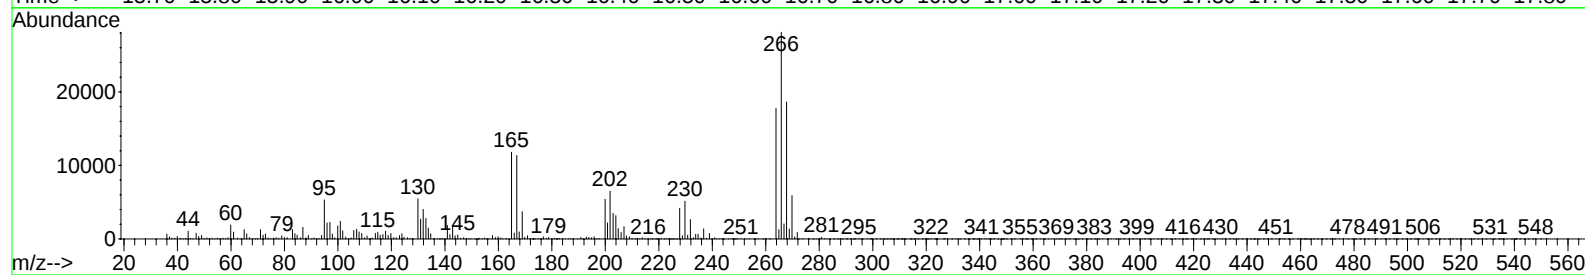


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP090920\
Data File : BP003237.D
Acq On : 09 Sep 2020 12:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 16:58:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 01 14:37:05 2020
Response via : Initial Calibration

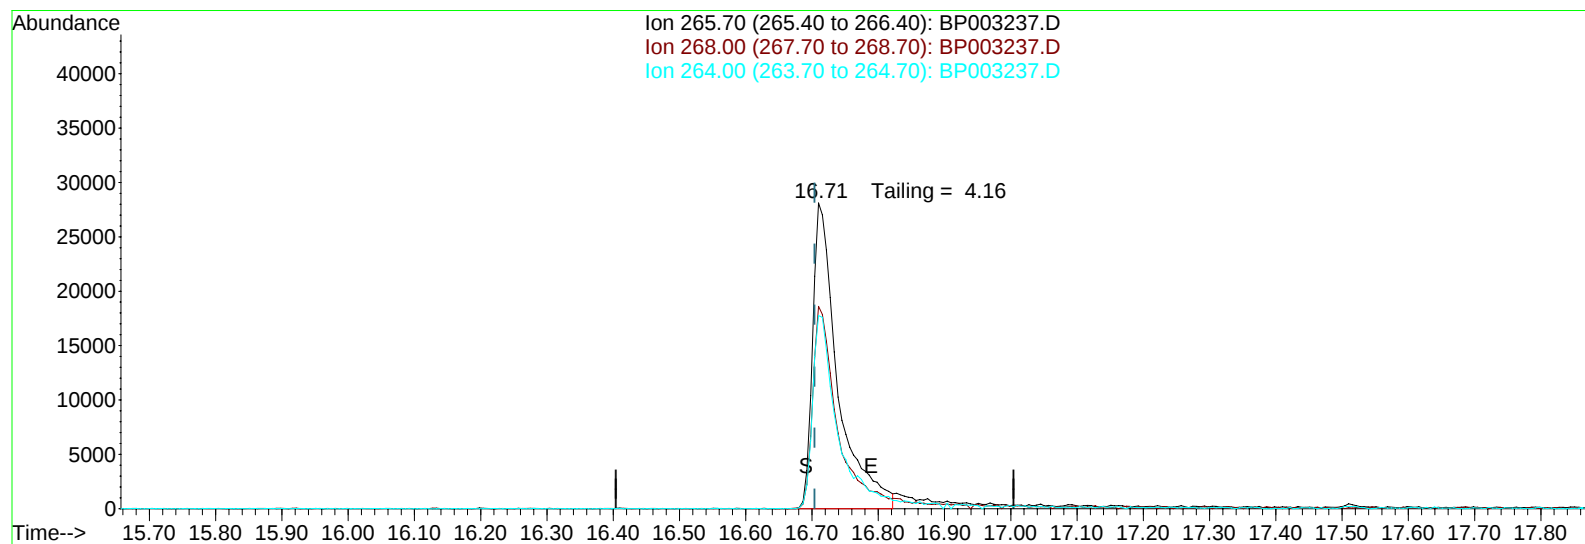

(70) Pentachlorophenol (C)




16.710min (+0.006) 205455.35ng

response 77457

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.22
264.00	63.30	63.15
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP090920\
 Data File : BP003237.D
 Acq On : 09 Sep 2020 12:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 16:58:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 01 14:37:05 2020
 Response via : Initial Calibration

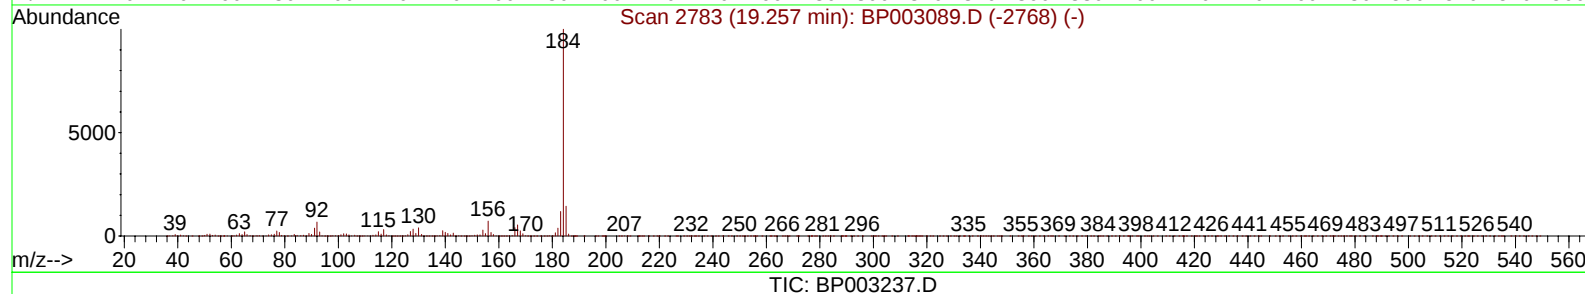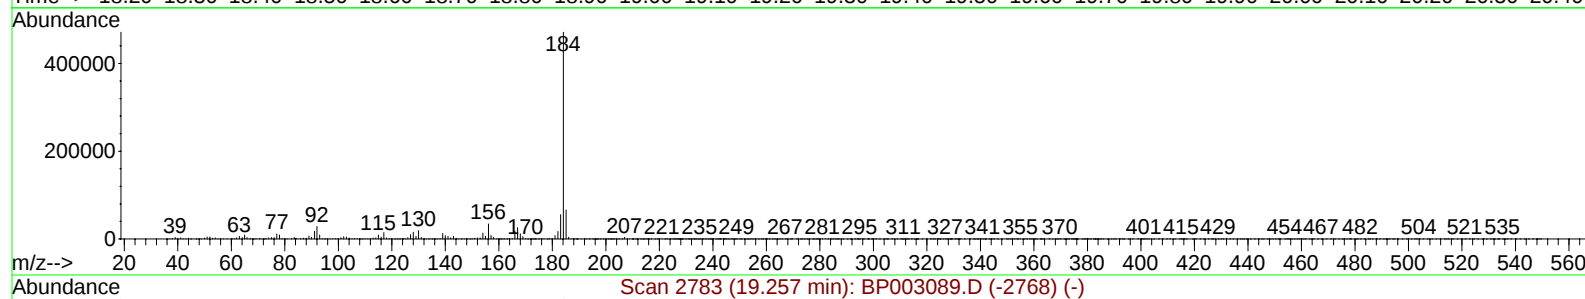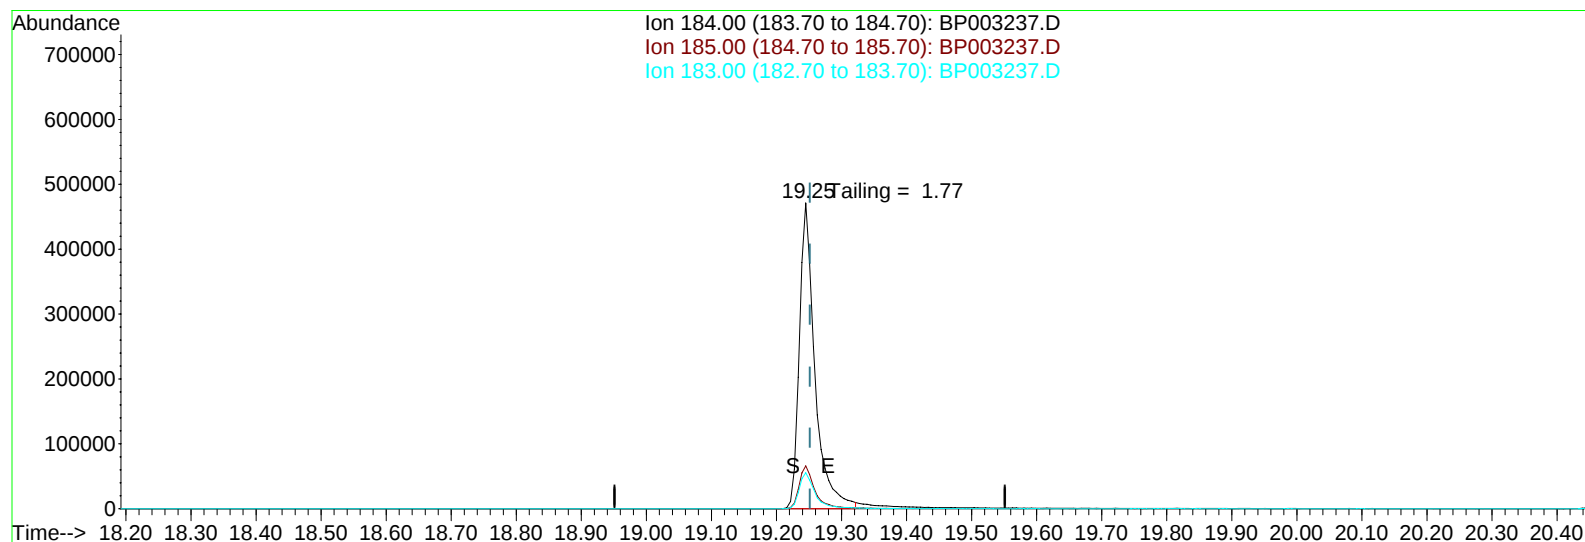

TIC: BP003237.D

(77) Benzidine

19.245min (-0.006) 54314.98ng

response 813095

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.01
183.00	12.00	11.80
0.00	0.00	0.00