


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP090920\
 Data File : BP003237.D
 Acq On : 09 Sep 2020 12:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 01 14:37:05 2020

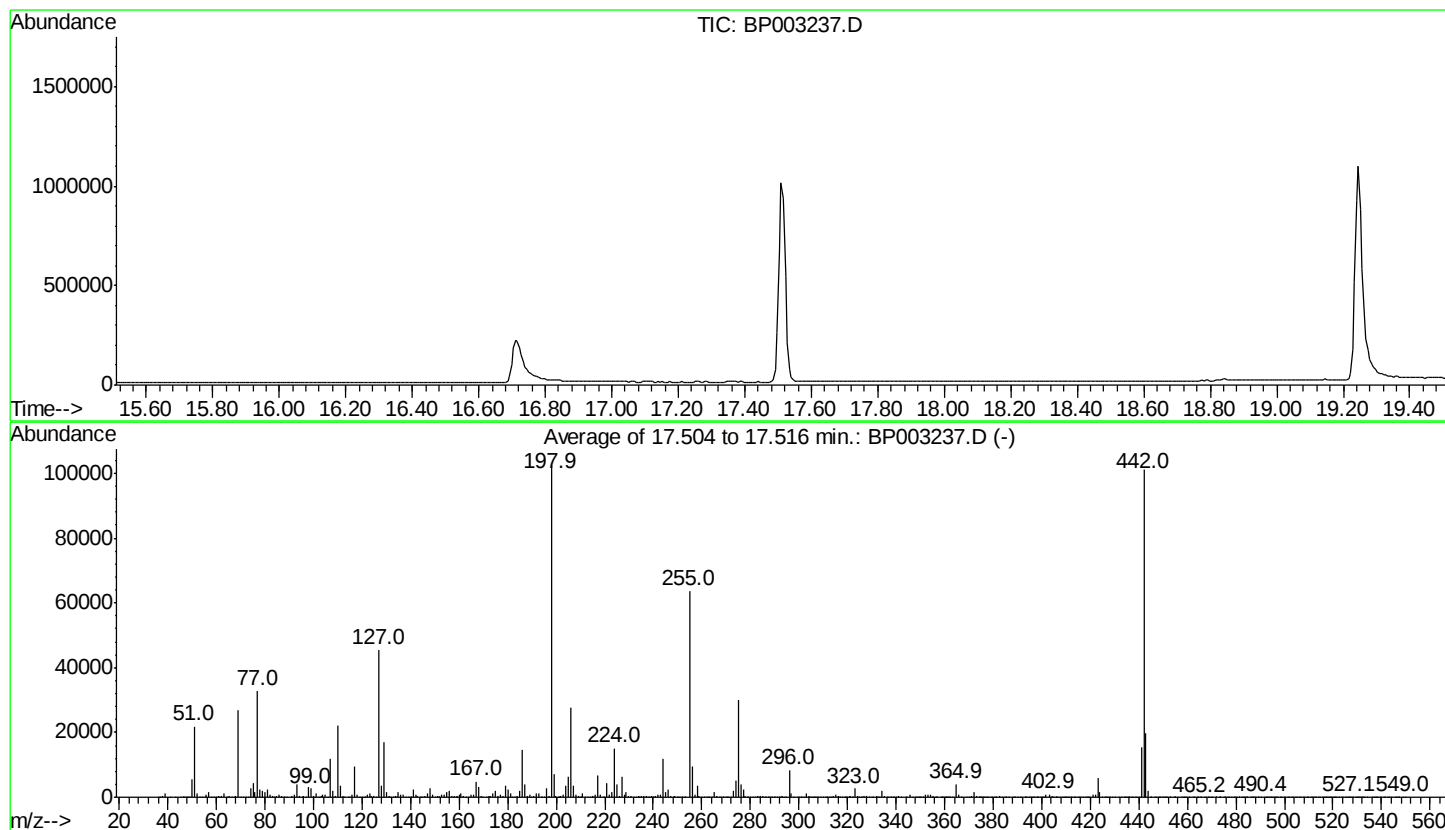

Spectrum Information: Average of 17.504 to 17.516 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.2	21732	PASS
68	69	0.00	2	1.9	505	PASS
69	198	0.00	100	26.2	26779	PASS
70	69	0.00	2	0.5	147	PASS
127	198	10	80	44.4	45488	PASS
197	198	0.00	2	0.2	249	PASS
198	198	100	100	100.0	102349	PASS
199	198	5	9	6.8	6985	PASS
275	198	10	60	29.4	30066	PASS
365	198	1	100	4.0	4110	PASS
441	198	0.01	100	15.0	15327	PASS
442	198	50	100	98.7	100984	PASS
443	442	15	24	19.5	19710	PASS