
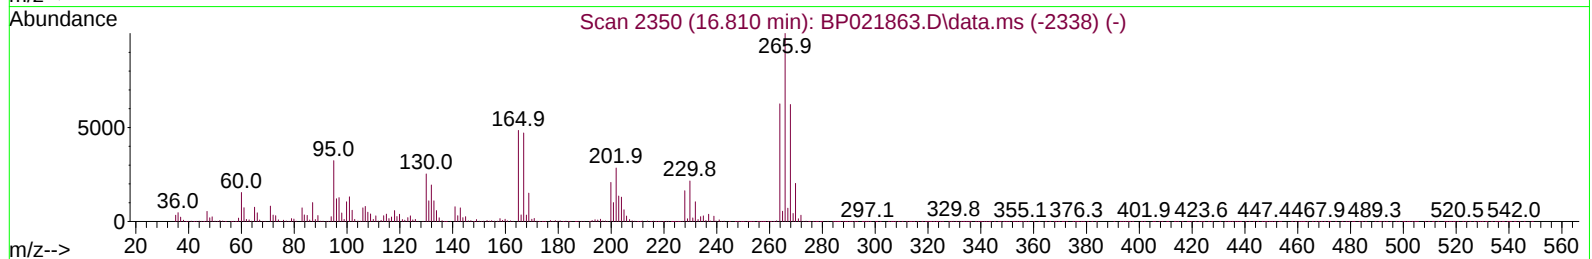
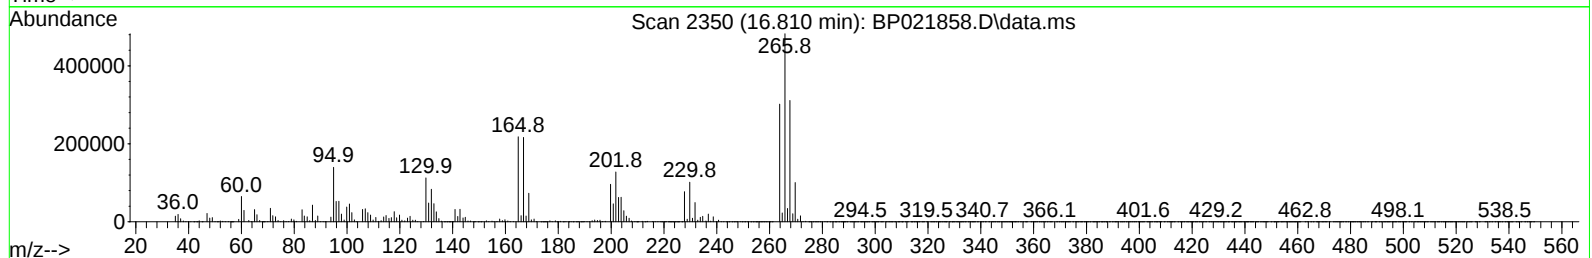


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP090924\  
Data File : BP021858.D  
Acq On : 09 Sep 2024 08:43  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 00:17:34 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP090924.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 10 00:09:47 2024  
Response via : Initial Calibration

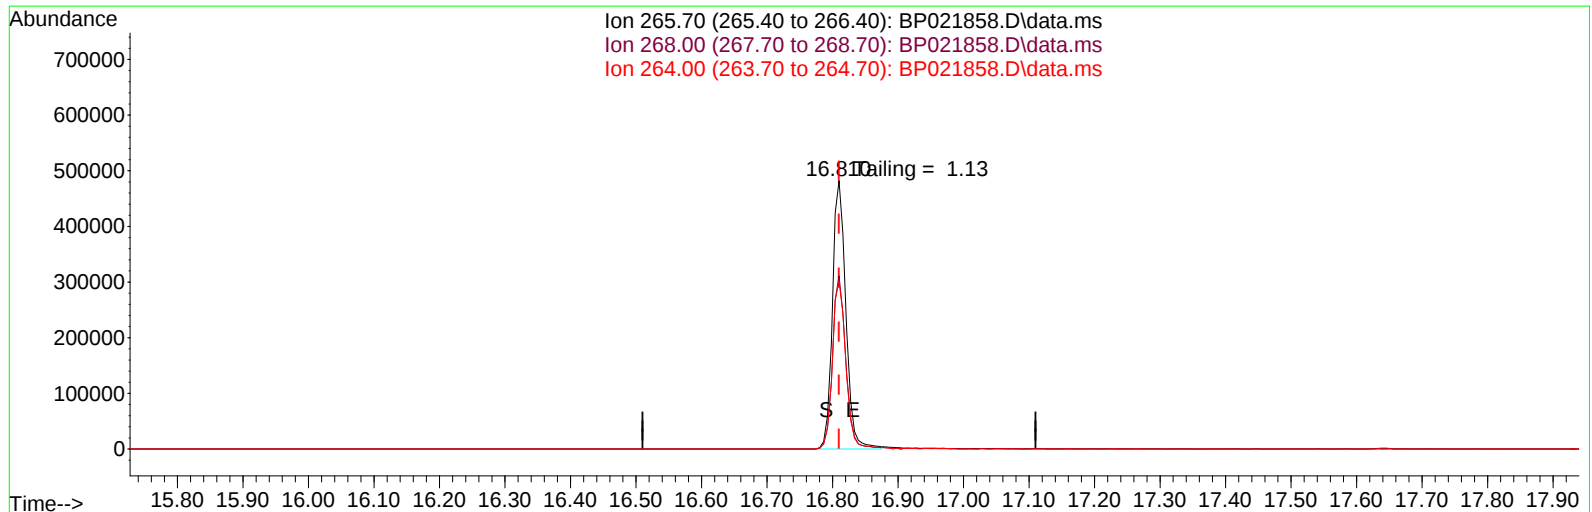

TIC: BP021858.D\data.ms

**(70) Pentachlorophenol (C)**




**16.810min (-0.000) 221230.16 ng**

**response 695170**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 64.49  |
| 264.00 | 62.50  | 62.54  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP090924\  
Data File : BP021858.D  
Acq On : 09 Sep 2024 08:43  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 00:17:34 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP090924.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 10 00:09:47 2024  
Response via : Initial Calibration

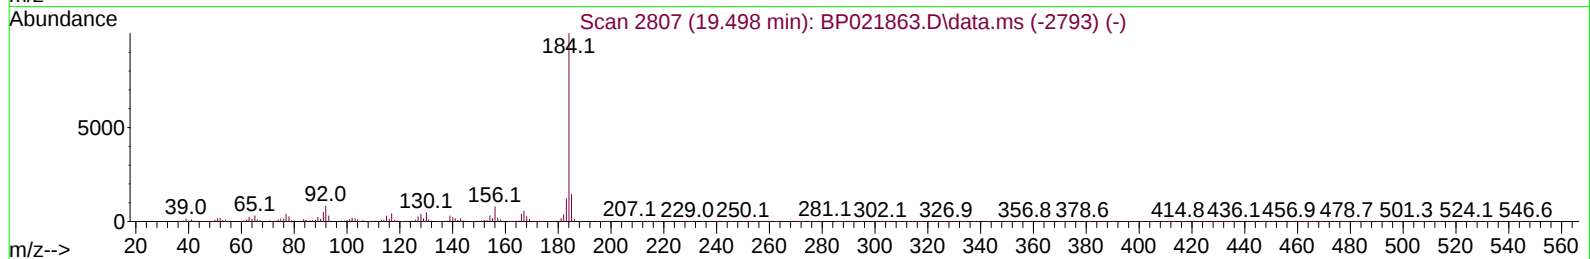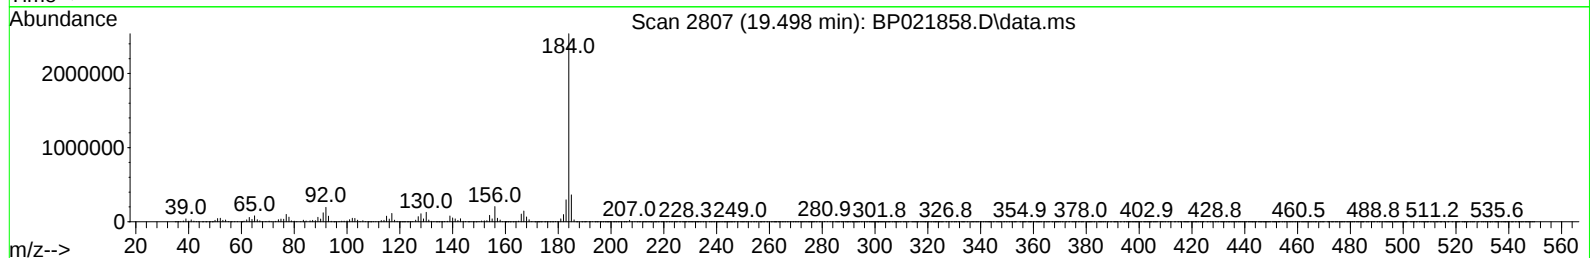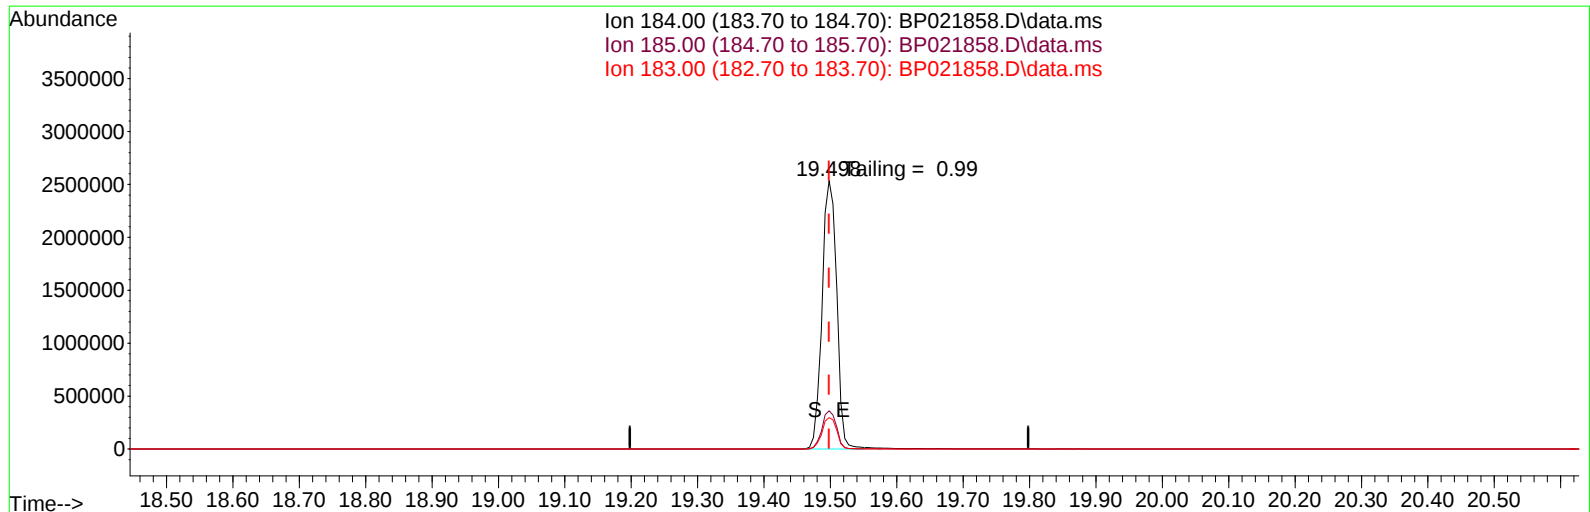

TIC: BP021858.D\data.ms

**(77) Benzidine****19.498min (-0.000) 140895.36 ng****response 3898830**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 14.28  |
| 183.00 | 12.10  | 11.70  |
| 0.00   | 0.00   | 0.00   |