
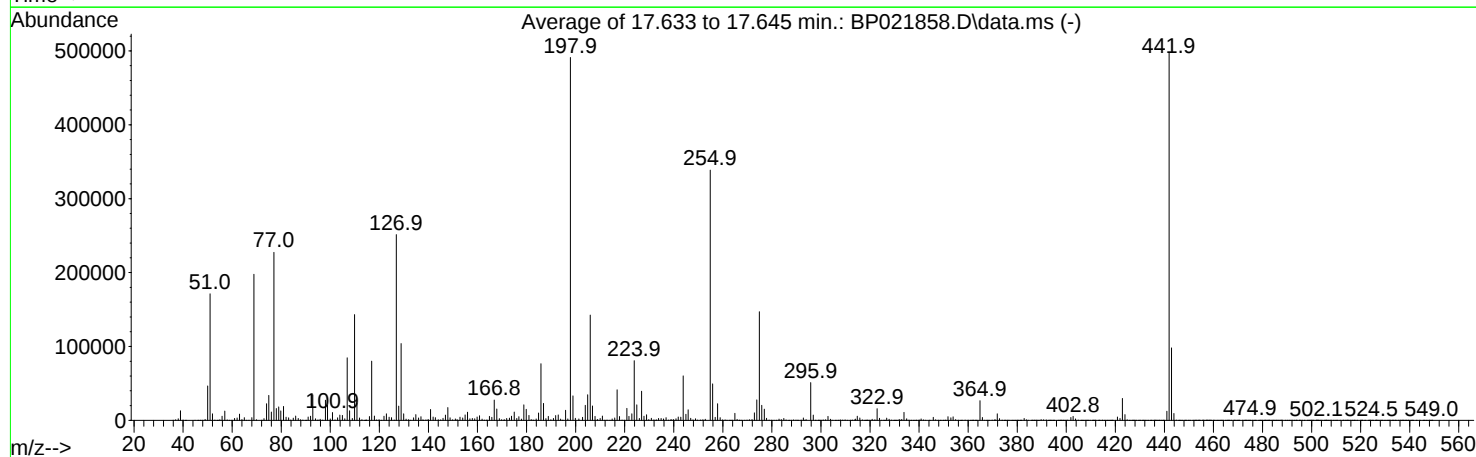


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090924\
Data File : BP021858.D
Acq On : 09 Sep 2024 08:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 10 00:09:47 2024

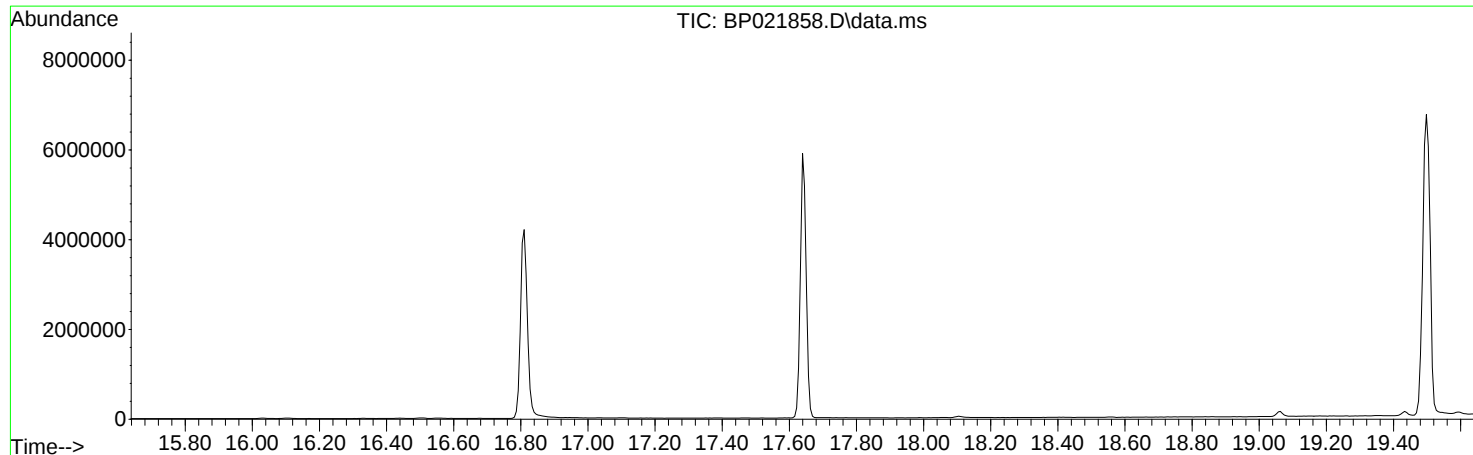




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	171239	PASS
68	69	0.00	2	1.9	3716	PASS
69	198	0.00	100	40.3	197749	PASS
70	69	0.00	2	0.5	898	PASS
127	198	10	80	51.2	251328	PASS
197	198	0.00	2	0.4	1895	PASS
198	198	100	100	100.0	491242	PASS
199	198	5	9	6.8	33179	PASS
275	198	10	60	30.0	147141	PASS
365	198	1	100	5.4	26587	PASS
441	198	0.01	100	2.5	12445	PASS
442	442	100	100	100.0	497856	PASS
443	442	15	24	19.7	98139	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090924\
Data File : BP021858.D
Acq On : 09 Sep 2024 08:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 10 00:17:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 00:09:47 2024
Response via : Initial Calibration

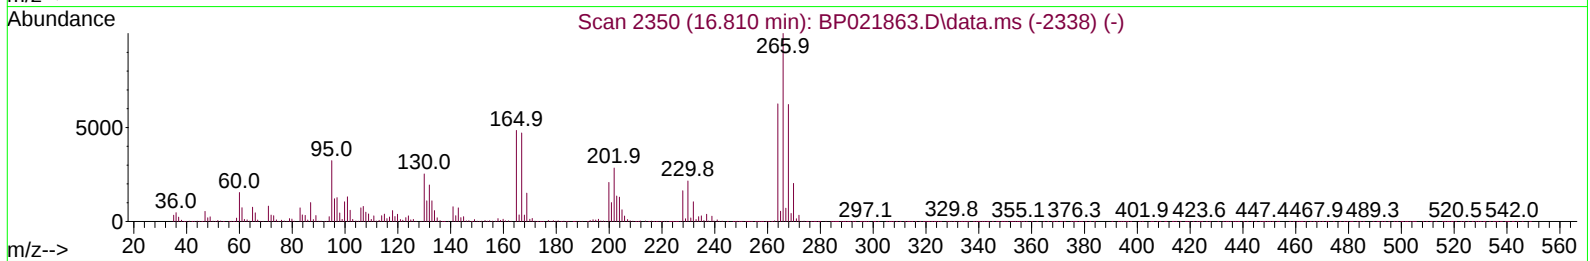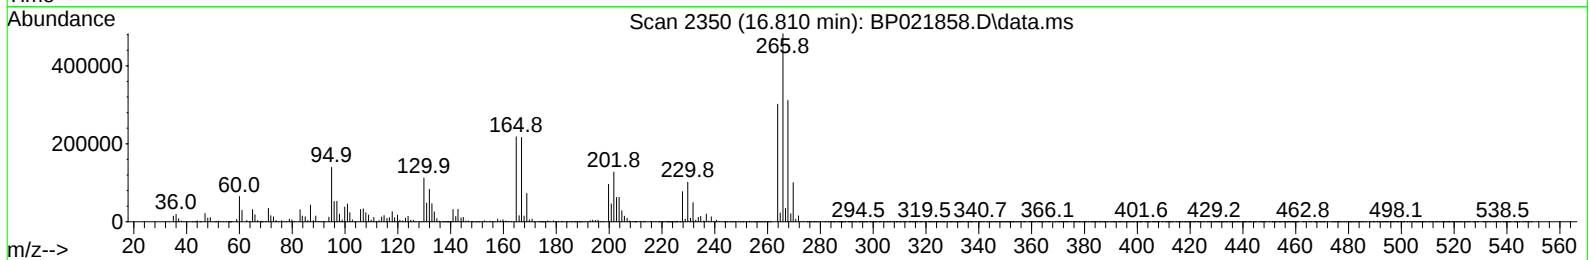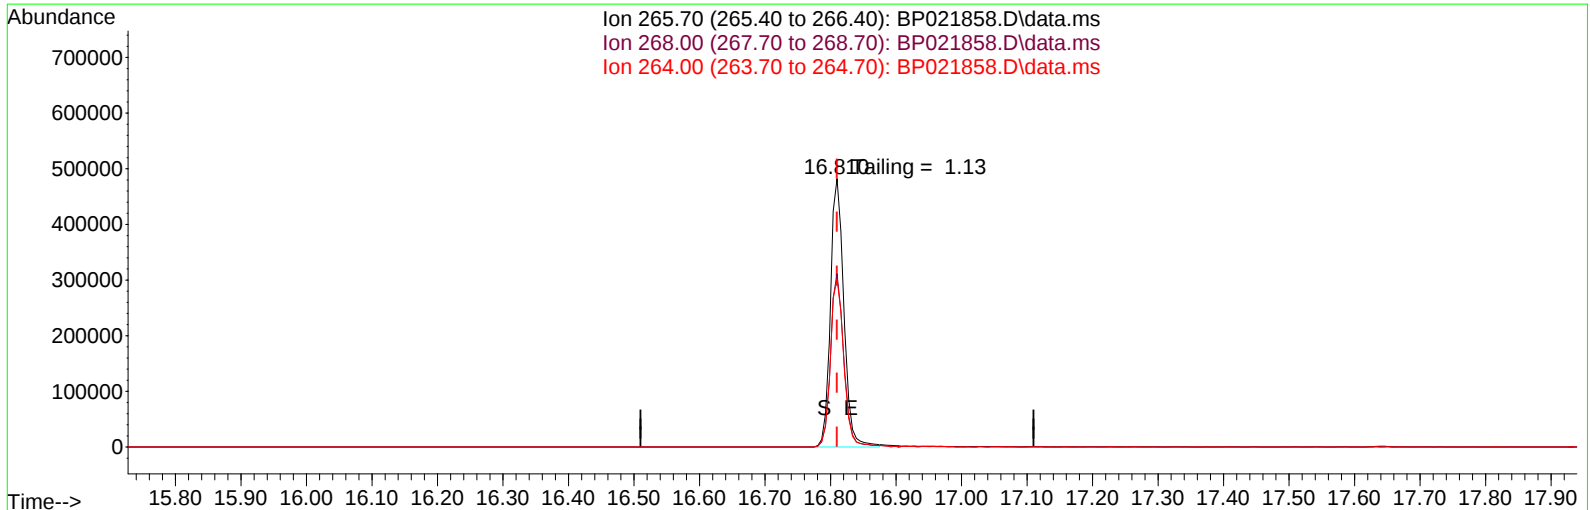

TIC: BP021858.D\data.ms

(70) Pentachlorophenol (C)

16.810min (-0.000) 221230.16 ng




response 695170

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.49
264.00	62.50	62.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090924\
Data File : BP021858.D
Acq On : 09 Sep 2024 08:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 10 00:17:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP090924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 00:09:47 2024
Response via : Initial Calibration

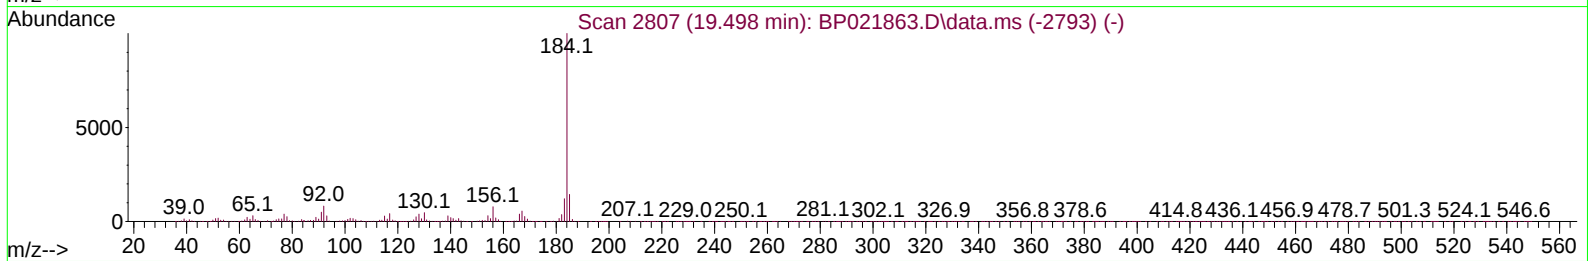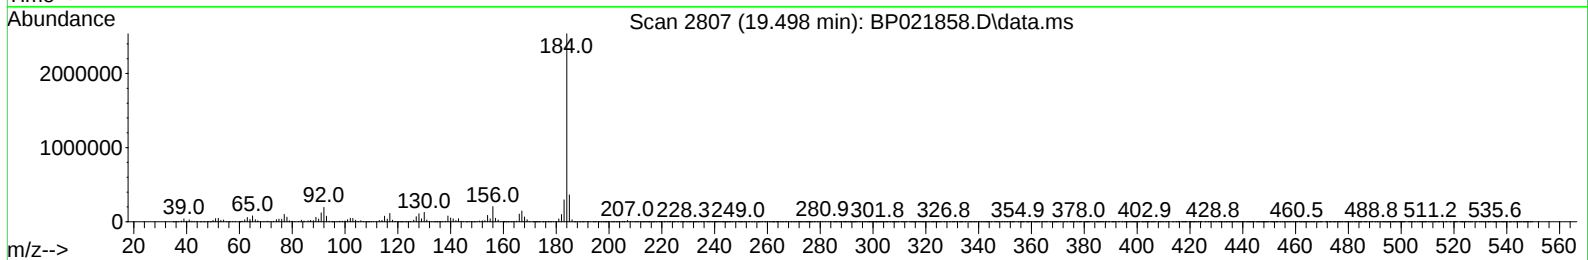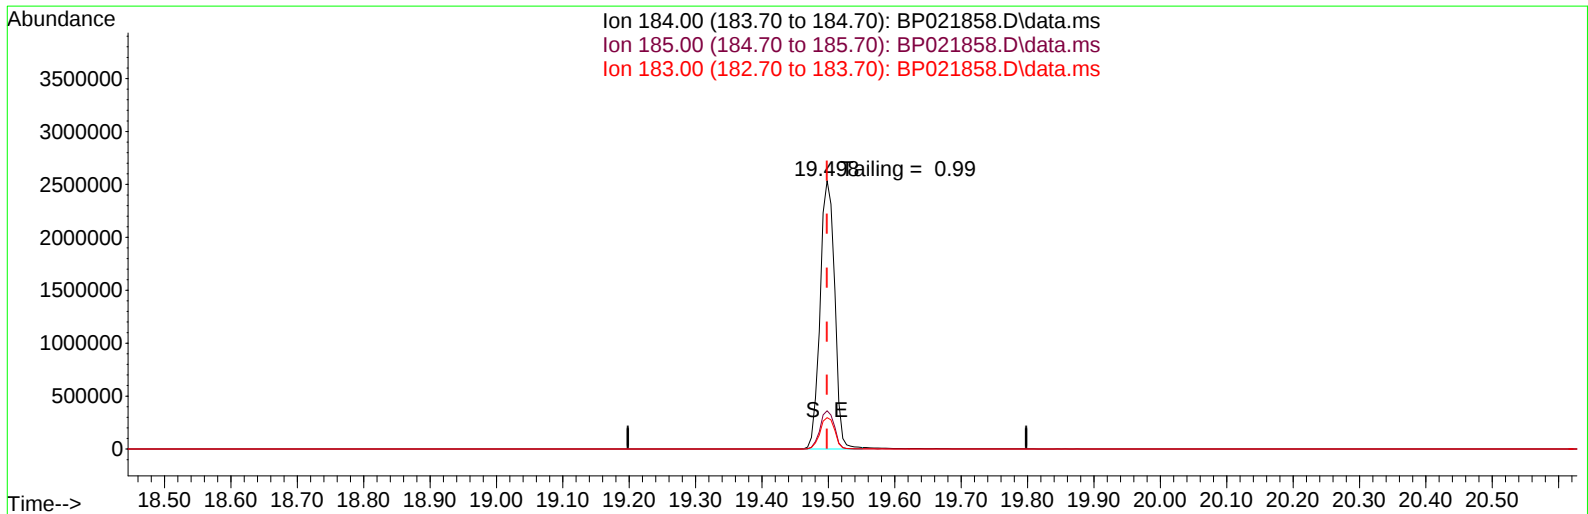

TIC: BP021858.D\data.ms

(77) Benzidine

19.498min (-0.000) 140895.36 ng

response 3898830

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.28
183.00	12.10	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/9/2024	BNA_P	<u>BP021858.D</u>
Compound Name	Response	Retention Time
DDT	1988652	20.786
DDD	59354	20.333
DDE	4028	19.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
63382	2052034	3.09

Instrument :
BNA_P
ClientSampleId :
DFTPP