


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP090925\
Data File : BP025691.D
Acq On : 09 Sep 2025 09:51
Operator : CG/JU
Sample : DFTPP628
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP628

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090825.MA.M
Title : SVOA CALIBRATION
Last Update : Tue Sep 09 09:26:50 2025

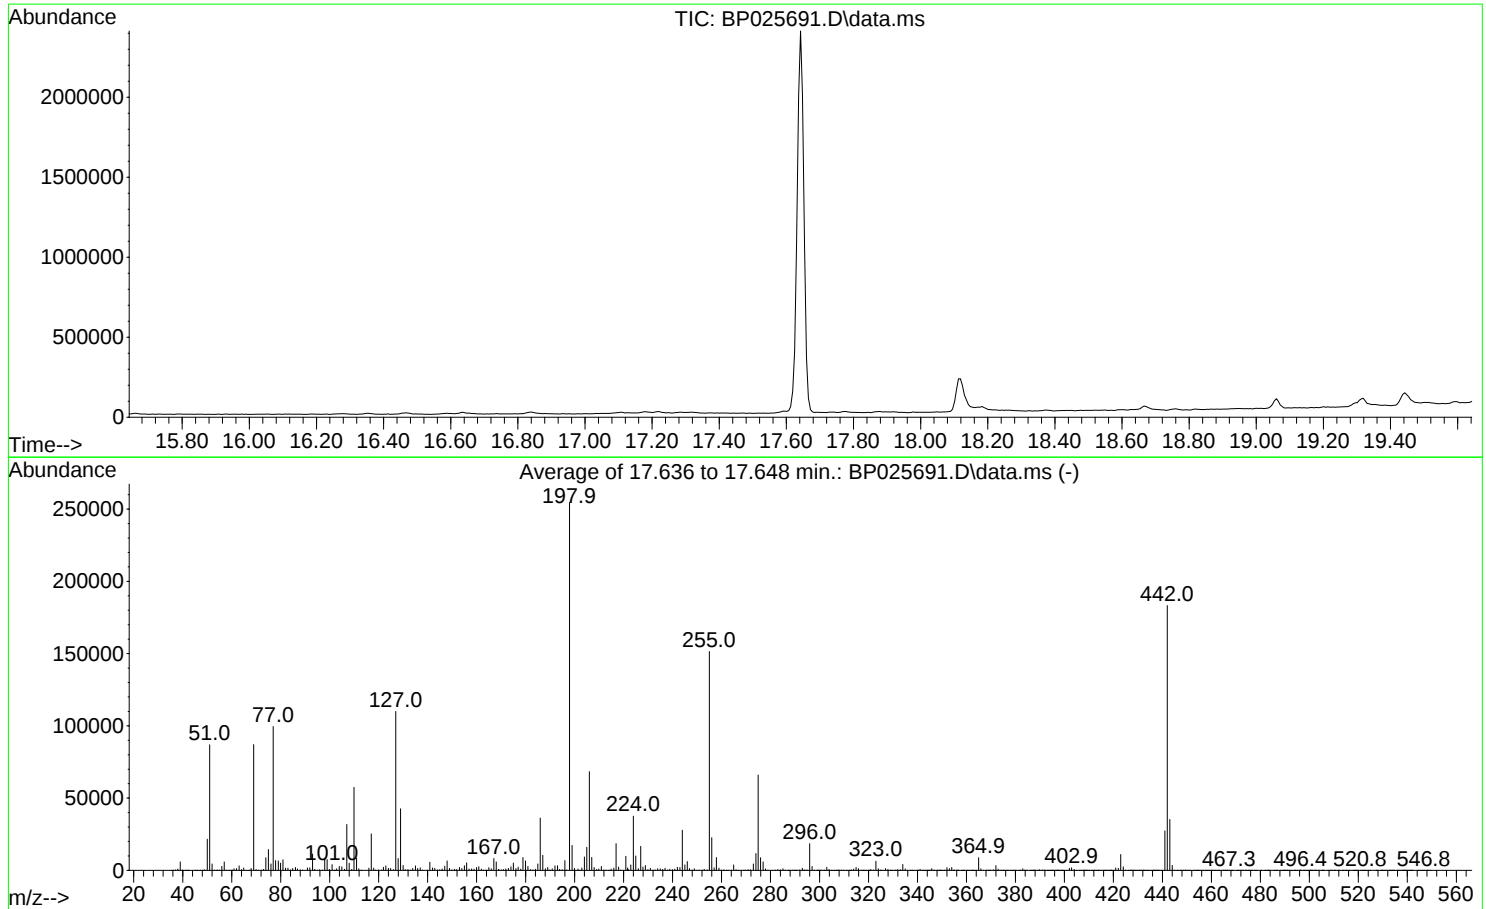

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	86936	PASS
68	69	0.00	2	1.5	1325	PASS
69	198	0.00	100	34.2	86995	PASS
70	69	0.00	2	0.6	552	PASS
127	198	10	80	43.2	109948	PASS
197	198	0.00	2	0.1	326	PASS
198	198	100	100	100.0	254571	PASS
199	198	5	9	6.8	17299	PASS
275	198	10	60	25.9	65959	PASS
365	198	1	100	3.4	8736	PASS
441	198	0.01	100	10.8	27408	PASS
442	198	50	100	72.0	183232	PASS
443	442	15	24	19.2	35197	PASS