
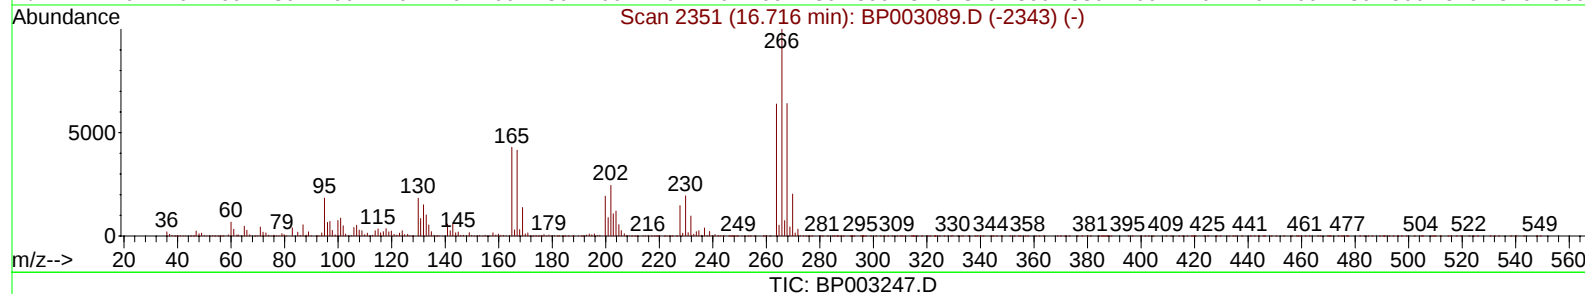
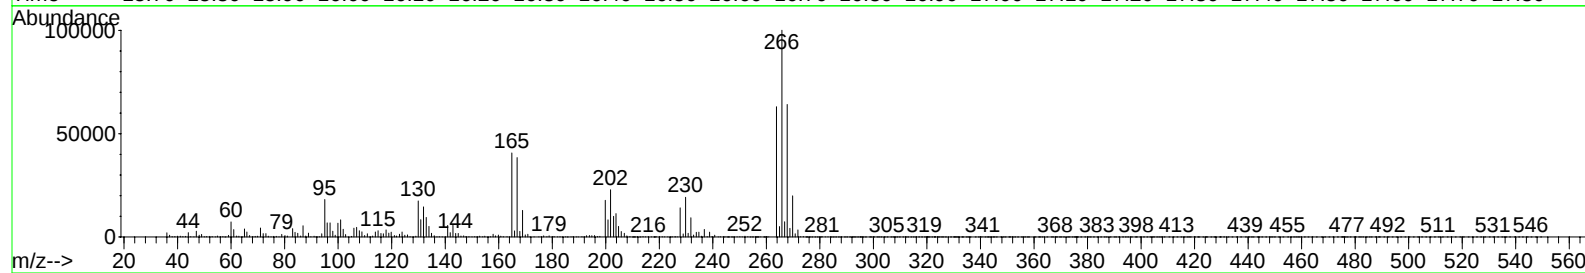


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091020\
 Data File : BP003247.D
 Acq On : 10 Sep 2020 13:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 18:19:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 01 14:37:05 2020
 Response via : Initial Calibration

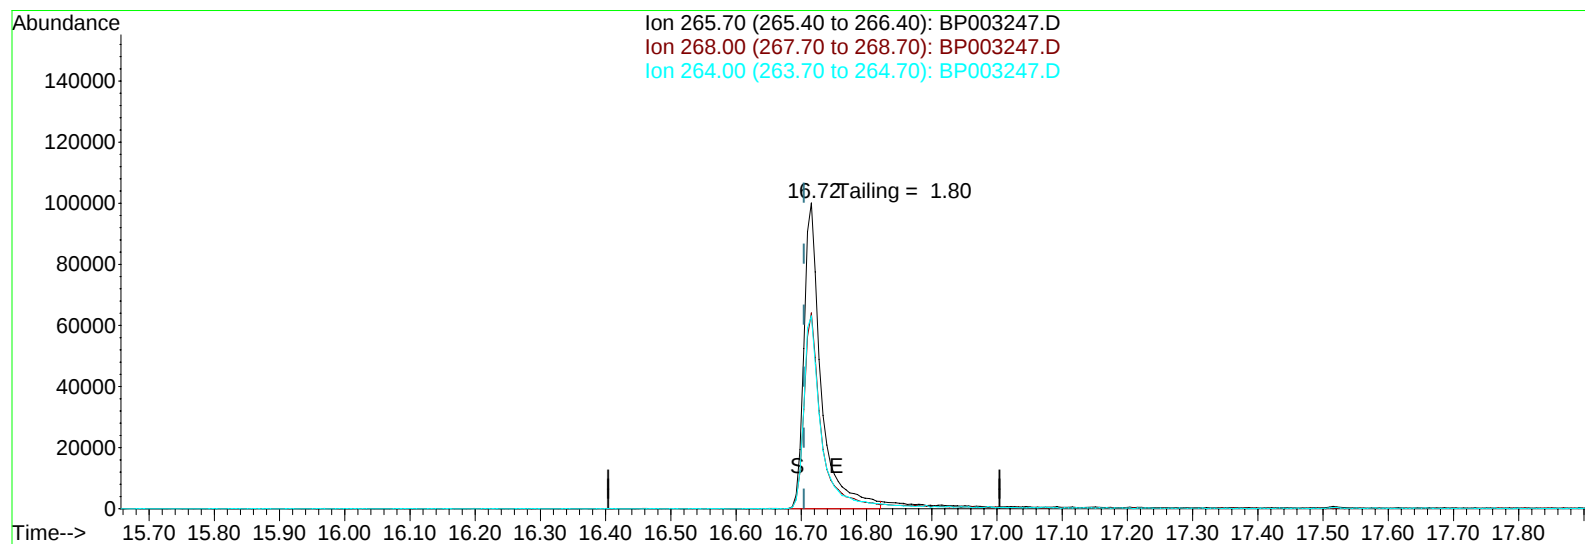

(70) Pentachlorophenol (C)




16.716min (+0.011) 205581.08ng

response 193761

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.07
264.00	63.30	63.03
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091020\
 Data File : BP003247.D
 Acq On : 10 Sep 2020 13:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 18:19:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 01 14:37:05 2020
 Response via : Initial Calibration

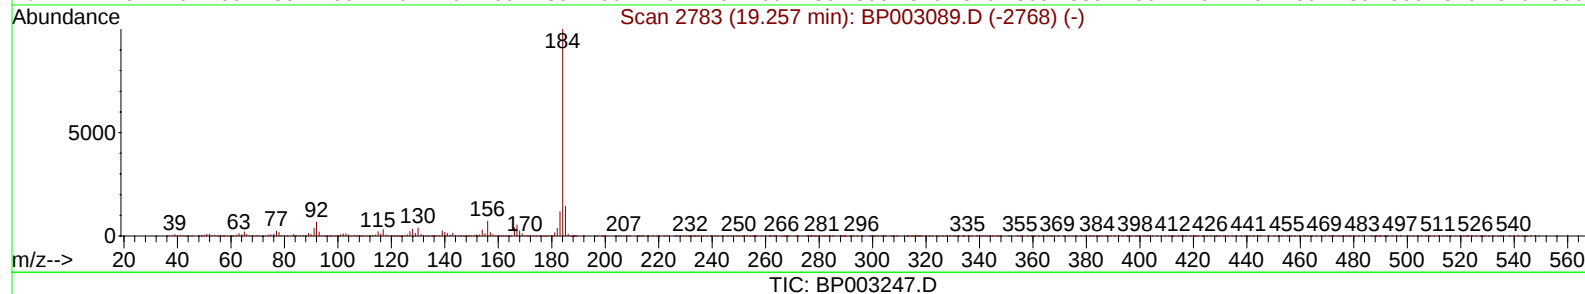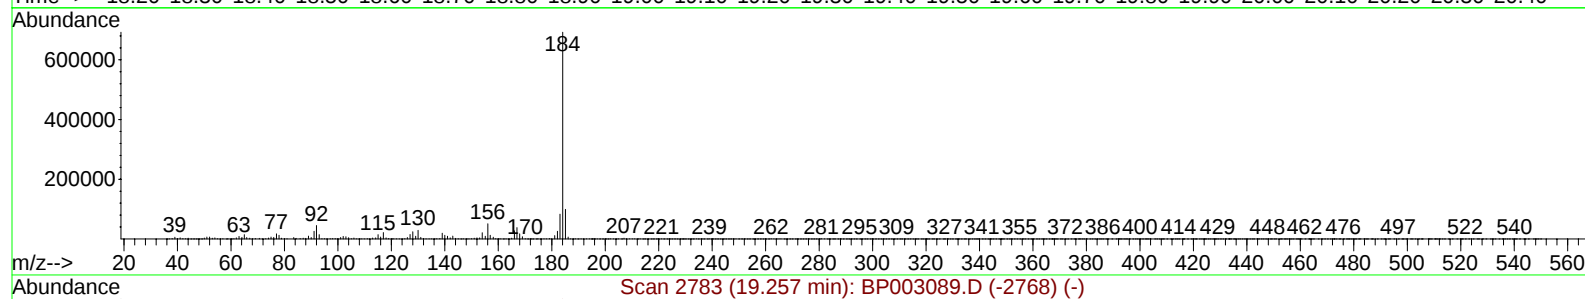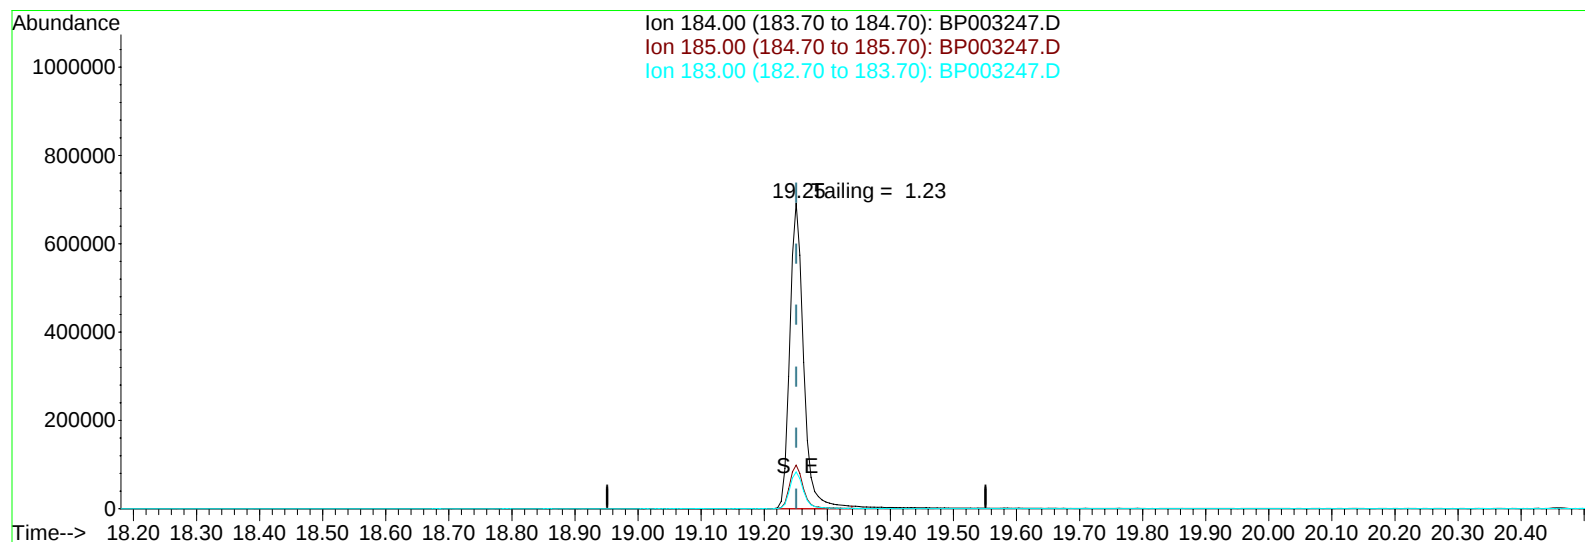

(77) Benzidine

19.251min (-0.000) 162939.39ng

response 1072504

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.30
183.00	12.00	12.02
0.00	0.00	0.00