

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091020\
 Data File : BP003249.D
 Acq On : 10 Sep 2020 15:40
 Operator : CG/JU
 Sample : PB131525BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB131525BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.263	397	404	419	rBV	2554320	3864638	39.61%	8.701%
2	6.840	664	672	694	rBV	2254549	3778458	38.73%	8.507%
3	7.645	802	809	821	rBV	713438	1111548	11.39%	2.503%
4	8.798	996	1005	1025	rBV	1574578	2809524	28.80%	6.326%
5	10.428	1272	1282	1307	rBV	805837	1558980	15.98%	3.510%
6	12.910	1696	1704	1727	rBV	4700317	7438639	76.24%	16.748%
7	14.292	1931	1939	1954	rBV2	1297526	2096223	21.49%	4.720%
8	15.792	2187	2194	2226	rBV	2866266	4882862	50.05%	10.994%
9	17.045	2400	2407	2422	rBV	1469353	2386024	24.46%	5.372%
10	19.627	2840	2846	2861	rBV	7184536	9756601	100.00%	21.967%
11	21.145	3099	3104	3112	rBV	1829455	2408782	24.69%	5.423%
12	23.380	3477	3484	3497	rVB2	1145327	2322574	23.81%	5.229%


Sum of corrected areas: 44414853

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091020\
Data File : BP003249.D
Acq On : 10 Sep 2020 15:40
Operator : CG/JU
Sample : PB131525BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131525BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

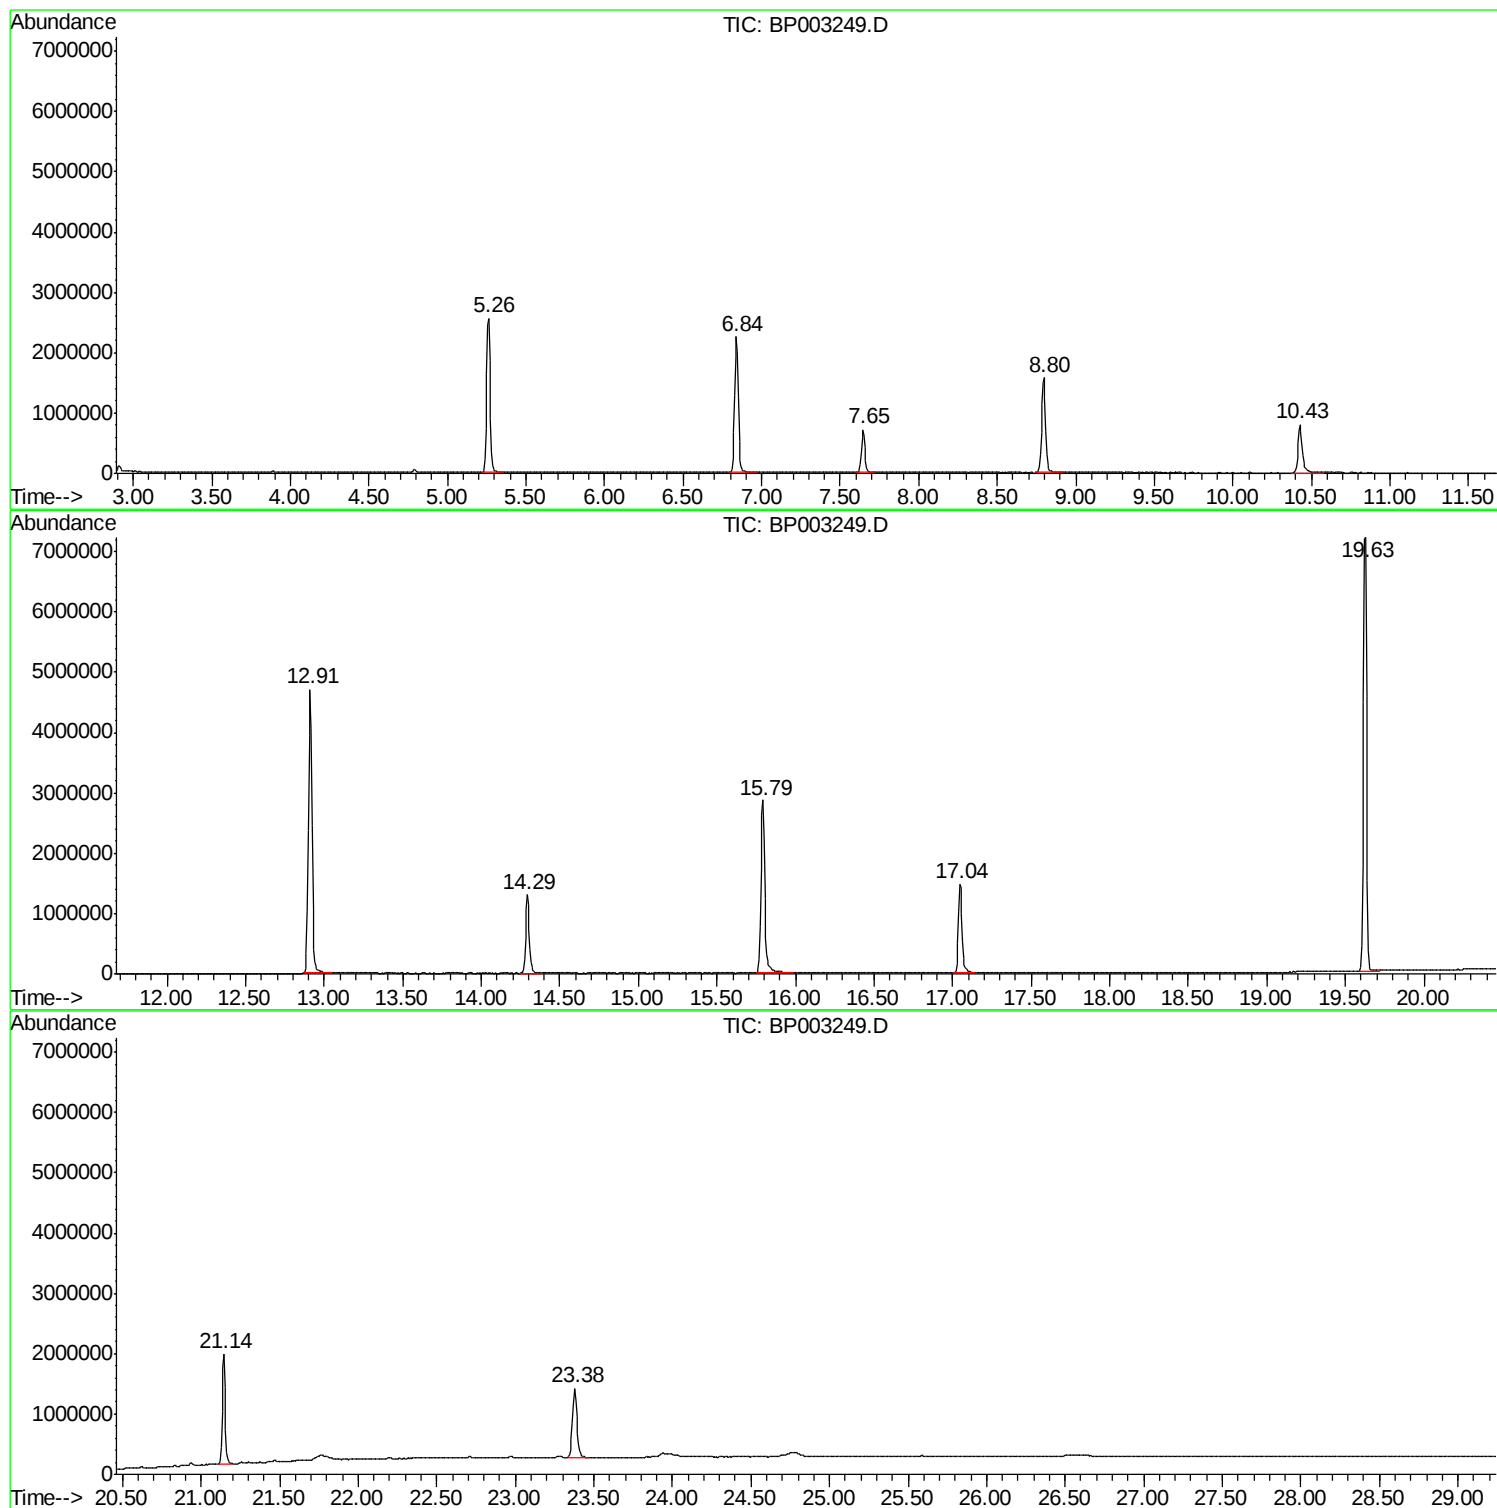

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091020\
Data File : BP003249.D
Acq On : 10 Sep 2020 15:40
Operator : CG/JU
Sample : PB131525BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131525BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091020\
Data File : BP003249.D
Acq On : 10 Sep 2020 15:40
Operator : CG/JU
Sample : PB131525BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131525BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc