


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091020\
 Data File : BP003247.D
 Acq On : 10 Sep 2020 13:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 01 14:37:05 2020

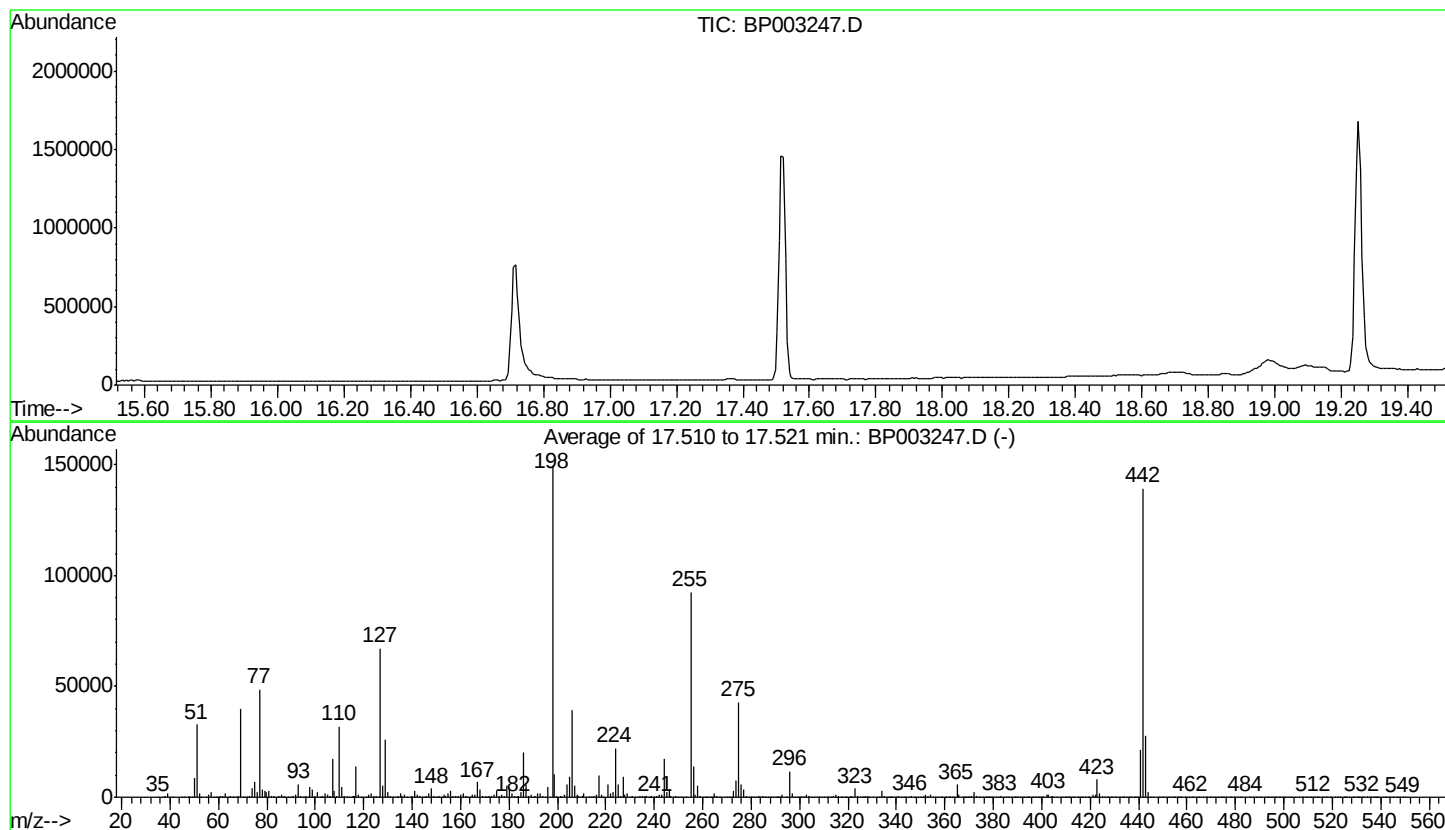

Spectrum Information: Average of 17.510 to 17.521 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.9	32800	PASS
68	69	0.00	2	0.9	358	PASS
69	198	0.00	100	26.5	39656	PASS
70	69	0.00	2	0.3	118	PASS
127	198	10	80	44.9	67162	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	149599	PASS
199	198	5	9	6.8	10190	PASS
275	198	10	60	28.6	42857	PASS
365	198	1	100	3.8	5696	PASS
441	198	0.01	100	14.4	21606	PASS
442	198	50	100	93.0	139184	PASS
443	442	15	24	19.8	27566	PASS