
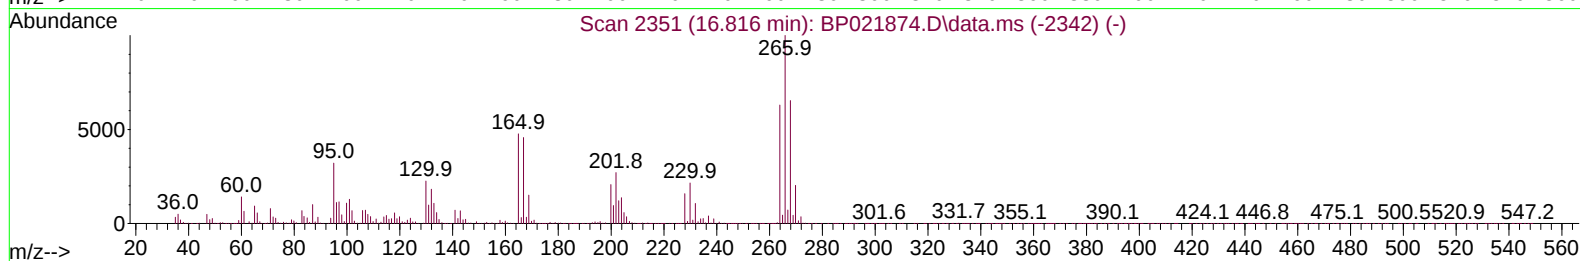
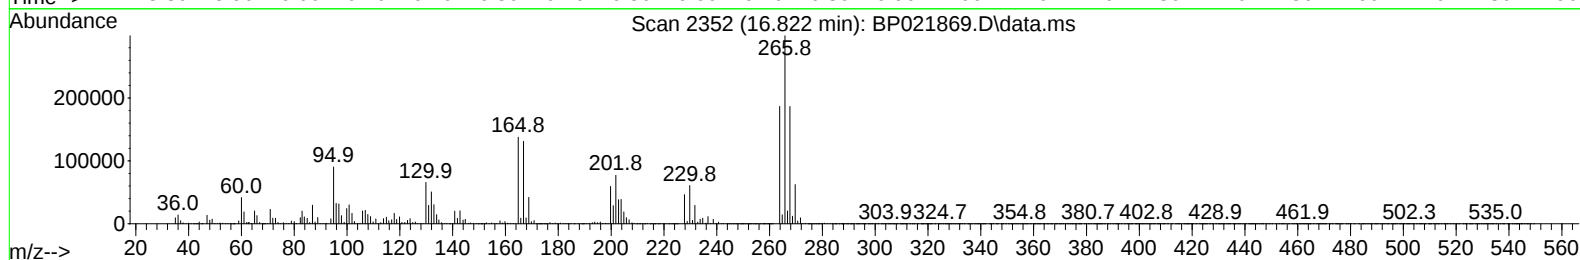


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091024\
Data File : BP021869.D
Acq On : 10 Sep 2024 09:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 11 02:37:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 17:57:20 2024
Response via : Initial Calibration

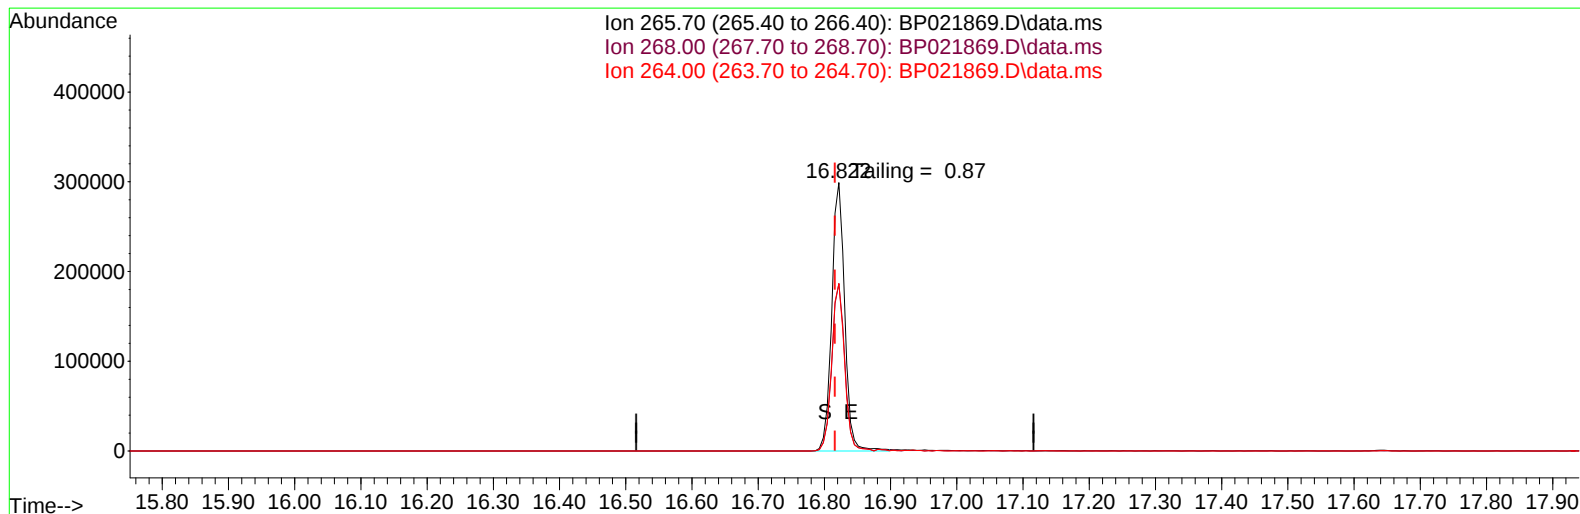

TIC: BP021869.D\data.ms

(70) Pentachlorophenol (C)




16.822min (+ 0.006) 696703.70 ng

response 411225

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.41
264.00	63.00	62.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091024\
Data File : BP021869.D
Acq On : 10 Sep 2024 09:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 11 02:37:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 17:57:20 2024
Response via : Initial Calibration

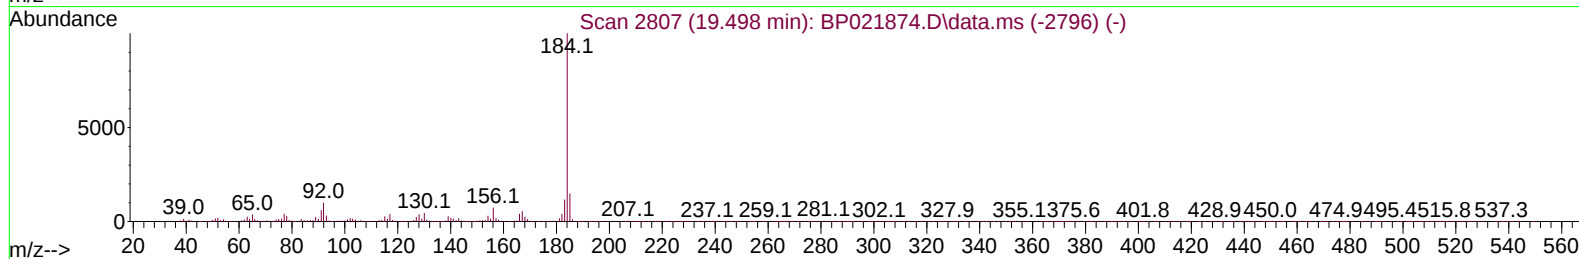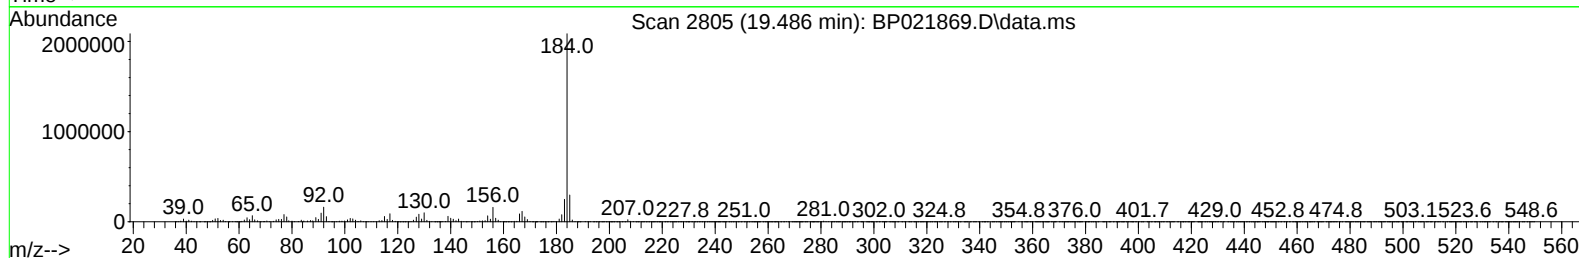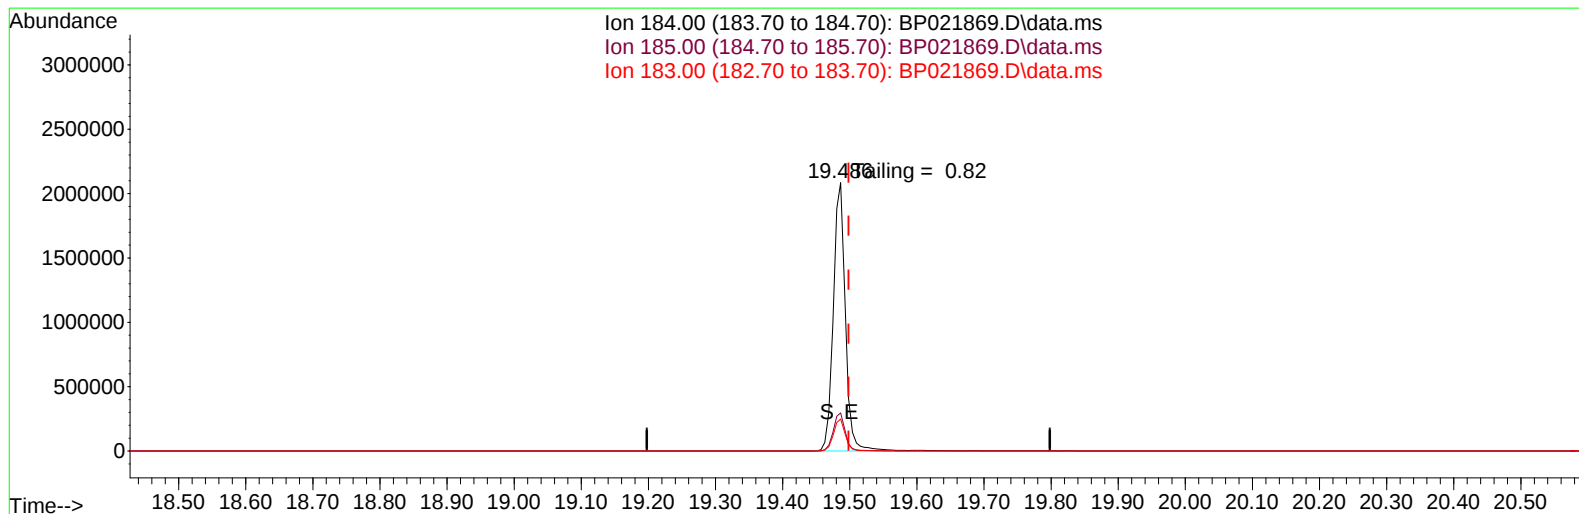

TIC: BP021869.D\data.ms

(77) Benzidine**19.486min (-0.012) 6298145.21 ng****response 2603940**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.22
183.00	11.50	11.92
0.00	0.00	0.00