
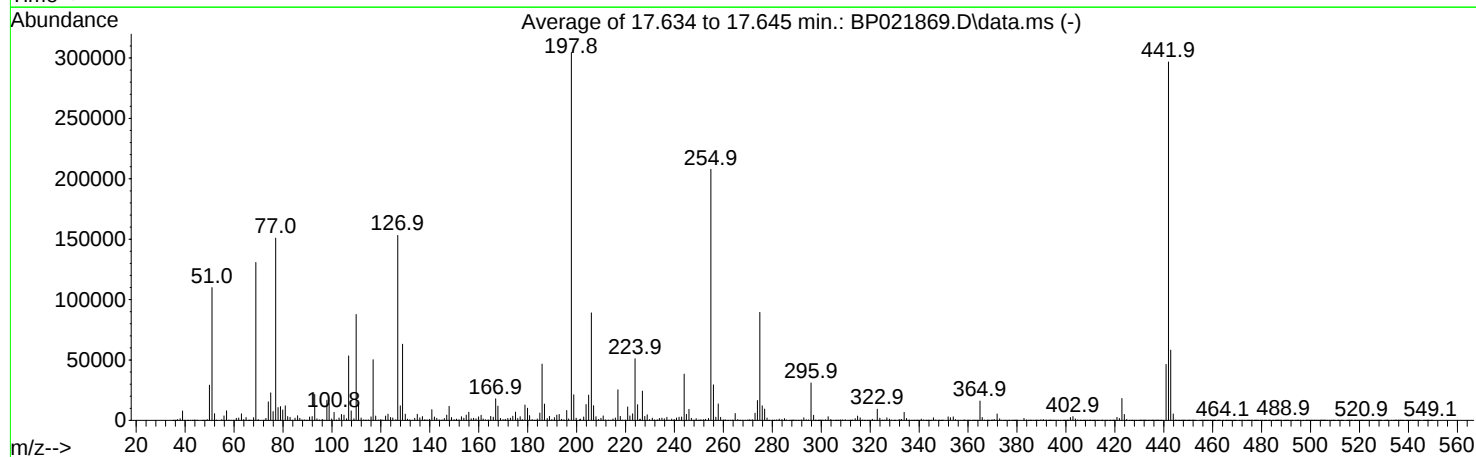


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091024\
Data File : BP021869.D
Acq On : 10 Sep 2024 09:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 10 17:57:20 2024

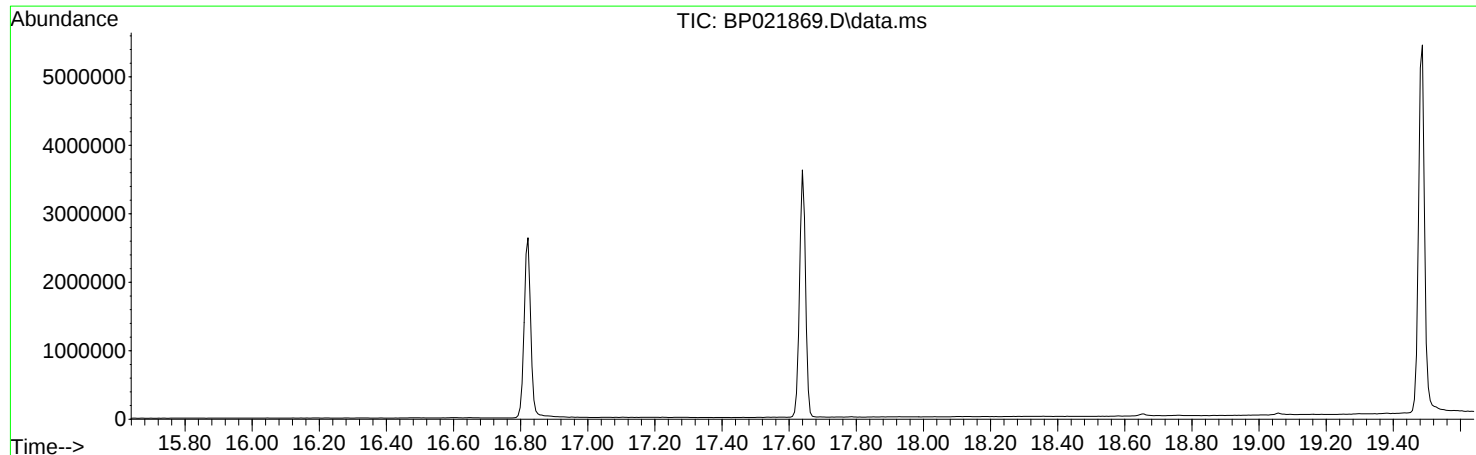

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	110013	PASS
68	69	0.00	2	1.8	2291	PASS
69	198	0.00	100	42.9	130753	PASS
70	69	0.00	2	0.5	707	PASS
127	198	10	80	50.3	153139	PASS
197	198	0.00	2	0.4	1165	PASS
198	198	100	100	100.0	304544	PASS
199	198	5	9	7.0	21183	PASS
275	198	10	60	29.4	89443	PASS
365	198	1	100	5.3	16072	PASS
441	198	0.01	100	15.2	46373	PASS
442	442	100	100	100.0	296704	PASS
443	442	15	24	19.6	58182	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/10/2024	BNA_P	<u>BP021869.D</u>
Compound Name	Response	Retention Time
DDT	1259322	20.775
DDD	21558	20.322
DDE	1778	19.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23336	1282658	1.82

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091024\
Data File : BP021869.D
Acq On : 10 Sep 2024 09:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 11 02:37:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 17:57:20 2024
Response via : Initial Calibration

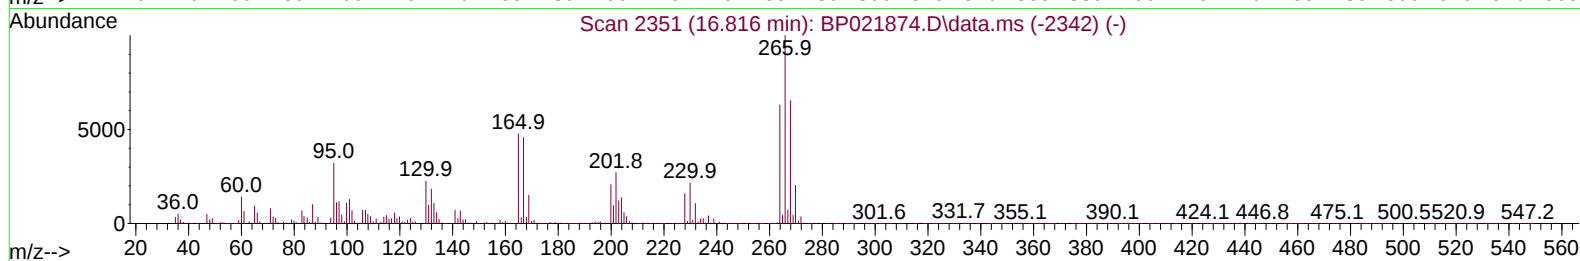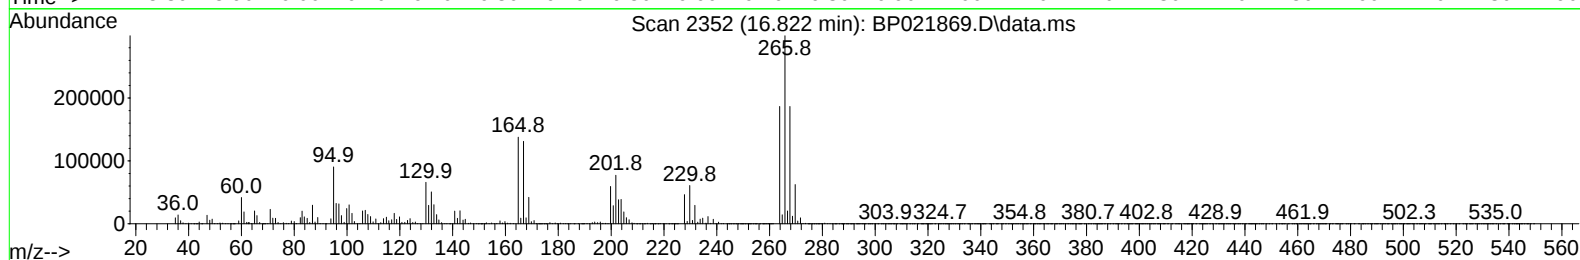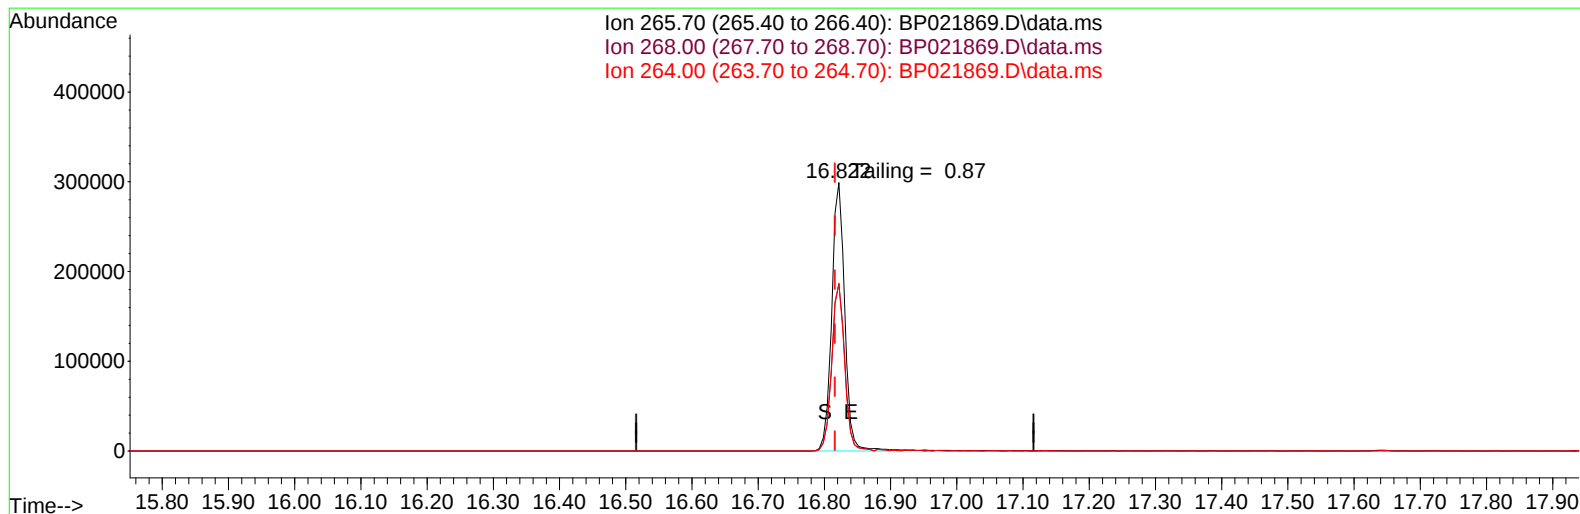

TIC: BP021869.D\data.ms

(70) Pentachlorophenol (C)

16.822min (+ 0.006) 696703.70 ng




response 411225

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.41
264.00	63.00	62.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091024\
 Data File : BP021869.D
 Acq On : 10 Sep 2024 09:25
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 11 02:37:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 17:57:20 2024
 Response via : Initial Calibration

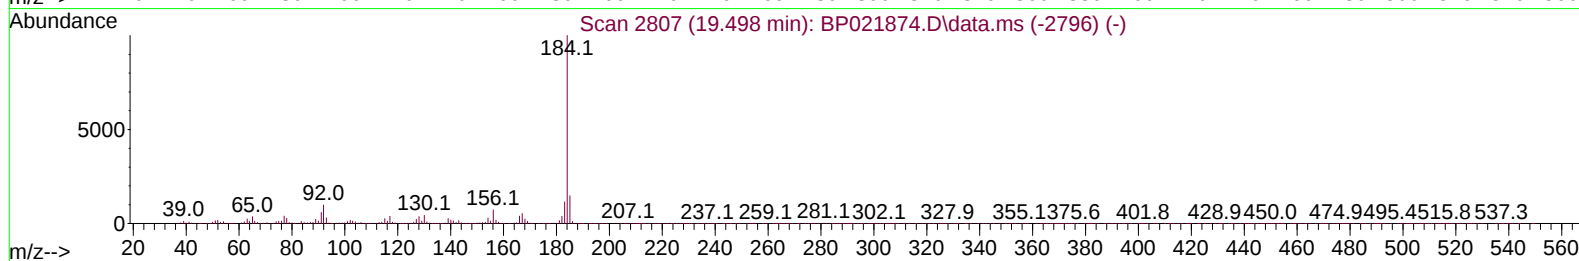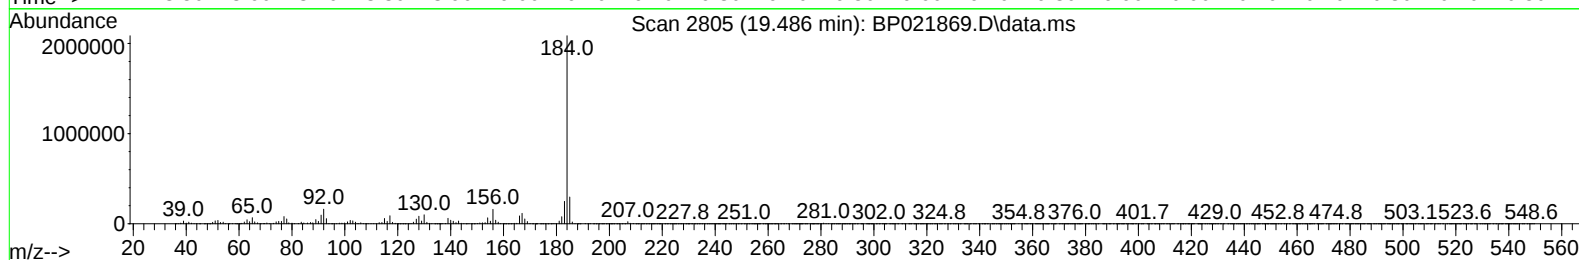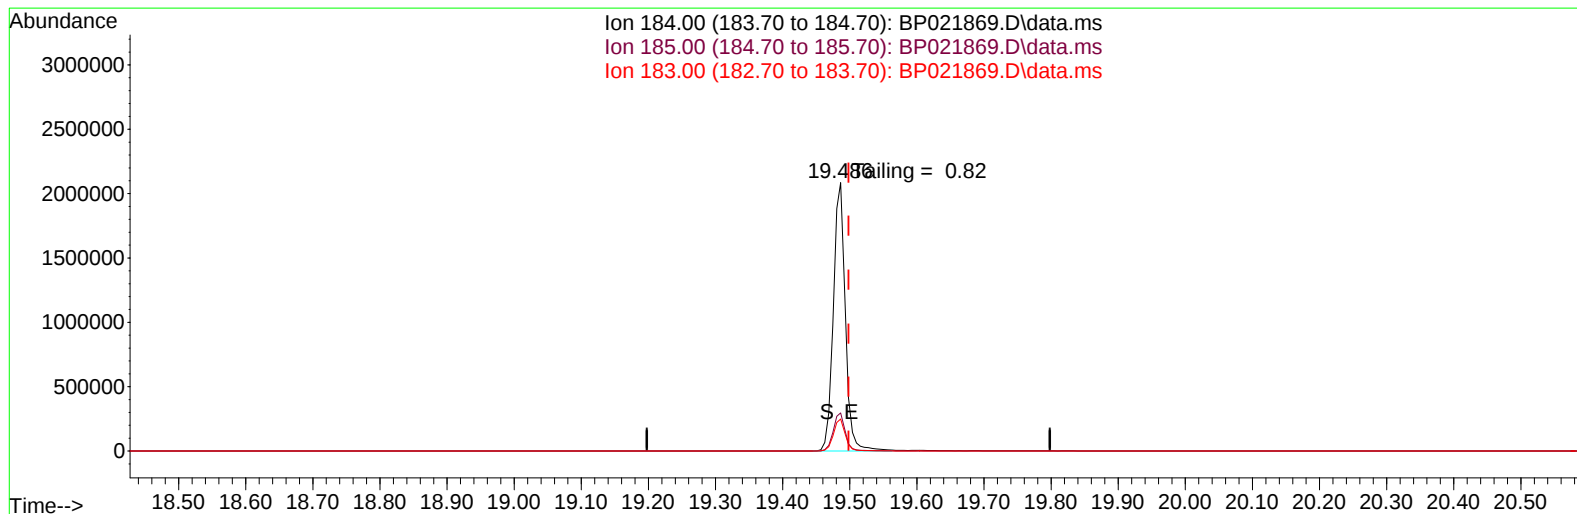

TIC: BP021869.D\data.ms

(77) Benzidine

19.486min (-0.012) 6298145.21 ng

response 2603940

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.22
183.00	11.50	11.92
0.00	0.00	0.00