


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091025\
Data File : BP025703.D
Acq On : 10 Sep 2025 09:13
Operator : CG/JU
Sample : DFTPP629
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP629

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP090825.MA.M
Title : SVOA CALIBRATION
Last Update : Tue Sep 09 09:26:50 2025

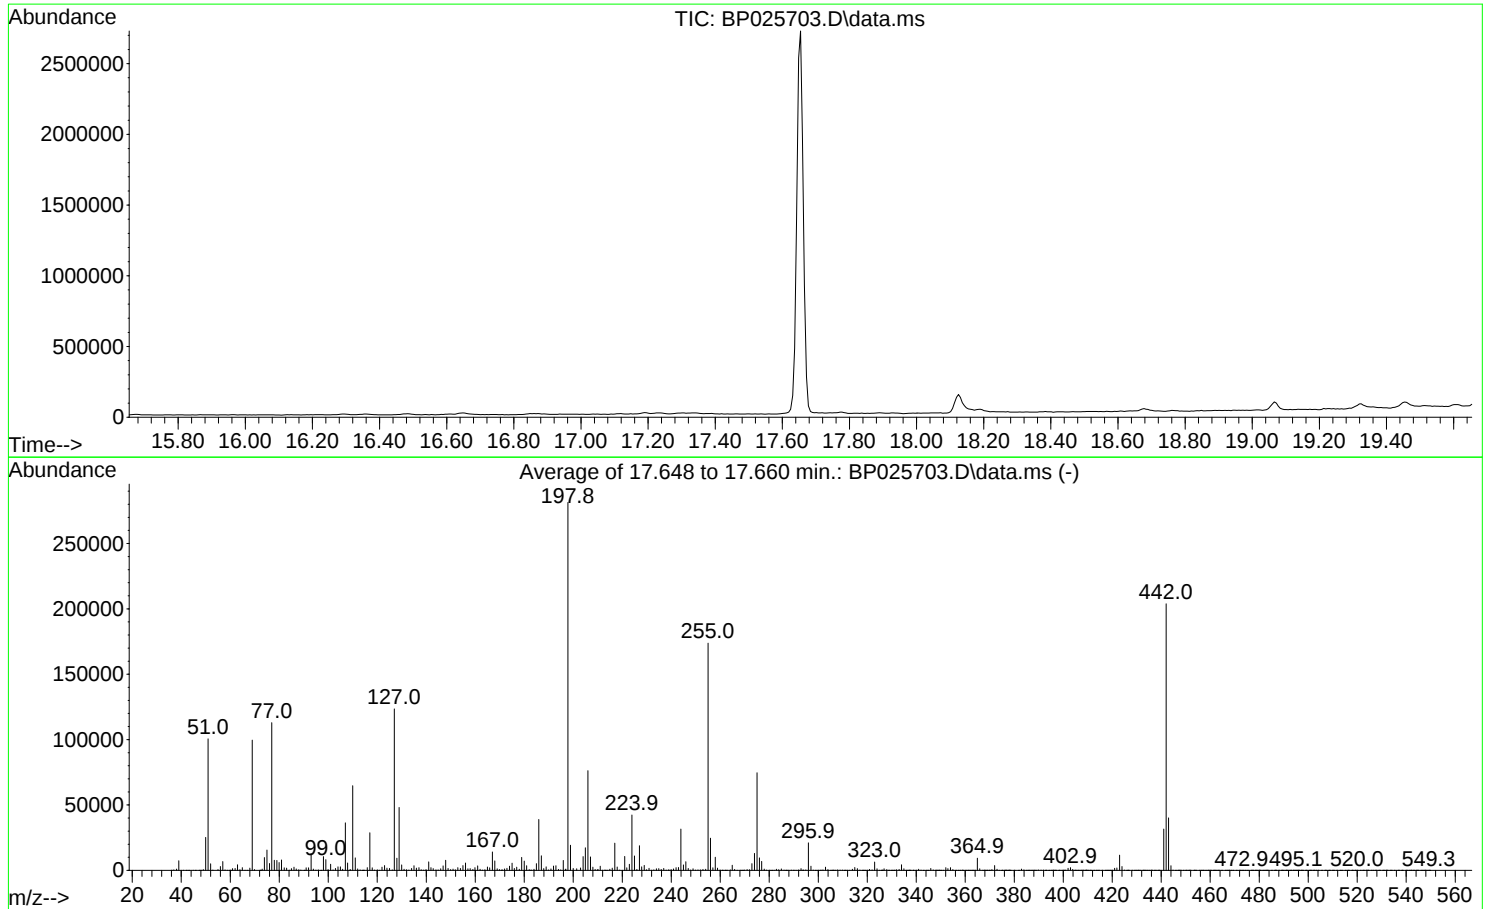

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	100649	PASS
68	69	0.00	2	1.7	1664	PASS
69	198	0.00	100	35.4	99582	PASS
70	69	0.00	2	0.6	587	PASS
127	198	10	80	43.9	123424	PASS
197	198	0.00	2	0.4	996	PASS
198	198	100	100	100.0	281354	PASS
199	198	5	9	6.8	19201	PASS
275	198	10	60	26.5	74699	PASS
365	198	1	100	3.3	9345	PASS
441	198	0.01	100	11.2	31560	PASS
442	198	50	100	72.5	203904	PASS
443	442	15	24	19.7	40115	PASS