

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091224\
 Data File : BP021894.D
 Acq On : 12 Sep 2024 13:30
 Operator : RC/JU
 Sample : PB163198BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK198

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021894.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.093	16	18	25	rVB5	6781	11013	0.37%	0.038%
2	3.258	42	46	57	rVB	27013	40220	1.35%	0.140%
3	3.664	111	115	136	rVB	300389	456341	15.29%	1.592%
4	3.987	167	170	179	rVB3	7615	11045	0.37%	0.039%
5	6.905	659	666	683	rBV	385473	620835	20.80%	2.166%
6	7.064	686	693	702	rVV	286360	449681	15.07%	1.569%
7	7.269	719	728	739	rBV	379864	627388	21.02%	2.189%
8	7.728	799	806	816	rBV	345626	598468	20.05%	2.088%
9	8.422	915	924	945	rBV	476525	786779	26.37%	2.745%
10	8.875	992	1001	1011	rBV	382912	620912	20.81%	2.166%
11	9.587	1115	1122	1136	rBV	287572	519985	17.42%	1.814%
12	10.128	1206	1214	1228	rBV	474136	819523	27.46%	2.859%
13	10.505	1268	1278	1290	rBV	482779	833555	27.93%	2.908%
14	10.634	1293	1300	1312	rBV	439590	777646	26.06%	2.713%
15	12.099	1544	1549	1556	rBV3	6318	12548	0.42%	0.044%
16	13.763	1824	1832	1846	rBV	953210	1413171	47.36%	4.930%
17	14.046	1868	1880	1892	rBV	1010225	1502223	50.34%	5.241%
18	14.357	1925	1933	1941	rBV	781257	1215855	40.74%	4.242%
19	14.557	1960	1967	1983	rBV	434398	719334	24.11%	2.510%
20	15.363	2096	2104	2116	rBV	1271618	1994757	66.85%	6.960%
21	15.481	2117	2124	2136	rVV	436191	642229	21.52%	2.241%
22	15.604	2140	2145	2150	rVB8	4750	9193	0.31%	0.032%
23	16.157	2236	2239	2243	rVB5	3456	5369	0.18%	0.019%
24	17.151	2401	2408	2417	rBV	1160915	1618498	54.24%	5.647%
25	17.251	2418	2425	2439	rVB	1724592	2278602	76.36%	7.950%
26	17.851	2525	2527	2532	rVB6	3222	3899	0.13%	0.014%
27	18.092	2565	2568	2569	rBV2	4011	3458	0.12%	0.012%
28	19.175	2747	2752	2756	rBV5	20577	32515	1.09%	0.113%
29	19.245	2761	2764	2773	rVB2	16762	27268	0.91%	0.095%
30	19.622	2822	2828	2838	rBV	1944435	2871140	96.21%	10.017%
31	20.463	2969	2971	2979	rVB2	72797	90899	3.05%	0.317%
32	21.592	3157	3163	3178	rBV	1386042	2017867	67.62%	7.040%
33	24.698	3681	3691	3704	rVB	1187723	2984144	100.00%	10.411%
34	24.916	3720	3728	3741	rVB2	739757	2045903	68.56%	7.138%

Sum of corrected areas: 28662263




Instrument :
BNA_P
ClientSampleId :
SBLK198

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091224\
Data File : BP021894.D
Acq On : 12 Sep 2024 13:30
Operator : RC/JU
Sample : PB163198BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK198

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

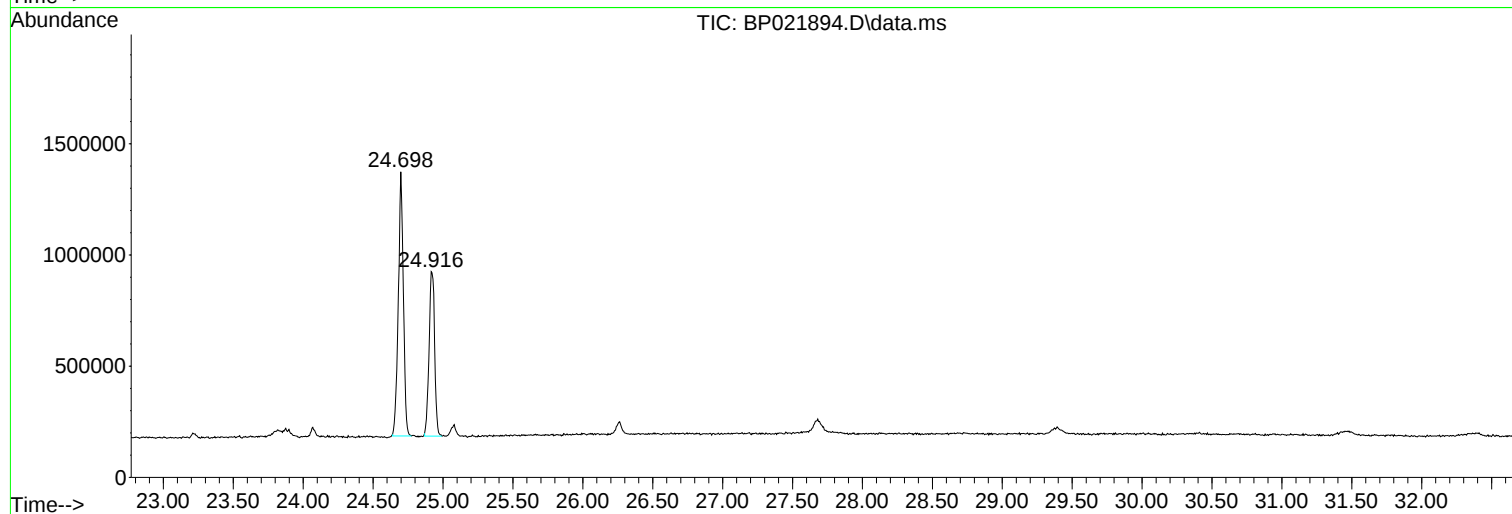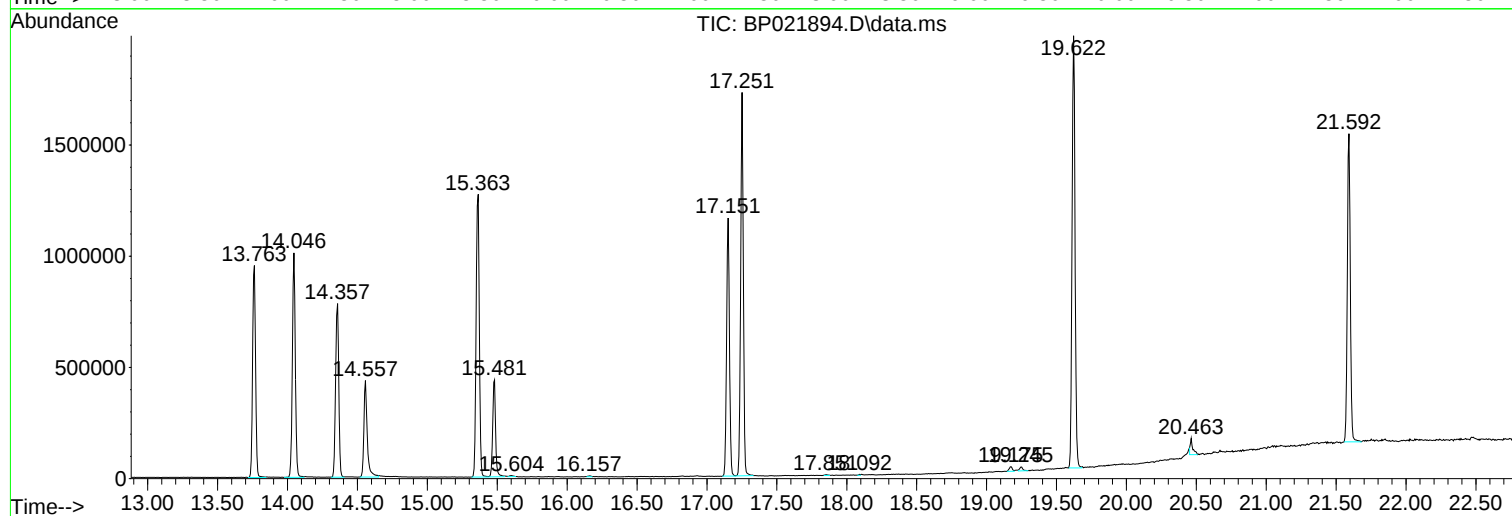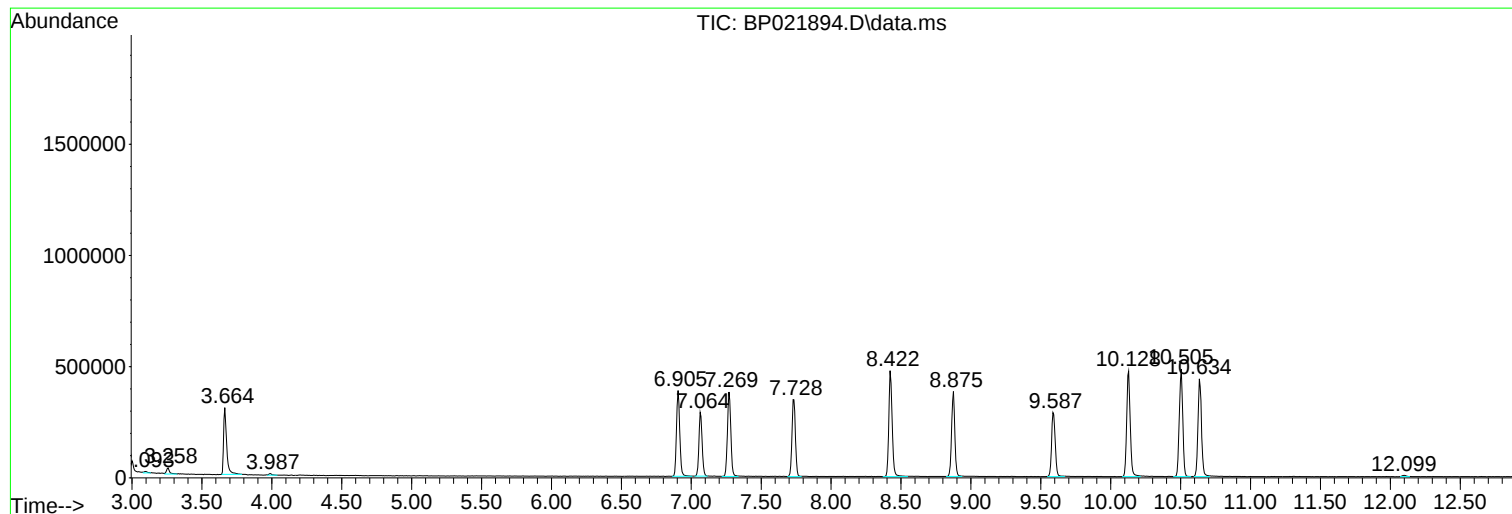

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091224\
Data File : BP021894.D
Acq On : 12 Sep 2024 13:30
Operator : RC/JU
Sample : PB163198BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK198

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091224\
Data File : BP021894.D
Acq On : 12 Sep 2024 13:30
Operator : RC/JU
Sample : PB163198BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK198

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc