

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091321\
 Data File : BP006963.D
 Acq On : 13 Sep 2021 16:23
 Operator : CG/JU
 Sample : M3263-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-QT4-2021-07

Manual Integrations
 APPROVED

mohammad
 9/14/2021 2:48:05 PM

Quant Time: Sep 13 16:52:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 13 14:04:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	403268	20.000	ng/ul	0.00
20) Naphthalene-d8	10.722	136	1741231	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.551	164	1188996	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.298	188	2446917	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.380	240	2192861	20.000	ng/ul	# 0.00
88) Perylene-d12	23.810	264	2023740	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	55676	5.494	ng/uL	0.00
4) Pyridine-d5	3.769	84	544615	20.624	ng/ul	0.00
7) Phenol-d5	7.075	99	899662	30.354	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.252	67	552882	32.480	ng/ul	0.00
11) 2-Chlorophenol-d4	7.452	132	754892	31.549	ng/ul	0.00
15) 4-Methylphenol-d8	8.622	113	737509	31.686	ng/ul	0.00
21) Nitrobenzene-d5	9.081	128	356490	33.801	ng/ul	0.00
24) 2-Nitrophenol-d4	9.804	143	380048	36.601	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.340	165	741212	30.274	ng/ul	0.00
31) 4-Chloroaniline-d4	10.857	131	1046813	30.917	ng/ul	0.00
46) Dimethylphthalate-d6	13.963	166	2376329	30.858	ng/ul	0.00
49) Acenaphthylene-d8	14.245	160	2761737	28.316	ng/ul	0.00
54) 4-Nitrophenol-d4	14.734	143	405084	30.278	ng/ul	0.00
60) Fluorene-d10	15.545	176	2047697	30.128	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	323516	29.887	ng/ul	0.00
73) Anthracene-d10	17.398	188	3071995	30.325	ng/ul	0.00
81) Pyrene-d10	19.633	212	3308713	32.218	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.651	264	3112714	31.883	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.387	88	10934	0.970	ng/uL#	92
5) Pyridine	3.793	79	106196	4.009	ng/ul#	55
6) Benzaldehyde	7.057	77	82609	4.374	ng/ul	92
8) Phenol	7.104	94	124047	4.049	ng/ul	93
10) Bis(2-Chloroethyl)ether	7.346	93	106470	4.341	ng/ul	99
12) 2-Chlorophenol	7.481	128	101092	4.118	ng/ul	93
13) 2-Methylphenol	8.357	108	88454	3.802	ng/ul	95
14) 2,2'-oxybis(1-Chloropr...	8.457	45	124079	4.379	ng/ul	98
16) Acetophenone	8.746	105	161465	4.524	ng/ul	87
17) N-Nitroso-di-n-propyla...	8.734	70	74963	4.507	ng/ul#	91
18) 4-Methylphenol	8.687	108	101756	4.078	ng/ul	94
19) Hexachloroethane	9.004	117	40058	4.007	ng/ul	88
22) Nitrobenzene	9.122	77	108836	4.264	ng/ul#	88
23) Isophorone	9.651	82	203739	4.019	ng/ul	95
25) 2-Nitrophenol	9.834	139	55606	4.791	ng/ul#	81
26) 2,4-Dimethylphenol	9.893	107	109430	3.892	ng/ul	89
27) Bis(2-Chloroethoxy)met...	10.134	93	141110	4.205	ng/ul	98
29) 2,4-Dichlorophenol	10.369	162	101749	4.196	ng/ul#	91
30) Naphthalene	10.775	128	341775	4.046	ng/ul	99
32) 4-Chloroaniline	10.881	127	143865	4.172	ng/ul	97
33) Hexachlorobutadiene	11.063	225	63984	3.825	ng/ul	99
34) Caprolactam	11.698	113	28432m	3.934	ng/ul	
35) 4-Chloro-3-methylphenol	11.998	107	91946	3.739	ng/ul	88
36) 2-Methylnaphthalene	12.381	142	236626	4.179	ng/ul	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091321\
 Data File : BP006963.D
 Acq On : 13 Sep 2021 16:23
 Operator : CG/JU
 Sample : M3263-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-QT4-2021-07

Manual Integrations
 APPROVED

mohammad
 9/14/2021 2:48:05 PM

Quant Time: Sep 13 16:52:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 13 14:04:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.598	142	236668	4.097	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.745	216	130837	3.843	ng/ul#	92
40) Hexachlorocyclopentadiene	12.734	237	100772	4.586	ng/ul	99
41) 2,4,6-Trichlorophenol	12.987	196	71393	3.623	ng/ul	97
42) 2,4,5-Trichlorophenol	13.051	196	81684	3.718	ng/ul	99
43) 1,1'-Biphenyl	13.387	154	322463	3.895	ng/ul	98
44) 2-Chloronaphthalene	13.428	162	248313	3.890	ng/ul#	91
45) 2-Nitroaniline	13.628	65	47240m	3.642	ng/ul	
47) Dimethylphthalate	14.010	163	311918	4.016	ng/ul	99
48) 2,6-Dinitrotoluene	14.122	165	45902	3.539	ng/ul#	84
50) Acenaphthylene	14.275	152	384541	3.800	ng/ul	100
51) 3-Nitroaniline	14.451	138	47721m	3.209	ng/ul	
52) Acenaphthene	14.616	153	263057	3.926	ng/ul	97
53) 2,4-Dinitrophenol	14.657	184	24589	3.375	ng/ul#	72
55) 4-Nitrophenol	14.751	109	39431	4.010	ng/ul#	85
56) Dibenzofuran	14.945	168	379451	3.924	ng/ul	87
57) 2,4-Dinitrotoluene	14.910	165	69759	3.763	ng/ul#	77
58) 2,3,4,6-Tetrachlorophenol	15.175	232	64352	3.635	ng/ul#	79
59) Diethylphthalate	15.369	149	296816	3.925	ng/ul	97
61) Fluorene	15.598	166	312465	4.054	ng/ul	97
62) 4-Chlorophenyl-phenyle...	15.592	204	158001	4.021	ng/ul#	83
63) 4-Nitroaniline	15.610	138	51050m	3.439	ng/ul	
66) 4,6-Dinitro-2-methylph...	15.669	198	44882	4.072	ng/ul#	93
67) N-Nitrosodiphenylamine	15.804	169	259821	4.032	ng/ul	99
68) 4-Bromophenyl-phenylether	16.492	248	88555	3.828	ng/ul#	79
69) Hexachlorobenzene	16.604	284	104552	3.898	ng/ul#	84
70) Atrazine	16.757	200	82609	3.385	ng/ul	94
71) Pentachlorophenol	16.951	266	56946	3.706	ng/ul	97
72) Phenanthrene	17.339	178	482765	3.961	ng/ul	100
74) Anthracene	17.433	178	491078	4.053	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.351	216	123383	3.598	ng/ul	98
76) Pentachlorobenzene	14.869	250	126771	3.819	ng/ul	98
77) Carbazole	17.698	167	398351	3.699	ng/ul	98
78) Di-n-butylphthalate	18.257	149	433627	3.553	ng/ul#	98
80) Fluoranthene	19.304	202	528928	4.141	ng/ul#	93
82) Pyrene	19.657	202	568897	4.342	ng/ul	94
83) Butylbenzylphthalate	20.533	149	168674	3.697	ng/ul#	88
84) 3,3'-Dichlorobenzidine	21.298	252	182165	4.003	ng/ul	98
85) Benzo(a)anthracene	21.363	228	507933	3.978	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.292	149	248514	3.654	ng/ul	97
87) Chrysene	21.416	228	494759	3.916	ng/ul	99
89) Di-n-octyl phthalate	22.227	149	377279	3.607	ng/ul	100
90) Benzo(b)fluoranthene	23.062	252	462653	3.907	ng/ul	98
91) Benzo(k)fluoranthene	23.110	252	448613	4.047	ng/ul	98
93) Benzo(a)pyrene	23.698	252	432324	3.795	ng/ul	97
94) Indeno(1,2,3-cd)pyrene	26.339	276	454301	3.437	ng/ul	96
95) Dibenzo(a,h)anthracene	26.356	278	384149	3.359	ng/ul	97
96) Benzo(g,h,i)perylene	27.115	276	374244	3.302	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091321\
 Data File : BP006963.D
 Acq On : 13 Sep 2021 16:23
 Operator : CG/JU
 Sample : M3263-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-QT4-2021-07

Manual Integrations
 APPROVED

mohammad
 9/14/2021 2:48:05 PM


Quant Time: Sep 13 16:52:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 13 14:04:43 2021
 Response via : Initial Calibration

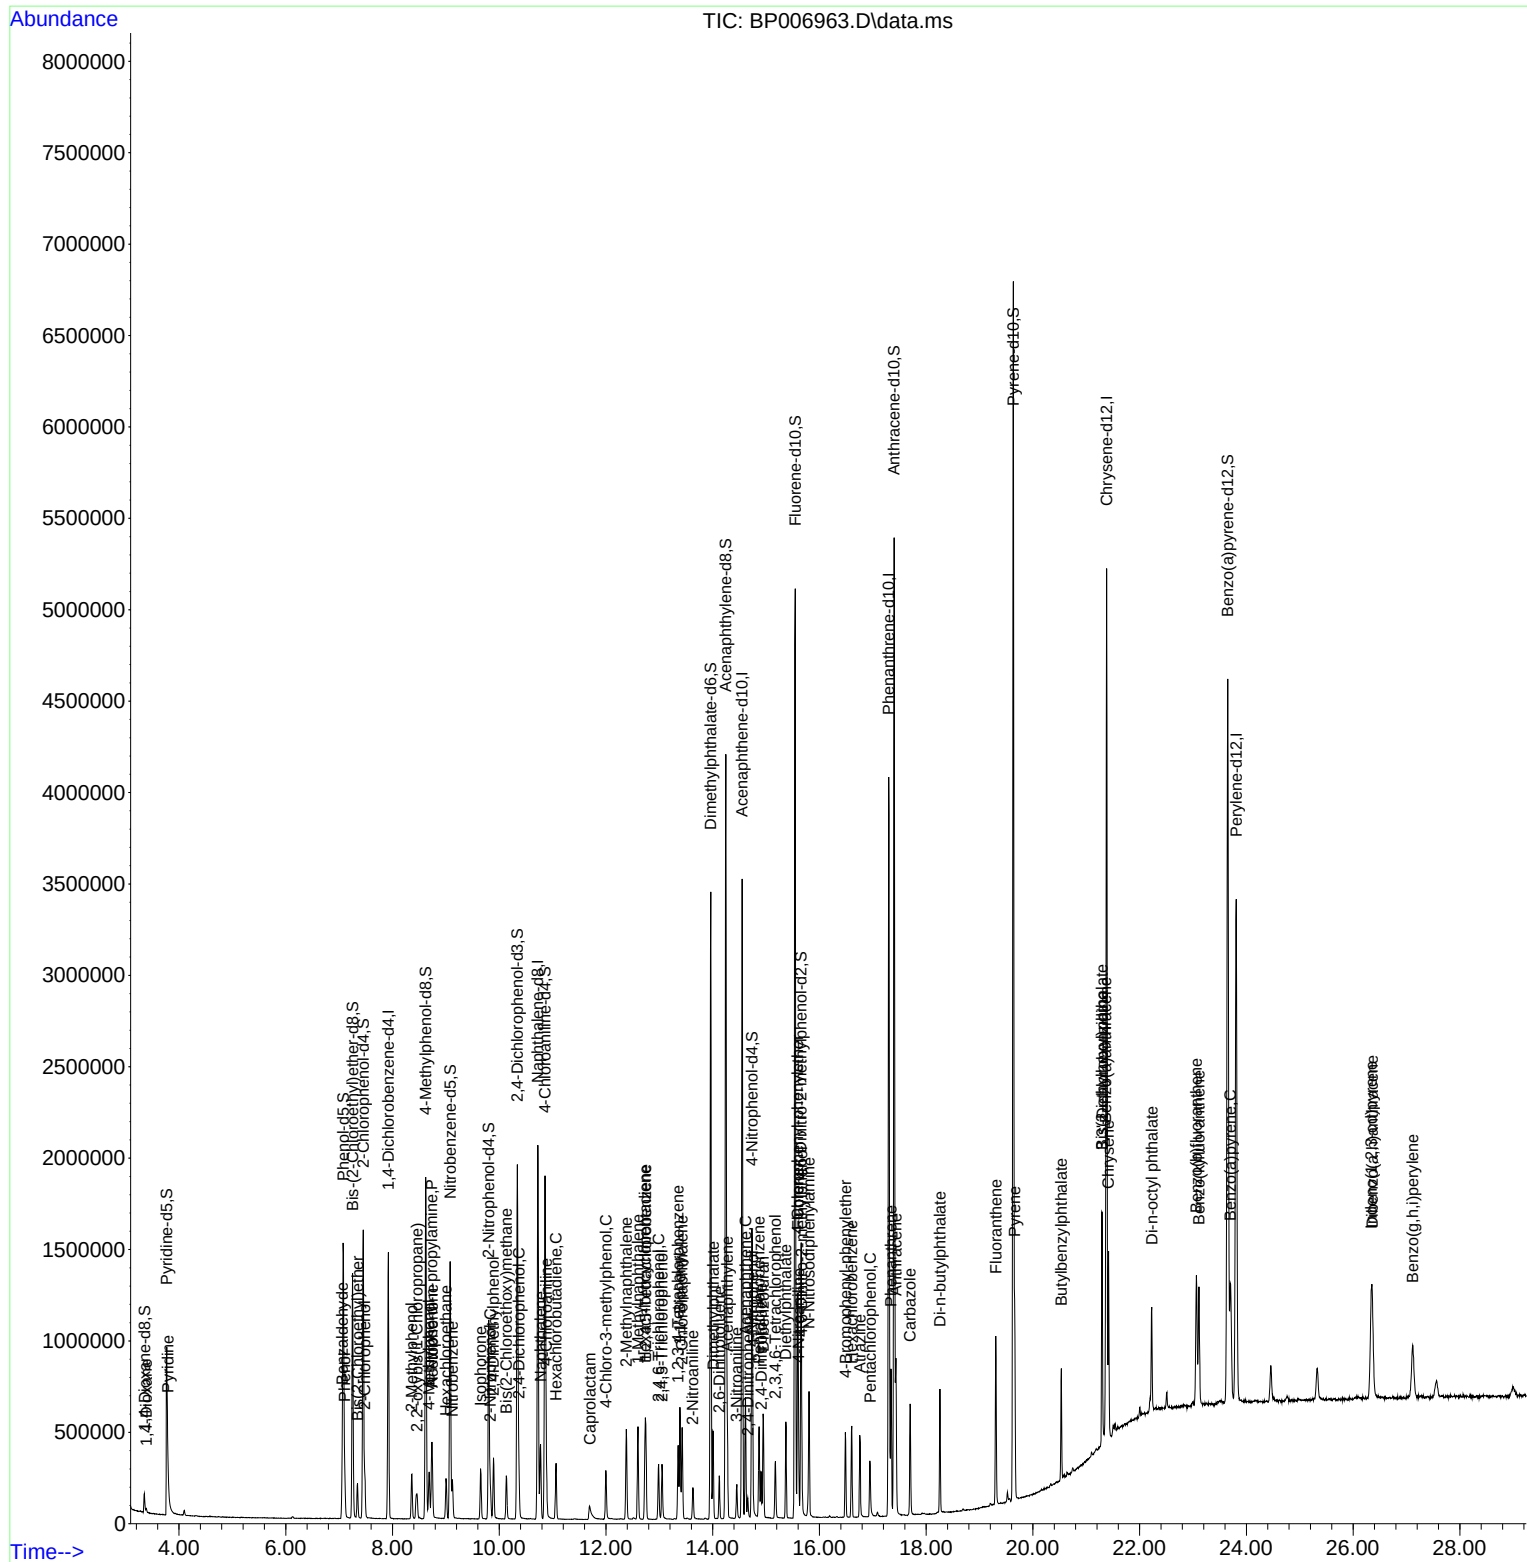



#2
1,4-Dioxane
Concen: 0.970 ng/uL
RT: 3.387 min Scan# 51
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07




Tgt Ion: 88 Resp: 10934
Ion Ratio Lower Upper
88 100
43 32.4 20.1 30.1#
58 64.5 48.4 72.6

Manual Integrations
APPROVED



mohammad
9/14/2021 2:48:05 PM

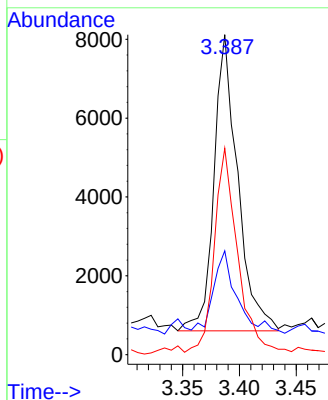


#5
Pyridine
Concen: 4.009 ng/uL
RT: 3.793 min Scan# 120
Delta R.T. 0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Tgt Ion: 79 Resp: 106196
Ion Ratio Lower Upper
79 100
52 106.3 49.2 73.8#
51 36.9 22.7 34.1#

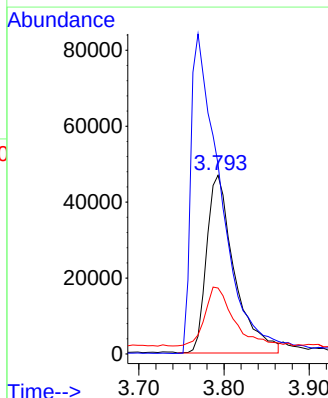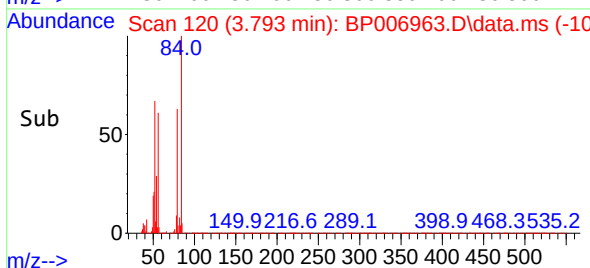



#6
Benzaldehyde
Concen: 4.374 ng/ul
RT: 7.057 min Scan# 675
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07



Tgt Ion: 77 Resp: 82609
Ion Ratio Lower Upper
77 100
105 98.4 74.4 111.6
106 98.1 70.3 105.5




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM



#8
Phenol
Concen: 4.049 ng/ul
RT: 7.104 min Scan# 683
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23

Tgt Ion: 94 Resp: 124047
Ion Ratio Lower Upper
94 100
65 26.5 24.4 36.6
66 35.5 31.8 47.6






#10

Bis(2-Chloroethyl)ether
Concen: 4.341 ng/ul
RT: 7.346 min Scan# 724
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07



Tgt Ion:	93	Resp:	106470
Ion	Ratio	Lower	Upper
93	100		
63	73.4	59.7	89.5
95	32.2	25.3	37.9

Manual Integrations
APPROVED




mohammad
9/14/2021 2:48:05 PM




#12

2-Chlorophenol
Concen: 4.118 ng/ul
RT: 7.481 min Scan# 747
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23


Tgt Ion:	128	Resp:	101092
Ion	Ratio	Lower	Upper
128	100		
64	43.8	40.6	60.8
130	32.3	26.4	39.6





#13
2-Methylphenol
Concen: 3.802 ng/ul
RT: 8.357 min Scan# 896
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07




Tgt Ion: 108 Resp: 88454
Ion Ratio Lower Upper
108 100
107 85.0 72.2 108.2

Manual Integrations
APPROVED



mohammad
9/14/2021 2:48:05 PM




#14
2,2'-oxybis(1-Chloropropane)
Concen: 4.379 ng/ul
RT: 8.457 min Scan# 913
Delta R.T. 0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Tgt Ion: 45 Resp: 124079
Ion Ratio Lower Upper
45 100
77 18.3 13.8 20.8
79 14.1 10.9 16.3

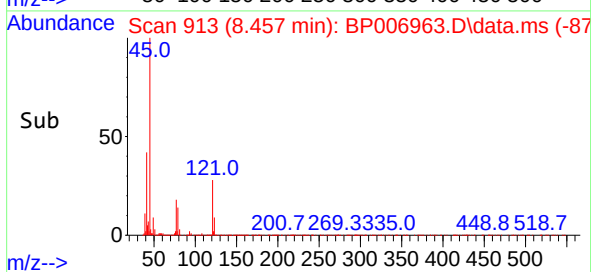



#16
Acetophenone
Concen: 4.524 ng/ul
RT: 8.746 min Scan# 962
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07




Tgt Ion:105 Resp: 161465
Ion Ratio Lower Upper
105 100
77 69.3 67.0 100.4
51 25.2 19.0 28.6

Manual Integrations
APPROVED



mohammad
9/14/2021 2:48:05 PM




#17
N-Nitroso-di-n-propylamine
Concen: 4.507 ng/ul
RT: 8.734 min Scan# 960
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23



Tgt Ion: 70 Resp: 74963
Ion Ratio Lower Upper
70 100
42 56.8 40.4 60.6
101 10.8 7.2 10.8#
130 23.4 14.9 22.3#

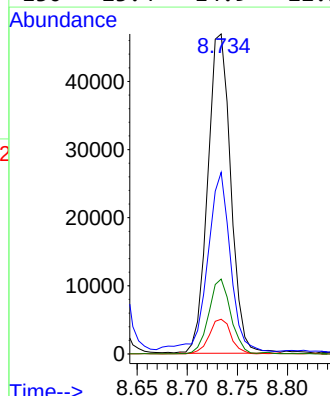







#18
4-Methylphenol
Concen: 4.078 ng/ul
RT: 8.687 min Scan# 952
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07

Tgt Ion:108 Resp: 101756
Ion Ratio Lower Upper
108 100
107 116.7 88.6 133.0




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM

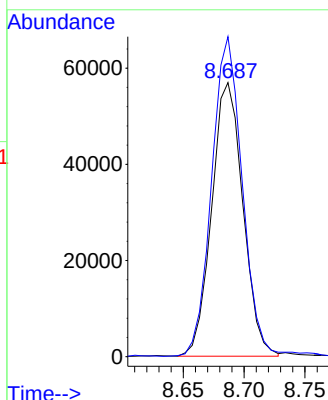

#19
Hexachloroethane
Concen: 4.007 ng/ul
RT: 9.004 min Scan# 1006
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23


Tgt Ion:117 Resp: 40058
Ion Ratio Lower Upper
117 100
201 97.8 68.2 102.2
199 60.6 43.5 65.3

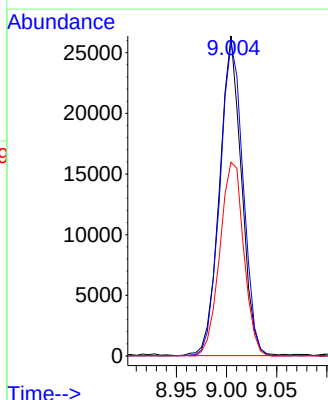

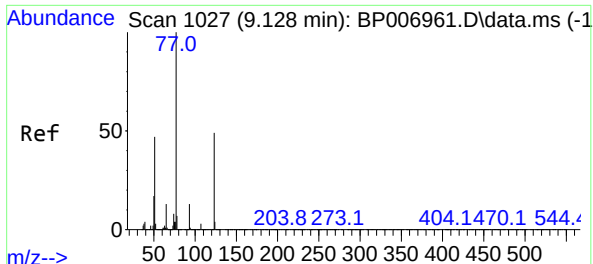

#22
Nitrobenzene
Concen: 4.264 ng/ul
RT: 9.122 min Scan# 1026
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07

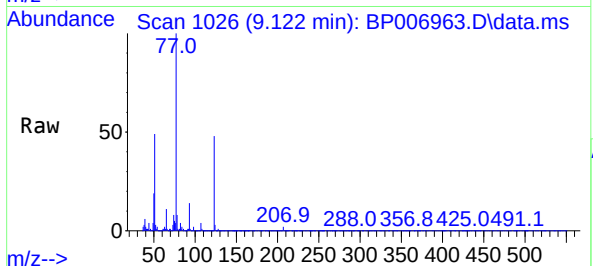


Tgt Ion: 77 Resp: 108836
Ion Ratio Lower Upper
77 100
123 47.5 31.1 46.7#
65 11.3 10.6 16.0

Manual Integrations
APPROVED



mohammad
9/14/2021 2:48:05 PM

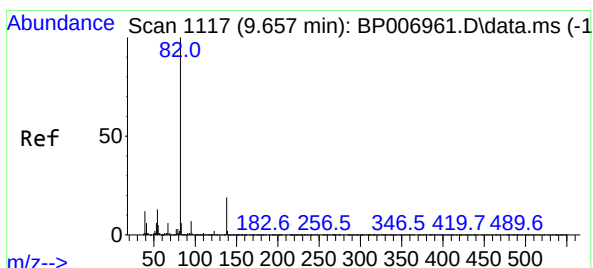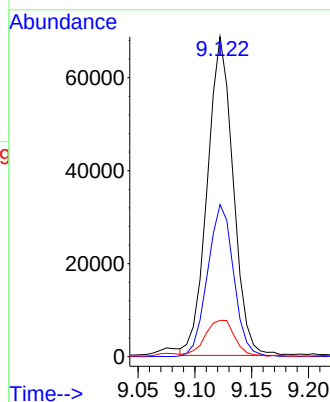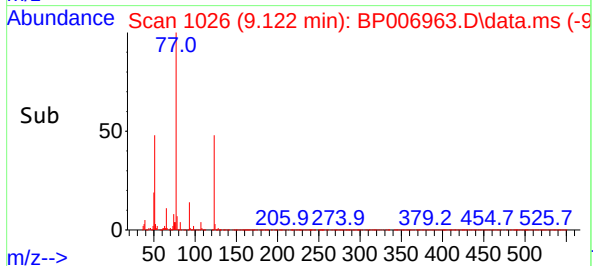


#23
Isophorone
Concen: 4.019 ng/ul
RT: 9.651 min Scan# 1116
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23

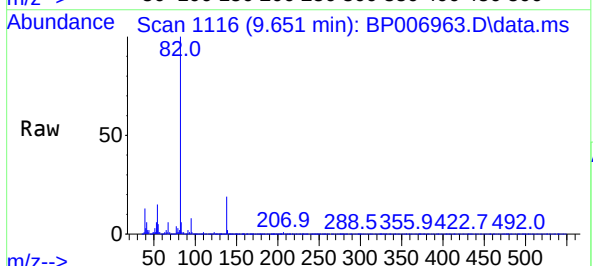

Tgt Ion: 82 Resp: 203739
Ion Ratio Lower Upper
82 100
95 7.5 5.8 8.8
138 18.6 12.5 18.7

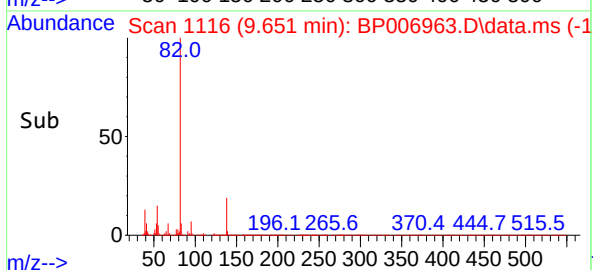

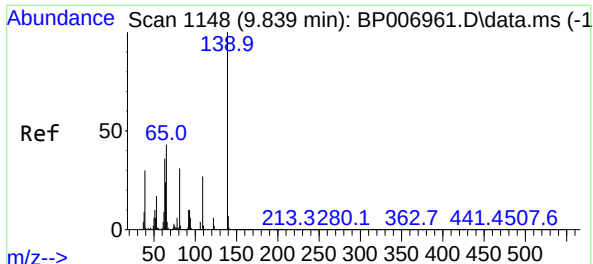





#25
2-Nitrophenol
Concen: 4.791 ng/ul
RT: 9.834 min Scan# 1147
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23

Tgt Ion	Ratio	Lower	Upper
139	100		
65	44.5	48.4	72.6#
109	26.3	28.2	42.2#

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM

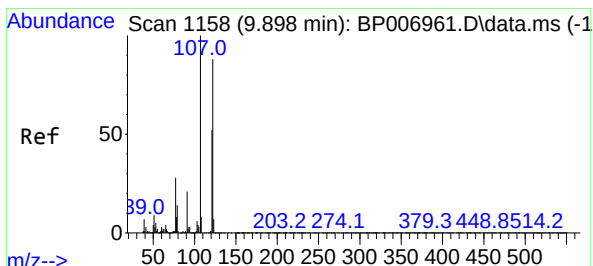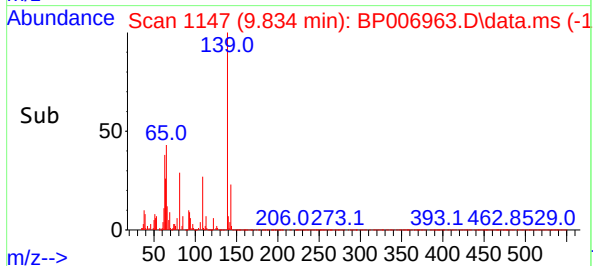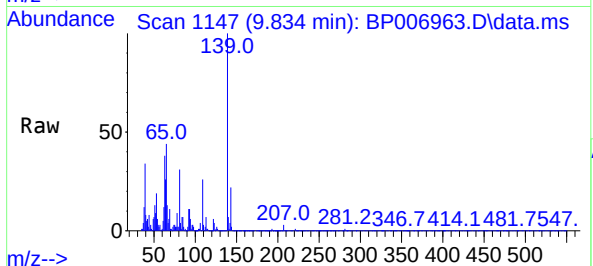

#26
2,4-Dimethylphenol
Concen: 3.892 ng/ul
RT: 9.893 min Scan# 1157
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23


Tgt Ion	Ratio	Lower	Upper
107	100		
121	54.3	38.1	57.1
122	90.5	64.2	96.4

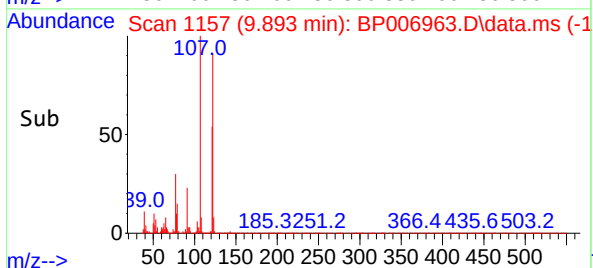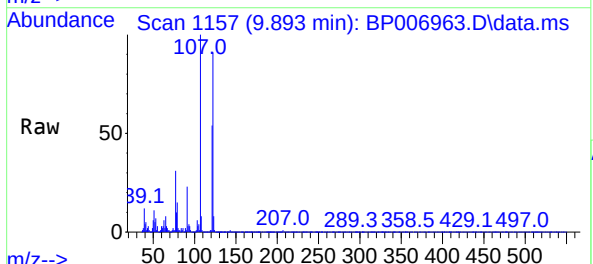



#27
Bis(2-Chloroethoxy)methane
Concen: 4.205 ng/ul
RT: 10.134 min Scan# 1198
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07



Tgt Ion: 93 Resp: 141110
Ion Ratio Lower Upper
93 100
95 33.1 25.6 38.4
123 11.4 8.2 12.4




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM



#29
2,4-Dichlorophenol
Concen: 4.196 ng/ul
RT: 10.369 min Scan# 1238
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23


Tgt Ion: 162 Resp: 101749
Ion Ratio Lower Upper
162 100
164 68.0 52.0 78.0
98 32.2 34.3 51.5#





#30
Naphthalene
Concen: 4.046 ng/ul
RT: 10.775 min Scan# 1307
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07



Tgt Ion:128 Resp: 341775
Ion Ratio Lower Upper
128 100
129 11.6 8.8 13.2
127 13.5 10.6 15.8




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM




#32
4-Chloroaniline
Concen: 4.172 ng/ul
RT: 10.881 min Scan# 1325
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23

Tgt Ion:127 Resp: 143865
Ion Ratio Lower Upper
127 100
129 30.2 25.7 38.5









#33
Hexachlorobutadiene
Concen: 3.825 ng/ul
RT: 11.063 min Scan# 1356
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23





Tgt Ion: 225 Resp: 63984
Ion Ratio Lower Upper
225 100
223 59.7 48.2 72.2
227 62.5 49.6 74.4



#34
Caprolactam
Concen: 3.934 ng/ul m
RT: 11.698 min Scan# 1464
Delta R.T. 0.041 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Tgt Ion: 113 Resp: 28432
Ion Ratio Lower Upper
113 100
55 149.6 125.8 188.6
56 98.9 98.2 147.2



Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07


Manual Integrations
APPROVED

mohammad
9/14/2021 2:48:05 PM



#35
4-Chloro-3-methylphenol
Concen: 3.739 ng/ul
RT: 11.998 min Scan# 1515
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07



Tgt Ion:107 Resp: 91946
Ion Ratio Lower Upper
107 100
144 27.8 18.8 28.2
142 83.7 58.4 87.6




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM



#36
2-Methylnaphthalene
Concen: 4.179 ng/ul
RT: 12.381 min Scan# 1580
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23


Tgt Ion:142 Resp: 236626
Ion Ratio Lower Upper
142 100
141 89.3 72.3 108.5





#37
1-Methylnaphthalene
Concen: 4.097 ng/ul
RT: 12.598 min Scan# 1617
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07




Tgt Ion:142 Resp: 236668
Ion Ratio Lower Upper
142 100
141 93.1 74.9 112.3
116 3.8 3.3 4.9

Manual Integrations
APPROVED



mohammad
9/14/2021 2:48:05 PM




#39
1,2,4,5-Tetrachlorobenzene
Concen: 3.843 ng/ul
RT: 12.745 min Scan# 1642
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23



Tgt Ion:216 Resp: 130837
Ion Ratio Lower Upper
216 100
214 75.7 64.3 96.5
179 20.1 19.3 28.9
108 16.3 19.8 29.6#

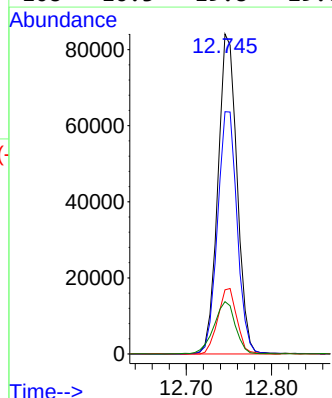







#40
Hexachlorocyclopentadiene
Concen: 4.586 ng/ul
RT: 12.734 min Scan# 1640
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07

Tgt Ion:237 Resp: 100772
Ion Ratio Lower Upper
237 100
235 63.7 50.4 75.6
272 13.8 9.7 14.5




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM



#41
2,4,6-Trichlorophenol
Concen: 3.623 ng/ul
RT: 12.987 min Scan# 1683
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23

Tgt Ion:196 Resp: 71393
Ion Ratio Lower Upper
196 100
198 99.0 76.2 114.4
200 31.4 24.6 36.8









#42
2,4,5-Trichlorophenol
Concen: 3.718 ng/ul
RT: 13.051 min Scan# 1694
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23

Tgt Ion:	196	Resp:	81684
Ion	Ratio	Lower	Upper
196	100		
198	98.2	79.3	118.9
200	30.9	25.8	38.8

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM



#43
1,1'-Biphenyl
Concen: 3.895 ng/ul
RT: 13.387 min Scan# 1751
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23


Tgt Ion:	154	Resp:	322463
Ion	Ratio	Lower	Upper
154	100		
153	40.9	32.4	48.6
76	13.3	12.9	19.3

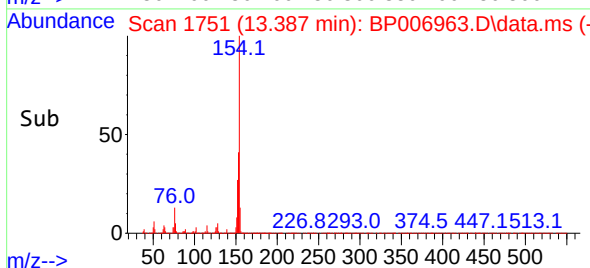



#44
2-Chloronaphthalene
Concen: 3.890 ng/ul
RT: 13.428 min Scan# 1758
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07



Tgt Ion:162 Resp: 248313
Ion Ratio Lower Upper
162 100
164 32.3 25.6 38.4
127 35.7 36.2 54.2#




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM



#45
2-Nitroaniline
Concen: 3.642 ng/ul m
RT: 13.628 min Scan# 1792
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23


Tgt Ion: 65 Resp: 47240
Ion Ratio Lower Upper
65 100
92 74.0 53.7 80.5
138 112.9 71.4 107.2#

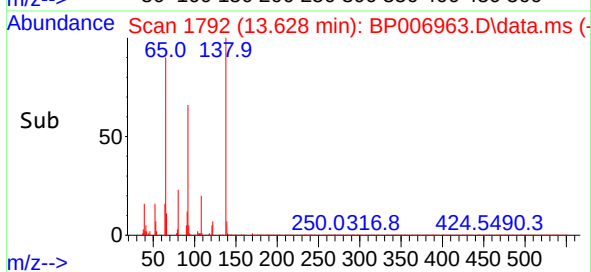



#47
Dimethylphthalate
Concen: 4.016 ng/ul
RT: 14.010 min Scan# 1857
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07




Tgt Ion:163 Resp: 311918
Ion Ratio Lower Upper
163 100
194 4.3 3.0 4.4
164 9.6 7.8 11.8

Manual Integrations
APPROVED



mohammad
9/14/2021 2:48:05 PM




#48
2,6-Dinitrotoluene
Concen: 3.539 ng/ul
RT: 14.122 min Scan# 1876
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Tgt Ion:165 Resp: 45902
Ion Ratio Lower Upper
165 100
89 60.3 62.2 93.2#
121 25.4 22.1 33.1





#50
Acenaphthylene
Concen: 3.800 ng/ul
RT: 14.275 min Scan# 1902
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07

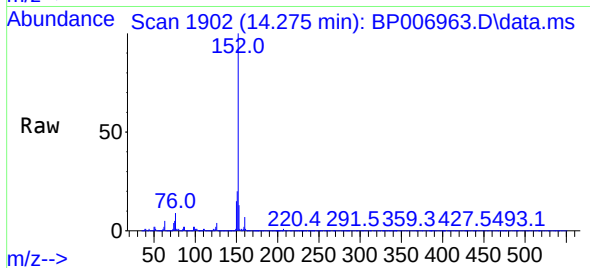

Tgt Ion:152 Resp: 384541
Ion Ratio Lower Upper
152 100
151 19.9 15.9 23.9
153 13.0 10.4 15.6




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM



#51
3-Nitroaniline
Concen: 3.209 ng/ul m
RT: 14.451 min Scan# 1932
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23


Tgt Ion:138 Resp: 47721
Ion Ratio Lower Upper
138 100
108 13.4 9.7 14.5
92 113.8 106.7 160.1

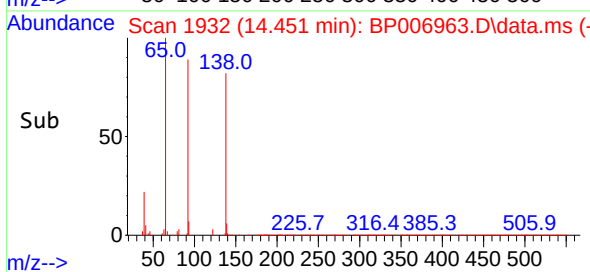



#52
Acenaphthene
Concen: 3.926 ng/ul
RT: 14.616 min Scan# 1960
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07




Tgt Ion:153 Resp: 263057
Ion Ratio Lower Upper
153 100
152 47.3 38.6 57.8
154 90.2 69.0 103.6

Manual Integrations
APPROVED



mohammad
9/14/2021 2:48:05 PM




#53
2,4-Dinitrophenol
Concen: 3.375 ng/ul
RT: 14.657 min Scan# 1967
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Tgt Ion:184 Resp: 24589
Ion Ratio Lower Upper
184 100
63 56.3 73.4 110.2#
154 61.0 59.4 89.0





#55
4-Nitrophenol
Concen: 4.010 ng/ul
RT: 14.751 min Scan# 1983
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07




Tgt Ion:109 Resp: 39431
Ion Ratio Lower Upper
109 100
139 138.3 90.3 135.5#
65 137.1 102.2 153.2

Manual Integrations
APPROVED



mohammad
9/14/2021 2:48:05 PM

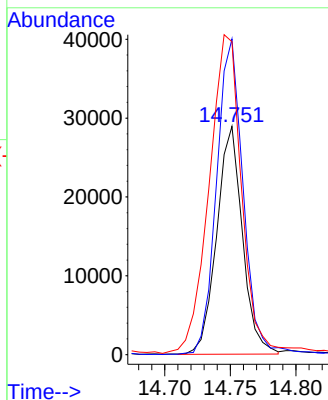


#56
Dibenzofuran
Concen: 3.924 ng/ul
RT: 14.945 min Scan# 2016
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Tgt Ion:168 Resp: 379451
Ion Ratio Lower Upper
168 100
139 35.6 35.3 52.9

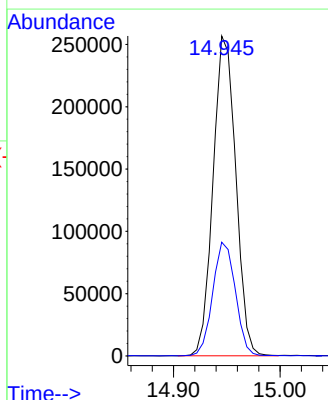



#57
2,4-Dinitrotoluene
Concen: 3.763 ng/ul
RT: 14.910 min Scan# 2010
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07




Tgt Ion:165 Resp: 69759
Ion Ratio Lower Upper
165 100
63 38.9 45.2 67.8#
182 3.1 1.9 2.9#

Manual Integrations
APPROVED



mohammad
9/14/2021 2:48:05 PM




#58
2,3,4,6-Tetrachlorophenol
Concen: 3.635 ng/ul
RT: 15.175 min Scan# 2055
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Tgt Ion:232 Resp: 64352
Ion Ratio Lower Upper
232 100
131 44.4 51.8 77.6#
130 2.4 3.1 4.7#
166 30.3 31.0 46.4#

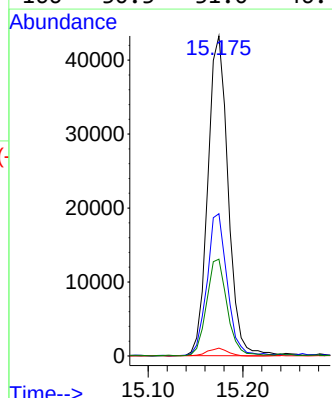



#59
Diethylphthalate
Concen: 3.925 ng/ul
RT: 15.369 min Scan# 2088
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07



Tgt Ion:149 Resp: 296816
Ion Ratio Lower Upper
149 100
177 21.2 15.5 23.3
150 11.8 9.9 14.9




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM



#61
Fluorene
Concen: 4.054 ng/ul
RT: 15.598 min Scan# 2127
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23


Tgt Ion:166 Resp: 312465
Ion Ratio Lower Upper
166 100
165 96.0 79.6 119.4
167 13.2 10.7 16.1





#62
4-Chlorophenyl-phenylether
Concen: 4.021 ng/ul
RT: 15.592 min Scan# 2126
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07



Tgt Ion:204 Resp: 158001
Ion Ratio Lower Upper
204 100
206 33.8 26.3 39.5
141 57.0 62.0 93.0#




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM



#63
4-Nitroaniline
Concen: 3.439 ng/ul m
RT: 15.610 min Scan# 2129
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23


Tgt Ion:138 Resp: 51050
Ion Ratio Lower Upper
138 100
92 49.8 47.1 70.7
108 72.0 73.8 110.8#

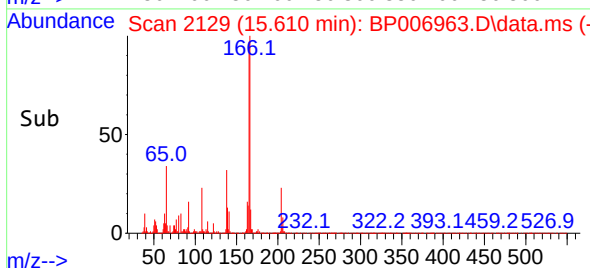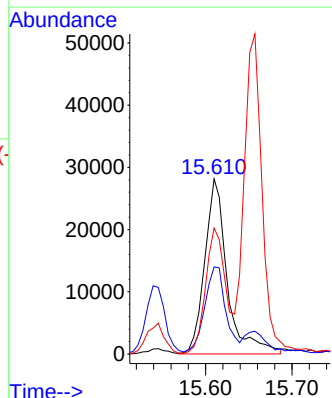



#66
4,6-Dinitro-2-methylphenol
Concen: 4.072 ng/ul
RT: 15.669 min Scan# 2139
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07




Tgt Ion:198 Resp: 44882
Ion Ratio Lower Upper
198 100
182 9.5 4.5 6.7#
77 35.6 31.7 47.5

Manual Integrations
APPROVED



mohammad
9/14/2021 2:48:05 PM




#67
N-Nitrosodiphenylamine
Concen: 4.032 ng/ul
RT: 15.804 min Scan# 2162
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23



Tgt Ion:169 Resp: 259821
Ion Ratio Lower Upper
169 100
168 67.8 53.9 80.9
167 36.3 30.0 45.0









#68
4-Bromophenyl-phenylether
Concen: 3.828 ng/ul
RT: 16.492 min Scan# 2279
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23

Tgt Ion:	248	Resp:	88555
Ion Ratio	Lower	Upper	
248	100		
250	95.0	78.4	117.6
141	63.1	80.6	121.0#

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM



#69
Hexachlorobenzene
Concen: 3.898 ng/ul
RT: 16.604 min Scan# 2298
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23

Tgt Ion:	284	Resp:	104552
Ion Ratio	Lower	Upper	
284	100		
142	31.9	37.8	56.6#
249	30.1	27.1	40.7

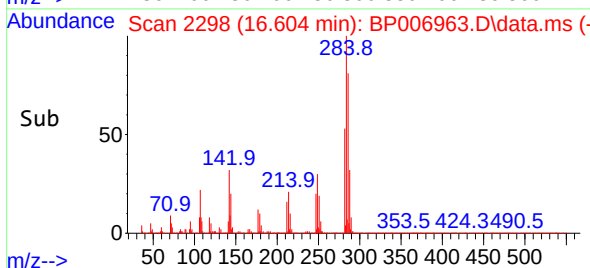







#70
Atrazine
Concen: 3.385 ng/ul
RT: 16.757 min Scan# 2324
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23

Tgt Ion:	200	Resp:	82609
Ion Ratio	Lower	Upper	
200	100		
173	28.7	22.2	33.4
215	50.1	35.4	53.0

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM



#71
Pentachlorophenol
Concen: 3.706 ng/ul
RT: 16.951 min Scan# 2357
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23


Tgt Ion:	266	Resp:	56946
Ion Ratio	Lower	Upper	
266	100		
264	62.5	51.0	76.4
268	58.2	49.4	74.2





#72
Phenanthrene
Concen: 3.961 ng/ul
RT: 17.339 min Scan# 2423
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07



Tgt Ion:178 Resp: 482765
Ion Ratio Lower Upper
178 100
179 15.2 12.0 18.0
176 19.3 15.6 23.4




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM



#74
Anthracene
Concen: 4.053 ng/ul
RT: 17.433 min Scan# 2439
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23


Tgt Ion:178 Resp: 491078
Ion Ratio Lower Upper
178 100
179 15.7 12.1 18.1
176 18.8 14.9 22.3





#75
1,2,3,4-Tetrachlorobenzene
Concen: 3.598 ng/uL
RT: 13.351 min Scan# 1745
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07



Tgt Ion:216 Resp: 123383
Ion Ratio Lower Upper
216 100
214 78.9 62.9 94.3
218 50.0 37.8 56.8




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM



#76
Pentachlorobenzene
Concen: 3.819 ng/uL
RT: 14.869 min Scan# 2003
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23


Tgt Ion:250 Resp: 126771
Ion Ratio Lower Upper
250 100
248 61.6 51.0 76.6
252 62.5 51.0 76.4

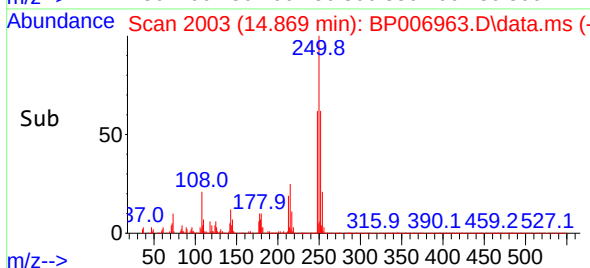



#77
Carbazole
Concen: 3.699 ng/ul
RT: 17.698 min Scan# 2484
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07




Tgt Ion:167 Resp: 398351
Ion Ratio Lower Upper
167 100
166 21.4 17.6 26.4
139 13.1 11.9 17.9

Manual Integrations
APPROVED



mohammad
9/14/2021 2:48:05 PM

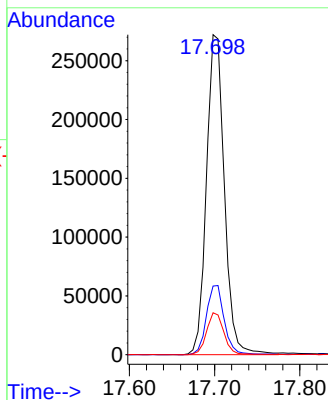


#78
Di-n-butylphthalate
Concen: 3.553 ng/ul
RT: 18.257 min Scan# 2579
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Tgt Ion:149 Resp: 433627
Ion Ratio Lower Upper
149 100
150 9.0 7.3 10.9
104 4.8 4.8 7.2#

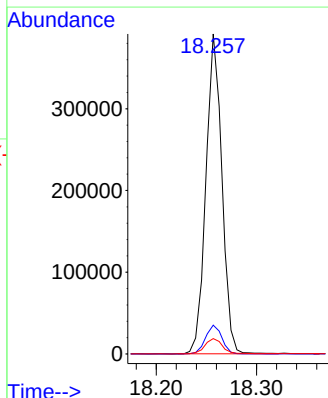



#80
Fluoranthene
Concen: 4.141 ng/ul
RT: 19.304 min Scan# 2757
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07




Tgt Ion:202 Resp: 528928
Ion Ratio Lower Upper
202 100
101 10.8 11.0 16.4#
100 8.3 8.3 12.5#

Manual Integrations
APPROVED



mohammad
9/14/2021 2:48:05 PM




#82
Pyrene
Concen: 4.342 ng/ul
RT: 19.657 min Scan# 2817
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Tgt Ion:202 Resp: 568897
Ion Ratio Lower Upper
202 100
101 13.1 12.6 19.0
100 10.8 10.6 15.8





#83
Butylbenzylphthalate
Concen: 3.697 ng/ul
RT: 20.533 min Scan# 2966
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07



Tgt Ion:149 Resp: 168674
Ion Ratio Lower Upper
149 100
91 67.8 63.0 94.6
206 21.3 14.1 21.1#




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM



#84
3,3'-Dichlorobenzidine
Concen: 4.003 ng/ul
RT: 21.298 min Scan# 3096
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23

Tgt Ion:252 Resp: 182165
Ion Ratio Lower Upper
252 100
254 65.1 51.6 77.4
126 11.2 10.7 16.1

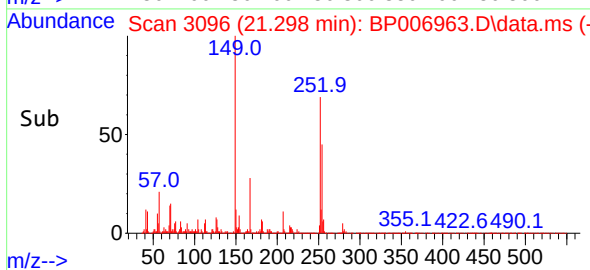







#85
Benzo(a)anthracene
Concen: 3.978 ng/ul
RT: 21.363 min Scan# 3107
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23

Tgt Ion:	228	Resp:	507933
Ion Ratio	Lower	Upper	
228	100		
229	19.3	15.8	23.8
226	26.7	21.6	32.4

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM



#86
Bis(2-ethylhexyl)phthalate
Concen: 3.654 ng/ul
RT: 21.292 min Scan# 3095
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23


Tgt Ion:	149	Resp:	248514
Ion Ratio	Lower	Upper	
149	100		
167	27.0	20.2	30.2
279	4.1	2.7	4.1





#87
Chrysene
Concen: 3.916 ng/ul
RT: 21.416 min Scan# 3116
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07



Tgt Ion:228 Resp: 494759
Ion Ratio Lower Upper
228 100
226 29.4 24.5 36.7
229 19.8 15.9 23.9




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM

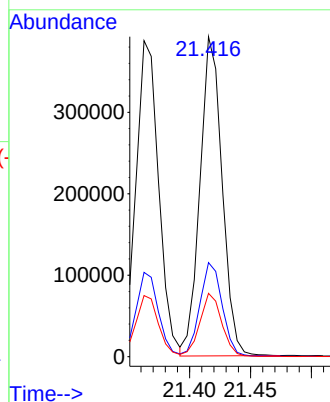

#89
Di-n-octyl phthalate
Concen: 3.607 ng/ul
RT: 22.227 min Scan# 3254
Delta R.T. 0.000 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23

Tgt Ion:149 Resp: 377279

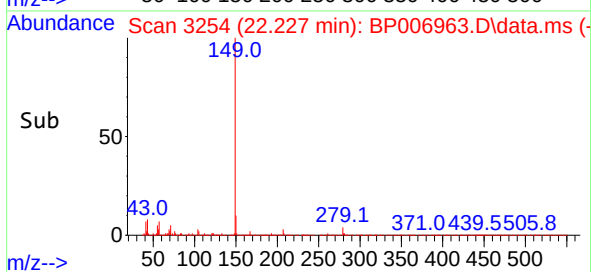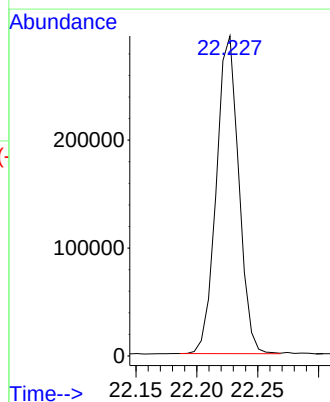







#90
Benzo(b)fluoranthene
Concen: 3.907 ng/ul
RT: 23.062 min Scan# 3396
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23

Tgt Ion:252 Resp: 462653
Ion Ratio Lower Upper
252 100
253 22.0 17.7 26.5
125 10.6 10.1 15.1

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07




Manual Integrations
APPROVED


mohammad
9/14/2021 2:48:05 PM



#91
Benzo(k)fluoranthene
Concen: 4.047 ng/ul
RT: 23.110 min Scan# 3404
Delta R.T. -0.011 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23


Tgt Ion:252 Resp: 448613
Ion Ratio Lower Upper
252 100
253 22.0 17.2 25.8
125 9.8 9.4 14.0

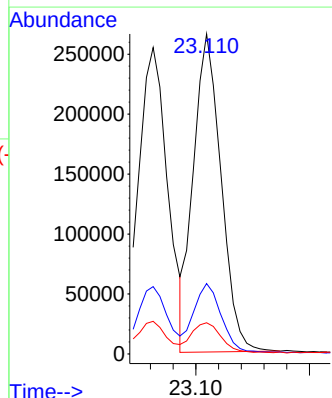



#93
Benzo(a)pyrene
Concen: 3.795 ng/ul
RT: 23.698 min Scan# 3504
Delta R.T. -0.006 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07




Tgt Ion:252 Resp: 432324
Ion Ratio Lower Upper
252 100
253 22.5 17.6 26.4
125 12.0 11.3 16.9

Manual Integrations
APPROVED



mohammad
9/14/2021 2:48:05 PM




#94
Indeno(1,2,3-cd)pyrene
Concen: 3.437 ng/ul
RT: 26.339 min Scan# 3953
Delta R.T. -0.012 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Tgt Ion:276 Resp: 454301
Ion Ratio Lower Upper
276 100
138 23.8 21.8 32.8
277 24.9 19.9 29.9





#95
Dibenzo(a,h)anthracene
Concen: 3.359 ng/ul
RT: 26.356 min Scan# 3956
Delta R.T. -0.017 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT4-2021-07



Tgt Ion:278 Resp: 384149
Ion Ratio Lower Upper
278 100
139 17.0 15.4 23.2
279 22.9 19.0 28.4

Manual Integrations
APPROVED

mohammad
9/14/2021 2:48:05 PM



#96
Benzo(g,h,i)perylene
Concen: 3.302 ng/ul
RT: 27.115 min Scan# 4085
Delta R.T. -0.017 min
Lab File: BP006963.D
Acq: 13 Sep 2021 16:23

Tgt Ion:276 Resp: 374244
Ion Ratio Lower Upper
276 100
138 22.2 20.7 31.1
277 24.8 19.0 28.4

