

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091321\
 Data File : BP006962.D
 Acq On : 13 Sep 2021 13:28
 Operator : CG/JU
 Sample : PB139010BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK010

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006962.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	41	45	52	rBV	136232	179402	1.64%	0.163%
2	3.770	113	116	136	rBV	1423540	2322447	21.25%	2.114%
3	4.099	168	172	177	rVB	22784	33302	0.30%	0.030%
4	7.081	670	679	690	rBV	1763692	2783190	25.46%	2.533%
5	7.252	702	708	720	rBV	1449291	2335575	21.37%	2.125%
6	7.452	734	742	756	rBV	1872938	3008992	27.53%	2.738%
7	7.922	815	822	833	rVB	1312023	2068968	18.93%	1.883%
8	8.628	934	942	957	rBV	2238360	3612609	33.05%	3.288%
9	9.081	1011	1019	1031	rBV	1689652	2760722	25.26%	2.512%
10	9.805	1134	1142	1156	rBV	1374949	2212672	20.24%	2.014%
11	10.340	1225	1233	1250	rBV	2250286	3783402	34.62%	3.443%
12	10.722	1290	1298	1307	rBV	1838890	3134675	28.68%	2.853%
13	10.858	1314	1321	1342	rBV	2230229	3884885	35.54%	3.535%
14	12.310	1561	1568	1577	rVB2	44188	75675	0.69%	0.069%
15	13.528	1765	1775	1780	rBV2	9592	20987	0.19%	0.019%
16	13.963	1842	1849	1862	rBV	4387732	6033324	55.20%	5.491%
17	14.246	1887	1897	1913	rBV	5029145	7400612	67.71%	6.735%
18	14.551	1942	1949	1960	rBV	3225716	4609710	42.18%	4.195%
19	14.734	1974	1980	2001	rBV	1816477	2713652	24.83%	2.470%
20	15.546	2110	2118	2131	rBV	6485504	9249679	84.63%	8.418%
21	15.657	2131	2137	2152	rVV	1687583	2423996	22.18%	2.206%
22	15.781	2154	2158	2163	rVB	78634	114703	1.05%	0.104%
23	16.216	2224	2232	2237	rBV	9734	26094	0.24%	0.024%
24	16.328	2246	2251	2256	rVB5	25080	36869	0.34%	0.034%
25	16.975	2358	2361	2367	rBV5	12986	19891	0.18%	0.018%
26	17.087	2376	2380	2389	rVB2	20036	37947	0.35%	0.035%
27	17.298	2409	2416	2426	rBV	3756735	5312754	48.61%	4.835%
28	17.398	2426	2433	2454	rVV	6657601	9654762	88.33%	8.786%
29	17.922	2520	2522	2527	rVB6	8618	12379	0.11%	0.011%
30	18.257	2575	2579	2585	rVB3	20322	34053	0.31%	0.031%
31	18.692	2650	2653	2658	rBV7	13457	17605	0.16%	0.016%
32	19.204	2737	2740	2745	rBV5	28130	35144	0.32%	0.032%
33	19.275	2748	2752	2757	rVB	78523	108973	1.00%	0.099%
34	19.522	2790	2794	2799	rBV	62163	86169	0.79%	0.078%
35	19.634	2807	2813	2823	rBV	8056271	10929754	100.00%	9.946%
36	21.381	3105	3110	3118	rBV	3940900	5066480	46.35%	4.611%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091321\
Data File : BP006962.D
Acq On : 13 Sep 2021 13:28
Operator : CG/JU
Sample : PB139010BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK010

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Title : SVOA CALIBRATION

37	23.651	3489	3496	3504	rBV2	4482659	8975946	82.12%	8.168%
38	23.810	3516	3523	3536	rVB2	2300062	4767911	43.62%	4.339%




Sum of corrected areas: 109885910

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091321\
Data File : BP006962.D
Acq On : 13 Sep 2021 13:28
Operator : CG/JU
Sample : PB139010BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK010

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

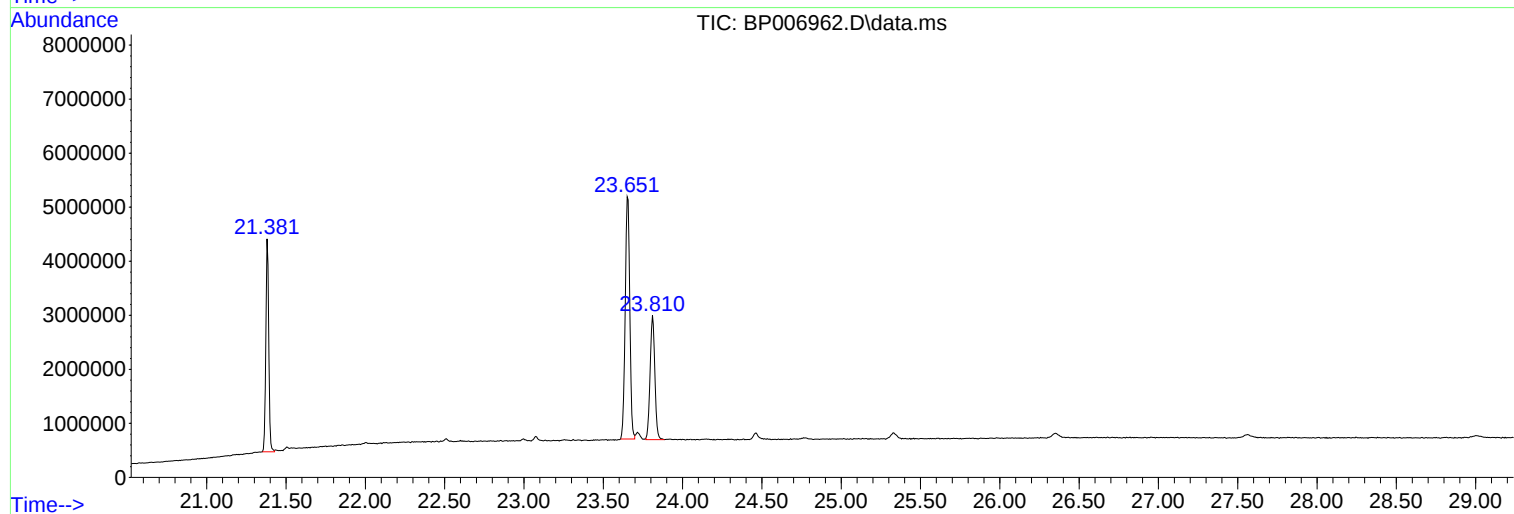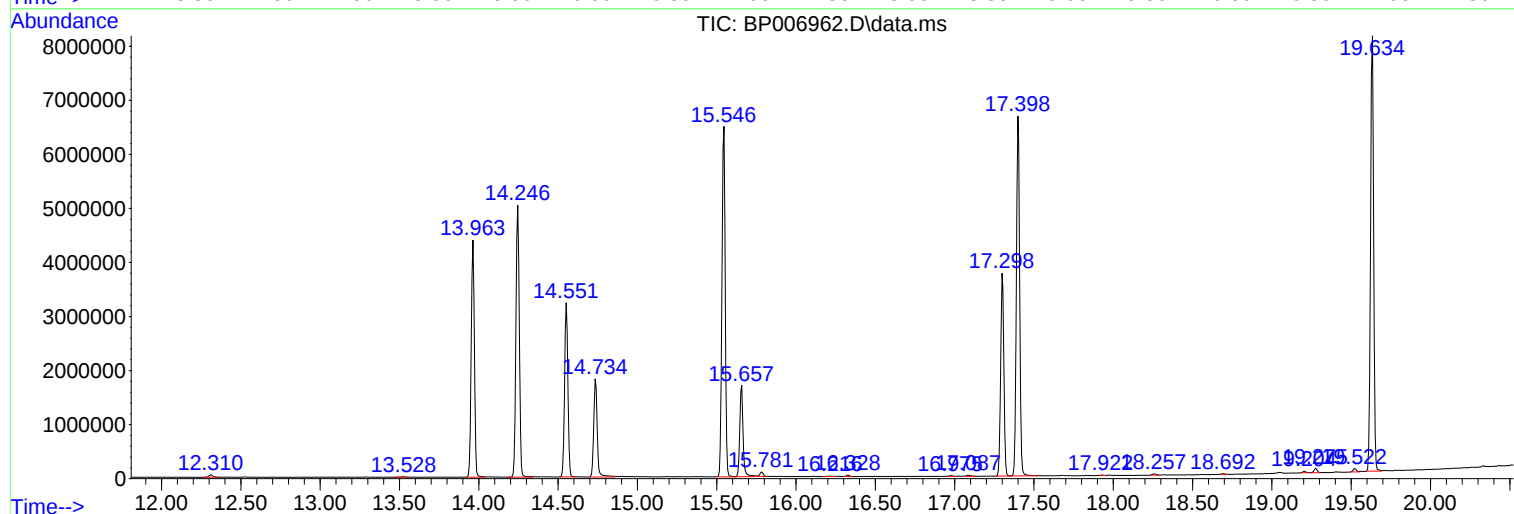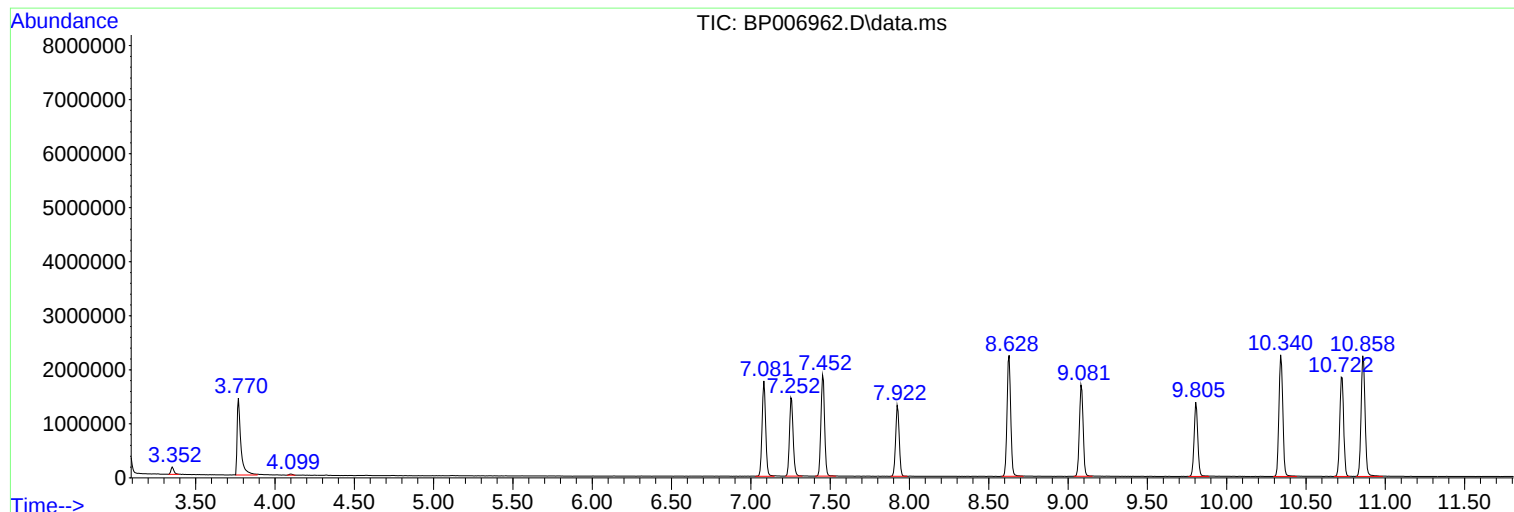

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091321\
Data File : BP006962.D
Acq On : 13 Sep 2021 13:28
Operator : CG/JU
Sample : PB139010BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK010

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091321\
Data File : BP006962.D
Acq On : 13 Sep 2021 13:28
Operator : CG/JU
Sample : PB139010BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK010

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP090821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc