



2-Nitrophenol

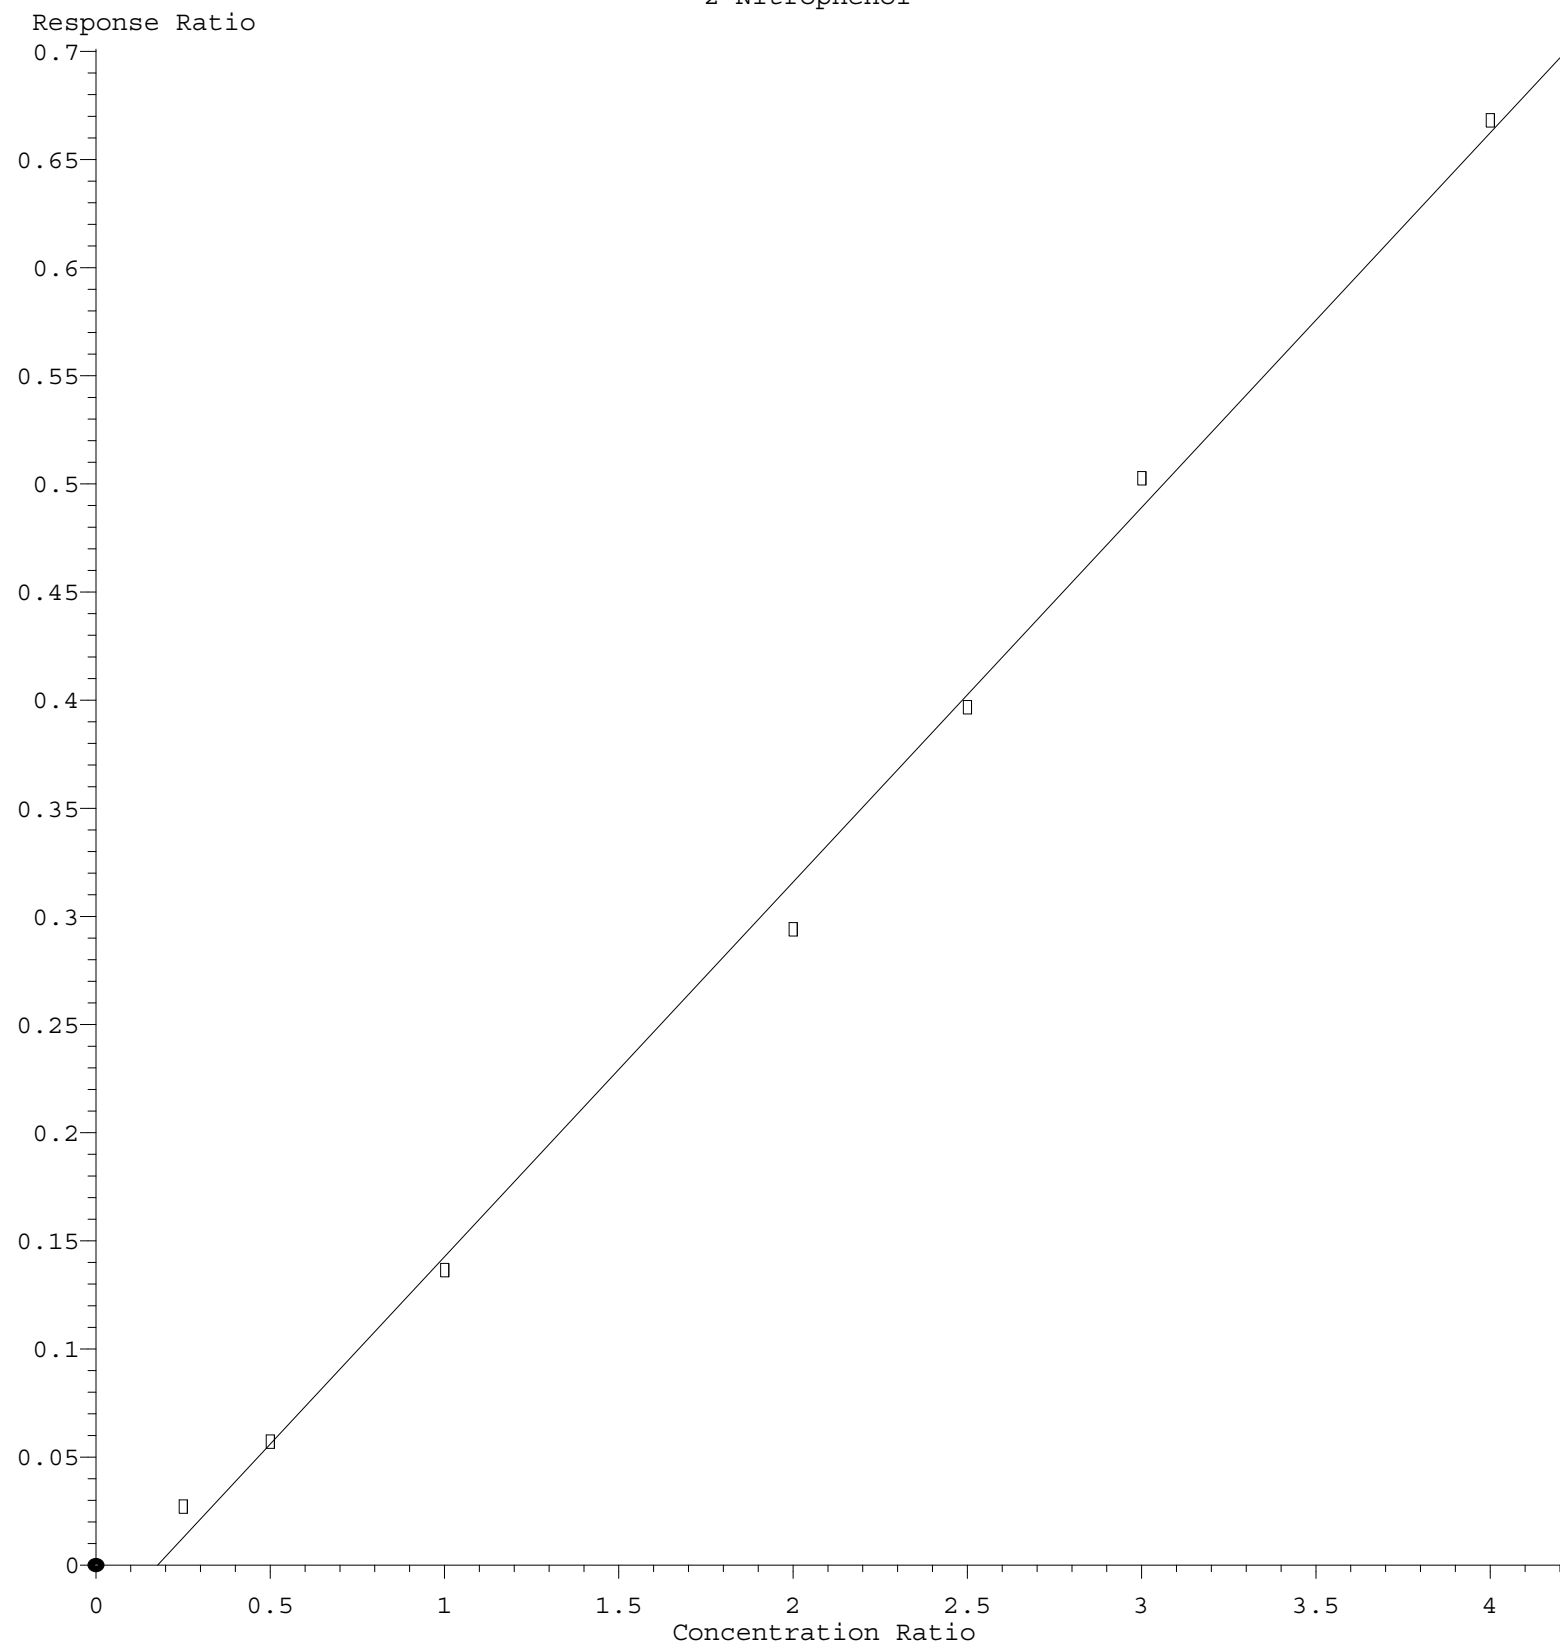

Response = $1.734e-001 * \text{Amt} - 3.075e-002$
 Coef of Det (r^2) = 0.997194 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP091322.M
 Calibration Table Last Updated: Tue Sep 13 15:49:51 2022

2-Nitroaniline

Response Ratio

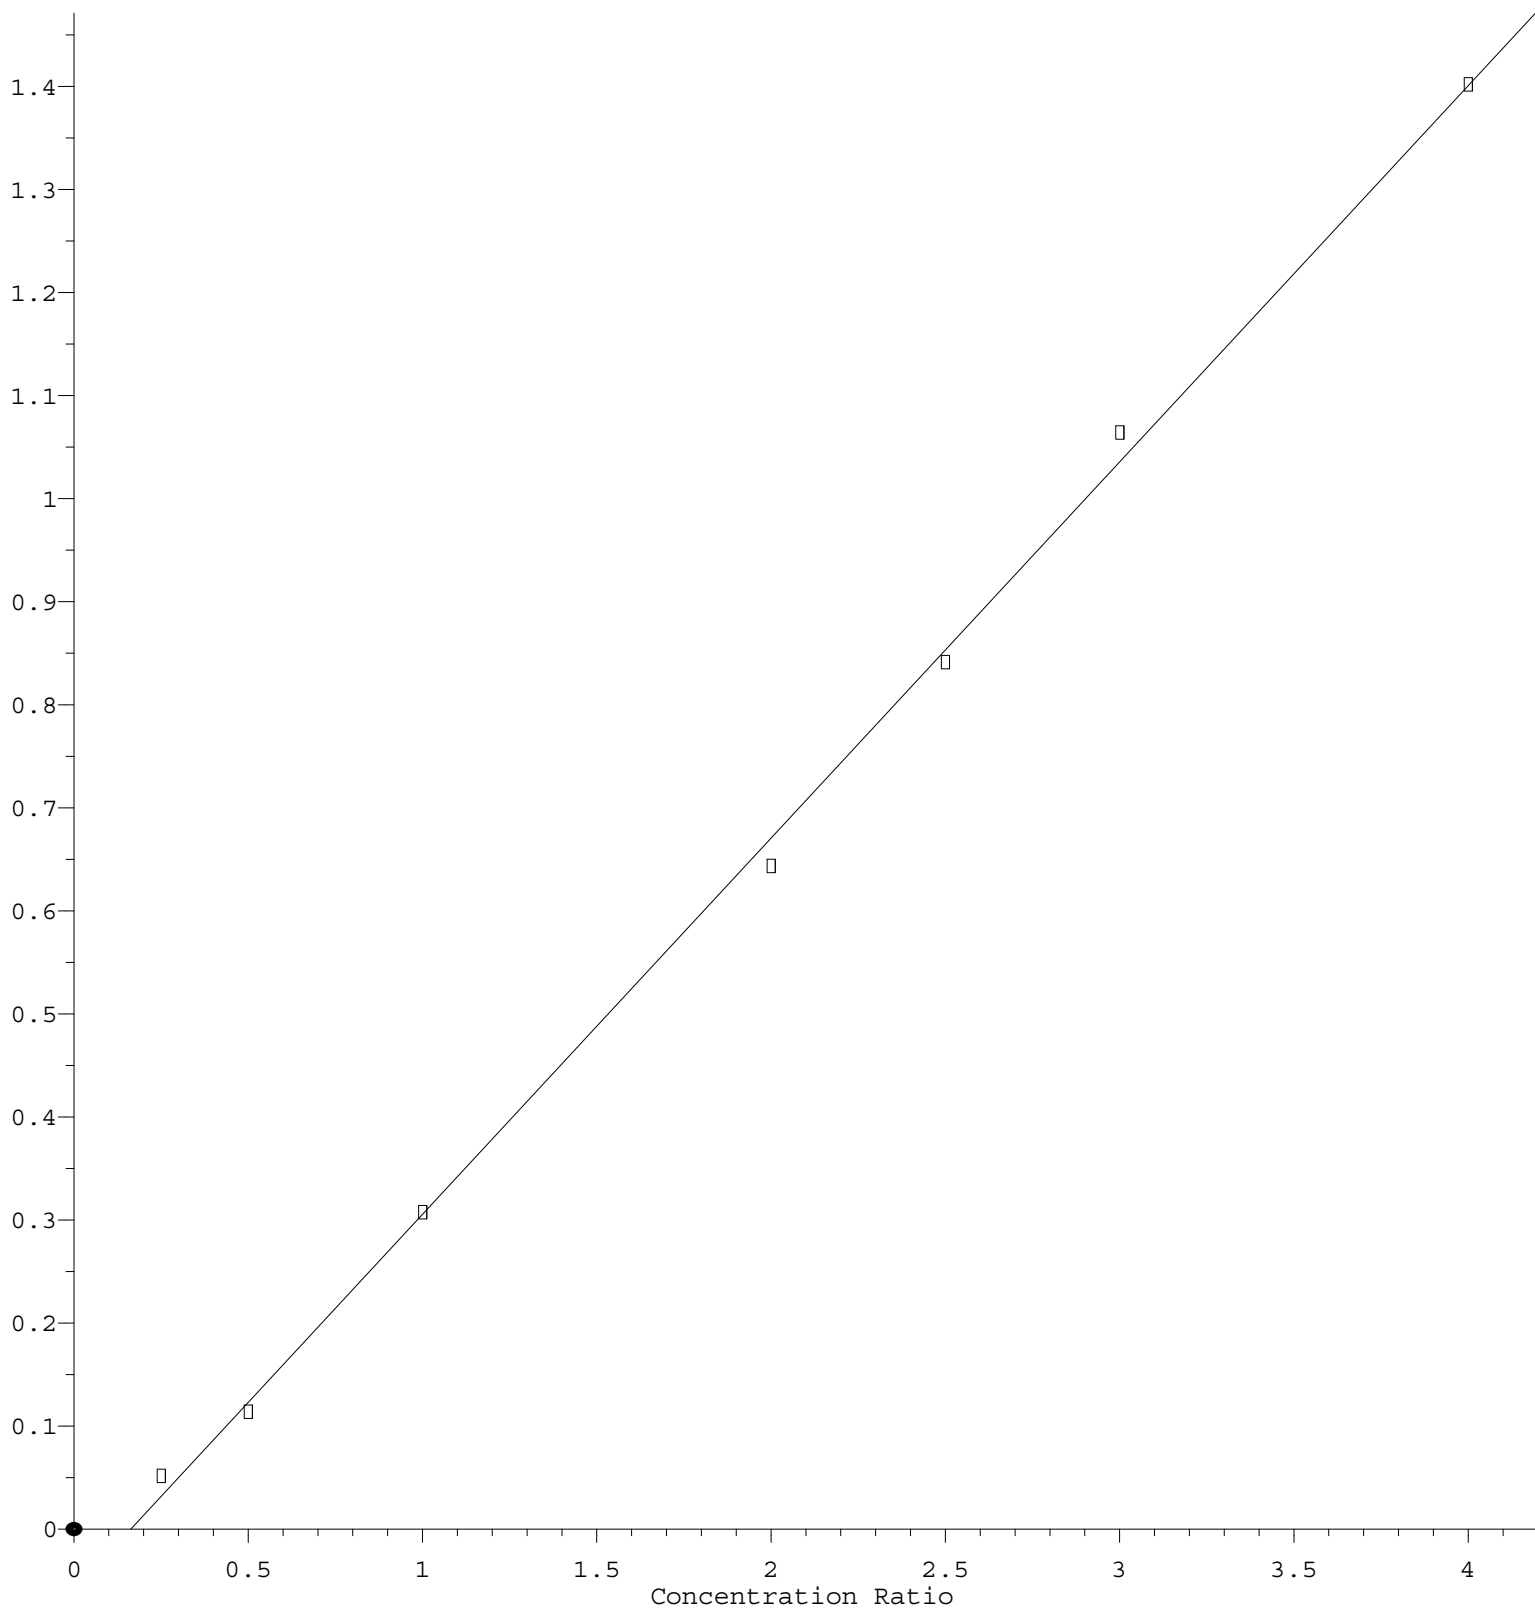

$$\text{Response} = 3.652\text{e-}001 * \text{Amt} - 5.936\text{e-}002$$


Coef of Det (r^2) = 0.998592 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP091322.M

Calibration Table Last Updated: Tue Sep 13 15:49:51 2022

Benzoic acid

Response Ratio

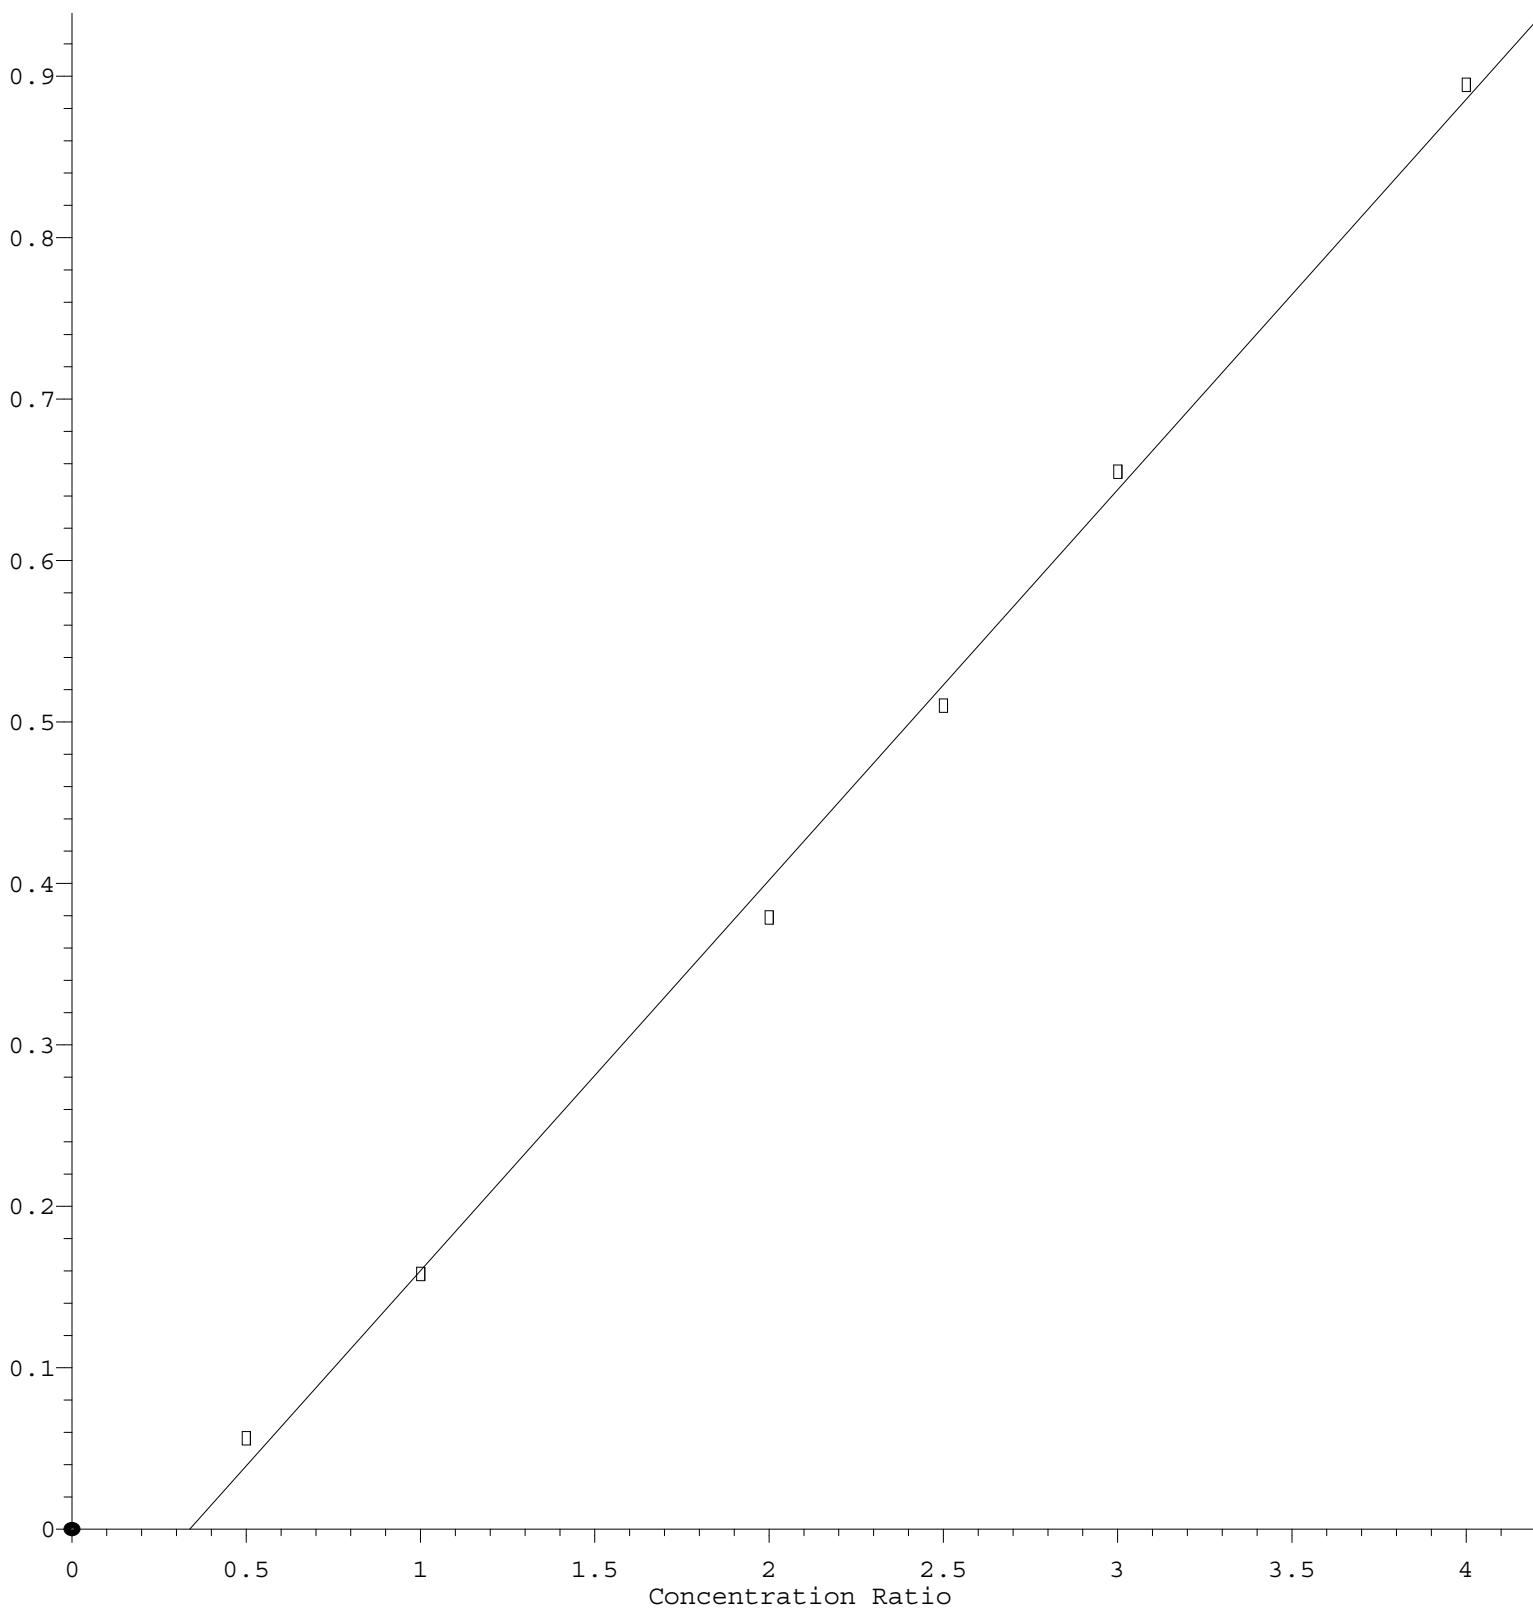


$$\text{Response} = 2.418\text{e-}001 * \text{Amt} - 8.163\text{e-}002$$

Coef of Det (r^2) = 0.997551 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP091322.M

Calibration Table Last Updated: Tue Sep 13 15:49:51 2022


2,4-Dinitrophenol

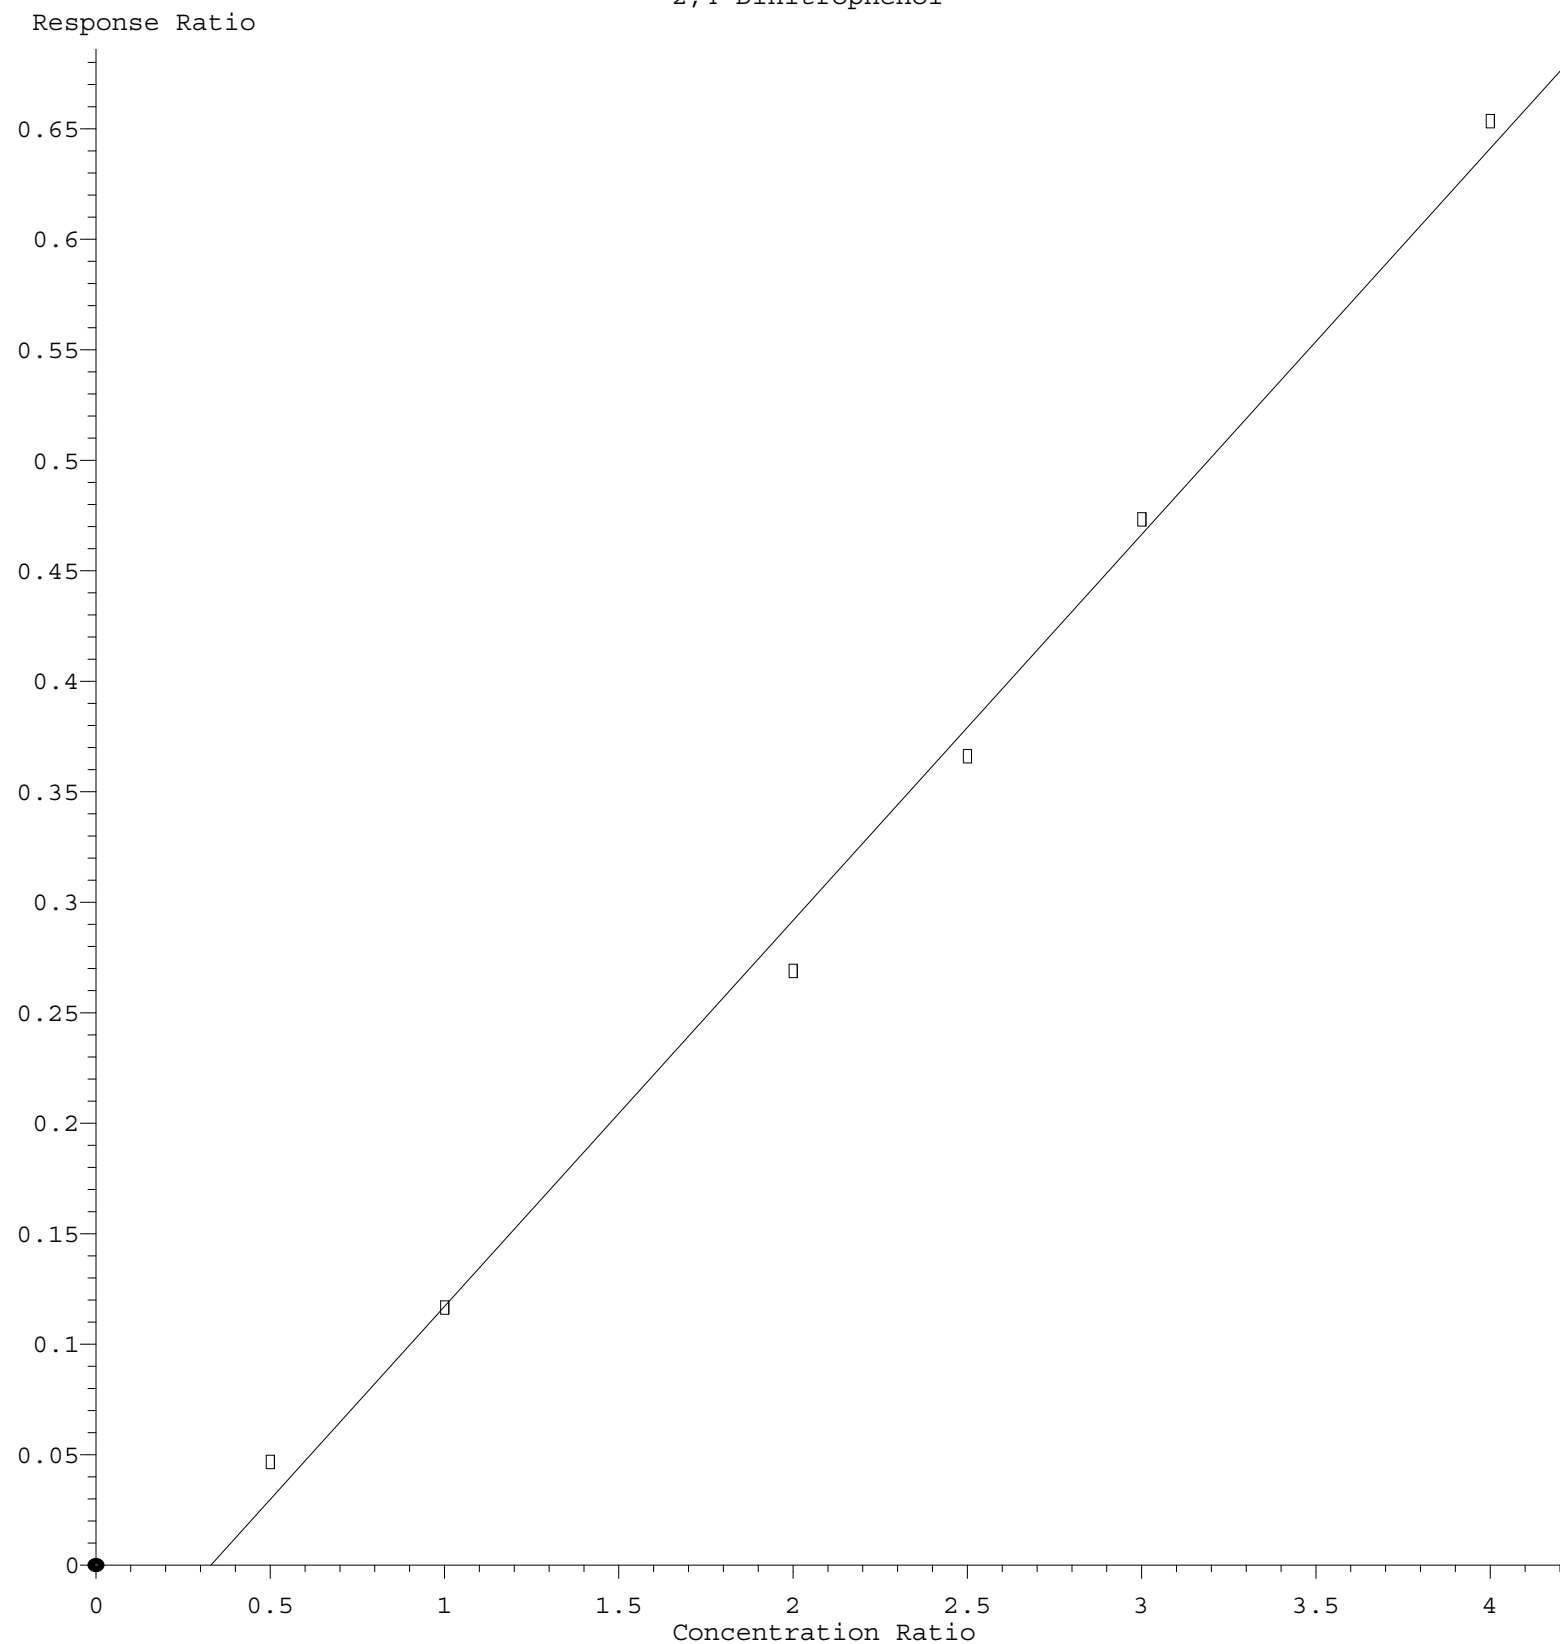

Response = $1.747 \times 10^{-1} \times \text{Amt} - 5.764 \times 10^{-2}$
 Coef of Det (r^2) = 0.995387 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP091322.M
 Calibration Table Last Updated: Tue Sep 13 15:49:51 2022

3-Nitroaniline

Response Ratio

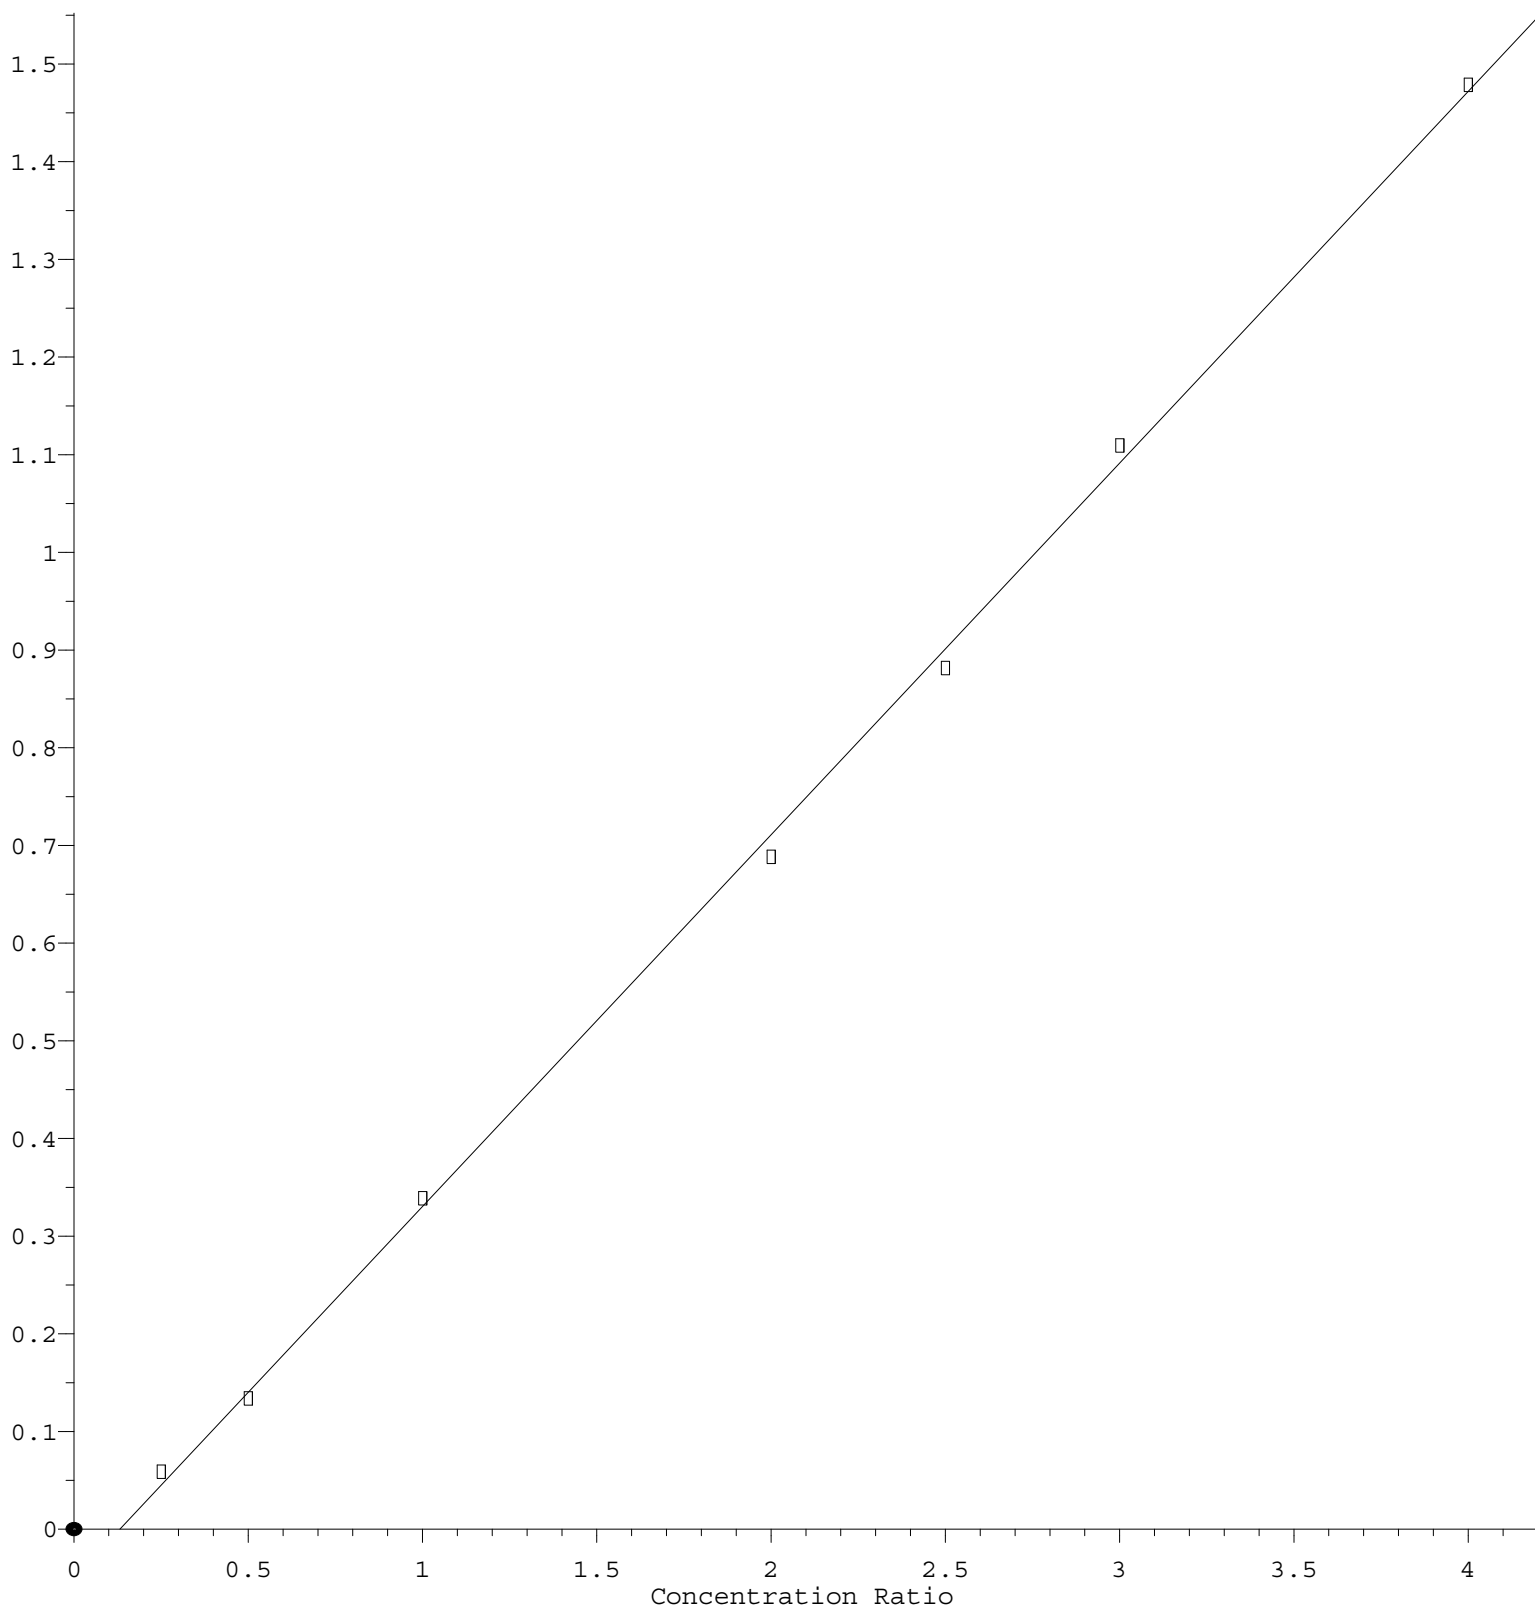

$$\text{Response} = 3.804\text{e-}001 * \text{Amt} - 5.013\text{e-}002$$


Coef of Det (r^2) = 0.999064 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP091322.M

Calibration Table Last Updated: Tue Sep 13 15:49:51 2022

2,4-Dinitrotoluene

Response Ratio

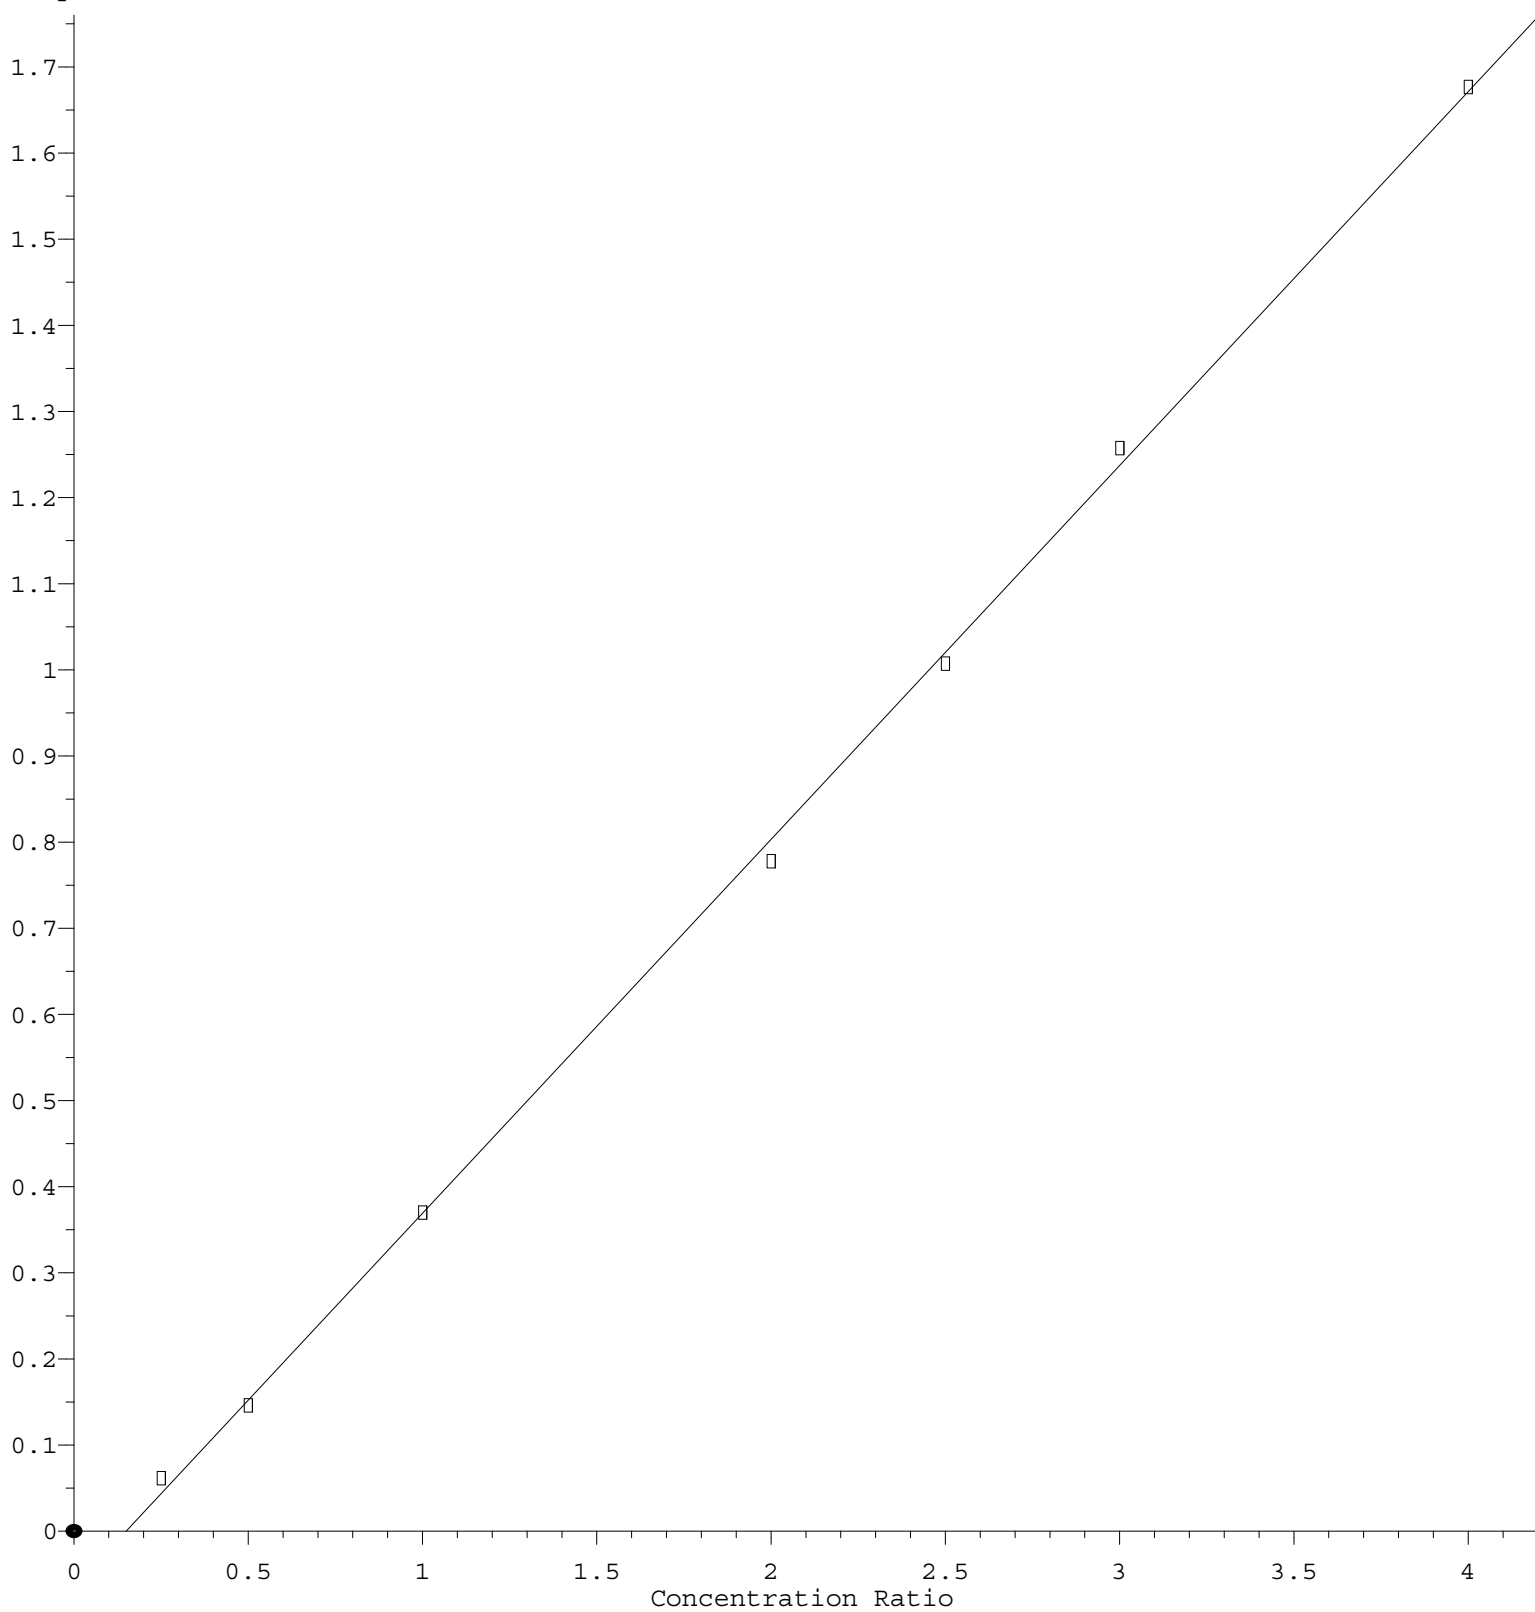

$$\text{Response} = 4.342\text{e-}001 * \text{Amt} - 6.523\text{e-}002$$


Coef of Det (r^2) = 0.999254 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP091322.M

Calibration Table Last Updated: Tue Sep 13 15:49:51 2022

4-Nitroaniline

Response Ratio

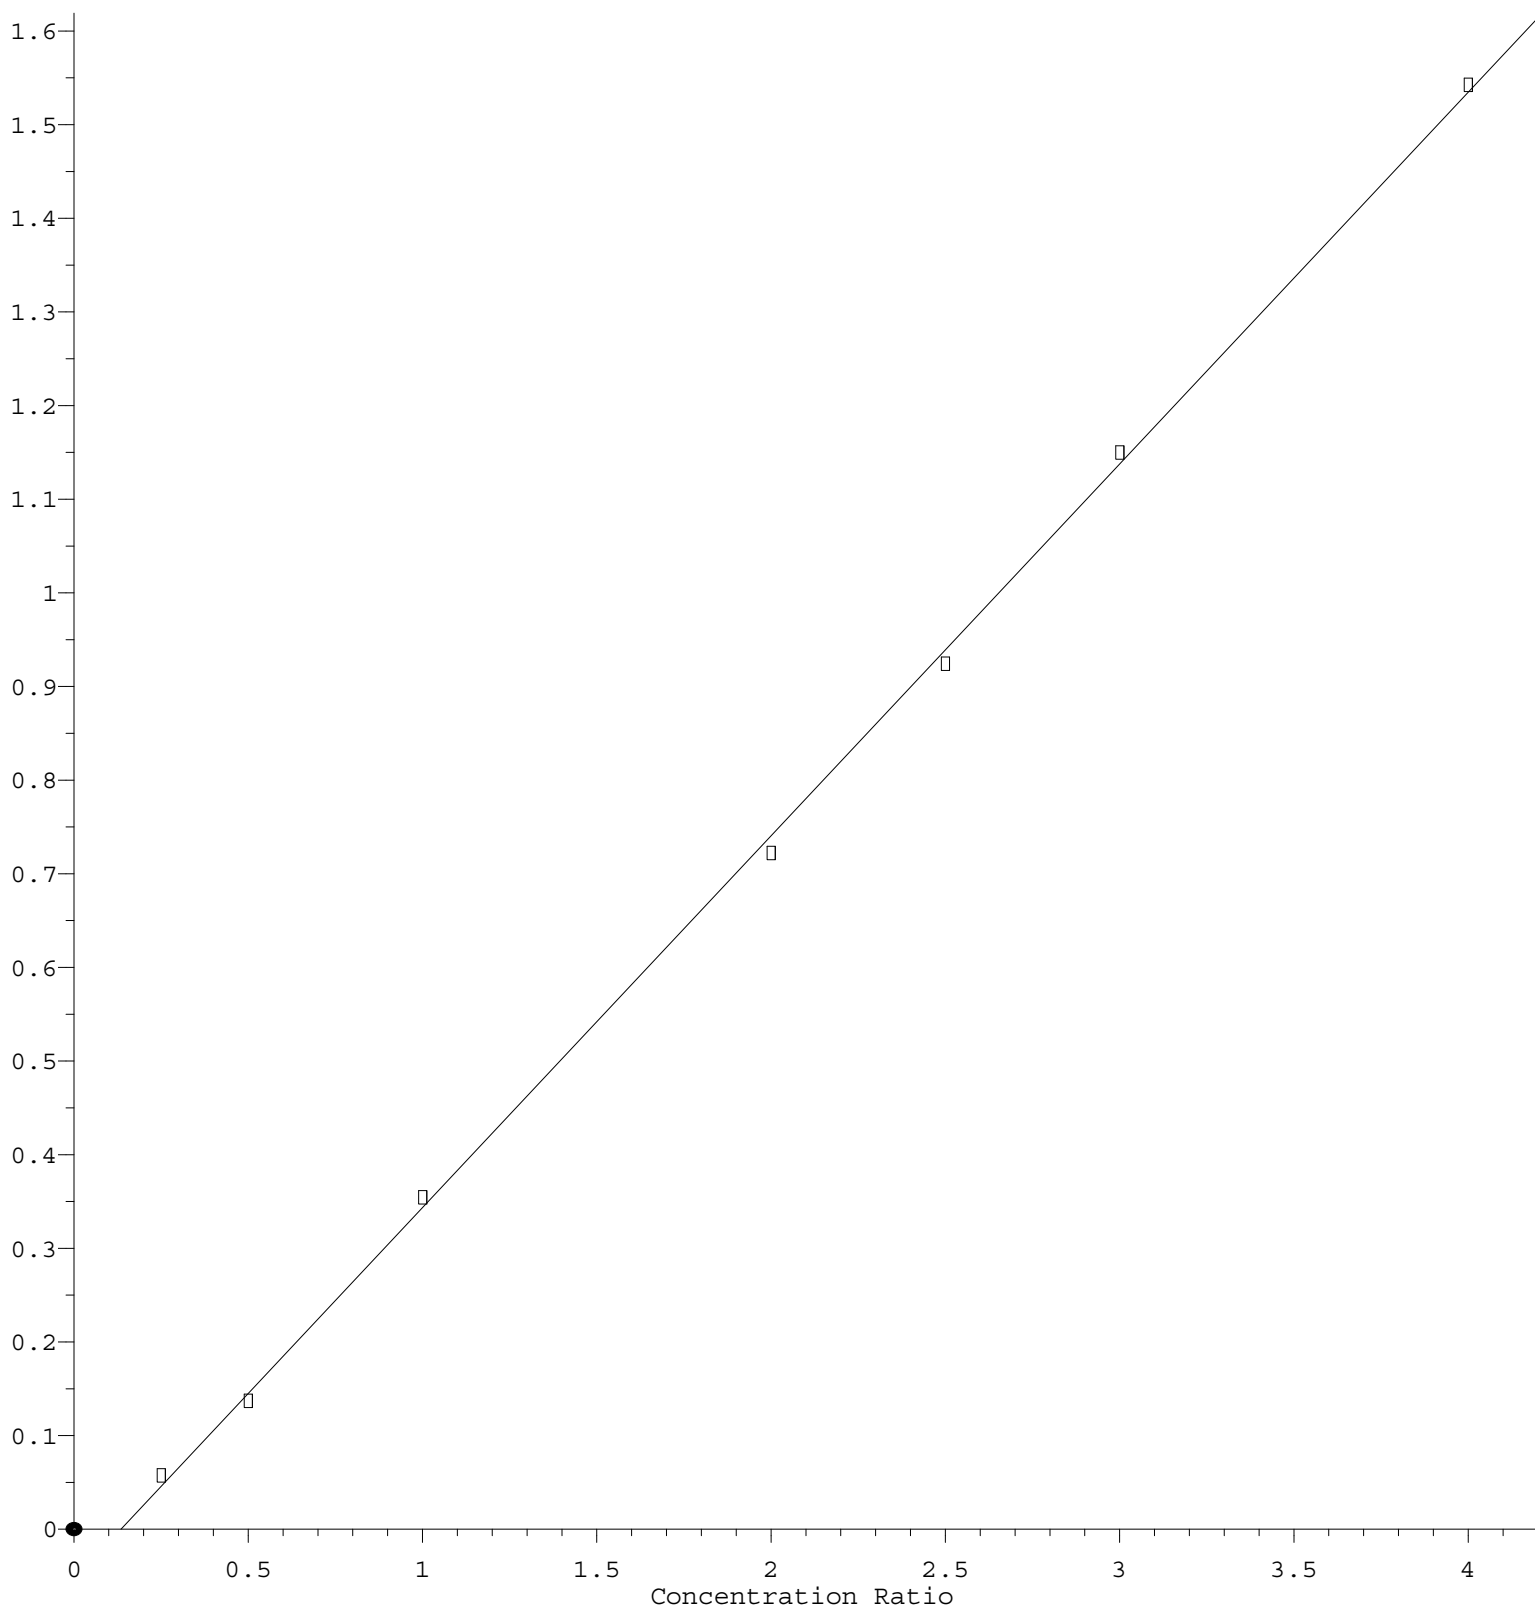


$$\text{Response} = 3.972\text{e-}001 * \text{Amt} - 5.356\text{e-}002$$

Coef of Det (r^2) = 0.999403 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP091322.M

Calibration Table Last Updated: Tue Sep 13 15:49:51 2022


4,6-Dinitro-2-methylphenol

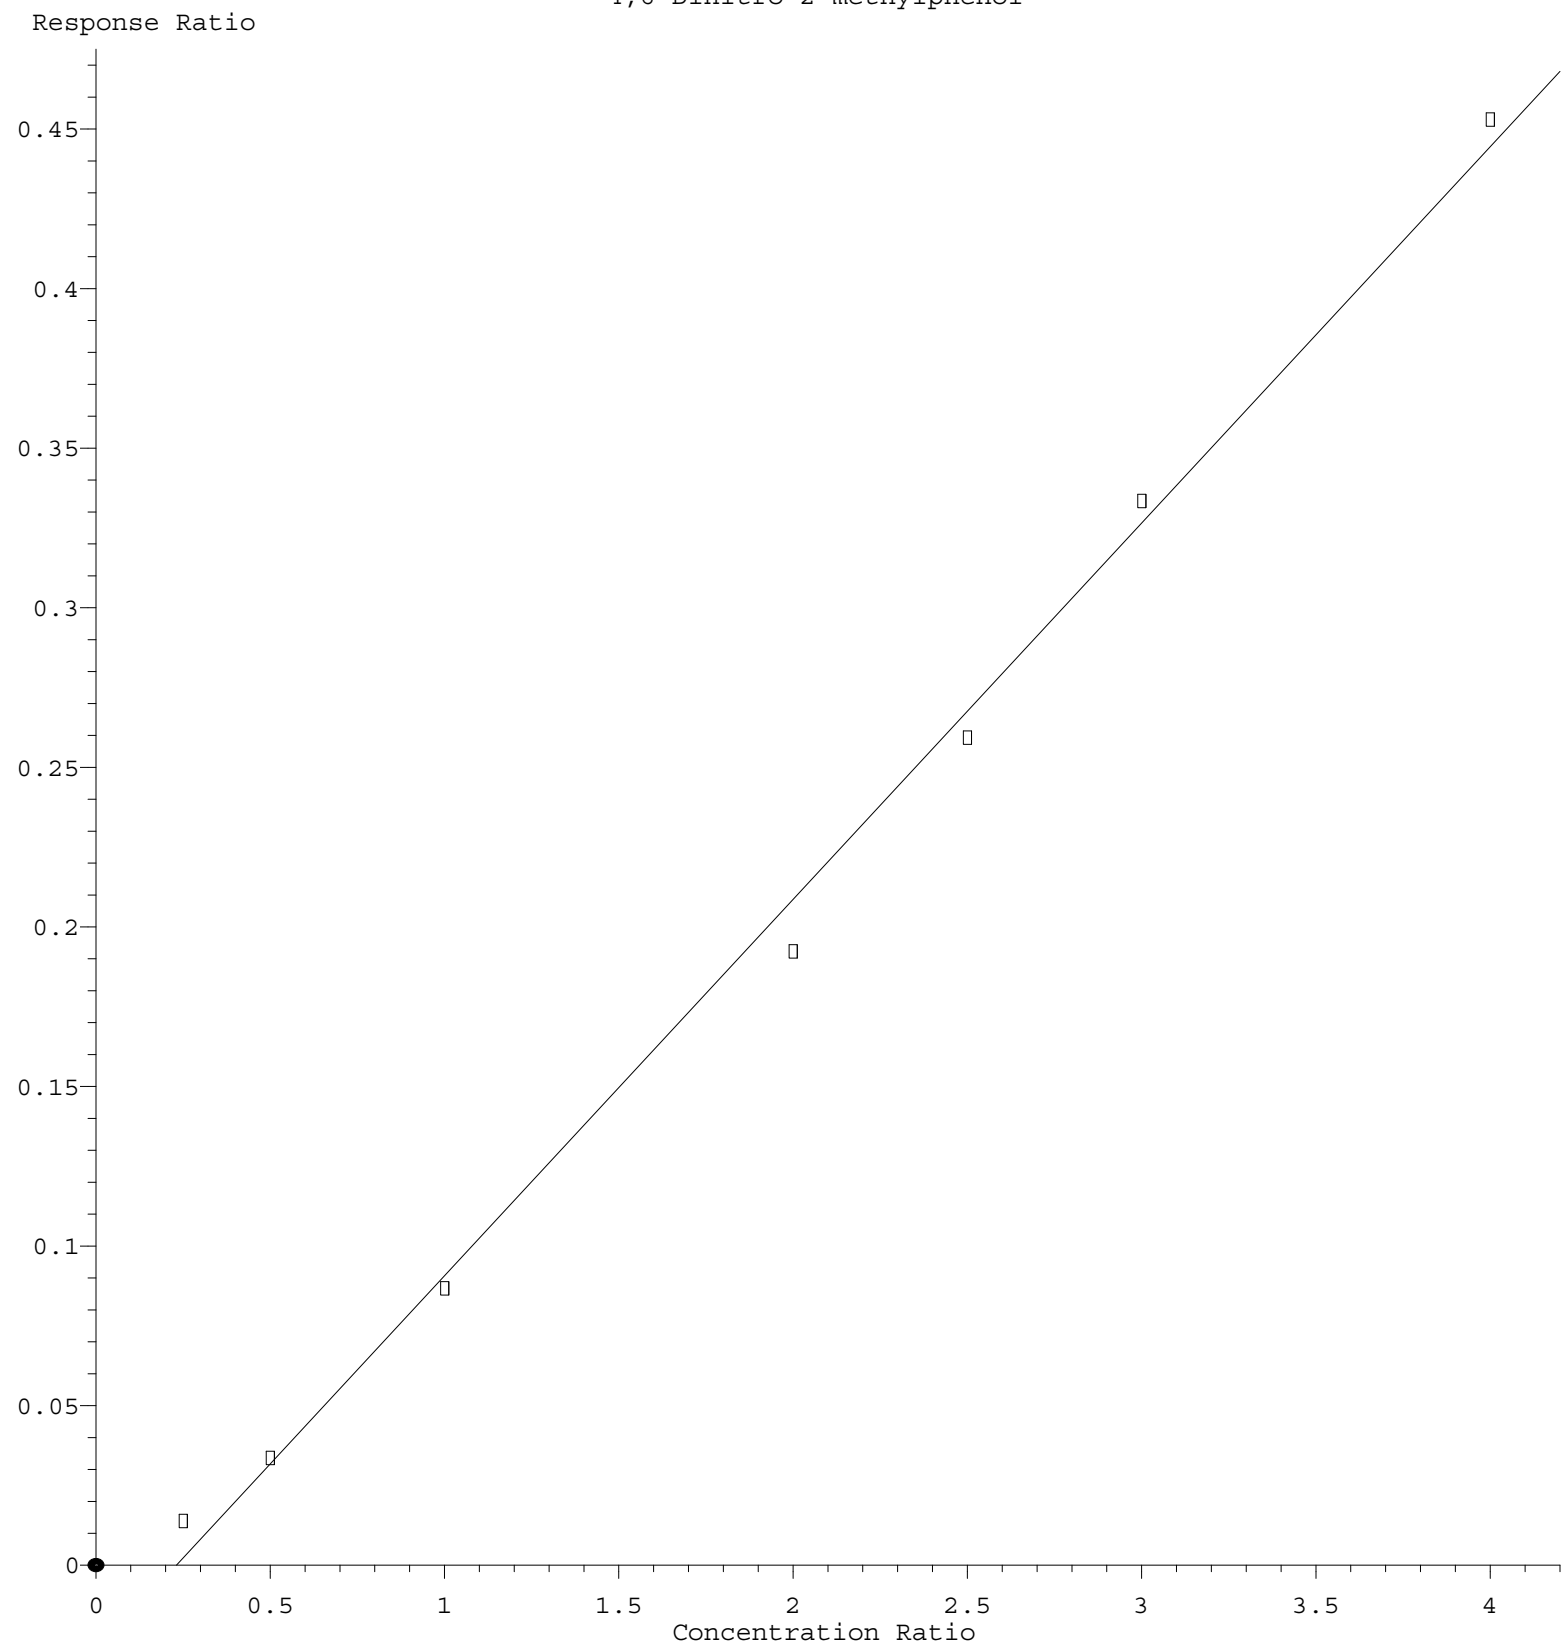

Response = $1.180 \times 10^{-1} \times \text{Amt} - 2.730 \times 10^{-2}$
 Coef of Det (r^2) = 0.996201 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP091322.M
 Calibration Table Last Updated: Tue Sep 13 15:49:51 2022

Butylbenzylphthalate

Response Ratio

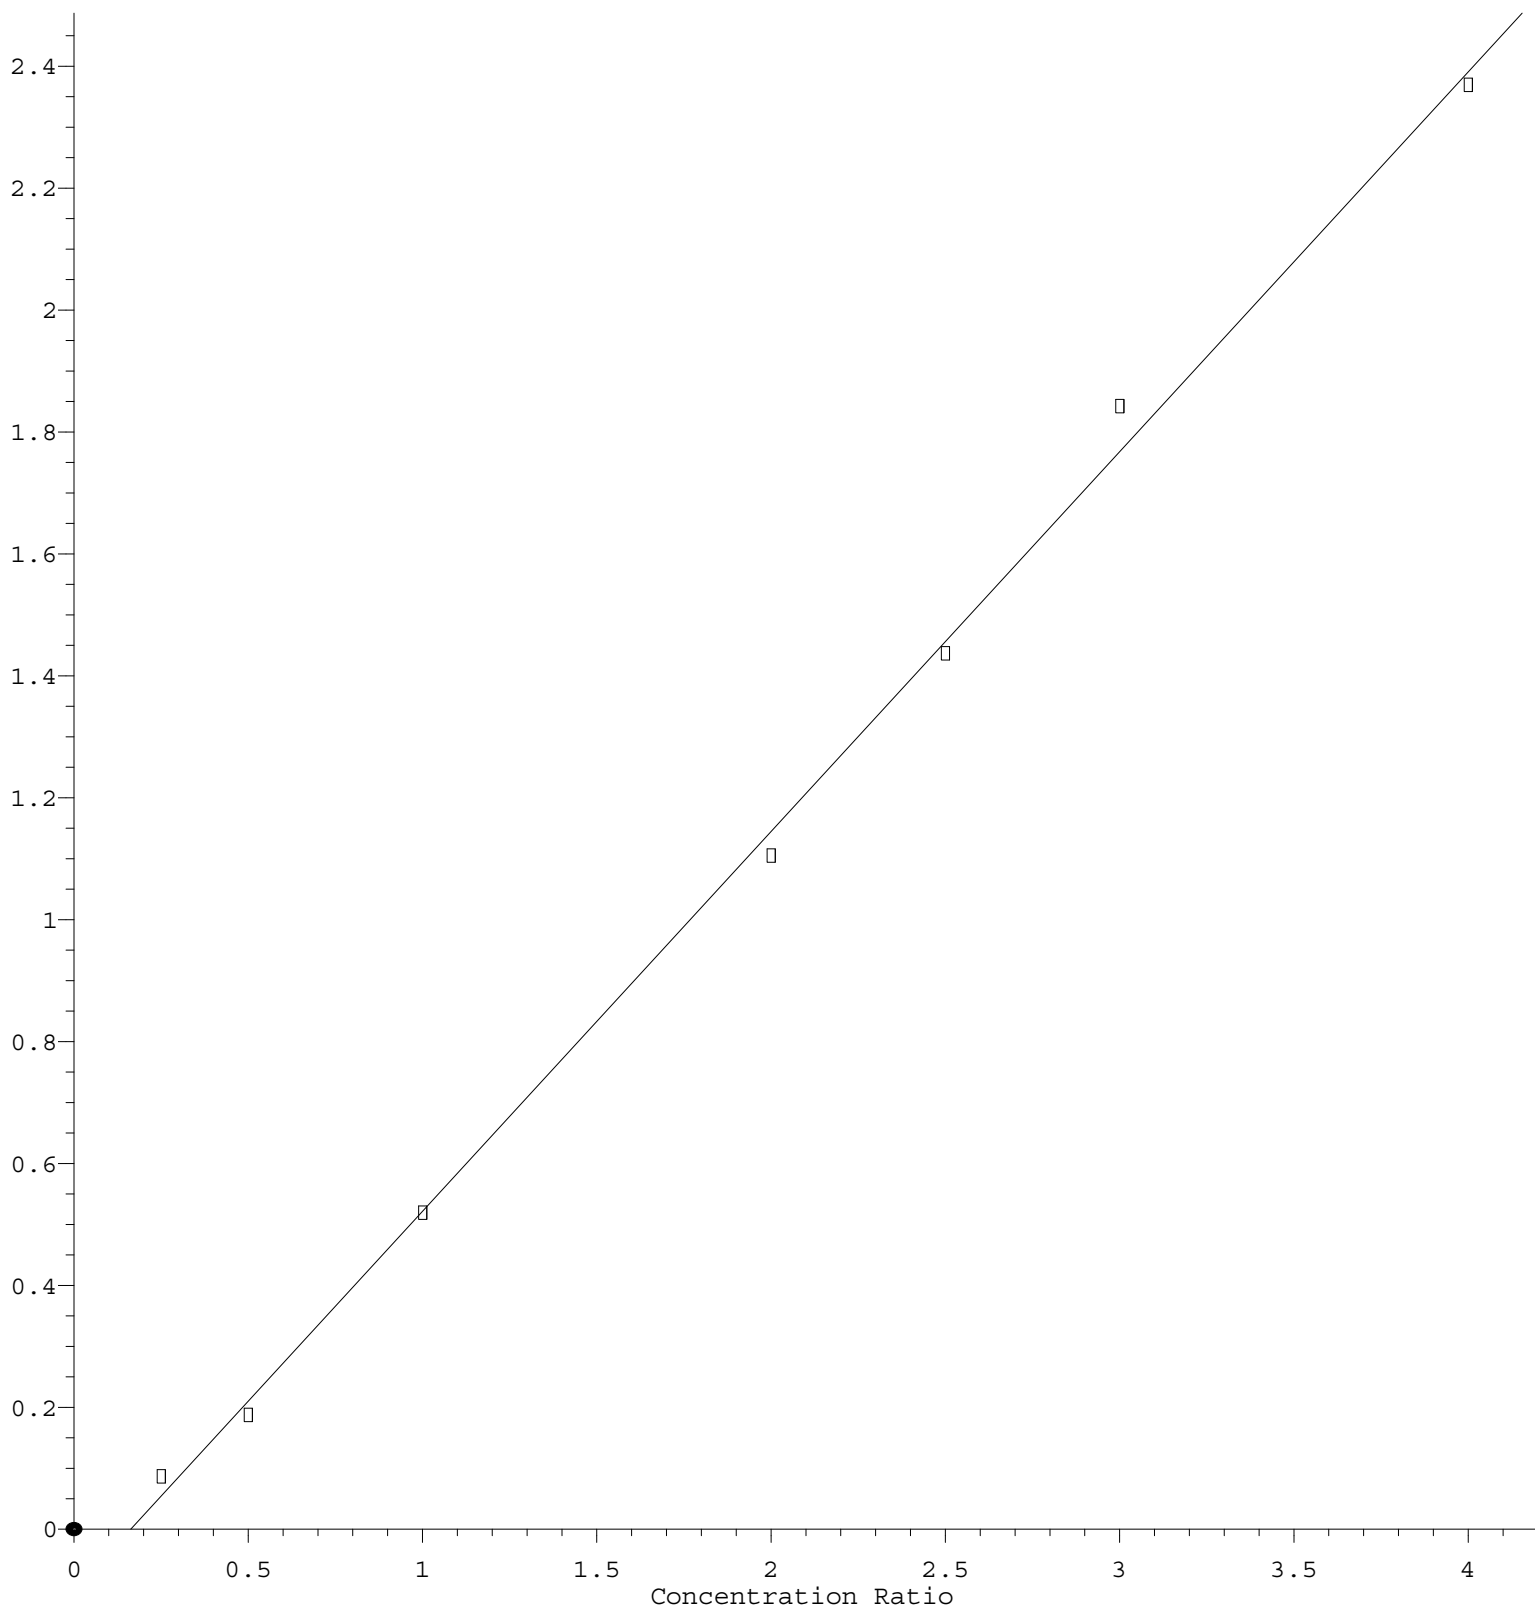

$$\text{Response} = 6.232\text{e-}001 * \text{Amt} - 1.015\text{e-}001$$


Coef of Det (r^2) = 0.997867 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP091322.M

Calibration Table Last Updated: Tue Sep 13 15:49:51 2022

Di-n-octyl phthalate

Response Ratio

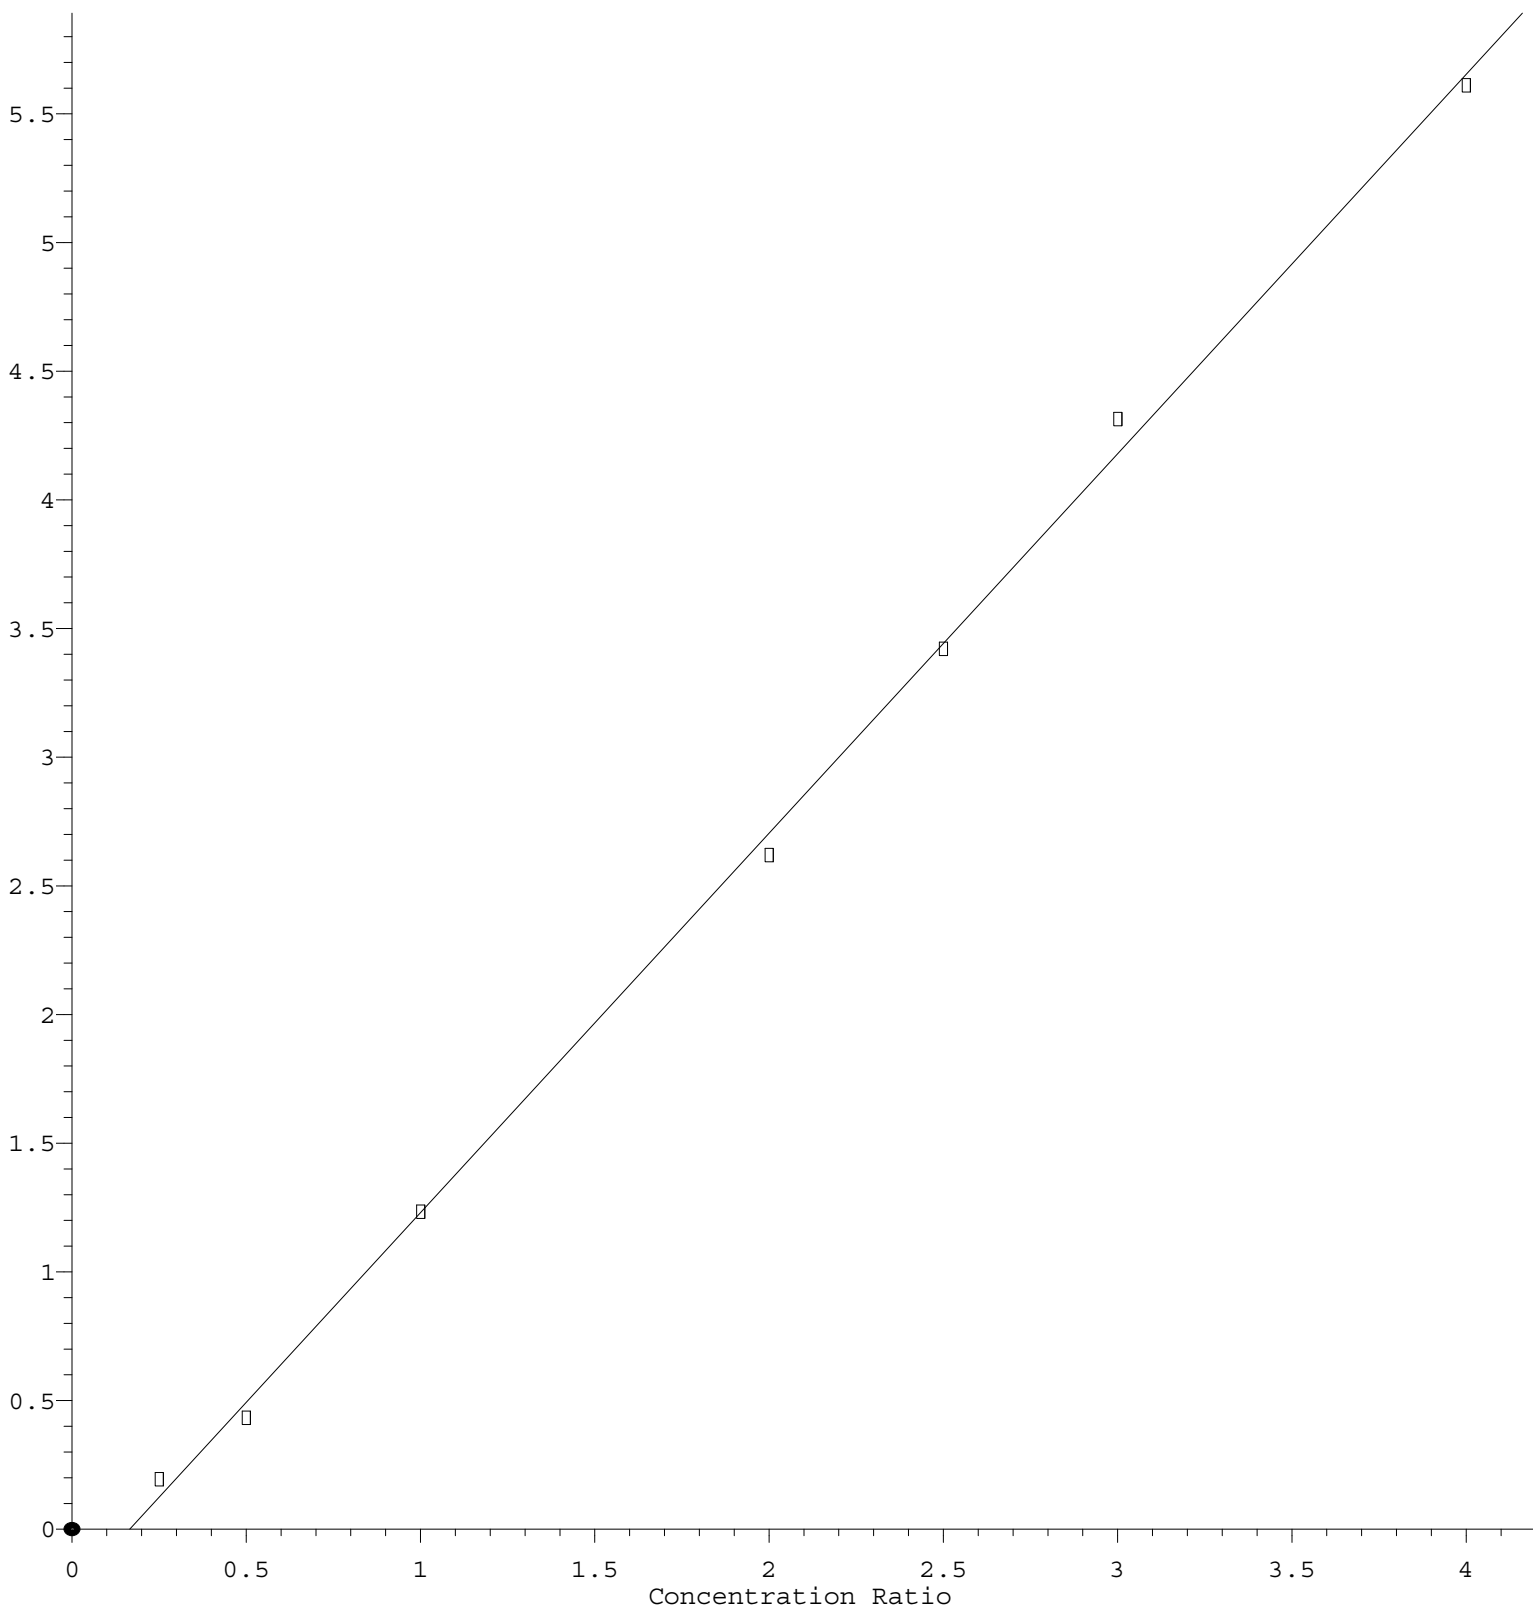

$$\text{Response} = 1.475\text{e}+000 * \text{Amt} - 2.450\text{e}-001$$


Coef of Det (r^2) = 0.998555 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP091322.M

Calibration Table Last Updated: Tue Sep 13 15:49:51 2022

Bis(2-ethylhexyl)phthalate

Response Ratio

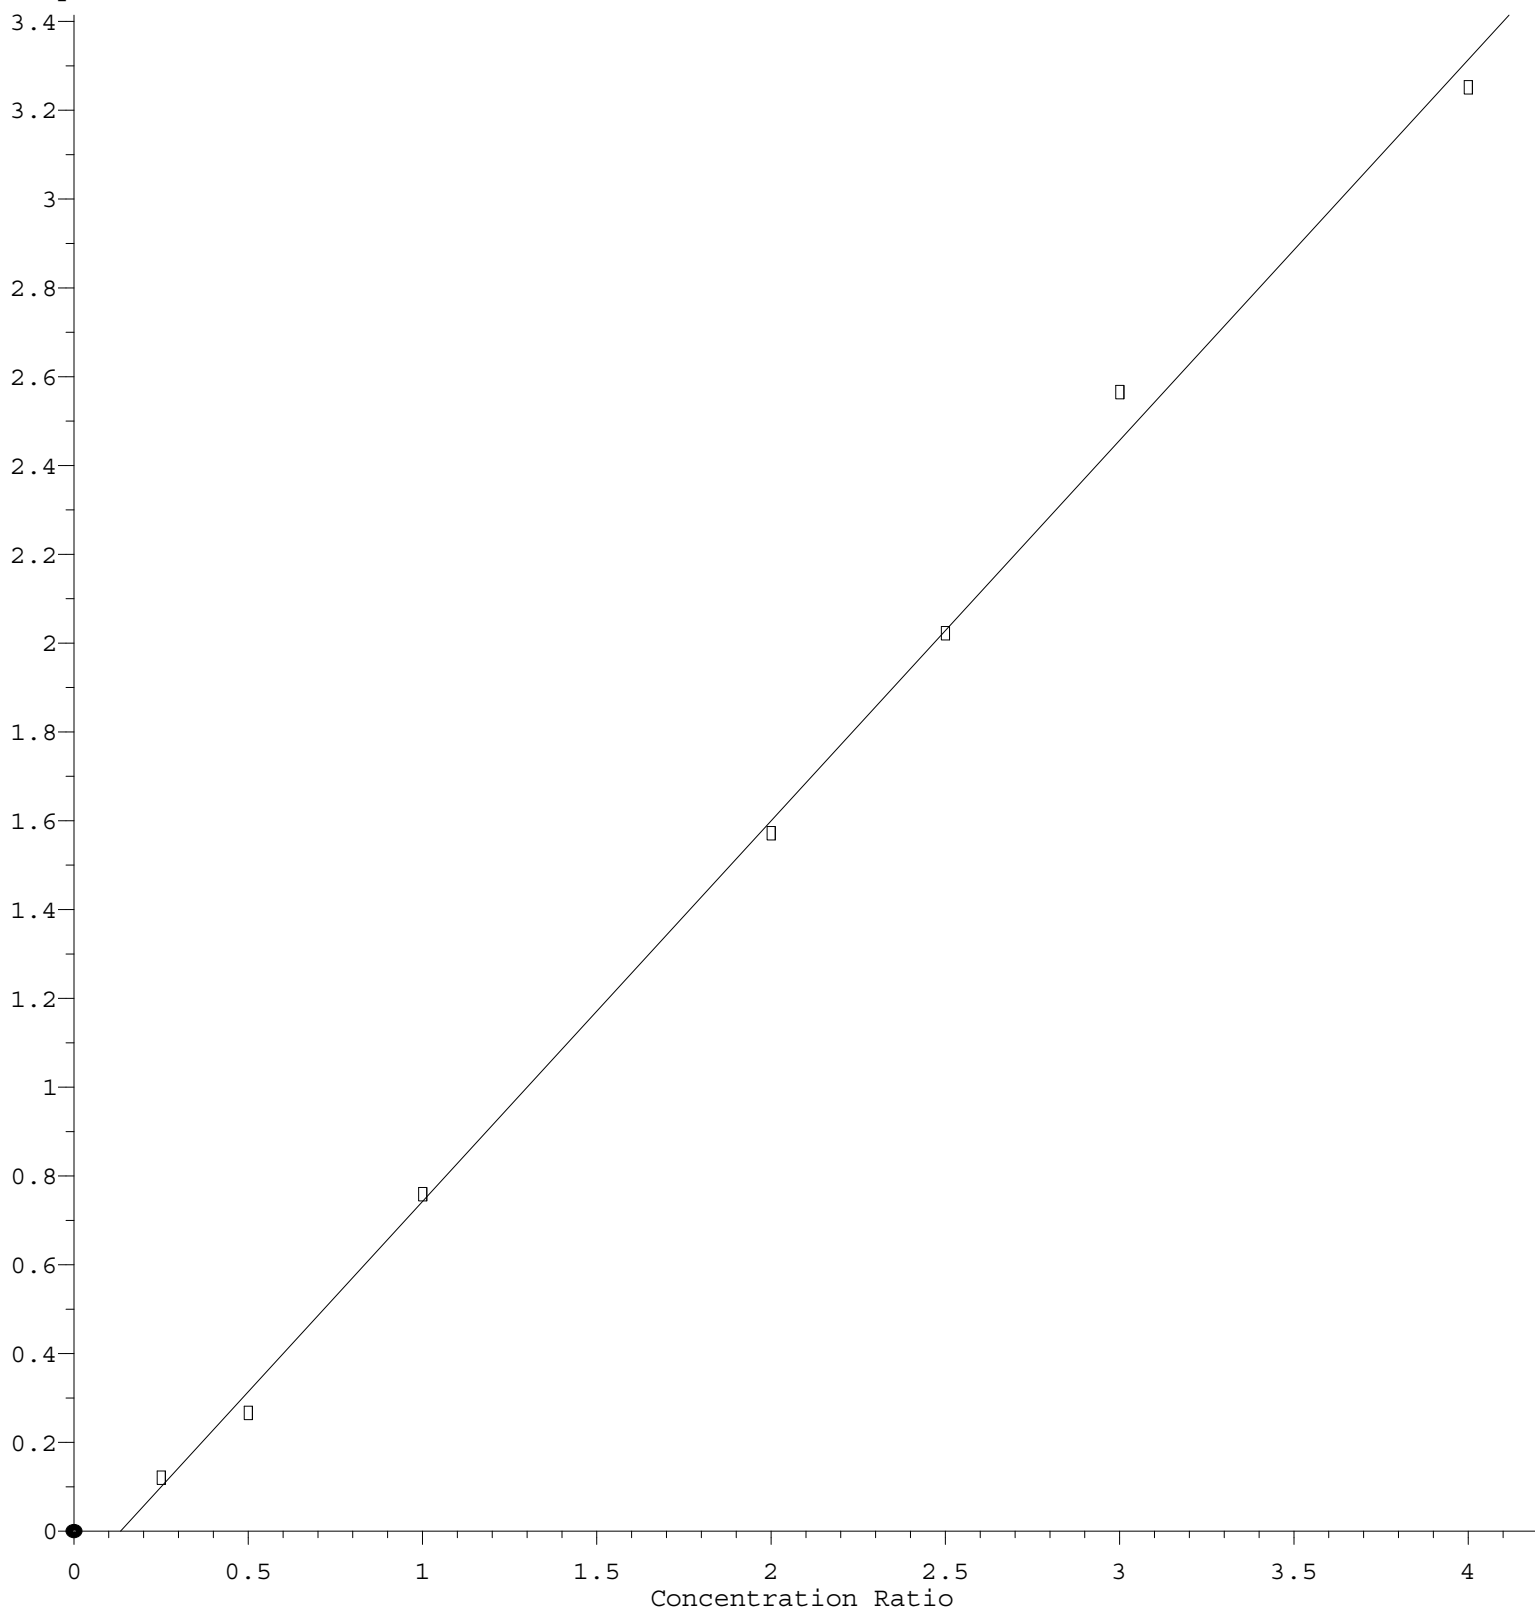

$$\text{Response} = 8.571\text{e-}001 * \text{Amt} - 1.145\text{e-}001$$

Coef of Det (r^2) = 0.997709 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP091322.M

Calibration Table Last Updated: Tue Sep 13 15:49:51 2022