
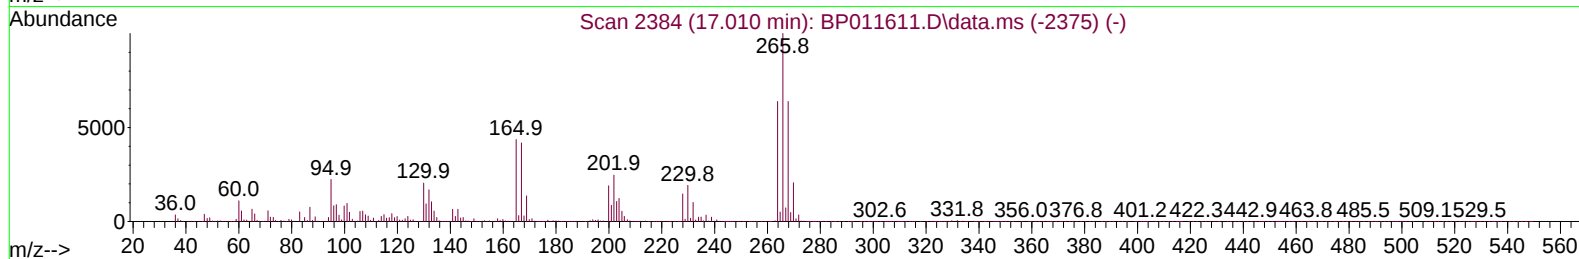
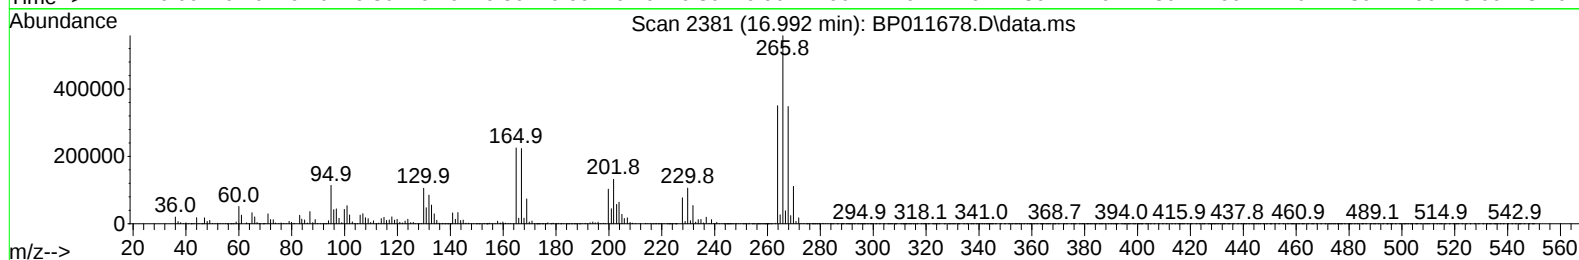


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091322\
 Data File : BP011678.D
 Acq On : 13 Sep 2022 10:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 14:04:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 13 13:59:15 2022
 Response via : Initial Calibration

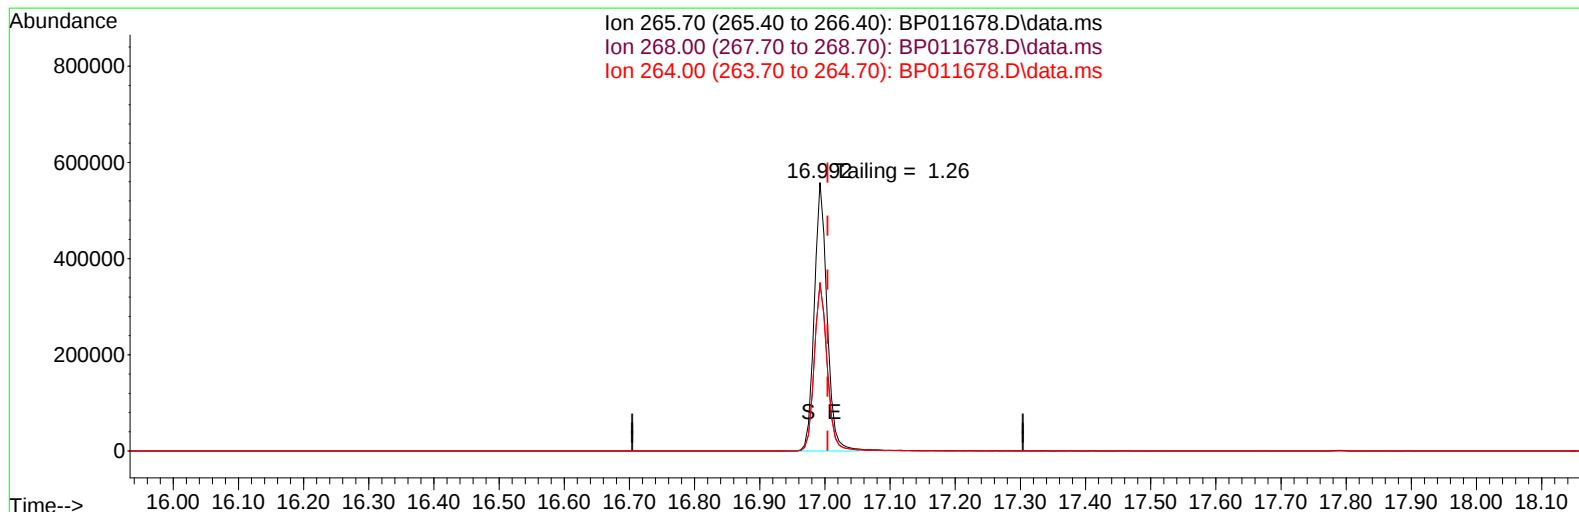

TIC: BP011678.D\data.ms

(70) Pentachlorophenol (C)




16.992min (-0.012) 2036500.24 ng

response 766718

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.40
264.00	63.00	62.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091322\
 Data File : BP011678.D
 Acq On : 13 Sep 2022 10:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 14:04:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 13 13:59:15 2022
 Response via : Initial Calibration

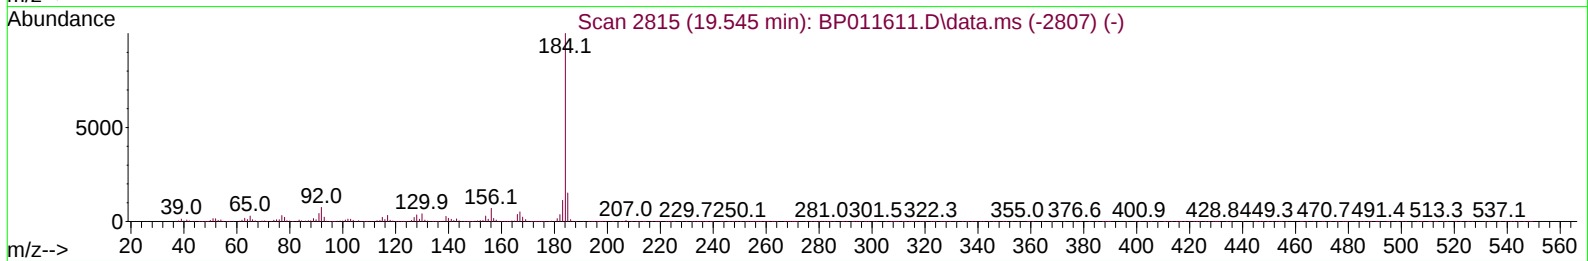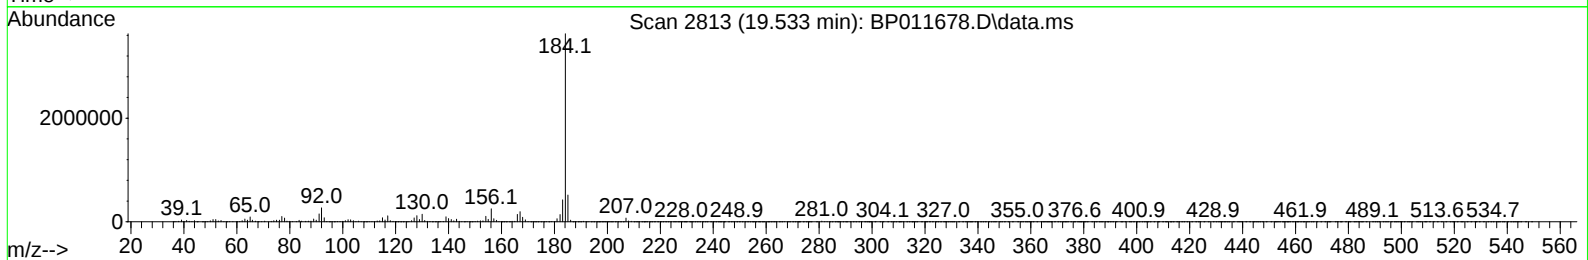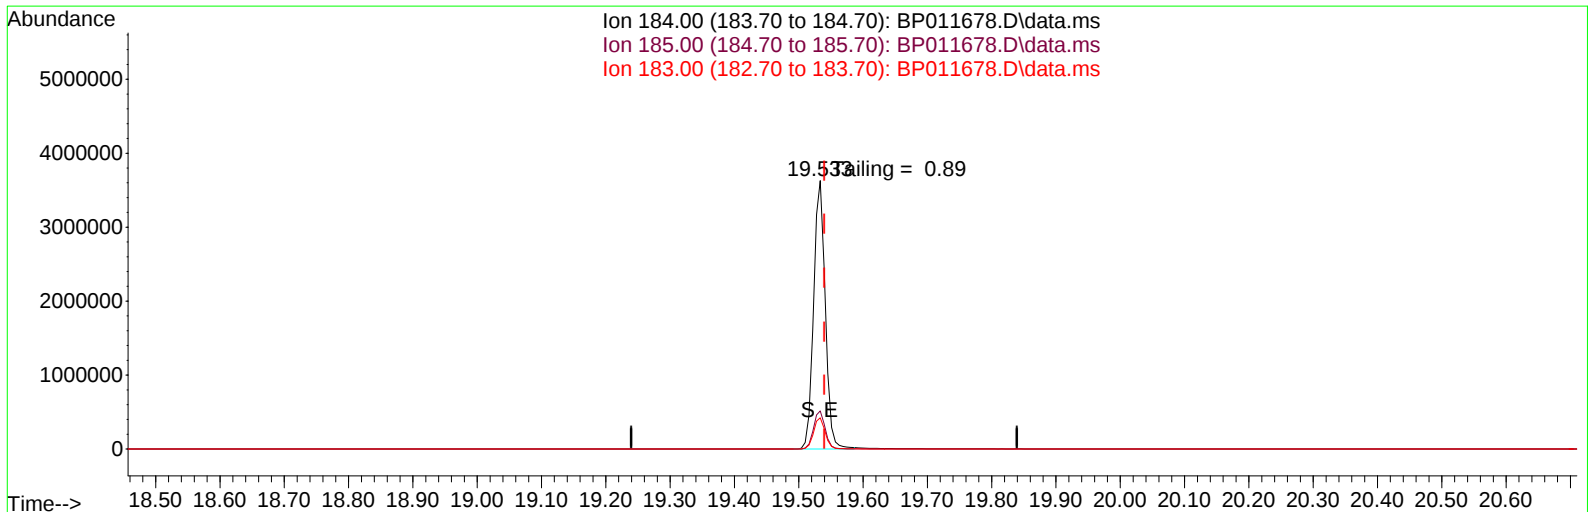

TIC: BP011678.D\data.ms

(77) Benzidine**19.533min (-0.006) 424004.01 ng****response 4643848**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.18
183.00	11.30	11.64
0.00	0.00	0.00