


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091322\
 Data File : BP011678.D
 Acq On : 13 Sep 2022 10:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 13 15:49:51 2022

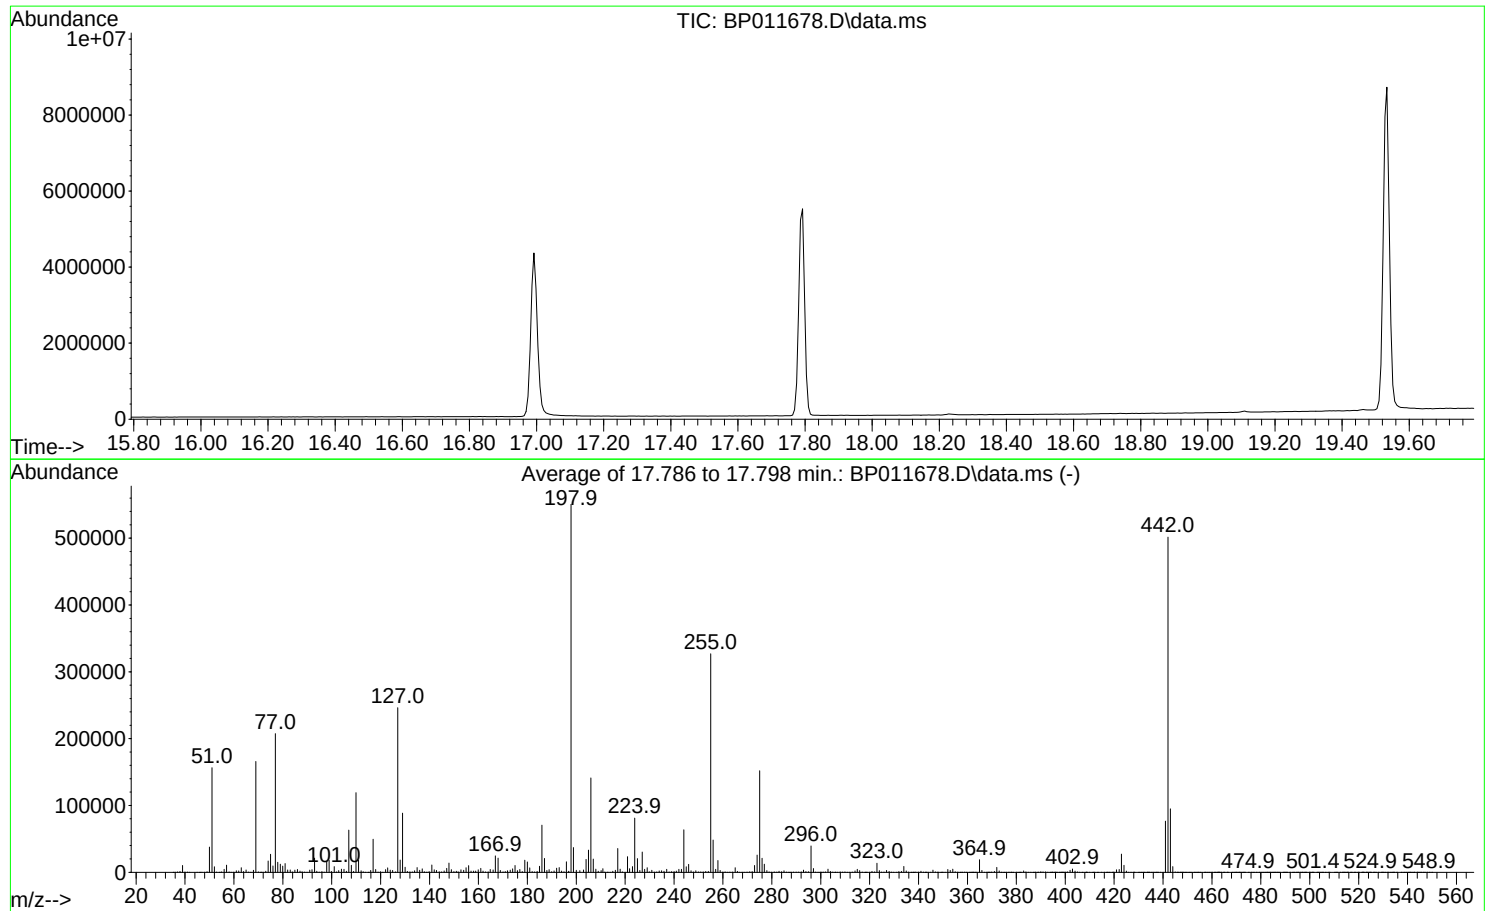




AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	156413	PASS
68	69	0.00	2	1.8	2916	PASS
69	198	0.00	100	30.1	165818	PASS
70	69	0.00	2	0.4	732	PASS
127	198	10	80	44.7	246236	PASS
197	198	0.00	2	0.3	1486	PASS
198	198	100	100	100.0	550528	PASS
199	198	5	9	6.7	37137	PASS
275	198	10	60	27.6	151842	PASS
365	198	1	100	3.4	18700	PASS
441	198	0.01	100	13.9	76581	PASS
442	442	100	100	100.0	501584	PASS
443	442	15	24	18.9	94882	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091322\
 Data File : BP011678.D
 Acq On : 13 Sep 2022 10:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 13 14:04:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 13 13:59:15 2022
 Response via : Initial Calibration

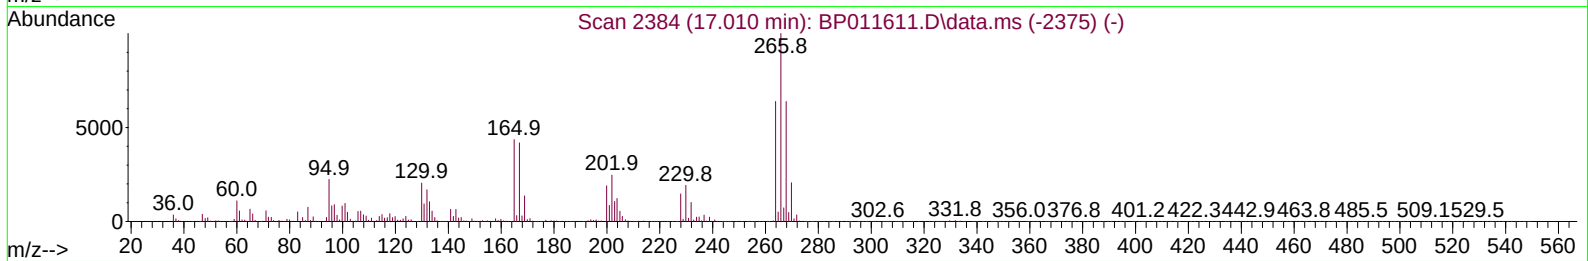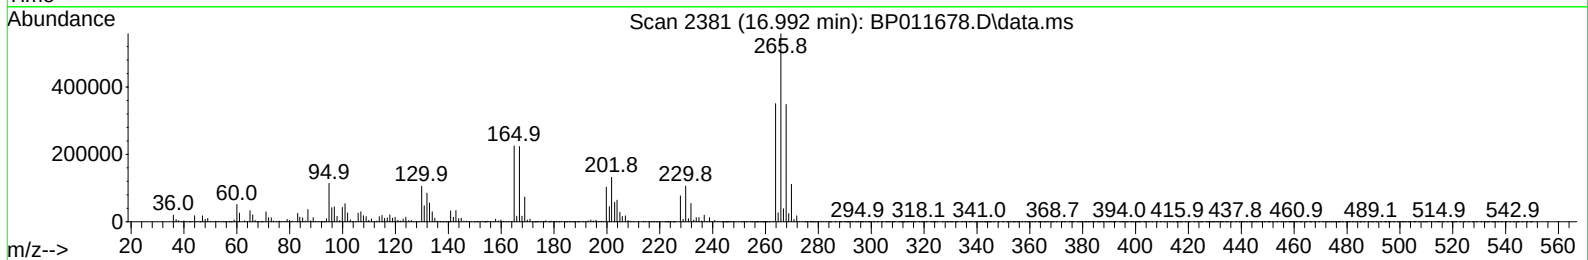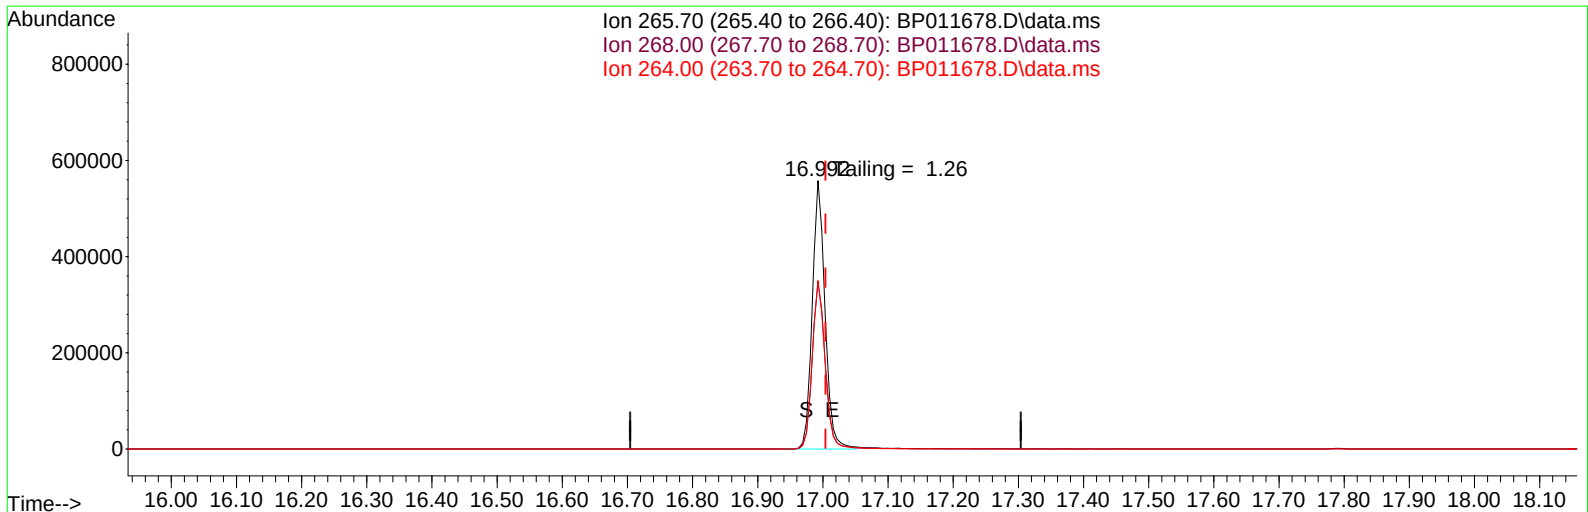

TIC: BP011678.D\data.ms

(70) Pentachlorophenol (C)

16.992min (-0.012) 2036500.24 ng




response 766718

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.40
264.00	63.00	62.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091322\
Data File : BP011678.D
Acq On : 13 Sep 2022 10:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 13 14:04:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 13 13:59:15 2022
Response via : Initial Calibration

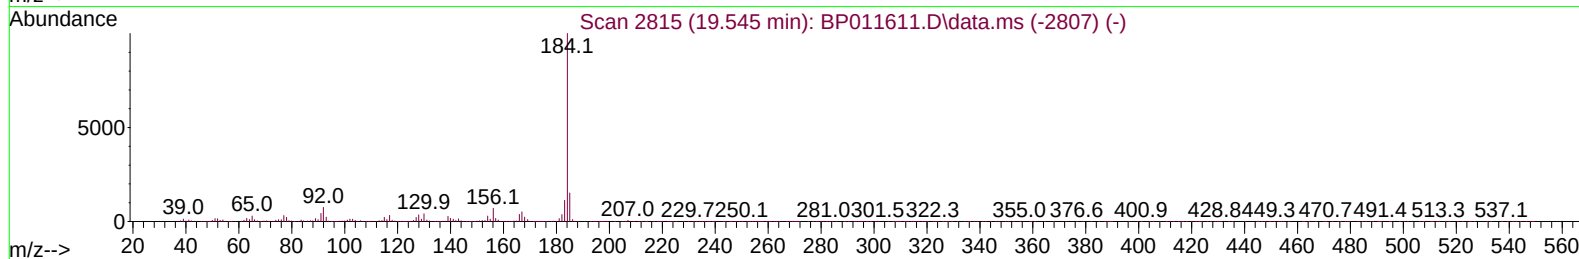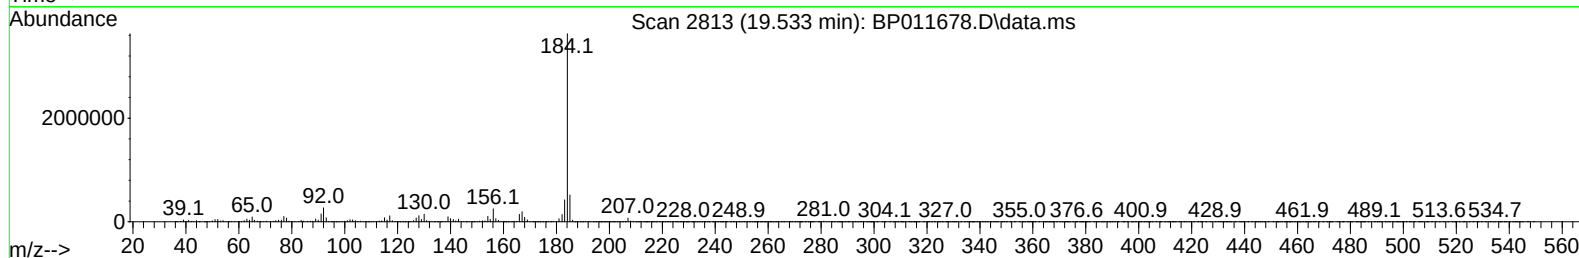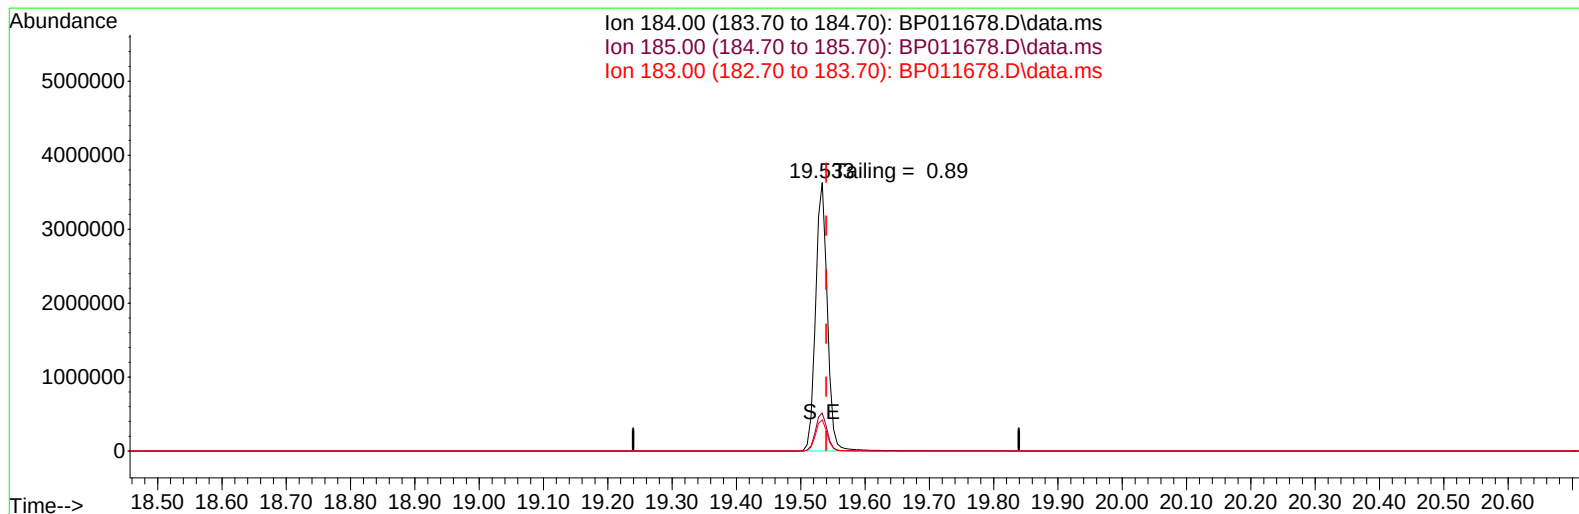

TIC: BP011678.D\data.ms

(77) Benzidine

19.533min (-0.006) 424004.01 ng

response 4643848

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.18
183.00	11.30	11.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/13/2022	BNA_P	<u>BP011678.D</u>
Compound Name	Response	Retention Time
DDT	2077884	20.73
DDD	11588	20.3
DDE	1141	19.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12729	2090613	0.61

Instrument :
BNA_P
ClientSampleId :
DFTPP