

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091324\
 Data File : BP021911.D
 Acq On : 13 Sep 2024 16:30
 Operator : RC/JU
 Sample : P3900-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DDCG6

Quant Time: Sep 13 17:11:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 12 12:48:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.757	152	95090	20.000	ng/u1	0.02
20) Naphthalene-d8	10.534	136	383018	20.000	ng/u1	0.03
38) Acenaphthene-d10	14.369	164	278791	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.151	188	655932	20.000	ng/u1	0.00
79) Chrysene-d12	21.592	240	579649	20.000	ng/u1	0.00
88) Perylene-d12	24.904	264	837782	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	10848	3.690	ng/uL	0.01
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	6.934	99	69123	8.507	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	7.093	67	109359	23.173	ng/u1	0.02
11) 2-Chlorophenol-d4	7.299	132	149137	26.368	ng/u1	0.02
15) 4-Methylphenol-d8	8.452	113	156488	24.123	ng/u1	0.02
21) Nitrobenzene-d5	8.899	128	93280	39.104	ng/u1	0.02
24) 2-Nitrophenol-d4	9.616	143	102259	37.709	ng/u1	0.02
28) 2,4-Dichlorophenol-d3	10.151	165	206123	34.324	ng/u1	0.02
31) 4-Chloroaniline-d4	10.657	131	42086	4.809	ng/u1	0.02
46) Dimethylphthalate-d6	13.769	166	738834	35.275	ng/u1	0.00
49) Acenaphthylene-d8	14.057	160	767174	33.391	ng/u1	0.00
54) 4-Nitrophenol-d4	14.575	143	38943	9.835	ng/u1	0.00
60) Fluorene-d10	15.369	176	642282	32.262	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.486	200	103589	27.604	ng/u1	0.00
73) Anthracene-d10	17.251	188	1120124	36.763	ng/u1	0.00
81) Pyrene-d10	19.622	212	1413925	44.089	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.680	264	1558711	35.750	ng/u1	-0.01
Target Compounds						
35) 4-Chloro-3-methylphenol	11.810	107	14177	2.041	ng/u1	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091324\
Data File : BP021911.D
Acq On : 13 Sep 2024 16:30
Operator : RC/JU
Sample : P3900-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCG6

Quant Time: Sep 13 17:11:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 12 12:48:41 2024
Response via : Initial Calibration

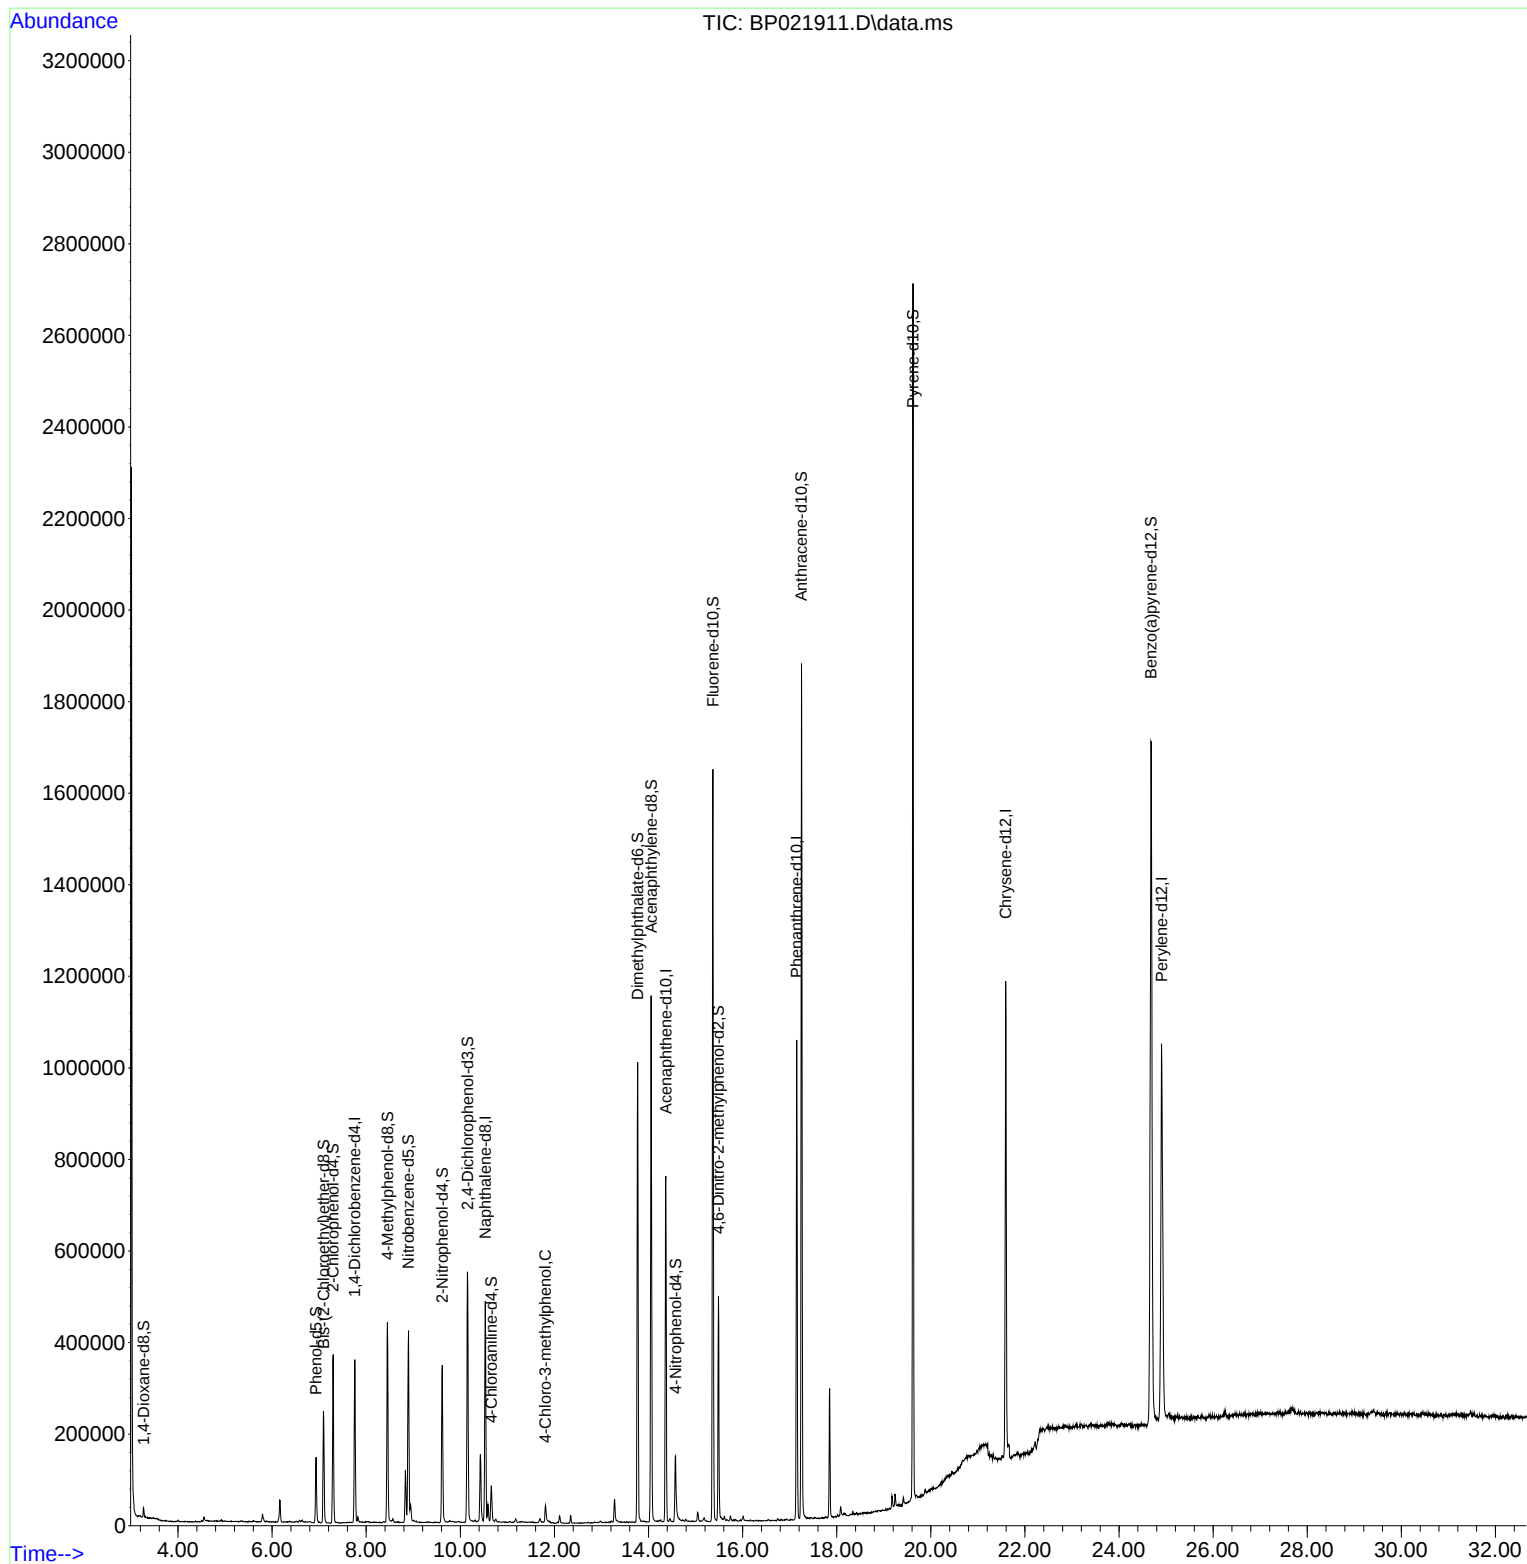

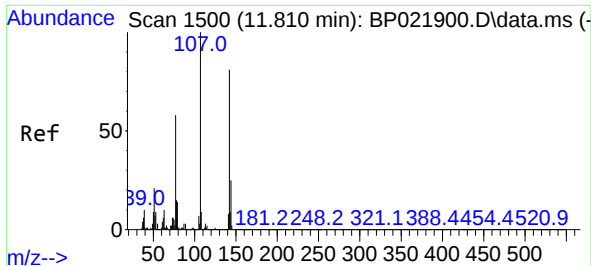

#35
 4-Chloro-3-methylphenol
 Concen: 2.041 ng/ul
 RT: 11.810 min Scan# 11
 Delta R.T. 0.018 min
 Lab File: BP021911.D
 Acq: 13 Sep 2024 16:30

Instrument :
 BNA_P
 ClientSampleId :
 DDCG6

Tgt Ion:107 Resp: 14177
 Ion Ratio Lower Upper
 107 100
 144 25.3 21.0 31.6
 142 82.9 61.8 92.8

