

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091324\
 Data File : BP021912.D
 Acq On : 13 Sep 2024 17:11
 Operator : RC/JU
 Sample : P3900-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DDCG7

Quant Time: Sep 13 18:01:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 12 12:48:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.757	152	109801	20.000	ng/u1	0.02
20) Naphthalene-d8	10.528	136	444241	20.000	ng/u1	0.02
38) Acenaphthene-d10	14.369	164	329801	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.157	188	779899	20.000	ng/u1	0.00
79) Chrysene-d12	21.592	240	825547	20.000	ng/u1	0.00
88) Perylene-d12	24.927	264	993945	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	10424	3.071	ng/uL	0.01
4) Pyridine-d5	3.687	84	18830	1.884	ng/u1	0.02
7) Phenol-d5	6.934	99	85593	9.123	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	7.093	67	146167	26.823	ng/u1	0.02
11) 2-Chlorophenol-d4	7.293	132	175802	26.919	ng/u1	0.02
15) 4-Methylphenol-d8	8.452	113	149634	19.976	ng/u1	0.02
21) Nitrobenzene-d5	8.899	128	91799	33.180	ng/u1	0.02
24) 2-Nitrophenol-d4	9.616	143	77601	24.673	ng/u1	0.02
28) 2,4-Dichlorophenol-d3	10.151	165	150924	21.669	ng/u1	0.02
31) 4-Chloroaniline-d4	10.657	131	187605	18.482	ng/u1	0.02
46) Dimethylphthalate-d6	13.769	166	746675	30.135	ng/u1	0.00
49) Acenaphthylene-d8	14.057	160	752724	27.695	ng/u1	0.00
54) 4-Nitrophenol-d4	14.581	143	21974	4.691	ng/u1	0.01
60) Fluorene-d10	15.369	176	641718	27.248	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.486	200	109659	24.577	ng/u1	0.00
73) Anthracene-d10	17.257	188	1186174	32.742	ng/u1	0.00
81) Pyrene-d10	19.633	212	1517779	33.230	ng/u1	0.01
92) Benzo(a)pyrene-d12	24.680	264	1677088	32.422	ng/u1	-0.01
Target Compounds						
					Qvalue	
35) 4-Chloro-3-methylphenol	11.804	107	14320	1.778	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091324\
Data File : BP021912.D
Acq On : 13 Sep 2024 17:11
Operator : RC/JU
Sample : P3900-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCG7


Quant Time: Sep 13 18:01:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 12 12:48:41 2024
Response via : Initial Calibration

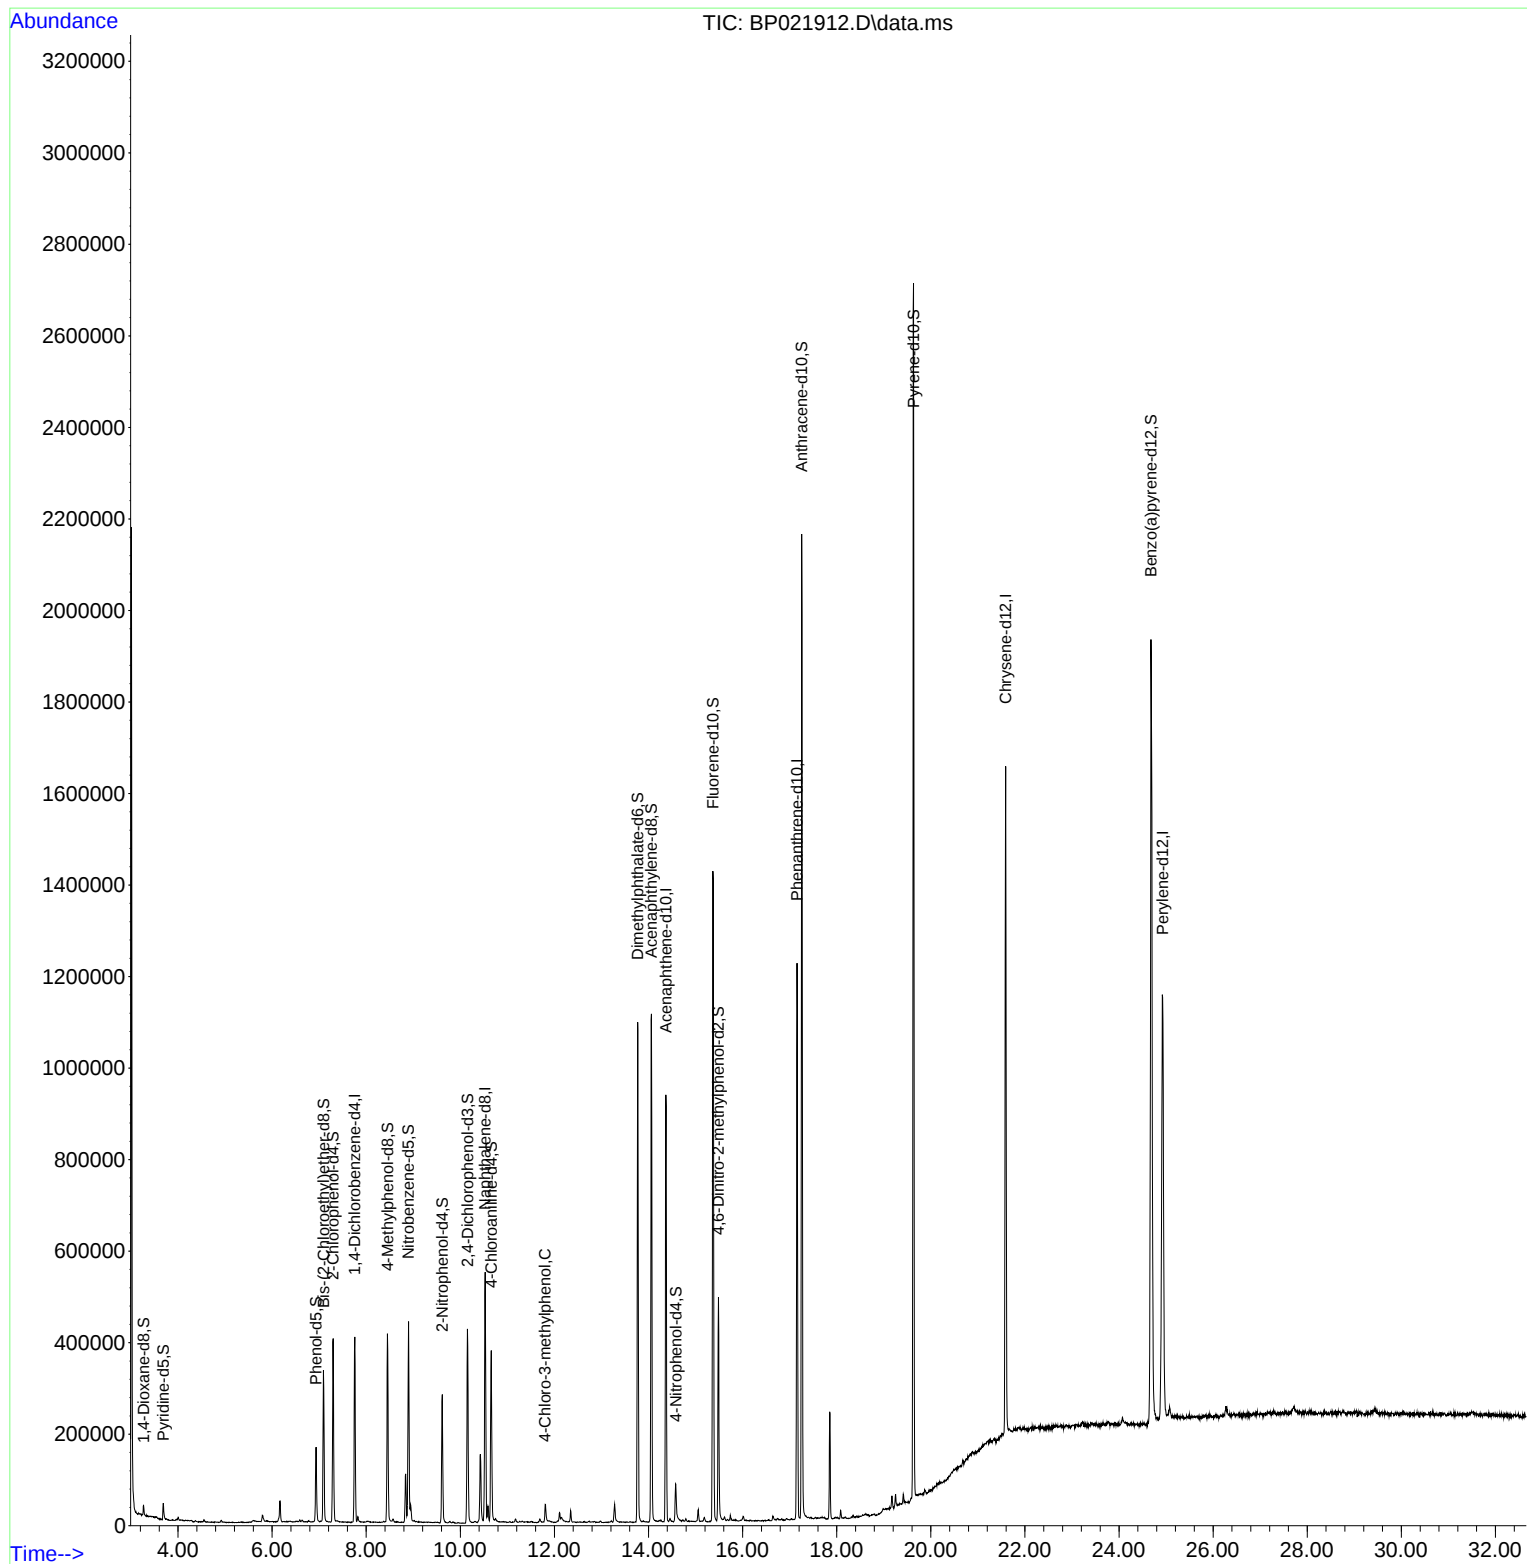

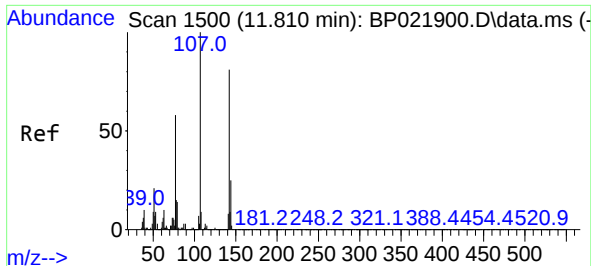

#35
4-Chloro-3-methylphenol
Concen: 1.778 ng/ul
RT: 11.804 min Scan# 14
Delta R.T. 0.012 min
Lab File: BP021912.D
Acq: 13 Sep 2024 17:11

Instrument :
BNA_P
ClientSampleId :
DDCG7

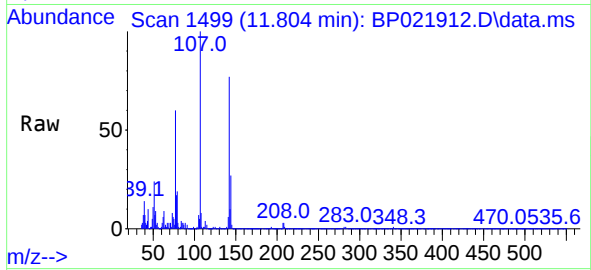

Tgt Ion:107 Resp: 14320
Ion Ratio Lower Upper
107 100
144 27.4 21.0 31.6
142 77.2 61.8 92.8

