
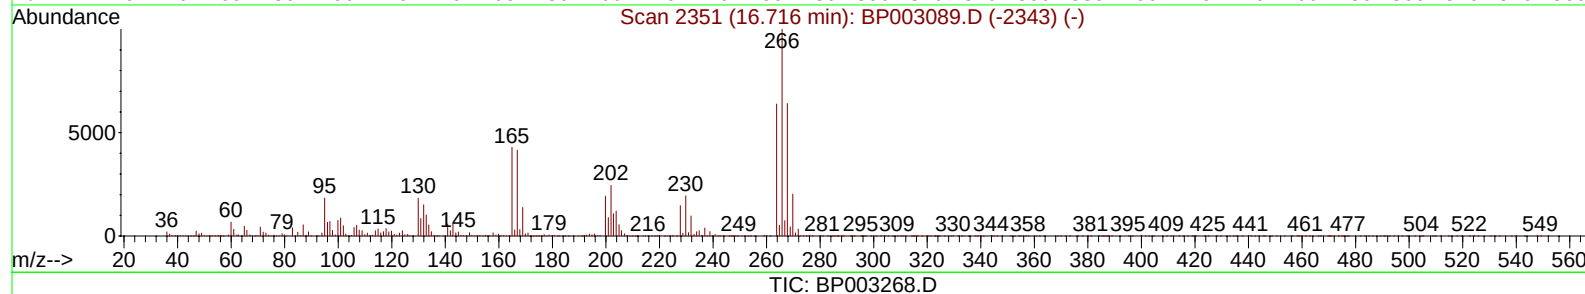
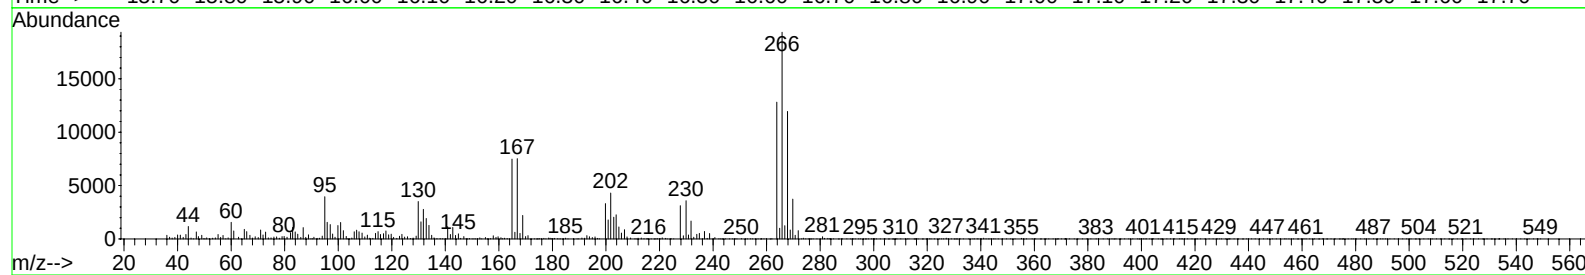


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091420\
Data File : BP003268.D
Acq On : 14 Sep 2020 14:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 18:43:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 01 14:37:05 2020
Response via : Initial Calibration

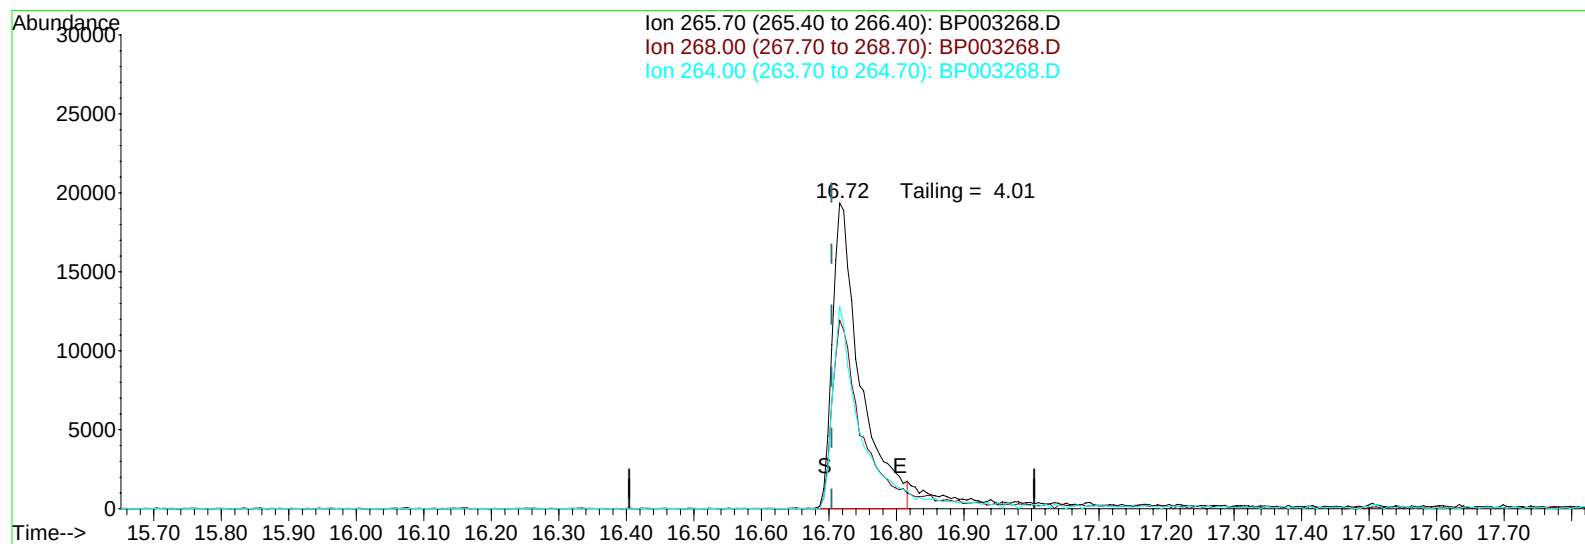

(70) Pentachlorophenol (C)




16.716min (+0.012) 248473.73ng

response 56205

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.70
264.00	63.30	66.20
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091420\
Data File : BP003268.D
Acq On : 14 Sep 2020 14:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 18:43:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 01 14:37:05 2020
Response via : Initial Calibration

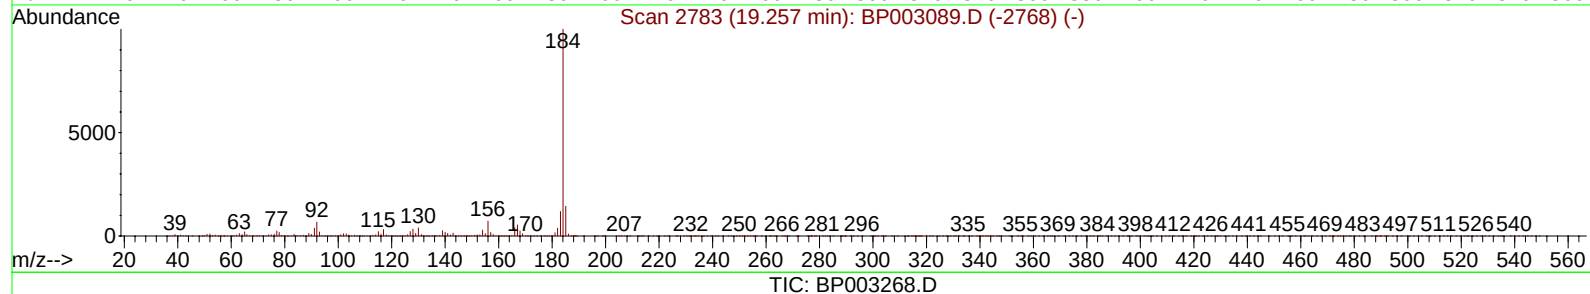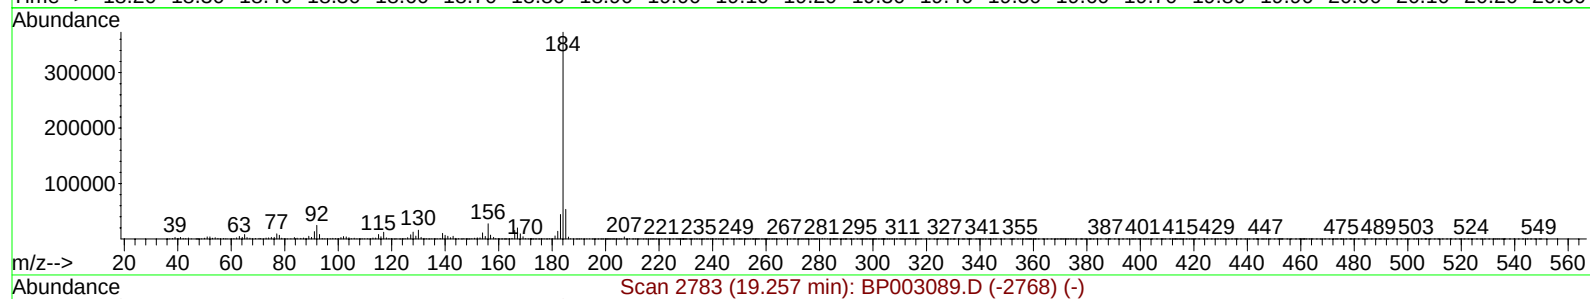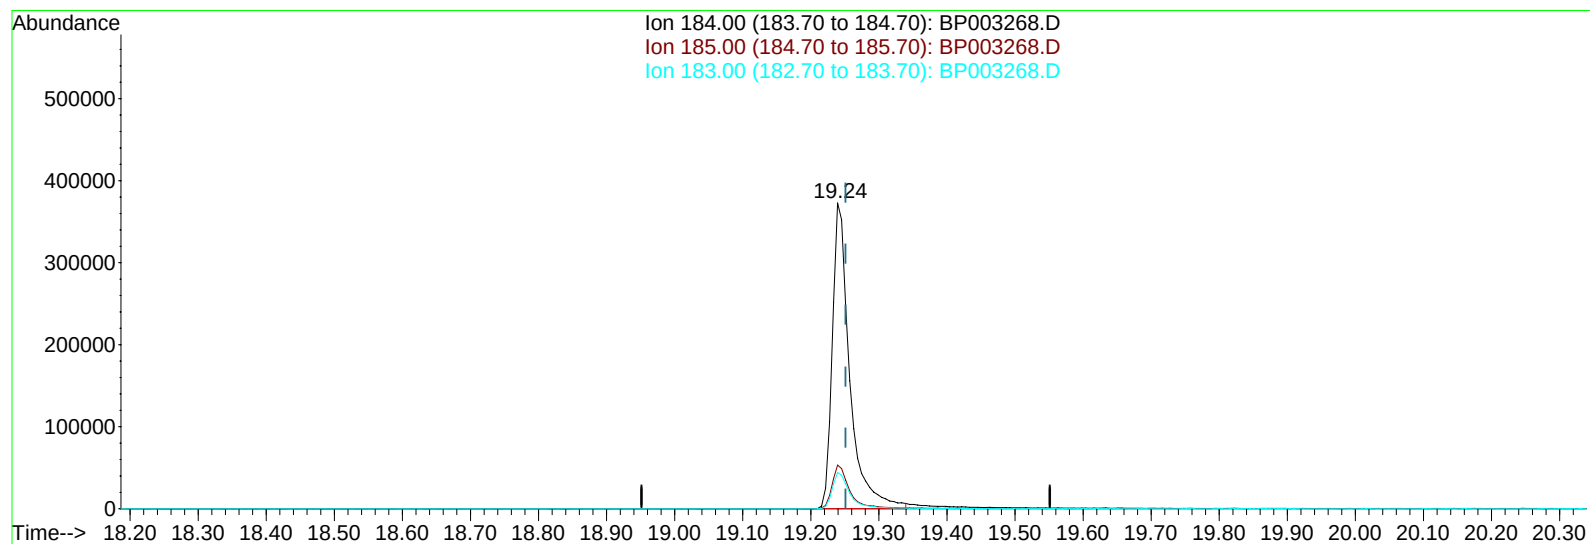

(77) Benzidine

19.239min (-0.012) 271426.06ng

response 663767

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.31
183.00	12.00	11.84
0.00	0.00	0.00